

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060619\
 Data File : VU032509.D
 Acq On : 06 Jun 2019 20:00
 Operator : JC/SP
 Sample : K3224-03
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0C60

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.396	89	95	108	rVB	66101	64490	10.41%	1.155%
2	1.675	175	182	197	rVB	58301	71516	11.55%	1.281%
3	2.267	357	366	378	rVB	116239	173136	27.95%	3.102%
4	2.421	411	414	415	rBV	461	269	0.04%	0.005%
5	2.569	458	460	464	rBV2	467	455	0.07%	0.008%
6	2.833	528	542	564	rVB	38419	83595	13.50%	1.498%
7	3.032	602	604	607	rVB	189	100	0.02%	0.002%
8	3.061	611	613	616	rVV2	148	83	0.01%	0.001%
9	3.174	640	648	649	rBV3	519	472	0.08%	0.008%
10	3.302	685	688	691	rVB2	223	160	0.03%	0.003%
11	3.354	701	704	708	rBV	166	129	0.02%	0.002%
12	3.437	728	730	734	rBV	201	126	0.02%	0.002%
13	3.662	796	800	801	rBV2	217	172	0.03%	0.003%
14	3.717	811	817	818	rBV	193	169	0.03%	0.003%
15	3.810	844	846	849	rVB	197	125	0.02%	0.002%
16	3.926	880	882	885	rVB	182	85	0.01%	0.002%
17	3.948	886	889	895	rVB	191	199	0.03%	0.004%
18	3.977	895	898	899	rBV	215	102	0.02%	0.002%
19	4.006	904	907	910	rBV	230	173	0.03%	0.003%
20	4.083	928	931	934	rVB	189	93	0.02%	0.002%
21	4.177	945	960	998	rBV3	102415	320723	51.78%	5.746%
22	4.643	1090	1105	1134	rVB2	110370	300089	48.45%	5.376%
23	4.797	1151	1153	1155	rVB2	227	87	0.01%	0.002%
24	4.817	1155	1159	1160	rBV2	514	283	0.05%	0.005%
25	4.842	1165	1167	1168	rBV2	216	96	0.02%	0.002%
26	4.926	1191	1193	1198	rBV2	263	188	0.03%	0.003%
27	5.090	1242	1244	1246	rBV2	164	91	0.01%	0.002%
28	5.193	1274	1276	1278	rVV	174	95	0.02%	0.002%
29	5.209	1278	1281	1284	rVB	160	94	0.02%	0.002%
30	5.334	1297	1320	1357	rBV2	209569	619358	100.00%	11.096%
31	5.794	1459	1463	1465	rBV2	371	284	0.05%	0.005%
32	5.881	1477	1490	1519	rBV	241299	473174	76.40%	8.477%
33	6.141	1567	1571	1572	rBV	232	158	0.03%	0.003%
34	6.170	1573	1580	1581	rBV3	2671	2455	0.40%	0.044%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060619\
 Data File : VU032509.D
 Acq On : 06 Jun 2019 20:00
 Operator : JC/SP
 Sample : K3224-03
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0C60

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Title : VOC Analysis

35	6.267	1608	1610	1613	rVB	245	140	0.02%	0.003%
36	6.325	1614	1628	1655	rBV	141041	283334	45.75%	5.076%
37	6.563	1700	1702	1703	rBV	152	86	0.01%	0.002%
38	6.617	1715	1719	1720	rBV	117	92	0.01%	0.002%
39	6.665	1731	1734	1739	rVB2	207	171	0.03%	0.003%
40	6.749	1757	1760	1765	rBV2	223	196	0.03%	0.004%
41	6.826	1782	1784	1787	rVV	315	172	0.03%	0.003%
42	6.887	1802	1803	1806	rVB	281	117	0.02%	0.002%
43	6.907	1806	1809	1812	rBV3	256	174	0.03%	0.003%
44	6.987	1830	1834	1835	rBV	197	113	0.02%	0.002%
45	7.035	1844	1849	1852	rBV	155	156	0.03%	0.003%
46	7.122	1869	1876	1882	rBV	156	250	0.04%	0.004%
47	7.161	1886	1888	1893	rBV	169	120	0.02%	0.002%
48	7.225	1895	1908	1931	rBV	79153	145824	23.54%	2.613%
49	7.386	1953	1958	1968	rVB6	1806	2873	0.46%	0.051%
50	7.456	1976	1980	1985	rVB3	291	365	0.06%	0.007%
51	7.482	1985	1988	1990	rBV	184	127	0.02%	0.002%
52	7.559	2000	2012	2034	rBV	288878	505210	81.57%	9.051%
53	7.845	2092	2101	2125	rBV	52883	94603	15.27%	1.695%
54	8.070	2169	2171	2176	rVB	142	101	0.02%	0.002%
55	8.231	2218	2221	2223	rBV	194	109	0.02%	0.002%
56	8.305	2234	2244	2282	rBV	183550	364241	58.81%	6.526%
57	8.524	2309	2312	2317	rVB3	636	463	0.07%	0.008%
58	8.620	2340	2342	2346	rVB	186	131	0.02%	0.002%
59	8.643	2348	2349	2354	rBV	99	95	0.02%	0.002%
60	8.707	2366	2369	2373	rBV	214	196	0.03%	0.004%
61	8.771	2386	2389	2391	rVB2	175	106	0.02%	0.002%
62	8.791	2392	2395	2398	rBV	207	134	0.02%	0.002%
63	8.980	2451	2454	2461	rBV	237	194	0.03%	0.003%
64	9.016	2463	2465	2467	rVB	245	98	0.02%	0.002%
65	9.083	2474	2486	2532	rBV	344931	595365	96.13%	10.666%
66	9.276	2544	2546	2549	rBV	243	162	0.03%	0.003%
67	9.328	2559	2562	2565	rBV	189	111	0.02%	0.002%
68	9.379	2573	2578	2582	rBV2	220	231	0.04%	0.004%
69	9.556	2631	2633	2636	rBV	209	108	0.02%	0.002%
70	9.675	2667	2670	2673	rVB	154	94	0.02%	0.002%
71	9.701	2676	2678	2681	rVB	176	92	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060619\
 Data File : VU032509.D
 Acq On : 06 Jun 2019 20:00
 Operator : JC/SP
 Sample : K3224-03
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0C60

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Title : VOC Analysis

72	9.746	2689	2692	2694	rBV	177	99	0.02%	0.002%
73	9.775	2698	2701	2702	rBV	146	84	0.01%	0.002%
74	9.804	2707	2710	2713	rVB	214	130	0.02%	0.002%
75	9.820	2713	2715	2718	rBV	177	122	0.02%	0.002%
76	9.861	2726	2728	2732	rVB2	152	92	0.01%	0.002%
77	9.916	2741	2745	2749	rVB2	206	166	0.03%	0.003%
78	9.939	2749	2752	2755	rBV	210	142	0.02%	0.003%
79	9.984	2762	2766	2771	rBV2	231	229	0.04%	0.004%
80	10.032	2776	2781	2784	rBV2	242	224	0.04%	0.004%
81	10.167	2820	2823	2824	rBV2	192	112	0.02%	0.002%
82	10.222	2838	2840	2843	rBV	177	119	0.02%	0.002%
83	10.324	2870	2872	2876	rBV	160	93	0.02%	0.002%
84	10.427	2891	2904	2929	rBV	215063	350453	56.58%	6.279%
85	10.556	2942	2944	2947	rVB	246	119	0.02%	0.002%
86	10.607	2953	2960	2966	rVB4	1133	1527	0.25%	0.027%
87	10.636	2966	2969	2972	rBV	278	244	0.04%	0.004%
88	10.704	2987	2990	2993	rVB	204	128	0.02%	0.002%
89	10.733	2997	2999	3001	rBV	151	84	0.01%	0.002%
90	10.836	3029	3031	3034	rBV	241	99	0.02%	0.002%
91	11.096	3107	3112	3114	rBV	294	265	0.04%	0.005%
92	11.244	3155	3158	3160	rBV	178	89	0.01%	0.002%
93	11.479	3219	3231	3250	rBV	359062	589957	95.25%	10.570%
94	11.803	3327	3332	3336	rVB3	380	435	0.07%	0.008%
95	11.855	3336	3348	3376	rBV	305477	526853	85.06%	9.439%
96	12.411	3519	3521	3523	rBV	313	170	0.03%	0.003%
97	12.533	3557	3559	3563	rVB	311	210	0.03%	0.004%
98	12.742	3622	3624	3627	rBV	250	157	0.03%	0.003%
99	12.774	3632	3634	3637	rBV	301	163	0.03%	0.003%
100	13.295	3794	3796	3798	rBV2	233	125	0.02%	0.002%


Sum of corrected areas: 5581668

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU060619\
Data File : VU032509.D
Acq On : 06 Jun 2019 20:00
Operator : JC/SP
Sample : K3224-03
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0C60

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

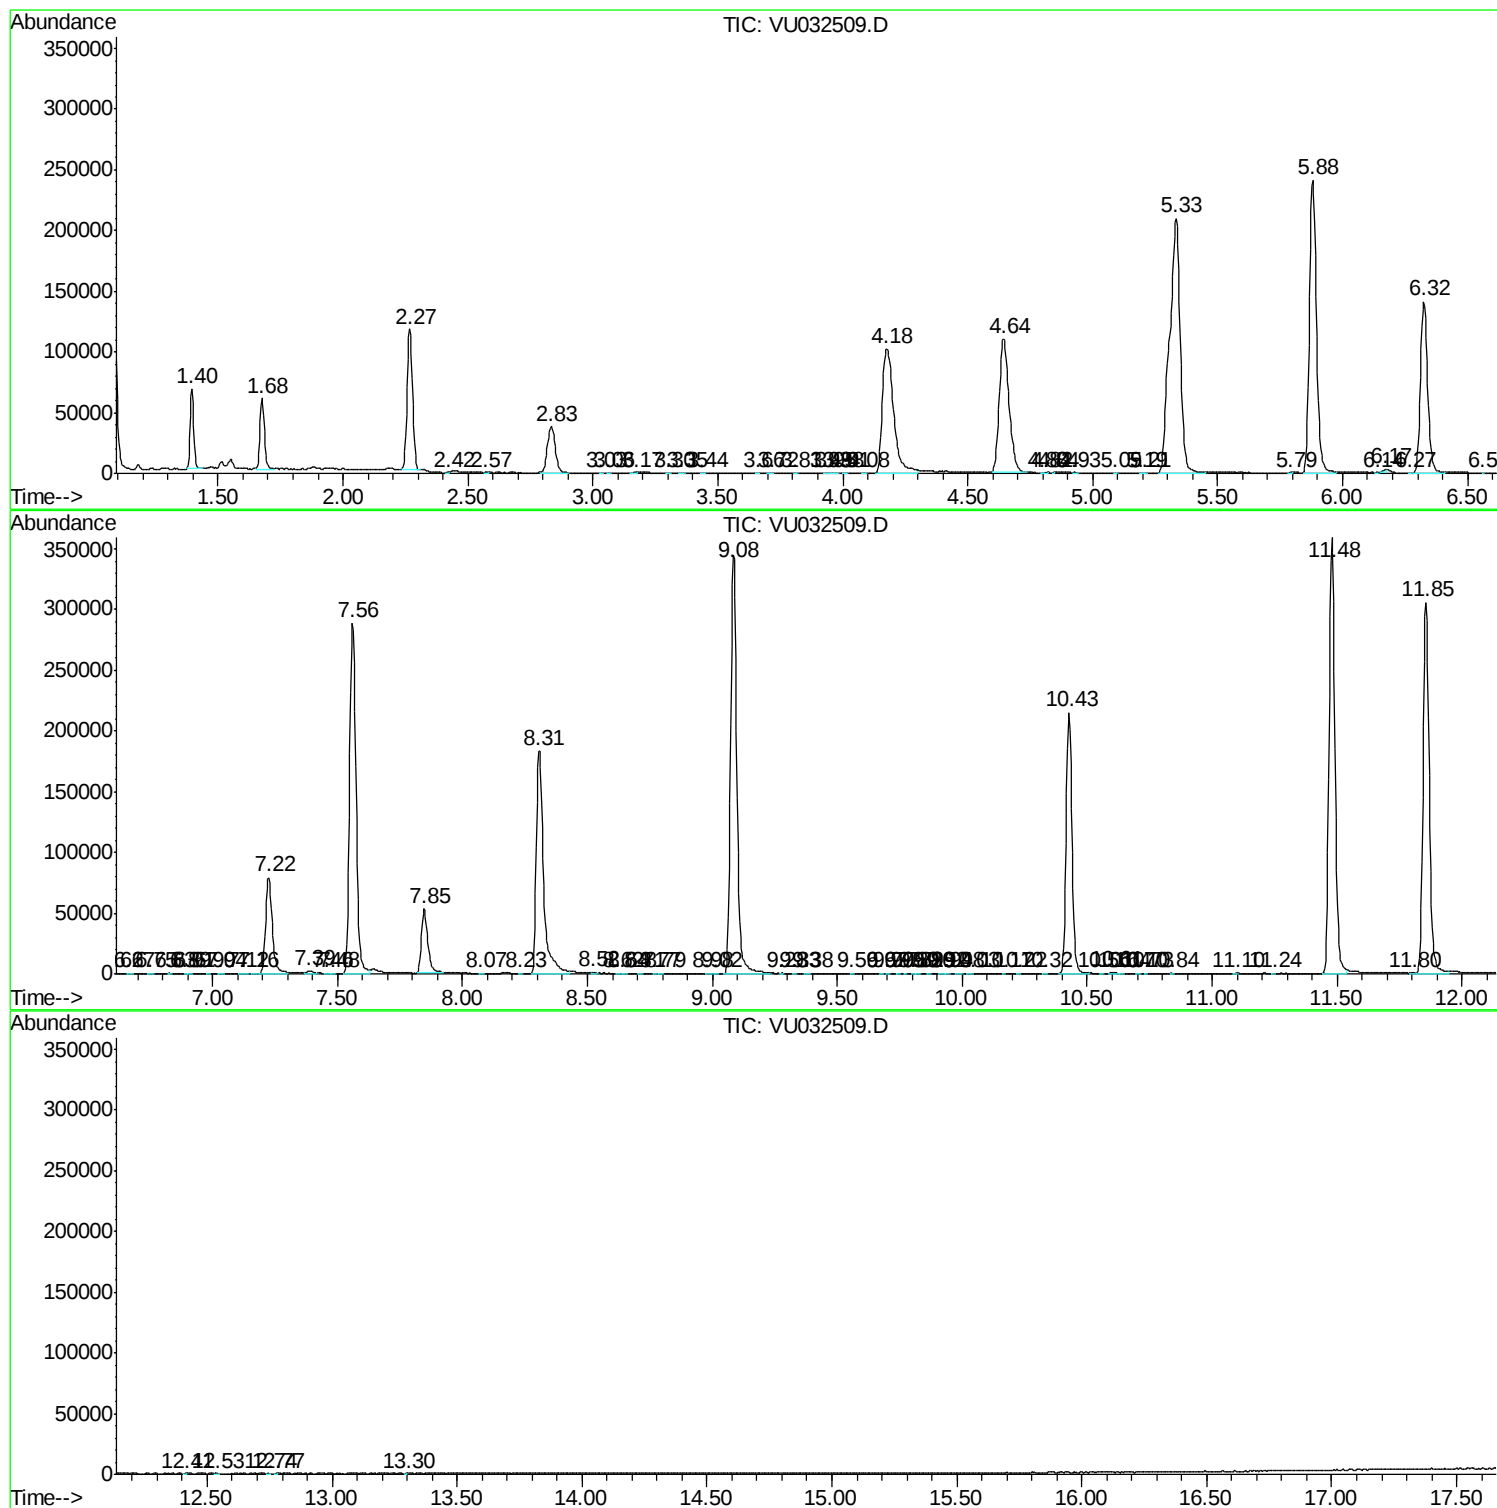

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU060619\
Data File : VU032509.D
Acq On : 06 Jun 2019 20:00
Operator : JC/SP
Sample : K3224-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0C60

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU060619\
Data File : VU032509.D
Acq On : 06 Jun 2019 20:00
Operator : JC/SP
Sample : K3224-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0C60

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc