

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060619\
 Data File : VU032511.D
 Acq On : 06 Jun 2019 20:46
 Operator : JC/SP
 Sample : K3224-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0C62

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.396	89	95	105	rVB	63388	65495	10.26%	1.170%
2	1.675	175	182	197	rVB	59424	74184	11.62%	1.325%
3	2.267	357	366	377	rVB	121185	178964	28.04%	3.196%
4	2.441	409	420	432	rBV	6693	12549	1.97%	0.224%
5	2.669	487	491	492	rBV	197	150	0.02%	0.003%
6	2.695	498	499	501	rBV	236	81	0.01%	0.001%
7	2.833	526	542	562	rBV	40033	87573	13.72%	1.564%
8	2.990	588	591	598	rVB2	196	181	0.03%	0.003%
9	3.074	613	617	619	rBV	409	304	0.05%	0.005%
10	3.148	638	640	642	rBV2	203	113	0.02%	0.002%
11	3.270	673	678	681	rBV2	239	179	0.03%	0.003%
12	3.296	681	686	689	rBV2	206	171	0.03%	0.003%
13	3.331	694	697	700	rVB	168	118	0.02%	0.002%
14	3.405	716	720	723	rBV	94	77	0.01%	0.001%
15	3.441	728	731	732	rBV	221	122	0.02%	0.002%
16	3.508	750	752	755	rVB2	209	119	0.02%	0.002%
17	3.540	755	762	764	rBV2	212	206	0.03%	0.004%
18	3.746	823	826	830	rVB2	152	110	0.02%	0.002%
19	3.865	860	863	866	rVB	208	145	0.02%	0.003%
20	3.913	876	878	883	rVB2	222	209	0.03%	0.004%
21	3.955	883	891	896	rBV2	220	270	0.04%	0.005%
22	3.984	897	900	904	rVB	165	142	0.02%	0.003%
23	4.061	919	924	928	rVB2	215	210	0.03%	0.004%
24	4.090	931	933	934	rBV2	162	70	0.01%	0.001%
25	4.177	943	960	999	rBV2	98337	310452	48.64%	5.544%
26	4.640	1090	1104	1132	rVB	111198	285197	44.69%	5.093%
27	4.791	1149	1151	1155	rVB2	403	263	0.04%	0.005%
28	4.810	1155	1157	1159	rBV	342	201	0.03%	0.004%
29	5.039	1224	1228	1232	rBV2	191	152	0.02%	0.003%
30	5.087	1241	1243	1249	rVB2	167	119	0.02%	0.002%
31	5.119	1249	1253	1254	rBV	233	138	0.02%	0.002%
32	5.141	1258	1260	1264	rBV	135	81	0.01%	0.001%
33	5.199	1271	1278	1280	rBV2	223	196	0.03%	0.004%
34	5.212	1280	1282	1285	rVB	174	86	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060619\
 Data File : VU032511.D
 Acq On : 06 Jun 2019 20:46
 Operator : JC/SP
 Sample : K3224-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0C62

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Title : VOC Analysis

35	5.228	1285	1287	1290	rBV2	211	130	0.02%	0.002%
36	5.334	1294	1320	1347	rBV2	216032	638201	100.00%	11.397%
37	5.514	1373	1376	1379	rBV	309	230	0.04%	0.004%
38	5.733	1442	1444	1447	rVB3	260	133	0.02%	0.002%
39	5.791	1457	1462	1463	rBV	436	367	0.06%	0.007%
40	5.881	1477	1490	1511	rBV	231599	452476	70.90%	8.081%
41	6.170	1573	1580	1592	rVB5	3771	7226	1.13%	0.129%
42	6.325	1614	1628	1647	rBV	147247	292409	45.82%	5.222%
43	6.456	1666	1669	1674	rBV4	521	511	0.08%	0.009%
44	6.579	1704	1707	1709	rBV	330	232	0.04%	0.004%
45	6.649	1726	1729	1732	rVB2	251	104	0.02%	0.002%
46	6.669	1732	1735	1738	rBV	211	132	0.02%	0.002%
47	6.820	1775	1782	1787	rBV3	330	545	0.09%	0.010%
48	6.926	1813	1815	1820	rVB	166	103	0.02%	0.002%
49	6.948	1820	1822	1823	rBV	146	78	0.01%	0.001%
50	7.000	1835	1838	1841	rBV2	185	120	0.02%	0.002%
51	7.016	1841	1843	1847	rVB2	182	108	0.02%	0.002%
52	7.061	1852	1857	1860	rVB2	181	144	0.02%	0.003%
53	7.077	1860	1862	1865	rBV	163	83	0.01%	0.001%
54	7.225	1896	1908	1935	rBV	81261	152583	23.91%	2.725%
55	7.469	1982	1984	1990	rBV	267	163	0.03%	0.003%
56	7.498	1990	1993	1996	rVB2	148	89	0.01%	0.002%
57	7.559	1999	2012	2035	rBV	297345	522838	81.92%	9.337%
58	7.845	2091	2101	2129	rBV	55070	99785	15.64%	1.782%
59	8.071	2165	2171	2172	rBV	248	163	0.03%	0.003%
60	8.173	2194	2203	2212	rVB4	1188	1895	0.30%	0.034%
61	8.260	2225	2230	2234	rBV2	196	178	0.03%	0.003%
62	8.305	2234	2244	2283	rBV2	191748	377175	59.10%	6.736%
63	8.611	2336	2339	2344	rBV	264	205	0.03%	0.004%
64	8.640	2344	2348	2351	rVB2	243	153	0.02%	0.003%
65	8.681	2356	2361	2367	rVB2	244	287	0.04%	0.005%
66	8.759	2383	2385	2388	rVB	158	74	0.01%	0.001%
67	8.775	2388	2390	2393	rBV	142	98	0.02%	0.002%
68	8.845	2410	2412	2415	rBV	141	74	0.01%	0.001%
69	8.894	2425	2427	2429	rBV	132	82	0.01%	0.001%
70	8.948	2441	2444	2447	rBV	138	78	0.01%	0.001%
71	8.997	2455	2459	2460	rBV	213	101	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060619\
 Data File : VU032511.D
 Acq On : 06 Jun 2019 20:46
 Operator : JC/SP
 Sample : K3224-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0C62

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Title : VOC Analysis

72	9.083	2475	2486	2516	rBV	330699	565165	88.56%	10.093%
73	9.312	2553	2557	2560	rVB3	274	204	0.03%	0.004%
74	9.334	2560	2564	2567	rBV	132	117	0.02%	0.002%
75	9.447	2596	2599	2602	rVB	197	138	0.02%	0.002%
76	9.585	2639	2642	2644	rBV2	102	74	0.01%	0.001%
77	9.633	2656	2657	2664	rVB	208	133	0.02%	0.002%
78	9.665	2664	2667	2672	rBV2	261	283	0.04%	0.005%
79	9.839	2718	2721	2724	rBV2	197	126	0.02%	0.002%
80	9.878	2730	2733	2735	rBV	200	128	0.02%	0.002%
81	10.048	2783	2786	2789	rVB	271	148	0.02%	0.003%
82	10.103	2801	2803	2806	rVB	161	106	0.02%	0.002%
83	10.132	2810	2812	2817	rVB	141	74	0.01%	0.001%
84	10.161	2817	2821	2829	rVB2	211	252	0.04%	0.005%
85	10.427	2891	2904	2926	rBV	221841	359591	56.34%	6.422%
86	10.601	2951	2958	2969	rBV2	2044	3174	0.50%	0.057%
87	10.710	2986	2992	2997	rBV	285	392	0.06%	0.007%
88	10.794	3016	3018	3020	rBV	194	112	0.02%	0.002%
89	10.849	3032	3035	3036	rBV	172	98	0.02%	0.002%
90	10.987	3074	3078	3079	rBV	158	117	0.02%	0.002%
91	11.074	3102	3105	3109	rBV2	159	140	0.02%	0.003%
92	11.160	3129	3132	3136	rVB	238	168	0.03%	0.003%
93	11.279	3166	3169	3173	rVB2	280	256	0.04%	0.005%
94	11.479	3219	3231	3262	rBV	347870	567346	88.90%	10.132%
95	11.855	3336	3348	3371	rBV	313783	532283	83.40%	9.506%
96	12.154	3439	3441	3442	rBV	274	139	0.02%	0.002%
97	12.723	3613	3618	3619	rBV	209	193	0.03%	0.003%
98	12.836	3651	3653	3656	rBV	309	201	0.03%	0.004%
99	13.074	3724	3727	3731	rBV2	316	283	0.04%	0.005%
100	13.276	3787	3790	3791	rBV2	280	137	0.02%	0.002%


Sum of corrected areas: 5599558

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU060619\
Data File : VU032511.D
Acq On : 06 Jun 2019 20:46
Operator : JC/SP
Sample : K3224-05
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0C62

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

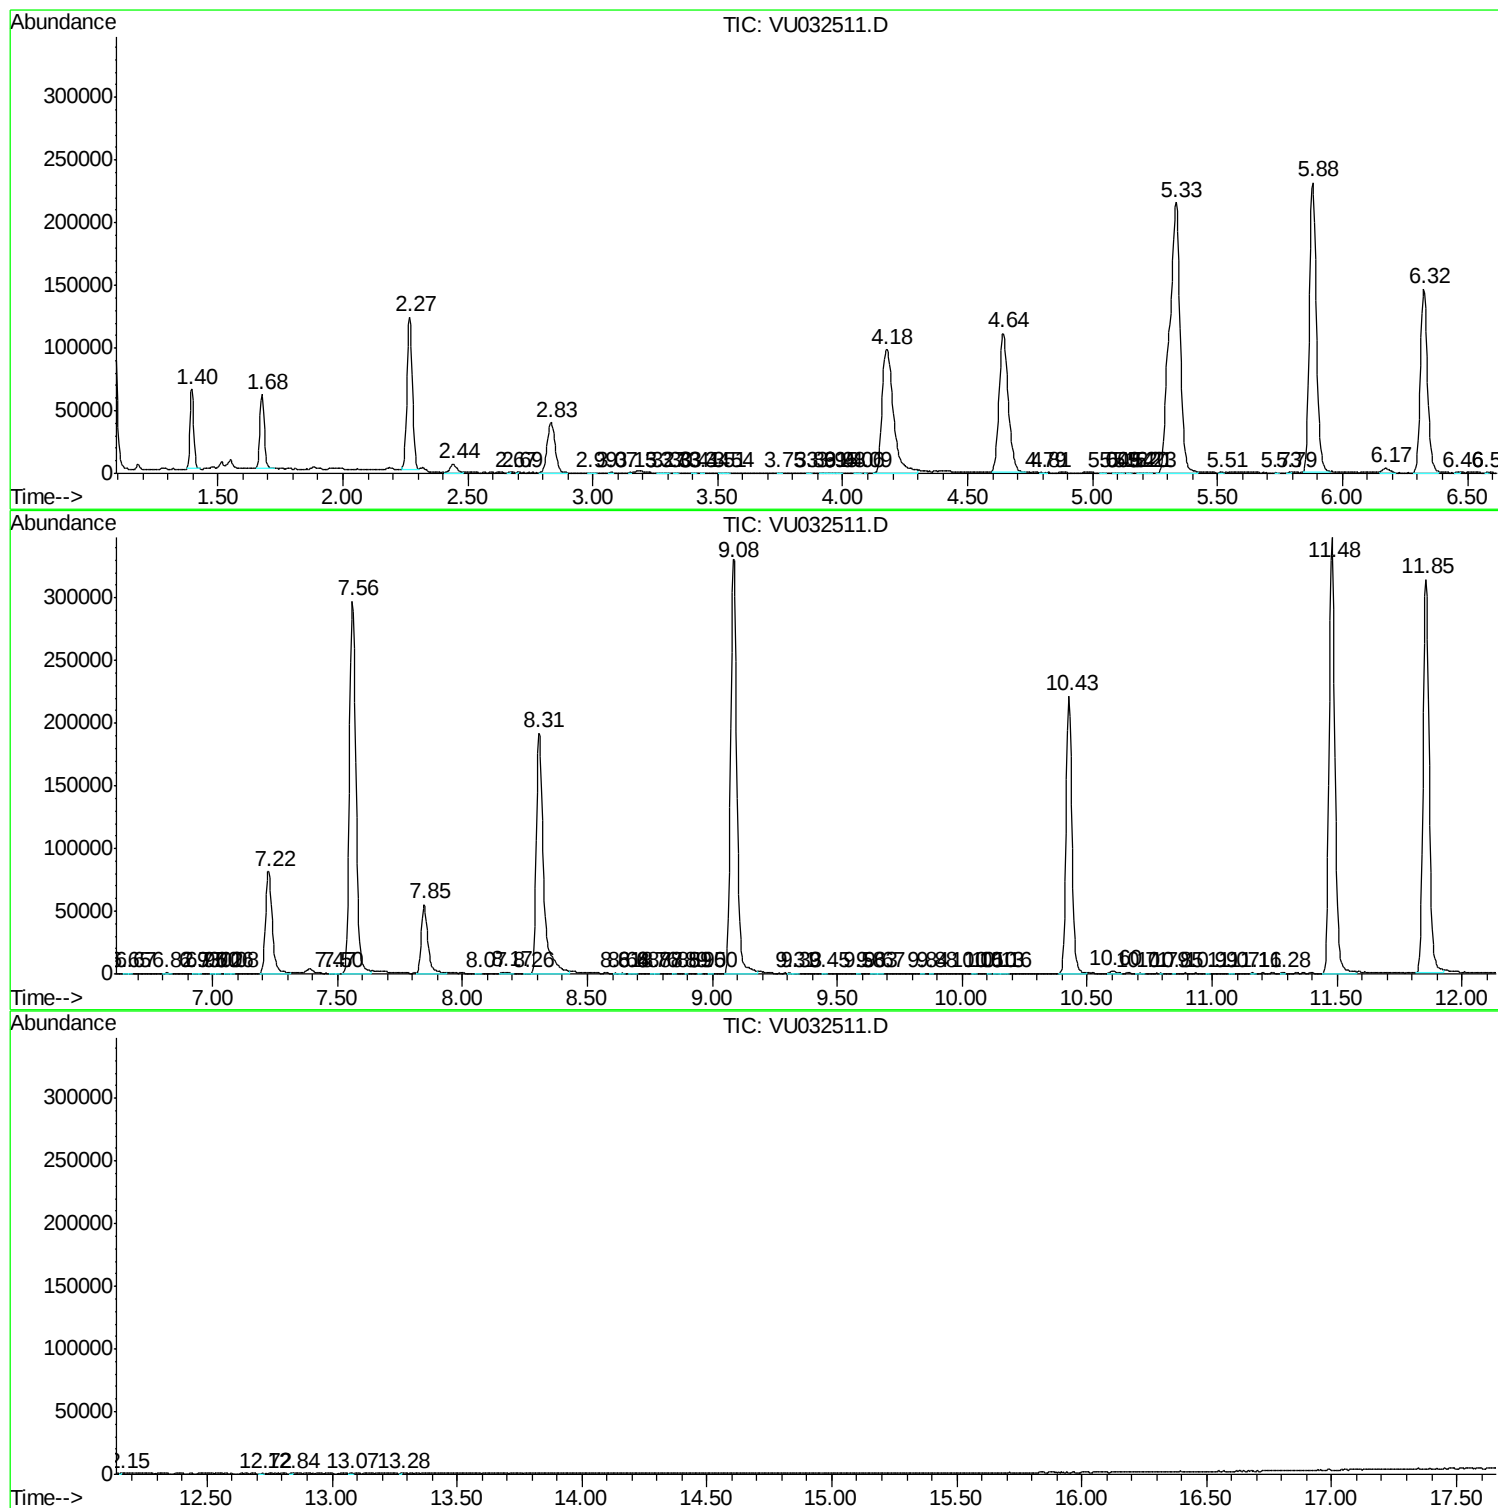

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU060619\
Data File : VU032511.D
Acq On : 06 Jun 2019 20:46
Operator : JC/SP
Sample : K3224-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0C62

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU060619\
Data File : VU032511.D
Acq On : 06 Jun 2019 20:46
Operator : JC/SP
Sample : K3224-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0C62

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc