


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU060619\
 Data File : VU032456.D
 Acq On : 05 Jun 2019 12:42
 Operator : JC/SP
 Sample : BFB48
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB48

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Title : VOC Analysis
 Last Update : Thu Jun 06 04:04:55 2019

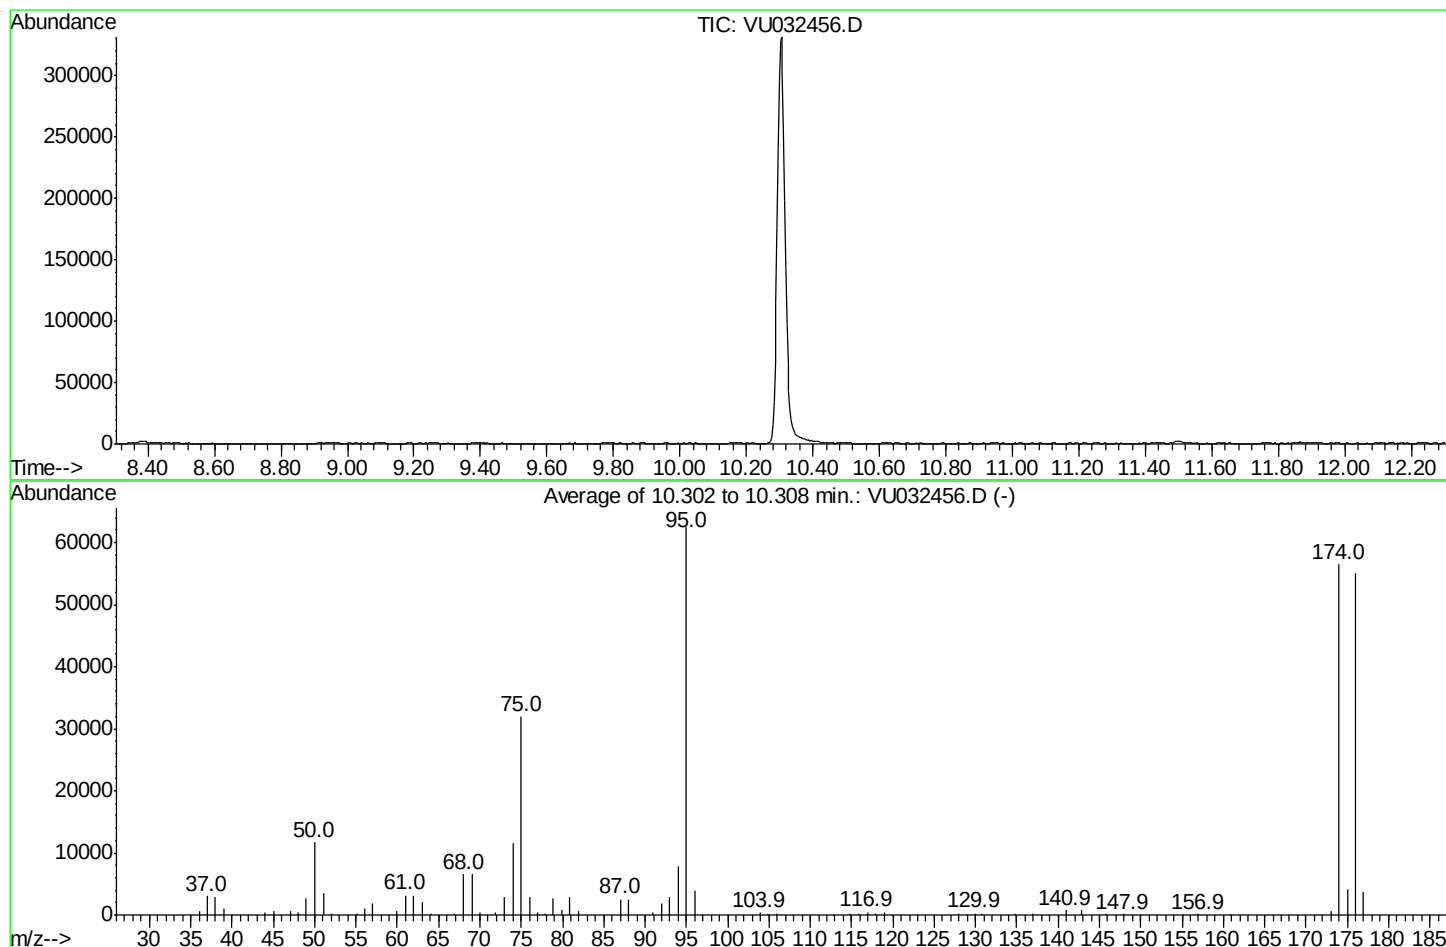

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	11659	PASS
75	95	30	80	51.2	31946	PASS
95	95	100	100	100.0	62445	PASS
96	95	5	9	6.3	3962	PASS
173	174	0.00	2	1.1	648	PASS
174	95	50	120	90.5	56482	PASS
175	174	5	9	7.2	4056	PASS
176	174	95	101	97.3	54962	PASS
177	176	5	9	6.8	3762	PASS

Scan 2853 (10.263 min): VU032456.D
BFB48

m/z	Abundance
39.90	113.0
43.90	464.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48

m/z	Abundance
36.00	580.0
37.00	3165.0
38.00	3124.0
39.00	1146.0
40.00	150.0
43.90	812.0
45.00	702.0
47.00	735.0
48.00	354.0
49.00	2798.0
50.00	12180.0
51.10	3678.0
51.90	155.0
55.10	208.0
56.00	1086.0
57.00	1863.0
58.00	112.0
60.00	595.0
61.00	3272.0
62.00	3179.0
63.00	2264.0
64.10	259.0
66.90	166.0
68.00	6949.0
69.00	7042.0
70.00	500.0
71.90	340.0
73.00	3105.0
74.00	11809.0
75.00	32968.0
76.00	3001.0
77.00	380.0
77.90	302.0
78.90	2646.0
79.90	767.0
80.90	3005.0
82.00	646.0
87.00	2469.0
88.00	2462.0
90.90	336.0
92.00	1808.0
93.00	2859.0
94.00	8077.0
95.00	63944.0
96.00	4122.0
97.00	148.0
103.90	361.0
104.80	115.0
105.90	315.0
112.80	114.0
114.80	115.0
115.90	302.0
116.90	491.0
117.90	227.0
118.90	350.0
127.90	246.0
129.00	135.0
129.90	259.0
130.80	109.0
134.80	136.0
137.00	157.0
140.90	785.0
142.90	770.0
145.90	167.0
147.90	139.0
150.00	106.0
155.00	135.0
156.90	144.0
160.90	120.0
173.10	640.0
174.00	56656.0
175.00	4052.0
176.00	55088.0
177.00	3761.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48

m/z	Abundance
36.00	546.0
37.00	3171.0
38.00	2949.0
39.00	1103.0
39.90	182.0
43.90	833.0
45.00	707.0
47.00	714.0
48.00	368.0
49.00	2790.0
50.00	12028.0
51.00	3641.0
52.00	142.0
55.10	243.0
56.00	1116.0
57.00	1859.0
58.00	102.0
60.00	548.0
61.00	3251.0
62.00	3251.0
63.00	2199.0
64.00	261.0
66.90	186.0
68.00	6760.0
69.00	6864.0
70.00	437.0
71.90	326.0
73.00	2897.0
74.00	11838.0
75.00	33000.0
76.00	3034.0
76.90	351.0
77.80	267.0
78.90	2739.0
79.90	745.0
80.90	3059.0
82.00	603.0
87.00	2617.0
88.00	2478.0
91.00	360.0
92.00	1848.0
93.00	2923.0
94.00	7975.0
95.00	64432.0
96.00	4029.0
97.00	146.0
103.90	350.0
104.90	123.0
105.90	295.0
114.90	131.0
115.90	323.0
116.90	496.0
117.90	239.0
118.90	341.0
127.90	269.0
128.90	134.0
129.90	262.0
130.80	119.0
134.80	171.0
136.90	158.0
140.90	812.0
142.90	841.0
145.90	131.0
147.90	134.0
149.90	102.0
155.00	132.0
156.90	145.0
160.80	120.0
173.10	671.0
174.00	58120.0
175.00	4179.0
176.00	56712.0
177.00	3883.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48

m/z	Abundance
36.00	482.0
37.00	2842.0
38.00	2572.0
39.00	1034.0
39.90	189.0
44.00	823.0
45.00	623.0
47.00	615.0
48.00	355.0
49.00	2476.0
50.00	10769.0
51.00	3257.0
52.10	130.0
55.00	235.0
56.00	1094.0
57.00	1729.0
60.00	457.0
61.00	2934.0
62.00	2918.0
63.00	1982.0
64.00	222.0
67.00	182.0
68.00	6036.0
69.00	6082.0
70.10	407.0
71.90	290.0
73.00	2462.0
74.00	10827.0
75.00	29872.0
76.00	2792.0
76.90	323.0
77.80	205.0
78.90	2553.0
79.90	691.0
80.90	2819.0
81.90	511.0
87.00	2449.0
88.00	2246.0
91.00	323.0
92.00	1720.0
93.00	2680.0
94.00	7252.0
95.00	58960.0
96.00	3737.0
103.90	319.0
104.90	119.0
105.90	292.0
114.90	106.0
115.90	299.0
116.90	448.0
117.90	227.0
118.90	319.0
127.90	255.0
129.90	255.0
130.80	111.0
134.80	149.0
136.90	152.0
140.90	828.0
142.90	815.0
145.80	110.0
147.90	138.0
157.00	137.0
173.10	634.0
174.00	54672.0
175.00	3939.0
176.00	53088.0
177.00	3644.0

Instrument :
MSVOA_U
ClientSampleId :
BFB48