


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060619\
 Data File : VU032482.D
 Acq On : 06 Jun 2019 08:28
 Operator : JC/SP
 Sample : BFB49
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB49

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Title : VOC Analysis
 Last Update : Fri Jun 07 11:53:52 2019

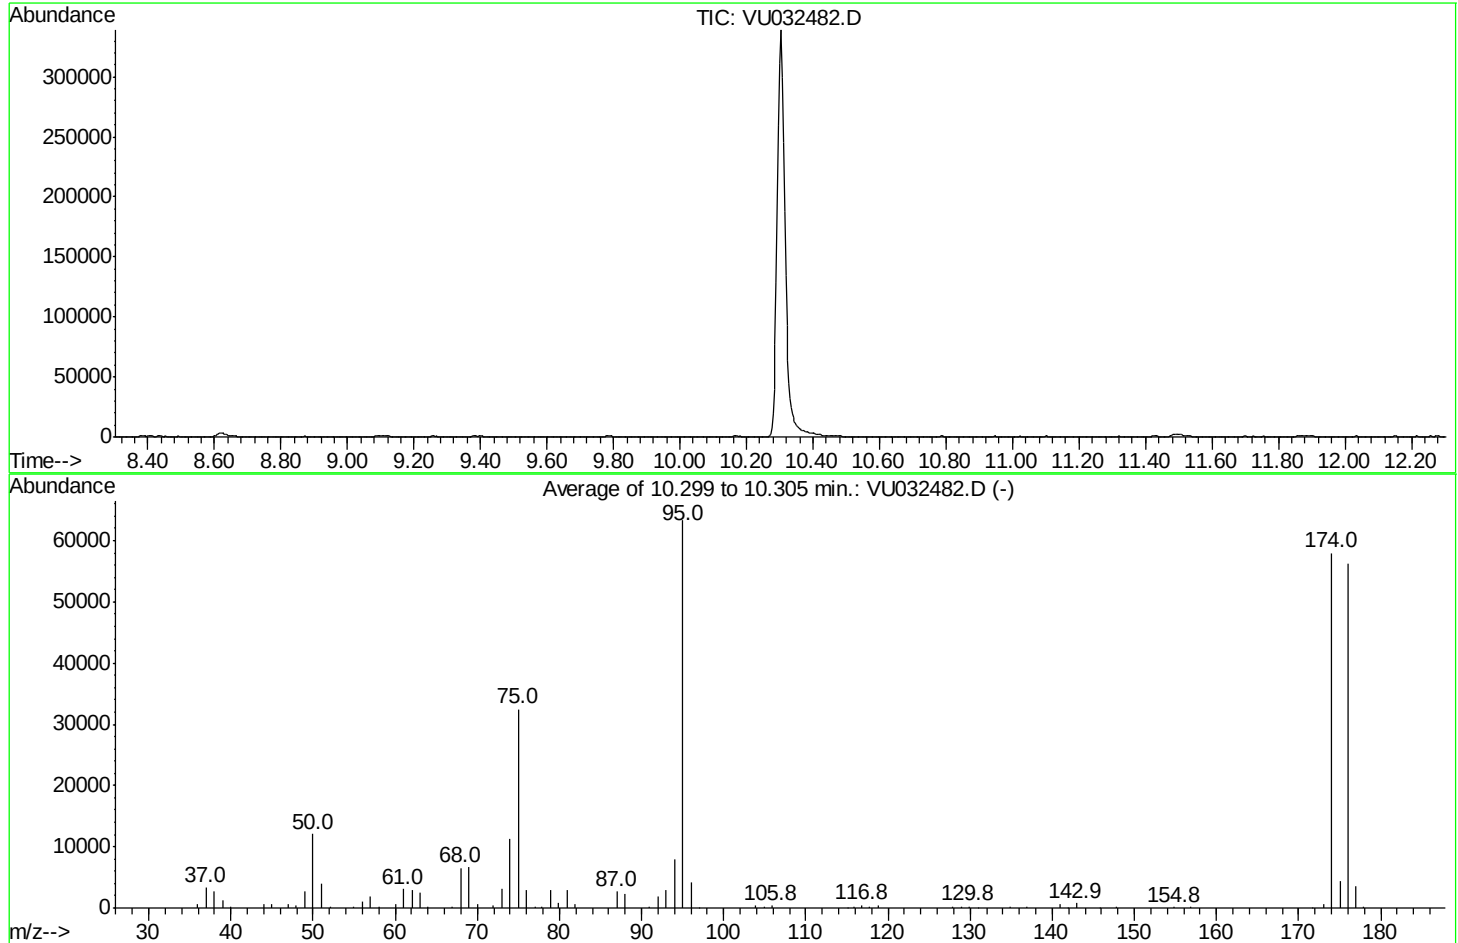

AutoFind: Scans 2864, 2865, 2866; Background Corrected with Scan 2853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	12081	PASS
75	95	30	80	51.3	32464	PASS
95	95	100	100	100.0	63312	PASS
96	95	5	9	6.6	4181	PASS
173	174	0.00	2	1.1	657	PASS
174	95	50	120	91.6	58010	PASS
175	174	5	9	7.7	4448	PASS
176	174	95	101	97.0	56261	PASS
177	176	5	9	6.5	3666	PASS

m/z	Abundance
43.90	315.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49

m/z	Abundance
35.90	490.0
37.00	3200.0
38.00	2744.0
39.00	1171.0
39.90	124.0
44.00	891.0
44.90	635.0
47.10	687.0
48.00	355.0
49.00	2632.0
50.00	11587.0
51.00	3822.0
52.10	151.0
55.00	216.0
56.00	1083.0
57.00	1953.0
58.00	111.0
60.10	581.0
61.00	2872.0
62.10	2749.0
63.00	2510.0
64.00	272.0
67.00	161.0
68.00	6259.0
69.00	6327.0
70.00	488.0
71.90	319.0
73.00	3015.0
74.00	10863.0
75.00	31296.0
76.00	2913.0
77.00	280.0
77.90	273.0
78.90	2737.0
79.90	697.0
80.90	2687.0
81.90	540.0
87.00	2565.0
88.00	2259.0
90.90	298.0
92.00	1814.0
93.00	2758.0
94.00	7776.0
95.00	60664.0
96.00	3982.0
97.00	108.0
103.90	294.0
104.90	135.0
105.80	337.0
115.80	237.0
116.90	514.0
117.80	289.0
118.80	350.0
127.90	240.0
128.90	132.0
129.90	261.0
134.90	152.0
136.80	133.0
140.90	677.0
141.90	103.0
143.00	818.0
147.70	108.0
154.80	135.0
156.80	132.0
171.70	107.0
173.10	622.0
174.00	53904.0
175.00	4097.0
176.00	52072.0
177.00	3460.0
177.80	116.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49

m/z	Abundance
36.00	555.0
37.00	3463.0
38.00	2894.0
39.00	1254.0
39.90	113.0
44.00	967.0
44.90	661.0
47.00	751.0
47.90	351.0
49.00	2713.0
50.00	12522.0
51.00	4034.0
52.10	176.0
55.00	202.0
56.00	1154.0
57.00	2048.0
58.00	126.0
60.00	657.0
61.00	3153.0
62.00	3166.0
63.00	2632.0
64.00	295.0
67.00	186.0
68.00	6759.0
69.00	6843.0
70.00	573.0
72.00	349.0
73.00	3290.0
74.00	11581.0
75.00	33480.0
76.00	3106.0
77.00	313.0
77.90	326.0
78.90	3015.0
79.90	788.0
80.90	2980.0
81.90	586.0
87.00	2834.0
87.90	2401.0
90.90	319.0
92.00	2007.0
93.00	2893.0
94.00	8246.0
95.00	65240.0
96.00	4258.0
103.90	350.0
104.90	143.0
105.80	369.0
115.90	238.0
116.80	535.0
117.80	324.0
118.80	397.0
127.90	259.0
128.90	126.0
129.80	278.0
134.90	192.0
136.90	141.0
140.90	739.0
141.90	111.0
142.90	840.0
147.80	123.0
154.80	140.0
156.80	119.0
171.60	107.0
173.10	690.0
174.00	59848.0
175.00	4579.0
176.00	58168.0
177.00	3822.0
177.90	135.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49

m/z	Abundance
36.00	576.0
37.00	3285.0
38.00	2819.0
39.00	1208.0
39.90	108.0
44.00	967.0
44.90	615.0
47.00	731.0
47.90	359.0
49.00	2610.0
50.00	12134.0
51.00	3837.0
52.10	197.0
55.00	208.0
56.00	1109.0
57.00	1953.0
58.10	123.0
60.00	675.0
61.00	3105.0
62.00	3193.0
63.00	2439.0
64.00	262.0
67.00	188.0
68.00	6655.0
69.00	6687.0
70.00	593.0
72.00	356.0
73.00	3103.0
74.00	11238.0
75.00	32616.0
76.00	2893.0
77.00	338.0
77.90	322.0
78.90	2940.0
79.90	814.0
80.90	2939.0
81.90	590.0
87.00	2745.0
87.90	2463.0
90.90	288.0
92.00	2037.0
93.00	2856.0
94.00	7896.0
95.00	64032.0
96.00	4305.0
103.90	383.0
104.90	126.0
105.90	372.0
115.00	101.0
115.90	249.0
116.80	533.0
117.80	318.0
118.80	395.0
127.90	255.0
128.90	117.0
129.80	263.0
130.90	105.0
134.90	169.0
136.90	135.0
140.90	801.0
141.90	101.0
142.90	795.0
145.80	109.0
147.80	159.0
154.90	153.0
156.80	113.0
173.10	661.0
174.00	60280.0
175.00	4670.0
176.00	58544.0
177.00	3717.0
177.90	120.0

Instrument :
MSVOA_U
ClientSampleId :
BFB49