
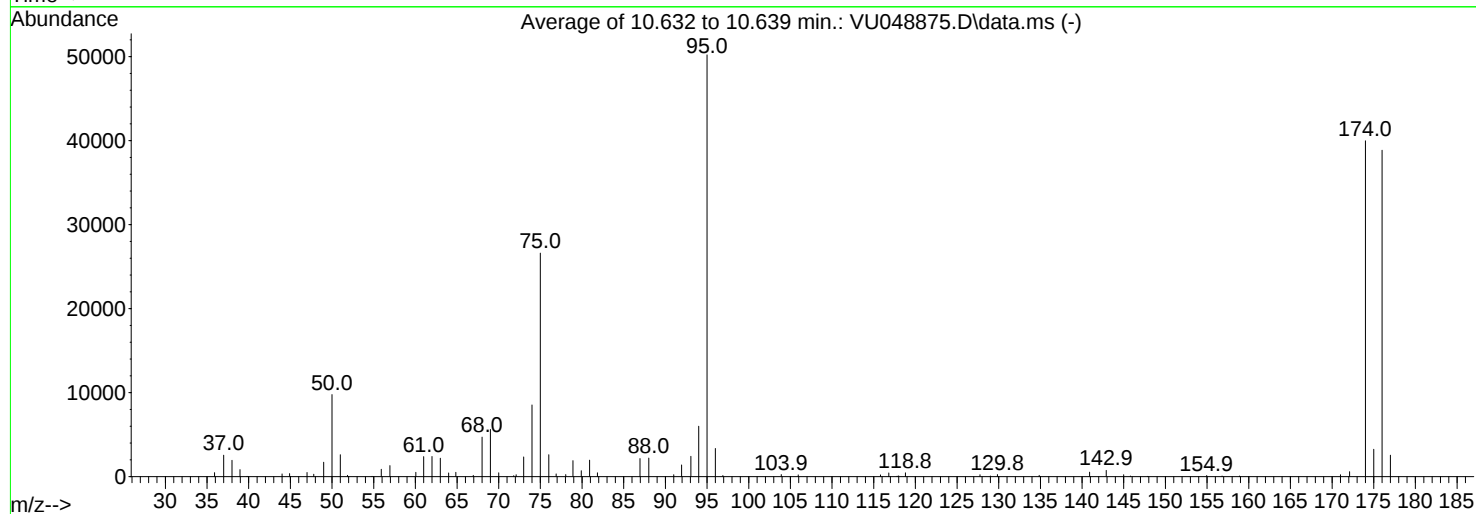


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060622\
Data File : VU048875.D
Acq On : 06 Jun 2022 09:23
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U052622W.M
Title : SW846 8260
Last Update : Fri May 27 06:42:31 2022

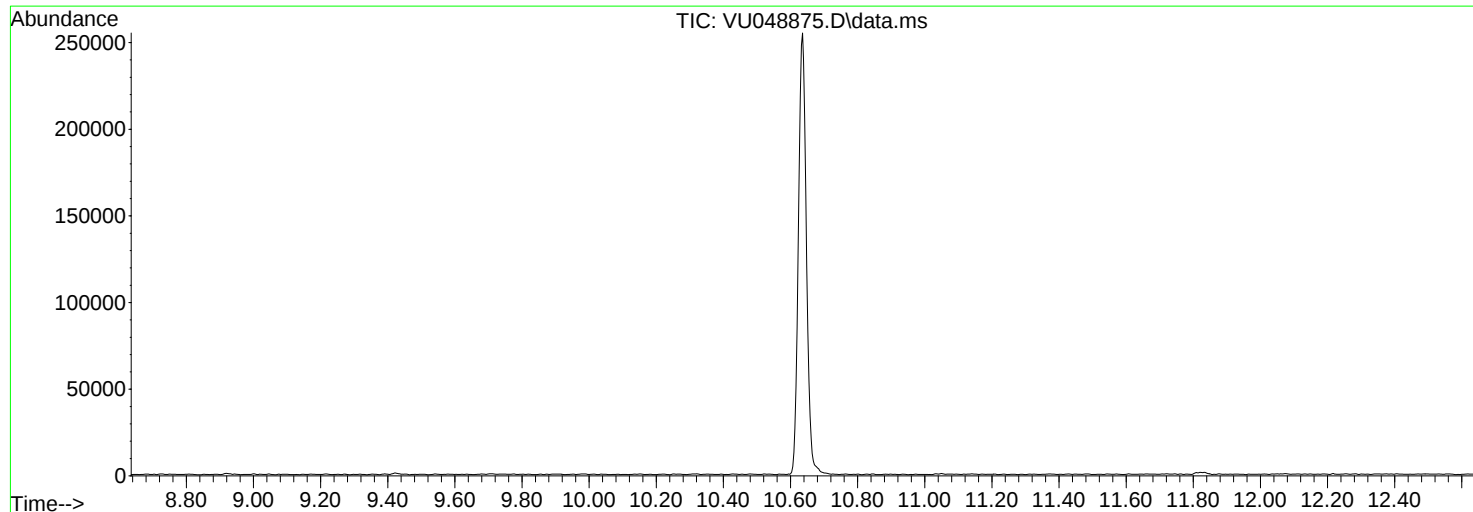

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	9772	PASS
75	95	30	60	53.0	26613	PASS
95	95	100	100	100.0	50221	PASS
96	95	5	9	6.7	3352	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	79.6	39997	PASS
175	174	5	9	8.2	3261	PASS
176	174	95	101	97.1	38856	PASS
177	176	5	9	6.6	2552	PASS