




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060625\
Data File : VU063365.D
Acq On : 06 Jun 2025 20:36
Operator : MD/SY
Sample : Q2117-01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
MDL-WATER-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/10/2025
Supervised By :Mahesh Dadoda 06/11/2025

Quant Time: Jun 09 11:58:23 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060625WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 09 11:34:08 2025
Response via : Initial Calibration

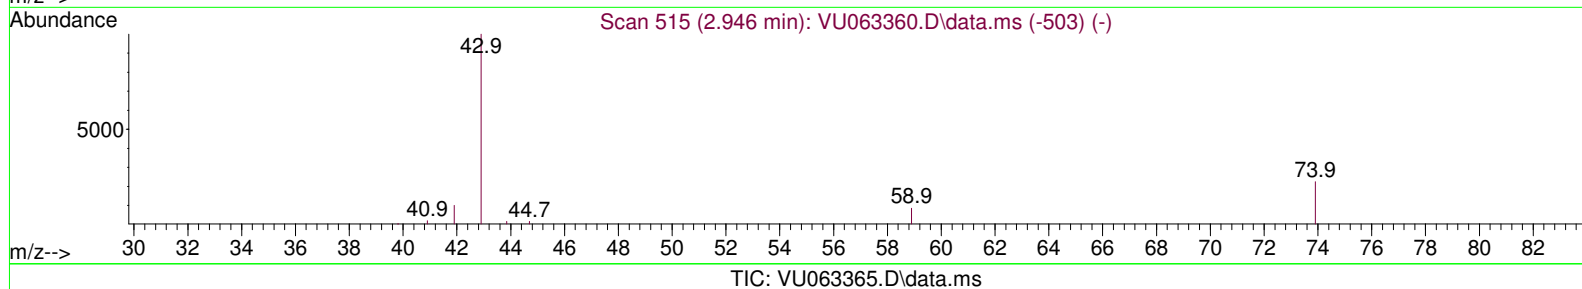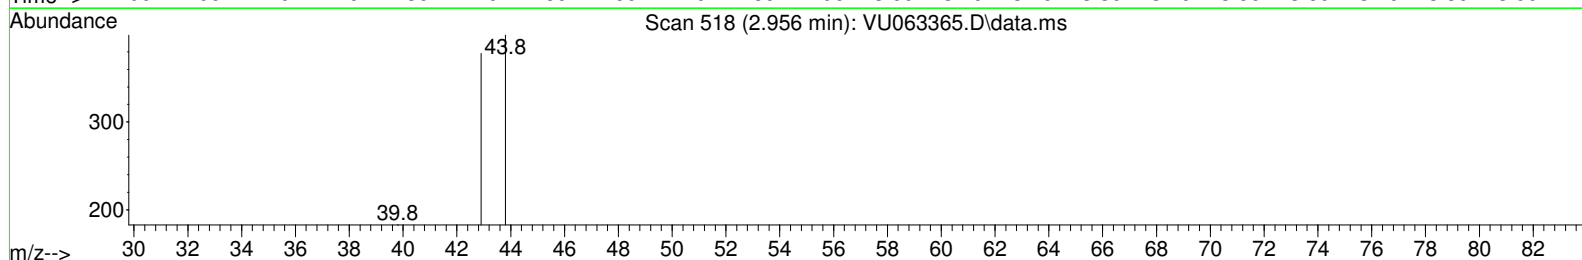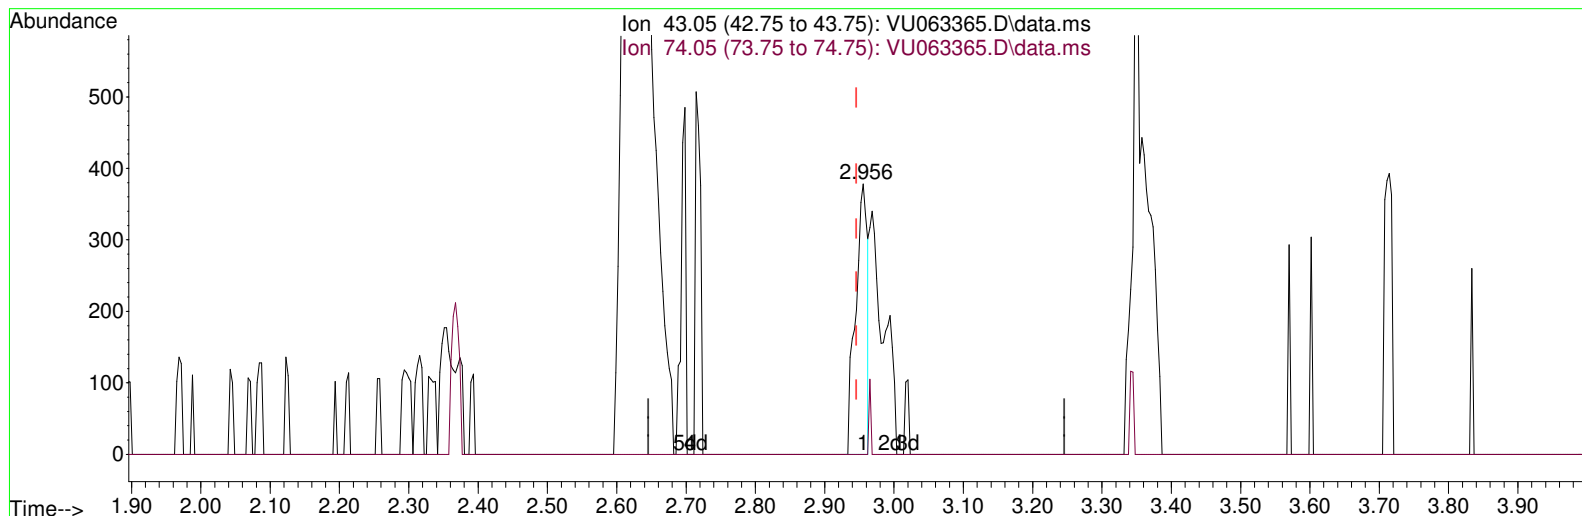

(15) Methyl Acetate (T)

2.956min (+ 0.010) 0.11 ug/L

response 446

Ion	Exp%	Act%
43.05	100.00	100.00
74.05	24.40	4.48#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060625\
Data File : VU063365.D
Acq On : 06 Jun 2025 20:36
Operator : MD/SY
Sample : Q2117-01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
MDL-WATER-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/10/2025
Supervised By :Mahesh Dadoda 06/11/2025

Quant Time: Jun 09 11:58:23 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060625WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 09 11:34:08 2025
Response via : Initial Calibration

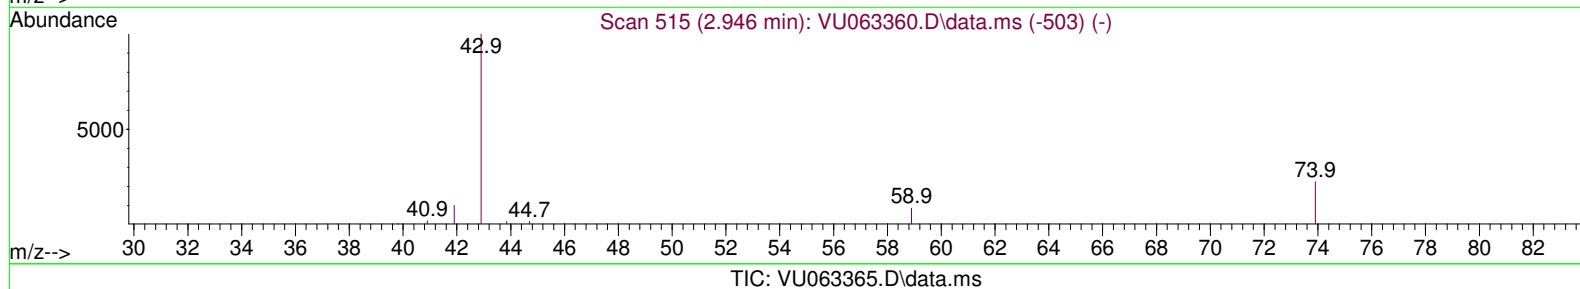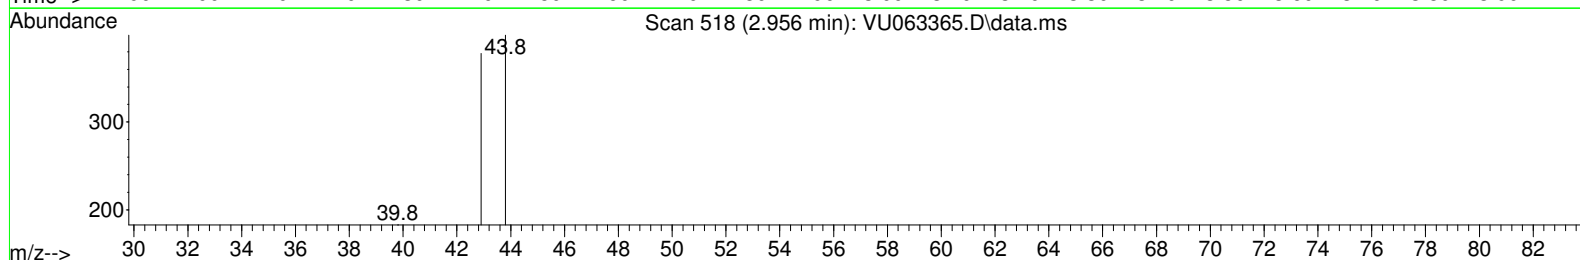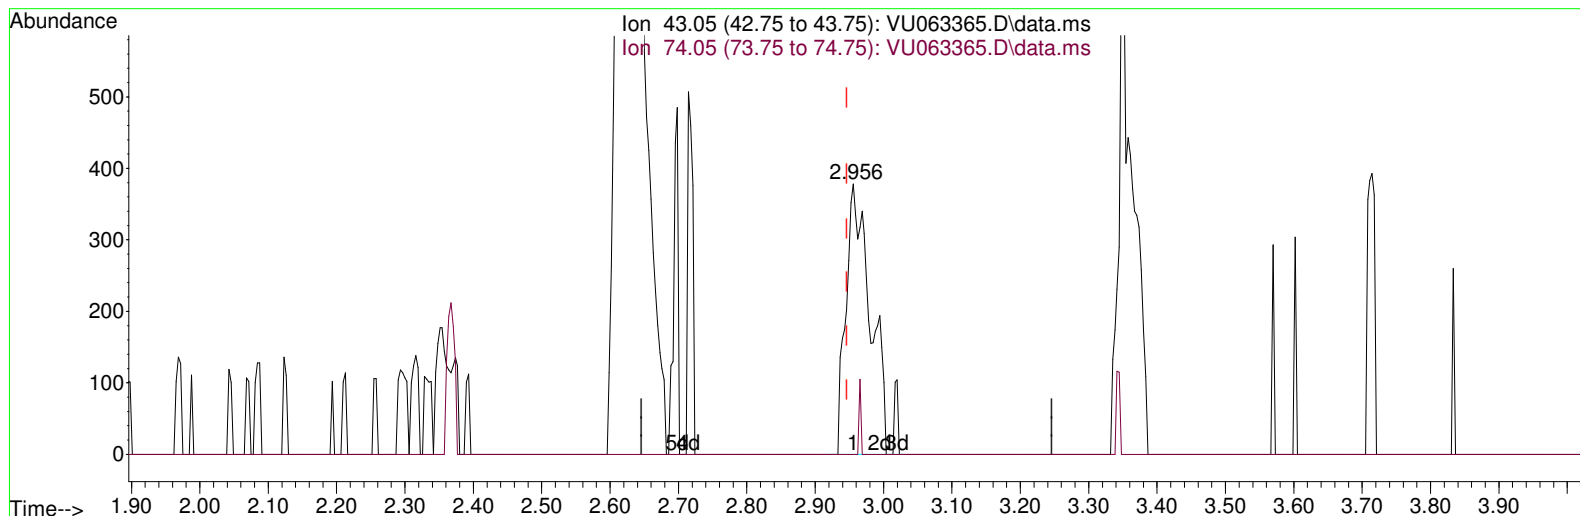

(15) Methyl Acetate (T)

2.956min (+ 0.010) 0.24 ug/L m

response 969

Ion	Exp%	Act%
43.05	100.00	100.00
74.05	24.40	2.06#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060625\
Data File : VU063365.D
Acq On : 06 Jun 2025 20:36
Operator : MD/SY
Sample : Q2117-01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
MDL-WATER-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/10/2025
Supervised By :Mahesh Dadoda 06/11/2025

Quant Time: Jun 09 11:58:23 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060625WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 09 11:34:08 2025
Response via : Initial Calibration

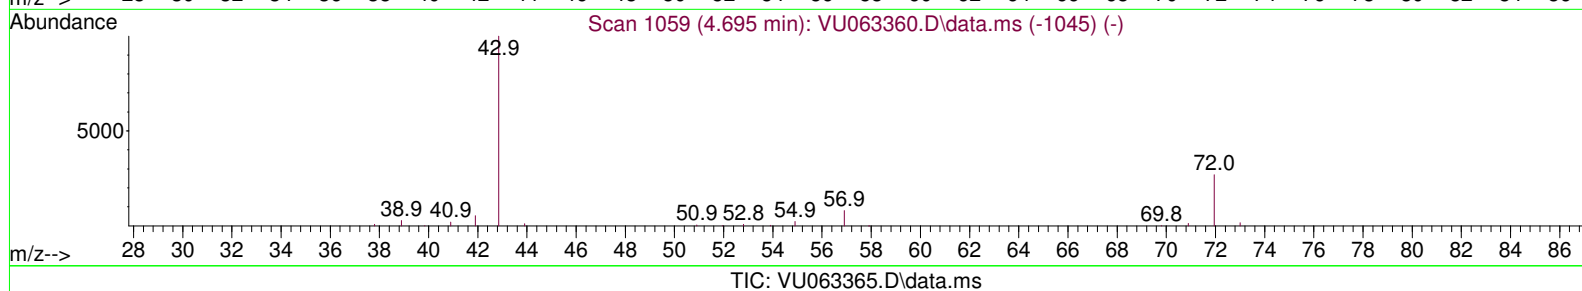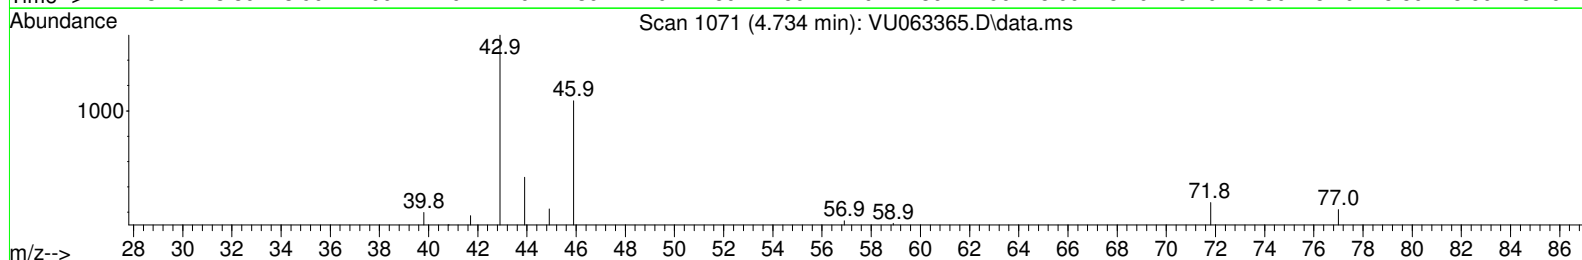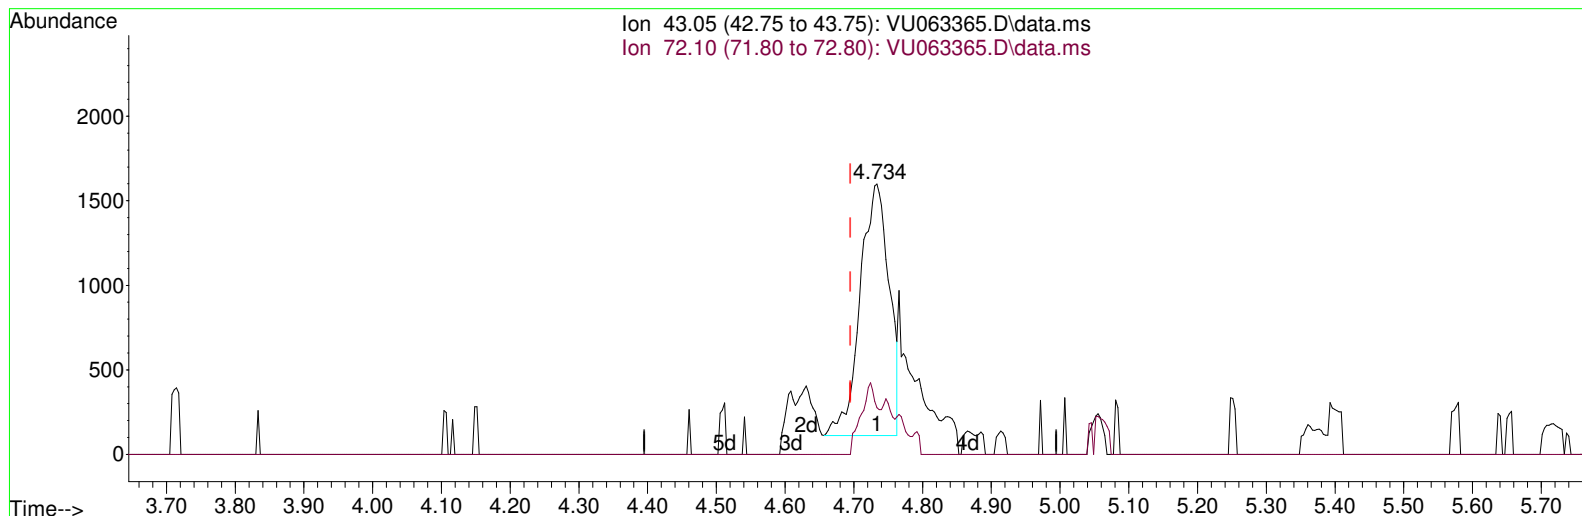

(21) 2-Butanone (T)

4.734min (+ 0.039) 1.87 ug/L

response 4333

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	27.80	16.87
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060625\
Data File : VU063365.D
Acq On : 06 Jun 2025 20:36
Operator : MD/SY
Sample : Q2117-01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
MDL-WATER-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/10/2025
Supervised By :Mahesh Dadoda 06/11/2025

Quant Time: Jun 09 11:58:23 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060625WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 09 11:34:08 2025
Response via : Initial Calibration

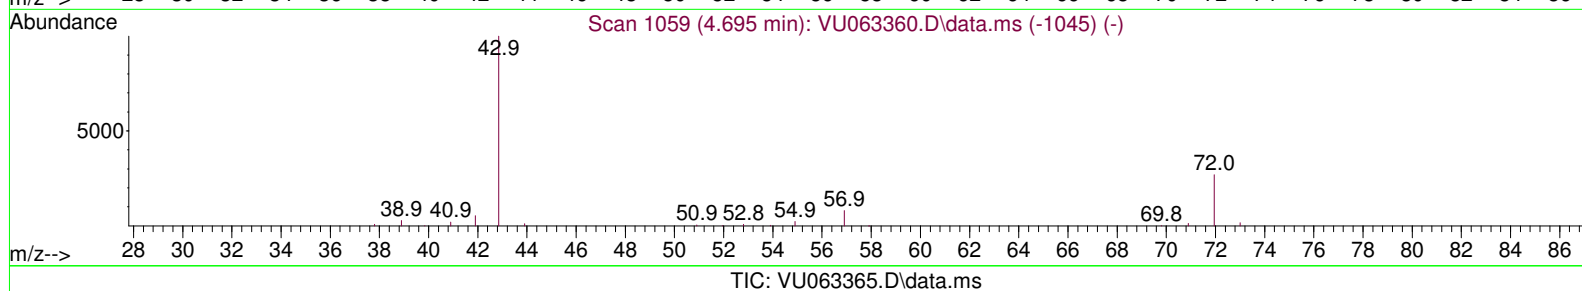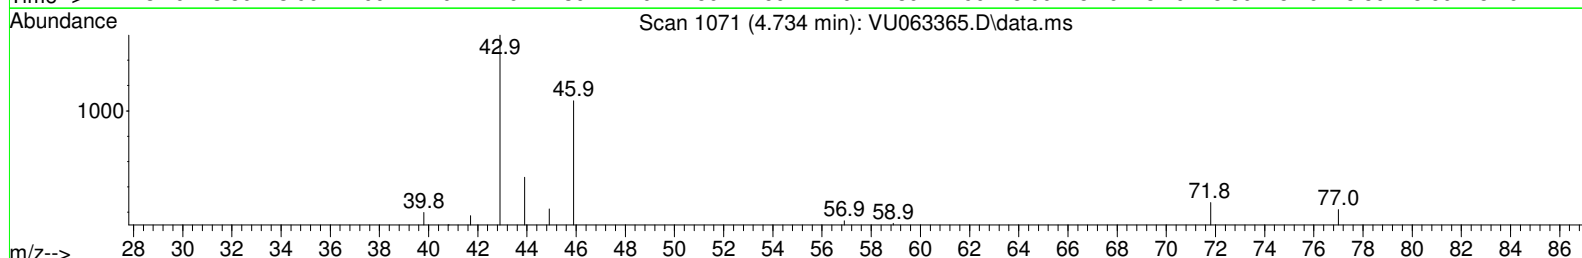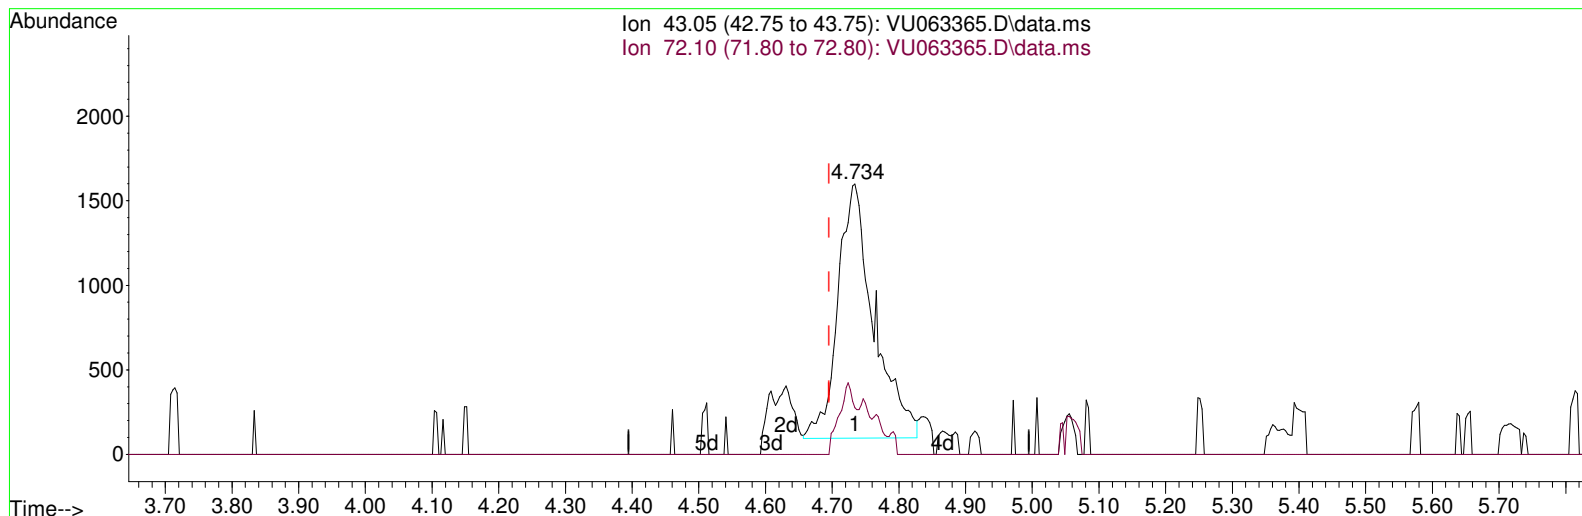

(21) 2-Butanone (T)

4.734min (+ 0.039) 2.43 ug/L m

response 5636

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	27.80	12.97#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060625\
Data File : VU063365.D
Acq On : 06 Jun 2025 20:36
Operator : MD/SY
Sample : Q2117-01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
MDL-WATER-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/10/2025
Supervised By :Mahesh Dadoda 06/11/2025

Quant Time: Jun 09 11:58:23 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060625WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 09 11:34:08 2025
Response via : Initial Calibration

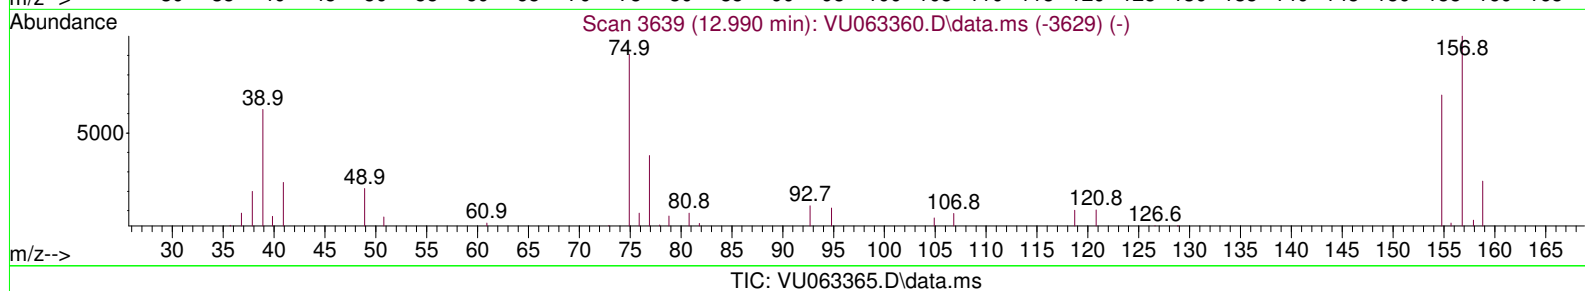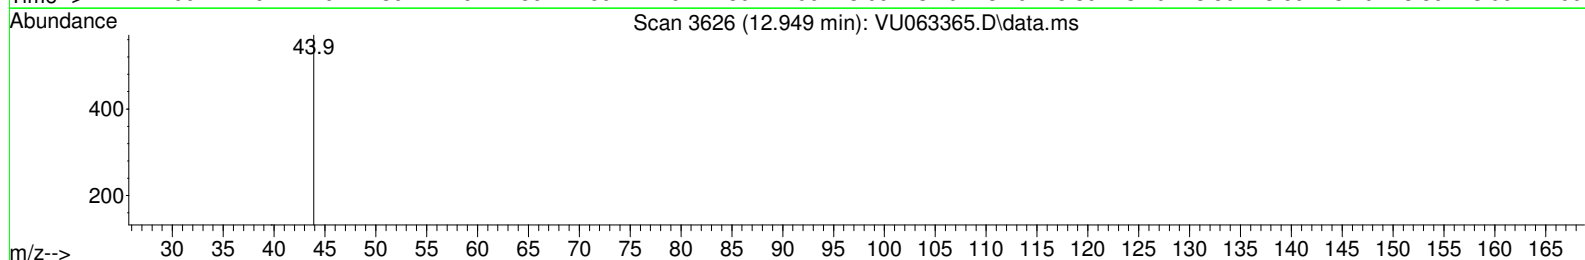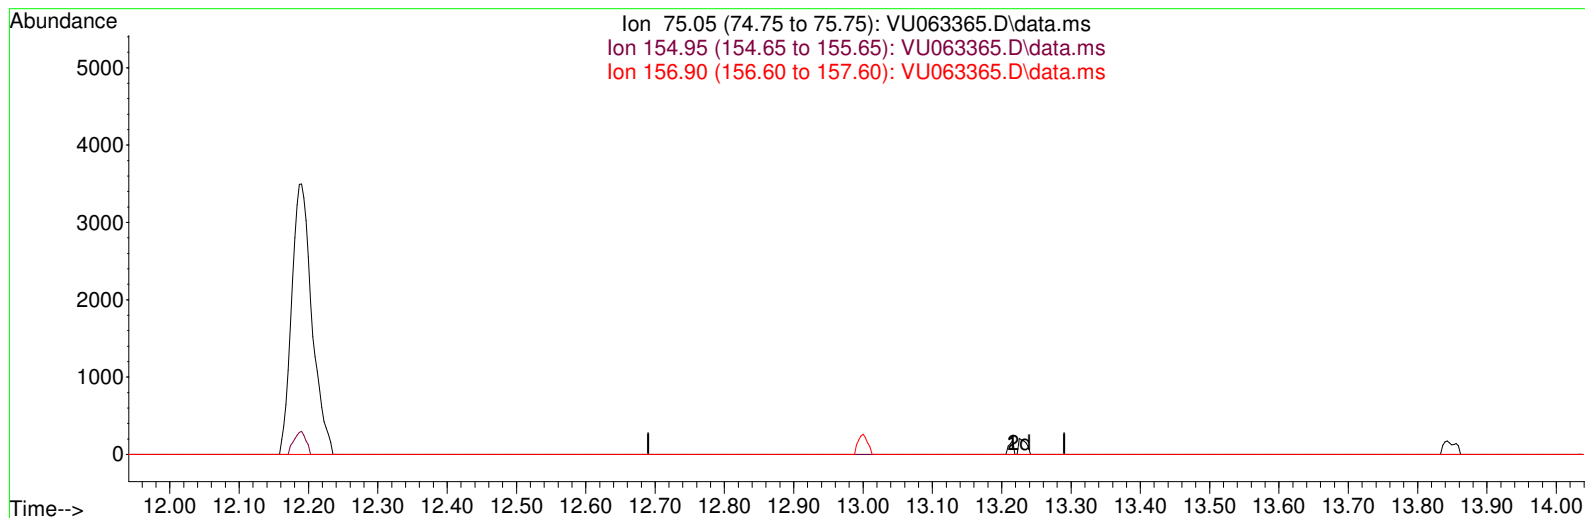

(68) 1,2-Dibromo-3-chloropropane (T)

12.949min (-0.042) 0.00 ug/L m

response 0

Ion	Exp%	Act%
75.05	100.00	0.00
154.95	77.00	0.00#
156.90	96.70	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060625\
Data File : VU063365.D
Acq On : 06 Jun 2025 20:36
Operator : MD/SY
Sample : Q2117-01
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
MDL-WATER-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/10/2025
Supervised By :Mahesh Dadoda 06/11/2025

Quant Time: Jun 09 11:58:23 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060625WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Jun 09 11:34:08 2025
Response via : Initial Calibration

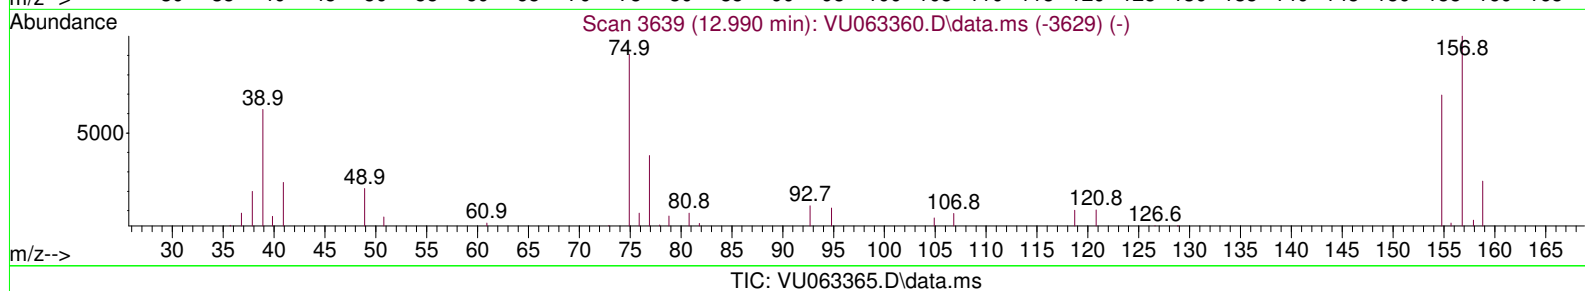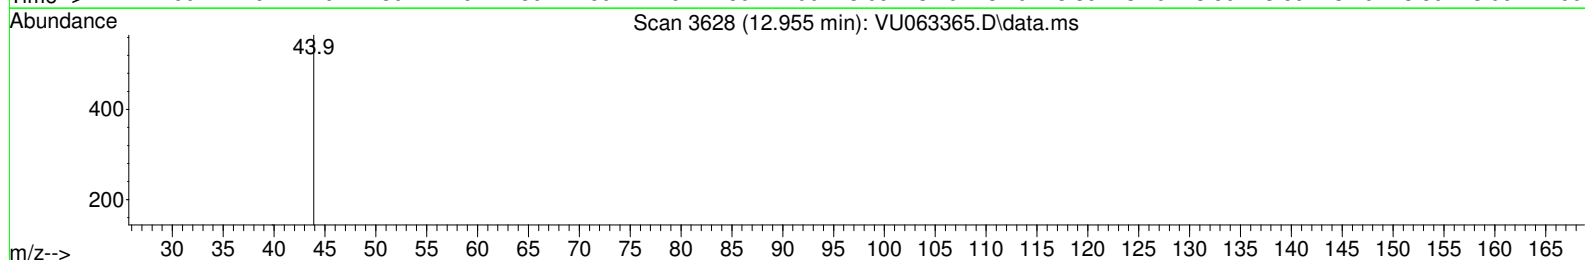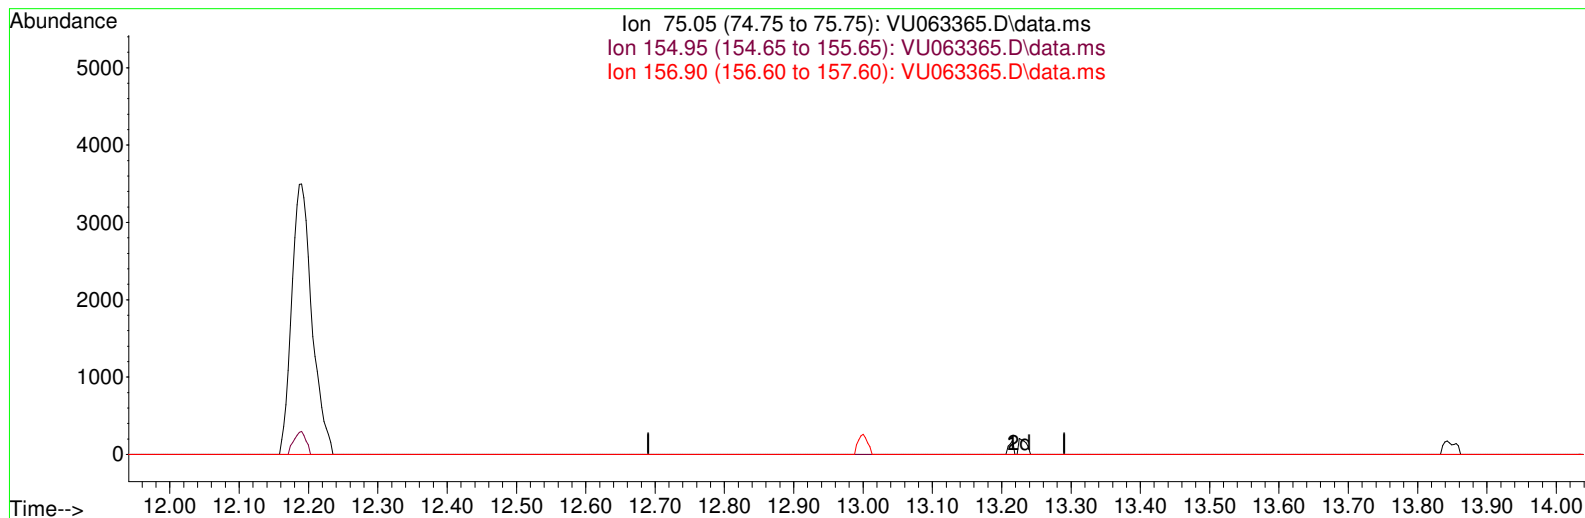

(68) 1,2-Dibromo-3-chloropropane (T)

12.955min (-0.035) 0.00 ug/L m

response 0

Ion	Exp%	Act%
75.05	100.00	0.00
154.95	77.00	0.00#
156.90	96.70	0.00#
0.00	0.00	0.00