
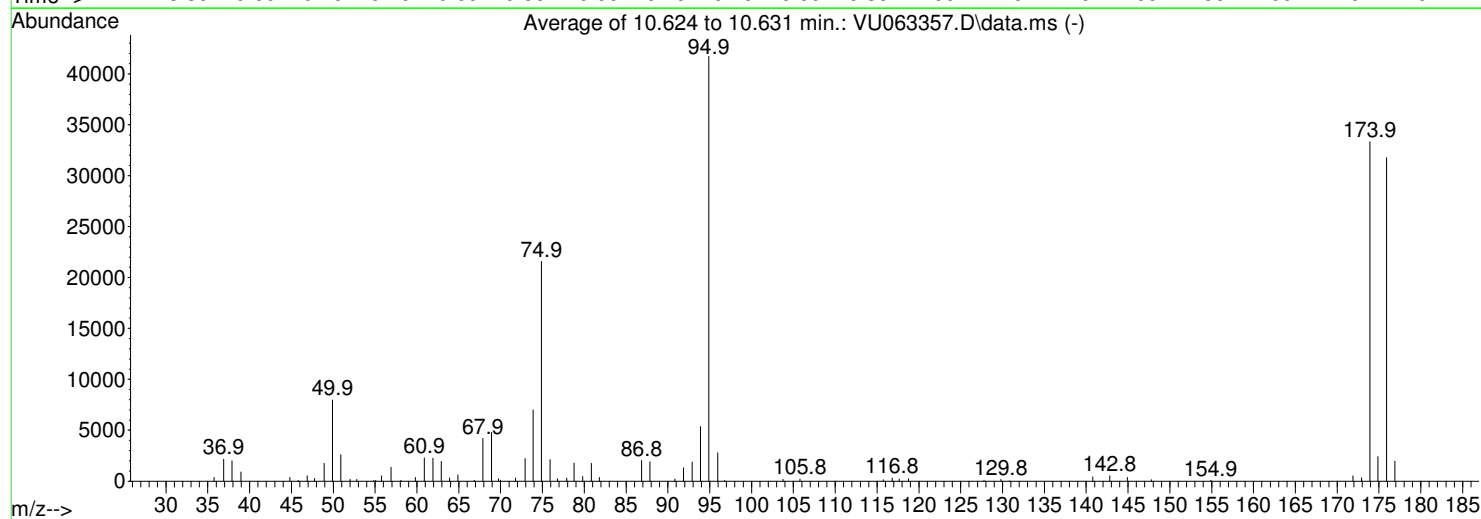


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060625\
Data File : VU063357.D
Acq On : 06 Jun 2025 09:23
Operator : MD/SY
Sample : BFB077
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB081

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060625WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Jun 09 11:34:08 2025

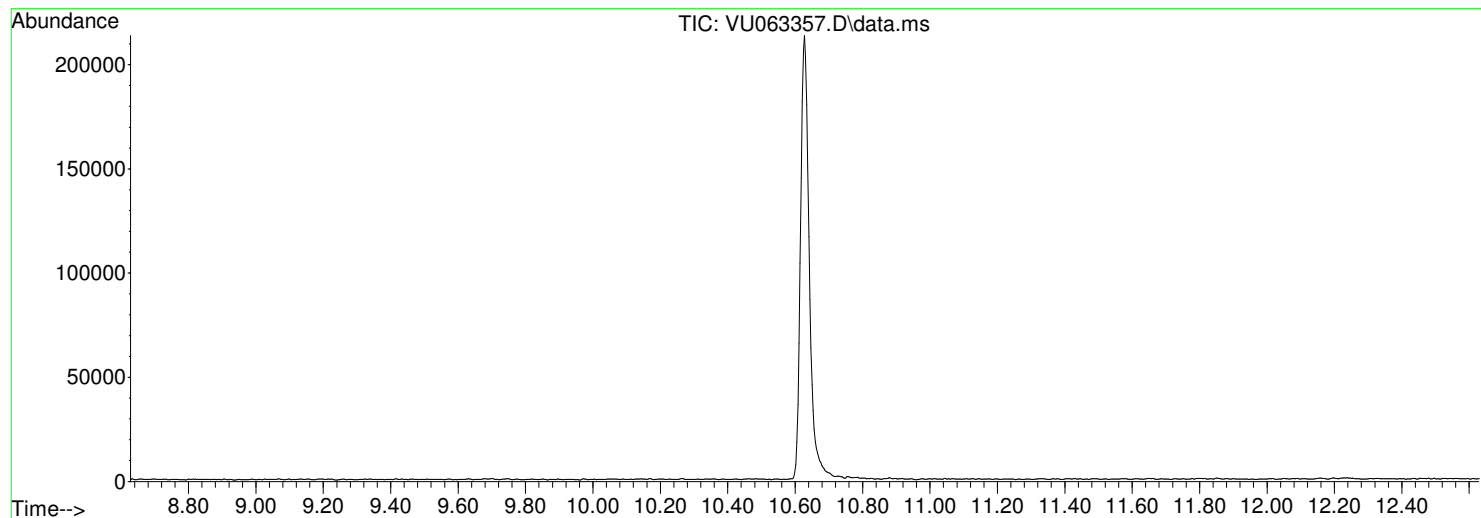

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.1	7959	PASS
75	95	30	80	51.7	21592	PASS
95	95	100	100	100.0	41728	PASS
96	95	5	9	6.7	2784	PASS
173	174	0.00	2	1.0	329	PASS
174	95	50	120	79.9	33336	PASS
175	174	5	9	7.2	2397	PASS
176	174	95	101	95.2	31752	PASS
177	176	5	9	6.2	1978	PASS

m/z	Abundance
39.80	452.0
43.90	827.0

Instrument :
MSVOA_U
ClientSampleId :
BFB081

m/z	Abundance
35.70	363.0
36.90	2041.0
37.90	2008.0
38.90	892.0
39.80	302.0
43.80	885.0
44.80	311.0
45.80	103.0
46.90	499.0
47.80	295.0
48.90	1734.0
49.90	8226.0
50.90	2591.0
51.90	197.0
52.80	148.0
54.80	186.0
55.80	499.0
56.90	1337.0
58.10	103.0
59.80	359.0
60.90	2377.0
61.90	2277.0
62.90	1971.0
63.90	312.0
64.90	525.0
66.90	157.0
67.90	4248.0
68.90	4606.0
69.70	234.0
70.00	205.0
71.80	305.0
72.90	2298.0
73.90	7299.0
74.90	22120.0
75.90	2024.0
76.80	197.0
77.90	261.0
78.80	1842.0
79.80	397.0
80.90	1778.0
81.80	268.0
86.80	2086.0
87.90	1961.0
90.80	179.0
91.80	1271.0
92.90	1781.0
93.90	5497.0
94.90	40952.0
95.90	2878.0
103.70	189.0
105.80	183.0
115.70	167.0
116.80	282.0
117.60	180.0
118.70	228.0
129.80	178.0
140.80	361.0
142.80	471.0
144.90	359.0
147.80	130.0
154.90	104.0
171.90	468.0
172.90	274.0
173.90	32880.0
174.90	2438.0
175.90	30648.0
176.90	1953.0

Instrument :
MSVOA_U
ClientSampleId :
BFB081

m/z	Abundance
35.70	358.0
36.90	2200.0
37.90	2124.0
38.90	899.0
39.90	255.0
43.80	774.0
44.80	385.0
45.80	104.0
46.90	529.0
47.80	270.0
48.90	1789.0
49.90	8096.0
50.90	2614.0
52.00	177.0
52.80	193.0
55.00	150.0
55.70	541.0
56.90	1438.0
58.10	102.0
59.80	347.0
60.90	2335.0
61.90	2327.0
62.90	1991.0
63.90	291.0
64.90	646.0
66.80	110.0
67.90	4366.0
68.90	5019.0
69.70	245.0
71.80	291.0
72.90	2253.0
73.90	7173.0
74.90	22408.0
75.90	2196.0
76.80	271.0
77.90	313.0
78.80	1800.0
79.80	498.0
80.90	1801.0
81.80	361.0
86.90	2042.0
87.90	1946.0
90.80	182.0
91.80	1334.0
92.90	1943.0
93.90	5576.0
94.90	42920.0
95.90	2831.0
96.80	113.0
103.70	173.0
105.80	193.0
115.70	152.0
116.80	320.0
117.60	207.0
118.80	247.0
127.80	124.0
129.80	185.0
140.80	435.0
142.80	549.0
144.90	391.0
147.80	164.0
154.90	111.0
171.90	515.0
172.90	328.0
173.90	34056.0
174.90	2454.0
175.90	32480.0
176.90	2023.0

Instrument :
MSVOA_U
ClientSampleId :
BFB081

m/z	Abundance
35.80	330.0
36.90	2210.0
37.90	1881.0
39.00	864.0
40.00	275.0
43.90	796.0
44.80	414.0
46.90	504.0
47.60	239.0
48.90	1748.0
49.90	7556.0
50.90	2559.0
52.10	112.0
52.80	178.0
55.10	126.0
55.70	546.0
56.90	1355.0
59.80	339.0
60.90	2090.0
61.90	2180.0
62.90	1846.0
63.90	280.0
64.90	647.0
67.90	4017.0
68.90	4739.0
69.80	233.0
71.80	258.0
73.00	2109.0
73.90	6539.0
74.90	20248.0
75.90	2142.0
76.80	260.0
77.90	320.0
78.80	1687.0
79.80	505.0
80.80	1671.0
81.80	452.0
86.90	1948.0
87.80	1773.0
90.90	236.0
91.90	1311.0
92.90	1910.0
93.90	5025.0
94.90	41312.0
96.00	2643.0
96.80	107.0
103.80	157.0
105.80	218.0
115.80	108.0
116.80	311.0
117.70	196.0
118.80	251.0
127.80	131.0
129.80	151.0
130.80	100.0
140.80	454.0
142.80	572.0
144.90	298.0
147.80	145.0
171.90	574.0
172.90	386.0
173.90	33072.0
174.80	2299.0
175.90	32128.0
176.90	1957.0

Instrument :
MSVOA_U
ClientSampleId :
BFB081