


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060719\
 Data File : VU032529.D
 Acq On : 07 Jun 2019 08:40
 Operator : JC/SP
 Sample : BFB50
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB50

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Title : VOC Analysis
 Last Update : Sat Jun 08 23:12:44 2019

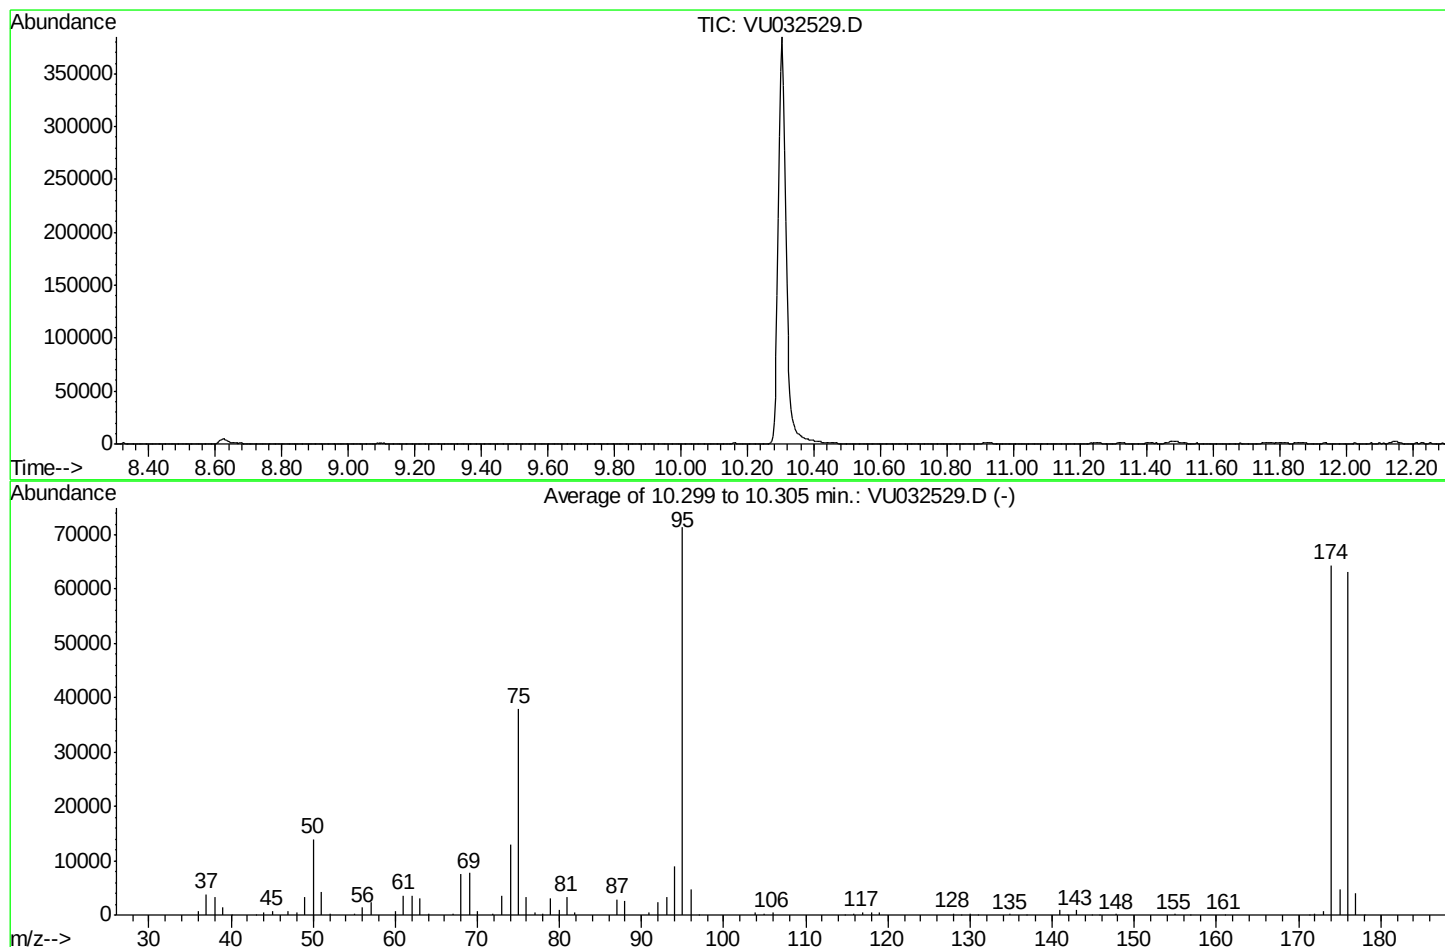

AutoFind: Scans 2864, 2865, 2866; Background Corrected with Scan 2853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	13975	PASS
75	95	30	80	53.2	37970	PASS
95	95	100	100	100.0	71381	PASS
96	95	5	9	6.8	4836	PASS
173	174	0.00	2	1.0	622	PASS
174	95	50	120	90.2	64365	PASS
175	174	5	9	7.3	4690	PASS
176	174	95	101	98.0	63066	PASS
177	176	5	9	6.5	4121	PASS

m/z	Abundance
43.90	355.0

Instrument :
MSVOA_U
ClientSampleId :
BFB50

m/z	Abundance
36.00	601.0
37.00	3770.0
38.00	3222.0
39.00	1462.0
44.00	850.0
45.00	746.0
47.00	746.0
48.00	443.0
49.00	3205.0
50.00	13493.0
51.00	4034.0
52.00	224.0
55.00	271.0
56.00	1381.0
57.00	2163.0
60.00	738.0
61.00	3510.0
62.00	3507.0
63.00	2977.0
64.00	230.0
67.00	229.0
68.00	7174.0
69.00	7333.0
70.00	651.0
71.90	277.0
73.00	3479.0
74.00	12368.0
75.00	36320.0
76.00	3273.0
77.10	446.0
78.00	321.0
78.90	2937.0
80.00	868.0
80.90	3138.0
81.90	544.0
87.00	2800.0
88.00	2478.0
90.90	370.0
92.00	2092.0
93.00	3021.0
94.00	8568.0
95.00	68128.0
96.00	4787.0
97.00	133.0
103.90	332.0
104.90	178.0
106.00	420.0
115.90	292.0
116.90	484.0
118.00	344.0
118.90	415.0
128.00	294.0
130.00	214.0
135.00	112.0
136.80	125.0
140.90	866.0
141.90	100.0
142.90	772.0
145.80	148.0
147.90	154.0
154.90	190.0
172.00	145.0
173.00	581.0
174.00	59984.0
175.00	4530.0
176.00	57992.0
177.00	3986.0
178.00	140.0

Instrument :
MSVOA_U
ClientSampleId :
BFB50

m/z	Abundance
36.10	669.0
37.00	3931.0
38.00	3465.0
39.00	1529.0
40.00	106.0
44.00	872.0
45.00	823.0
47.00	824.0
47.90	477.0
49.00	3420.0
50.00	14475.0
51.00	4440.0
52.00	202.0
55.10	265.0
56.00	1432.0
57.00	2415.0
60.00	766.0
61.00	3777.0
62.00	3710.0
63.00	3120.0
64.10	263.0
67.00	250.0
68.00	7847.0
69.00	7944.0
70.00	660.0
71.90	324.0
73.00	3716.0
74.00	13344.0
75.00	39208.0
76.00	3354.0
77.00	461.0
78.00	326.0
78.90	3163.0
79.90	907.0
80.90	3436.0
81.90	573.0
87.00	2939.0
88.00	2764.0
90.90	416.0
92.00	2352.0
93.00	3318.0
94.00	9140.0
95.00	73816.0
96.00	4989.0
97.00	122.0
103.90	396.0
105.00	162.0
106.00	458.0
114.70	108.0
115.90	274.0
116.90	532.0
118.00	386.0
118.90	448.0
128.00	315.0
128.90	109.0
130.00	239.0
131.00	101.0
134.80	136.0
136.80	122.0
140.90	926.0
141.80	110.0
143.00	931.0
145.80	130.0
147.90	168.0
154.90	228.0
156.80	123.0
161.00	138.0
172.00	138.0
173.00	645.0
174.00	66480.0
175.00	4842.0
176.00	65360.0
177.00	4261.0
178.00	109.0

Instrument :
MSVOA_U
ClientSampleId :
BFB50

m/z	Abundance
36.00	663.0
37.00	3736.0
38.00	3403.0
39.00	1418.0
40.00	128.0
43.00	104.0
44.00	853.0
45.00	769.0
47.00	807.0
47.90	502.0
49.00	3269.0
50.00	13959.0
51.00	4327.0
52.00	167.0
55.10	249.0
56.00	1334.0
57.00	2324.0
59.90	689.0
61.00	3655.0
62.00	3612.0
63.00	2942.0
64.10	271.0
67.00	261.0
68.00	7622.0
69.00	7727.0
70.00	663.0
71.90	354.0
73.00	3562.0
74.00	13014.0
75.00	38384.0
76.00	3171.0
77.00	413.0
77.90	322.0
78.90	3123.0
79.90	811.0
80.90	3341.0
81.90	583.0
87.00	2781.0
88.00	2797.0
90.90	390.0
92.00	2315.0
93.00	3273.0
94.00	8862.0
95.00	72200.0
96.00	4732.0
103.90	413.0
104.90	119.0
105.90	422.0
114.70	107.0
115.80	291.0
116.90	526.0
118.00	362.0
118.90	470.0
127.90	301.0
128.90	146.0
130.00	228.0
131.00	122.0
134.80	149.0
136.80	121.0
141.00	874.0
141.80	102.0
143.00	979.0
144.80	104.0
145.70	104.0
147.80	161.0
154.90	227.0
156.80	161.0
161.00	149.0
171.30	106.0
172.00	133.0
173.00	640.0
174.00	66632.0
175.00	4698.0
176.00	65848.0
177.00	4116.0

Instrument :
MSVOA_U
ClientSampleId :
BFB50