


# Methylene Chloride

Response Ratio

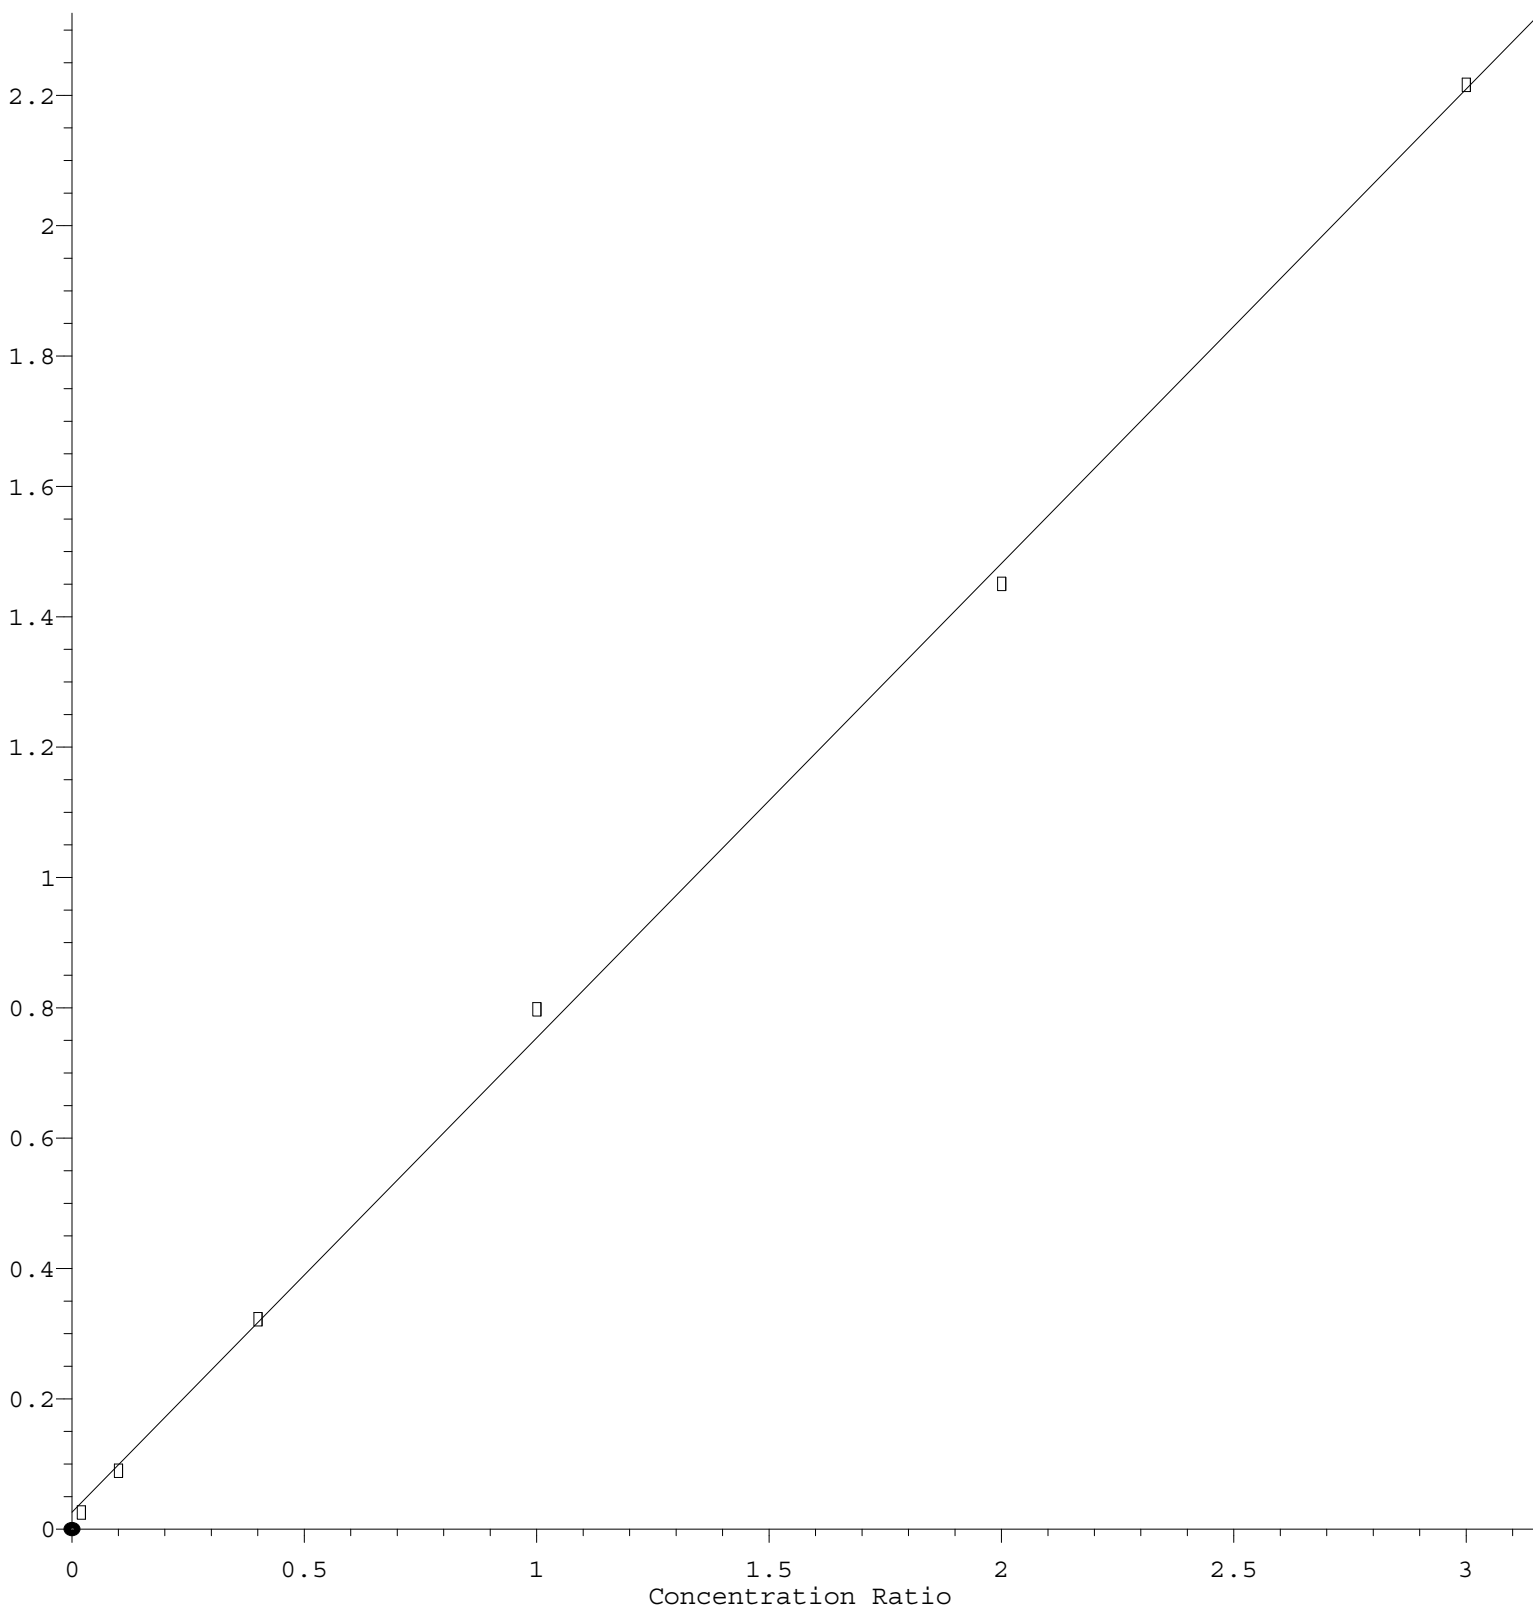

$$\text{Response} = 7.281\text{e-}001 * \text{Amt} + 2.561\text{e-}002$$


Coef of Det ( $r^2$ ) = 0.999133 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U060721W.M

Calibration Table Last Updated: Tue Jun 08 17:38:51 2021

## Chloromethane

Response Ratio

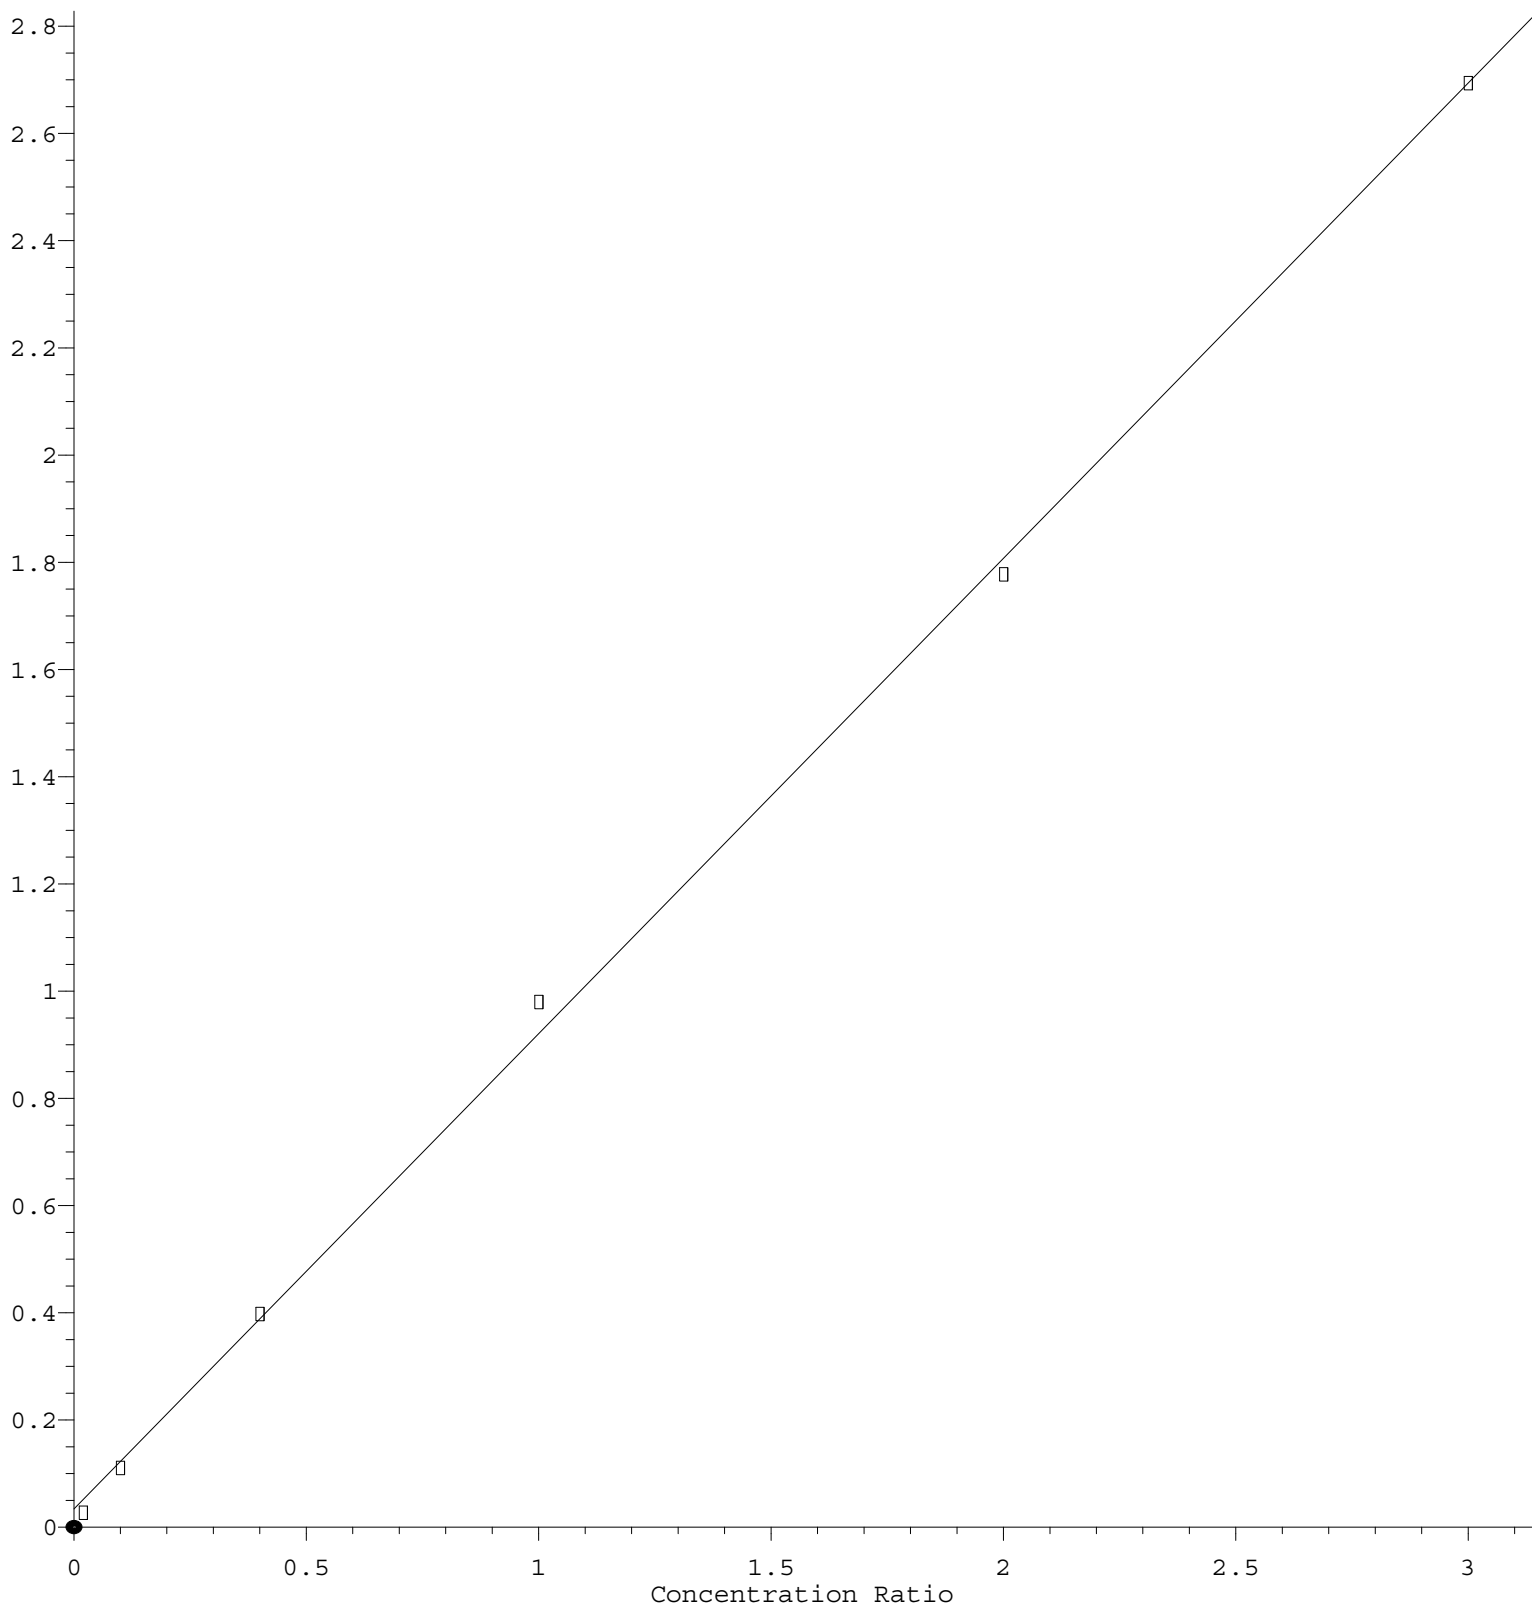

$$\text{Response} = 8.867\text{e-}001 * \text{Amt} + 3.408\text{e-}002$$


Coef of Det ( $r^2$ ) = 0.999066 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U060721W.M

Calibration Table Last Updated: Tue Jun 08 17:38:51 2021

## Ethyl methacrylate

Response Ratio

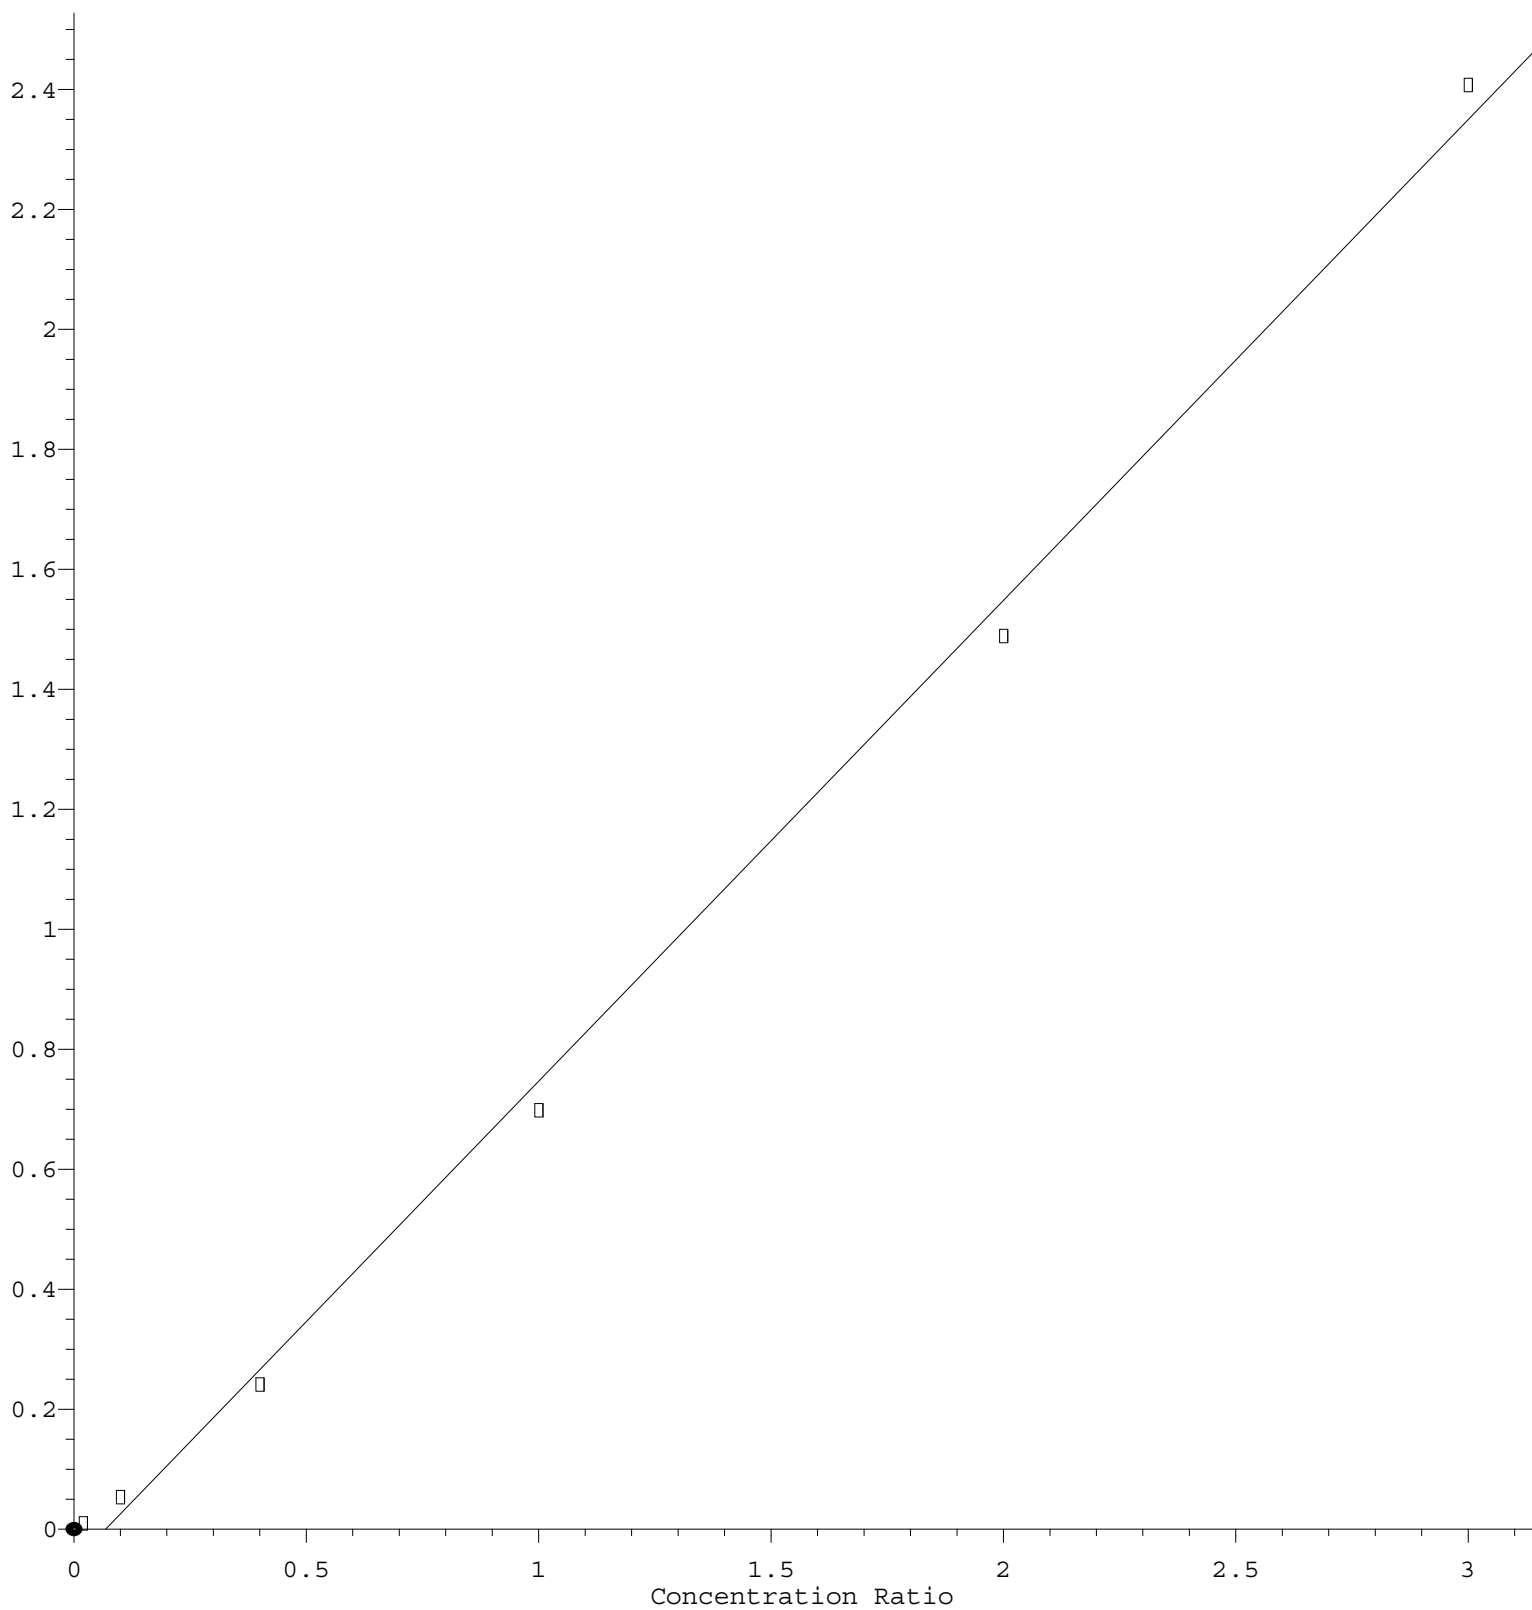

$$\text{Response} = 8.012\text{e-}001 * \text{Amt} - 5.425\text{e-}002$$


Coef of Det ( $r^2$ ) = 0.997174 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U060721W.M

Calibration Table Last Updated: Tue Jun 08 17:38:51 2021

# 2-Chloroethyl Vinyl ether

Response Ratio

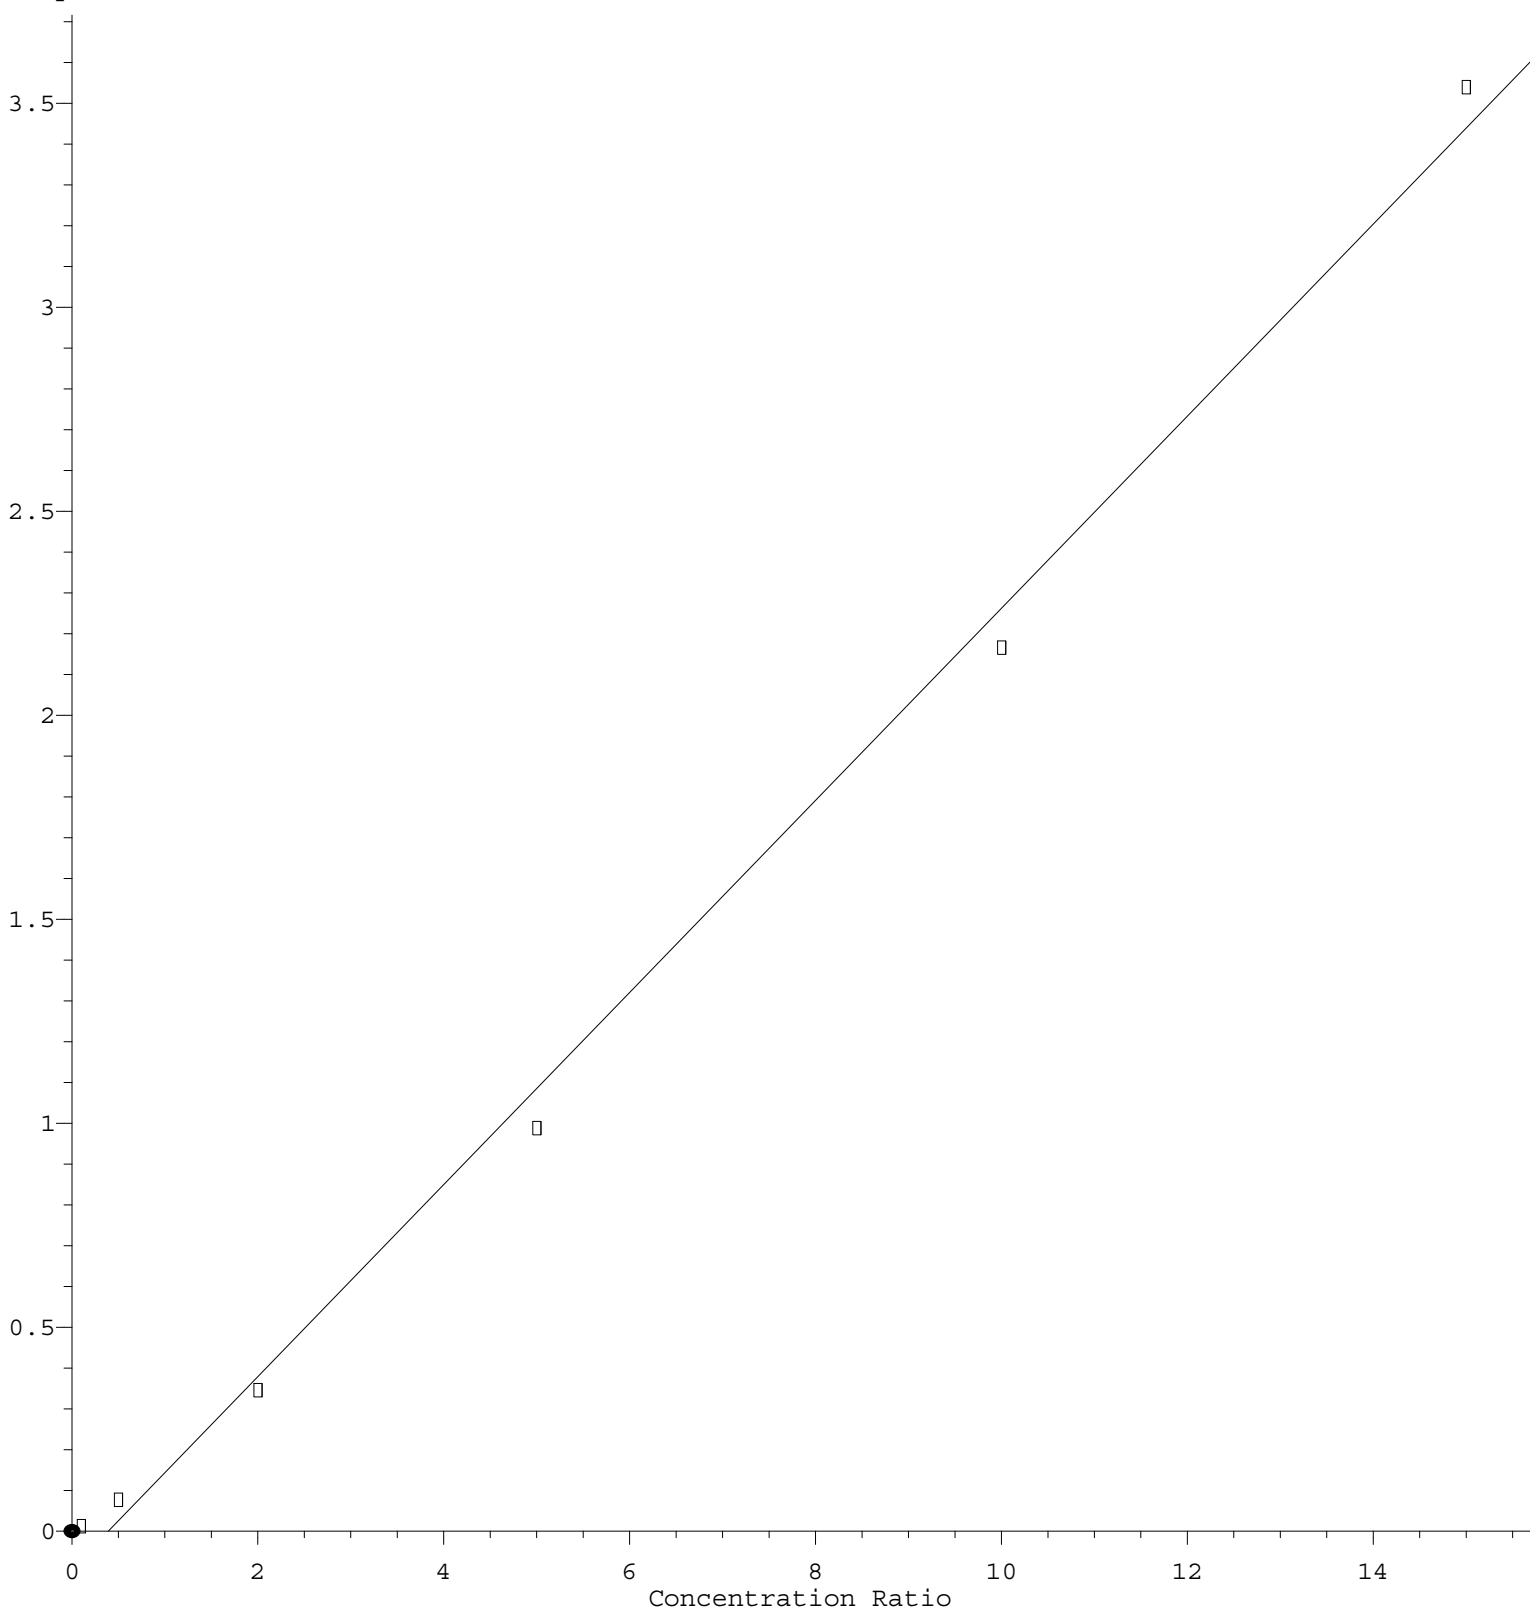

$$\text{Response} = 2.354\text{e-}001 * \text{Amt} - 9.087\text{e-}002$$


Coef of Det ( $r^2$ ) = 0.996040 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U060721W.M

Calibration Table Last Updated: Tue Jun 08 17:38:51 2021

# 1,2,4-Trimethylbenzene

Response Ratio

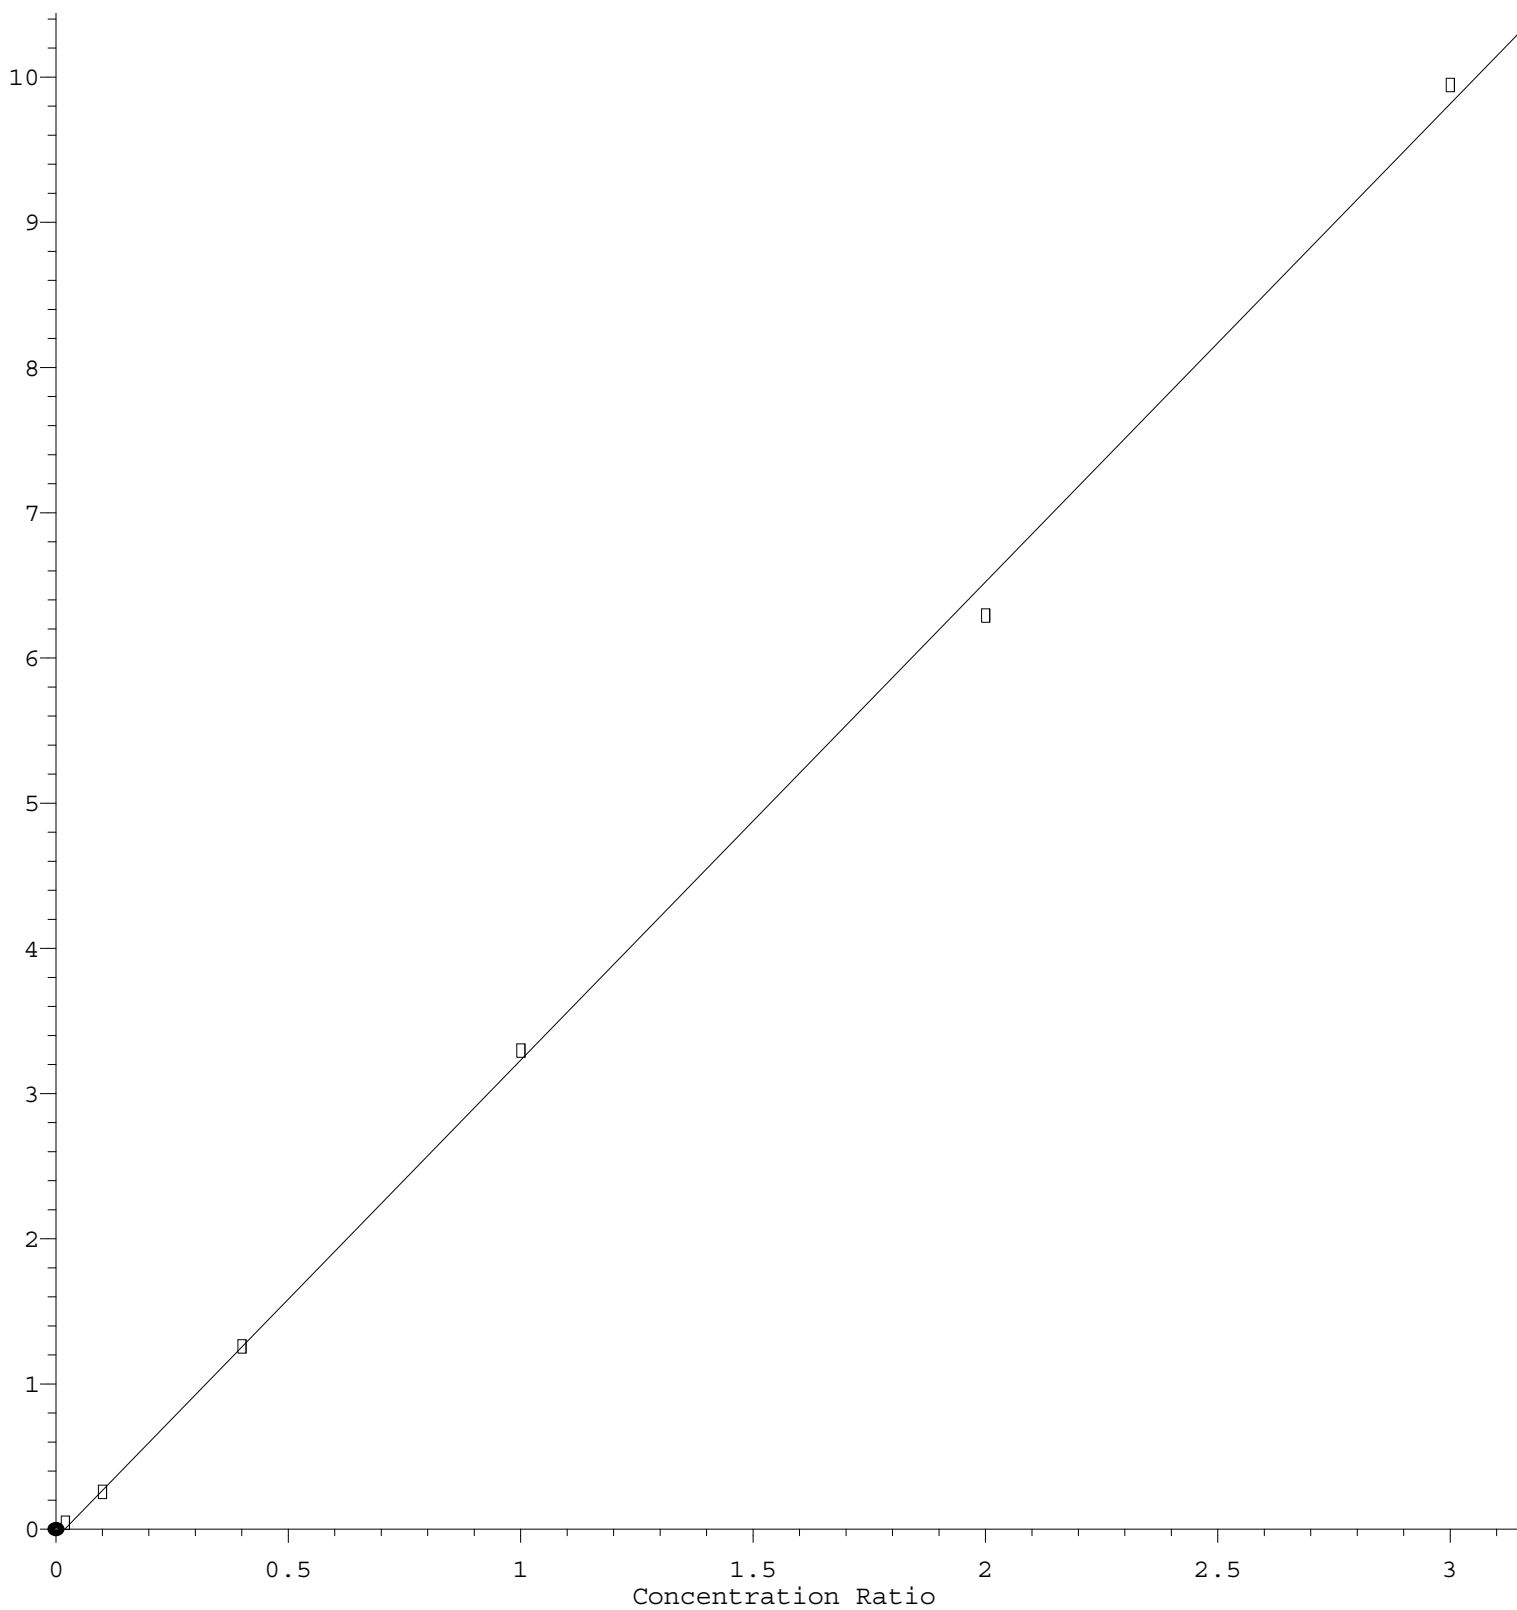

$$\text{Response} = 3.292\text{e}+000 * \text{Amt} - 6.247\text{e}-002$$


Coef of Det ( $r^2$ ) = 0.999005 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U060721W.M

Calibration Table Last Updated: Tue Jun 08 17:38:51 2021

# Naphthalene

Response Ratio

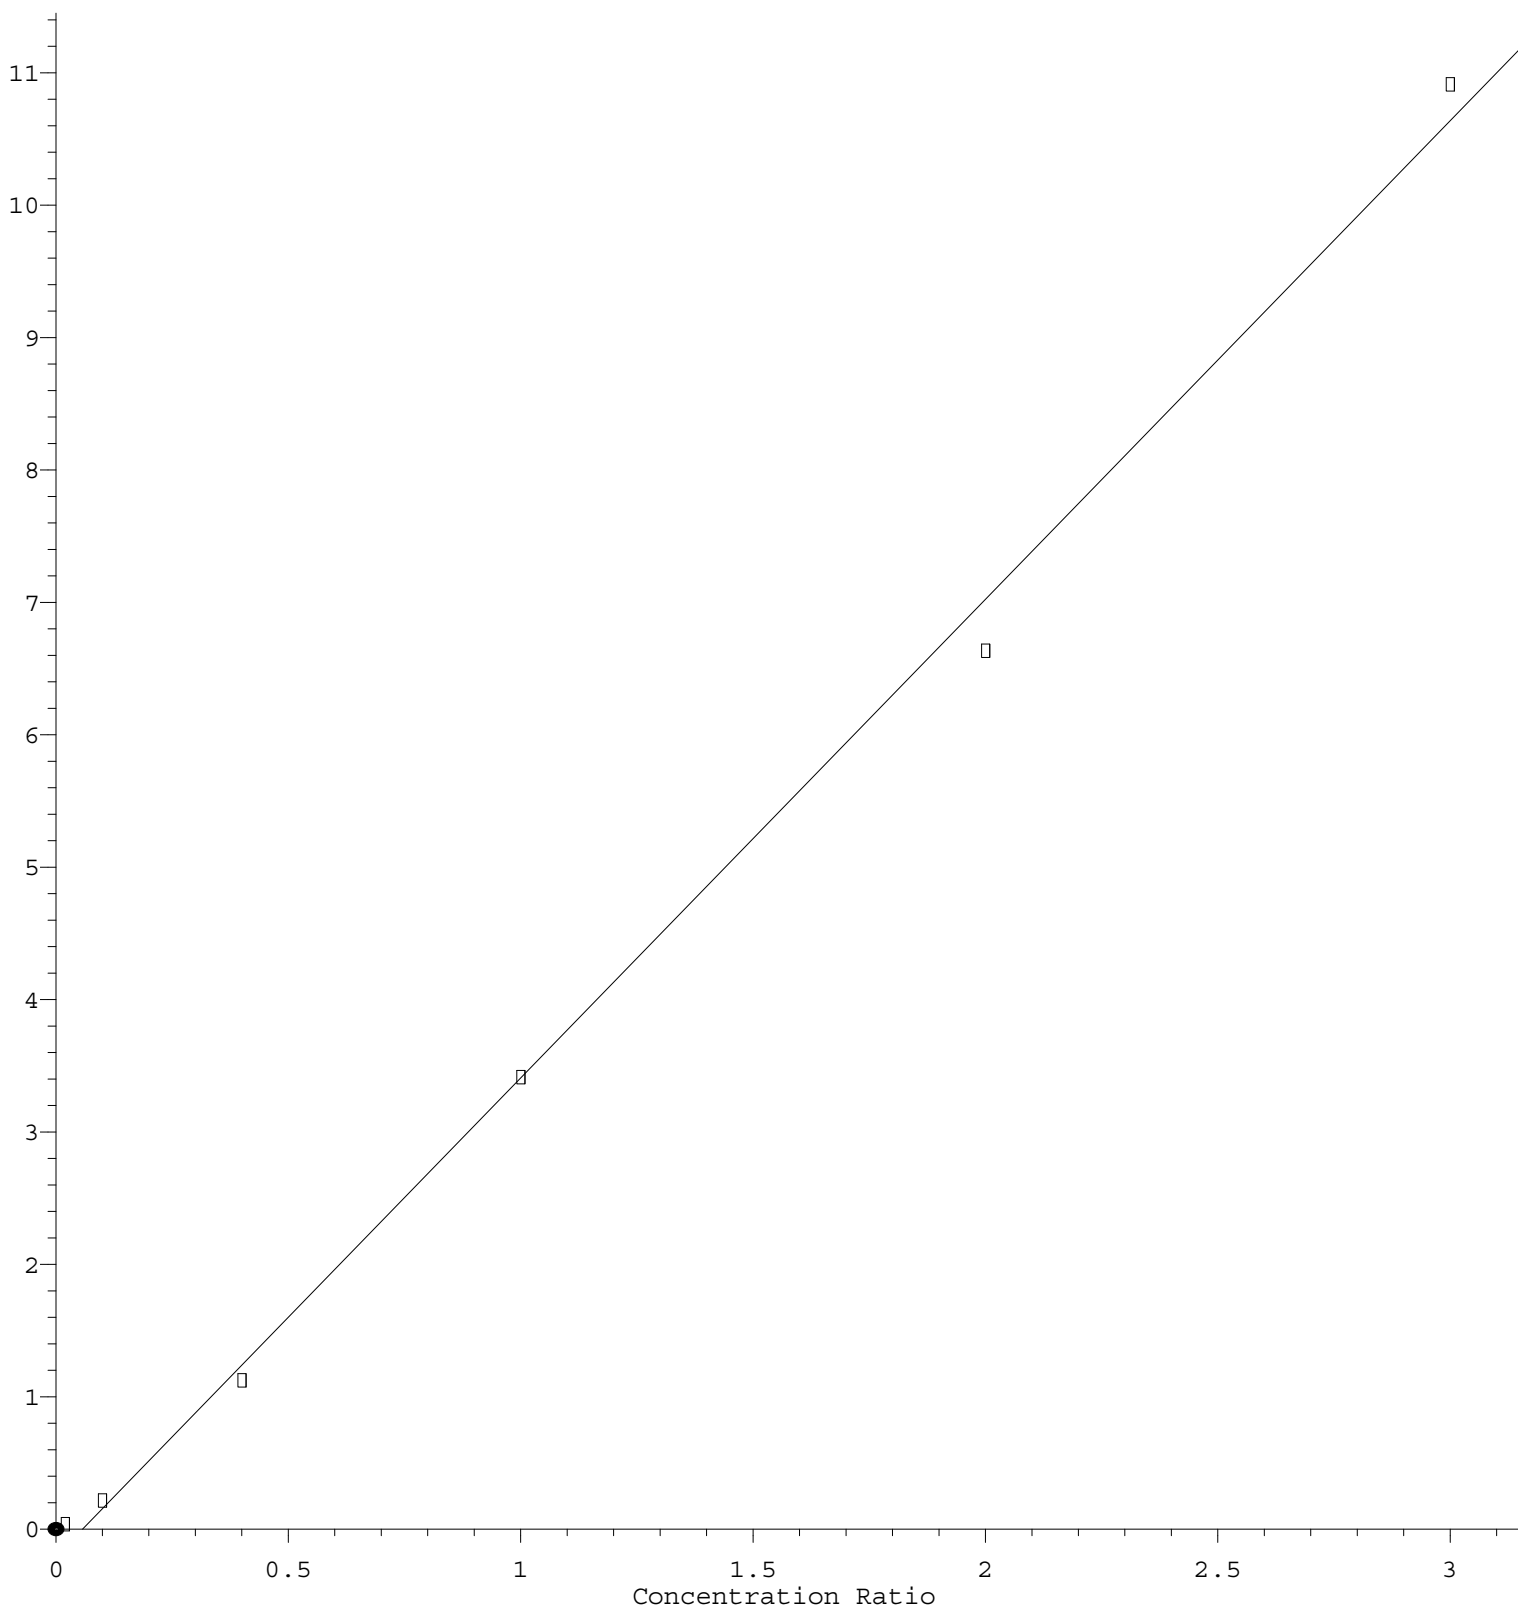

$$\text{Response} = 3.615\text{e}+000 * \text{Amt} - 2.058\text{e}-001$$

Coef of Det ( $r^2$ ) = 0.997063 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U060721W.M

Calibration Table Last Updated: Tue Jun 08 17:38:51 2021