

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060721\
 Data File : VU044063.D
 Acq On : 07 Jun 2021 18:19
 Operator : SY/MD
 Sample : VU0607WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0607WBL01

Quant Time: Jun 08 05:44:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U060721W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 08 05:21:34 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.382	168	209778	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.256	114	419057	50.000	ug/l	0.00
63) Chlorobenzene-d5	9.423	117	419474	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.819	152	197304	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.710	65	192769	52.764	ug/l	0.00
Spiked Amount	50.000		Recovery	=	105.520%	
35) Dibromofluoromethane	5.298	113	149386	49.954	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.900%	
50) Toluene-d8	7.906	98	560335	48.577	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.160%	
62) 4-Bromofluorobenzene	10.639	95	205826	45.069	ug/l	0.00
Spiked Amount	50.000		Recovery	=	90.140%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060721\
Data File : VU044063.D
Acq On : 07 Jun 2021 18:19
Operator : SY/MD
Sample : VU0607WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0607WBL01

Quant Time: Jun 08 05:44:20 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U060721W.M
Quant Title : SW846 8260
QLast Update : Tue Jun 08 05:21:34 2021
Response via : Initial Calibration




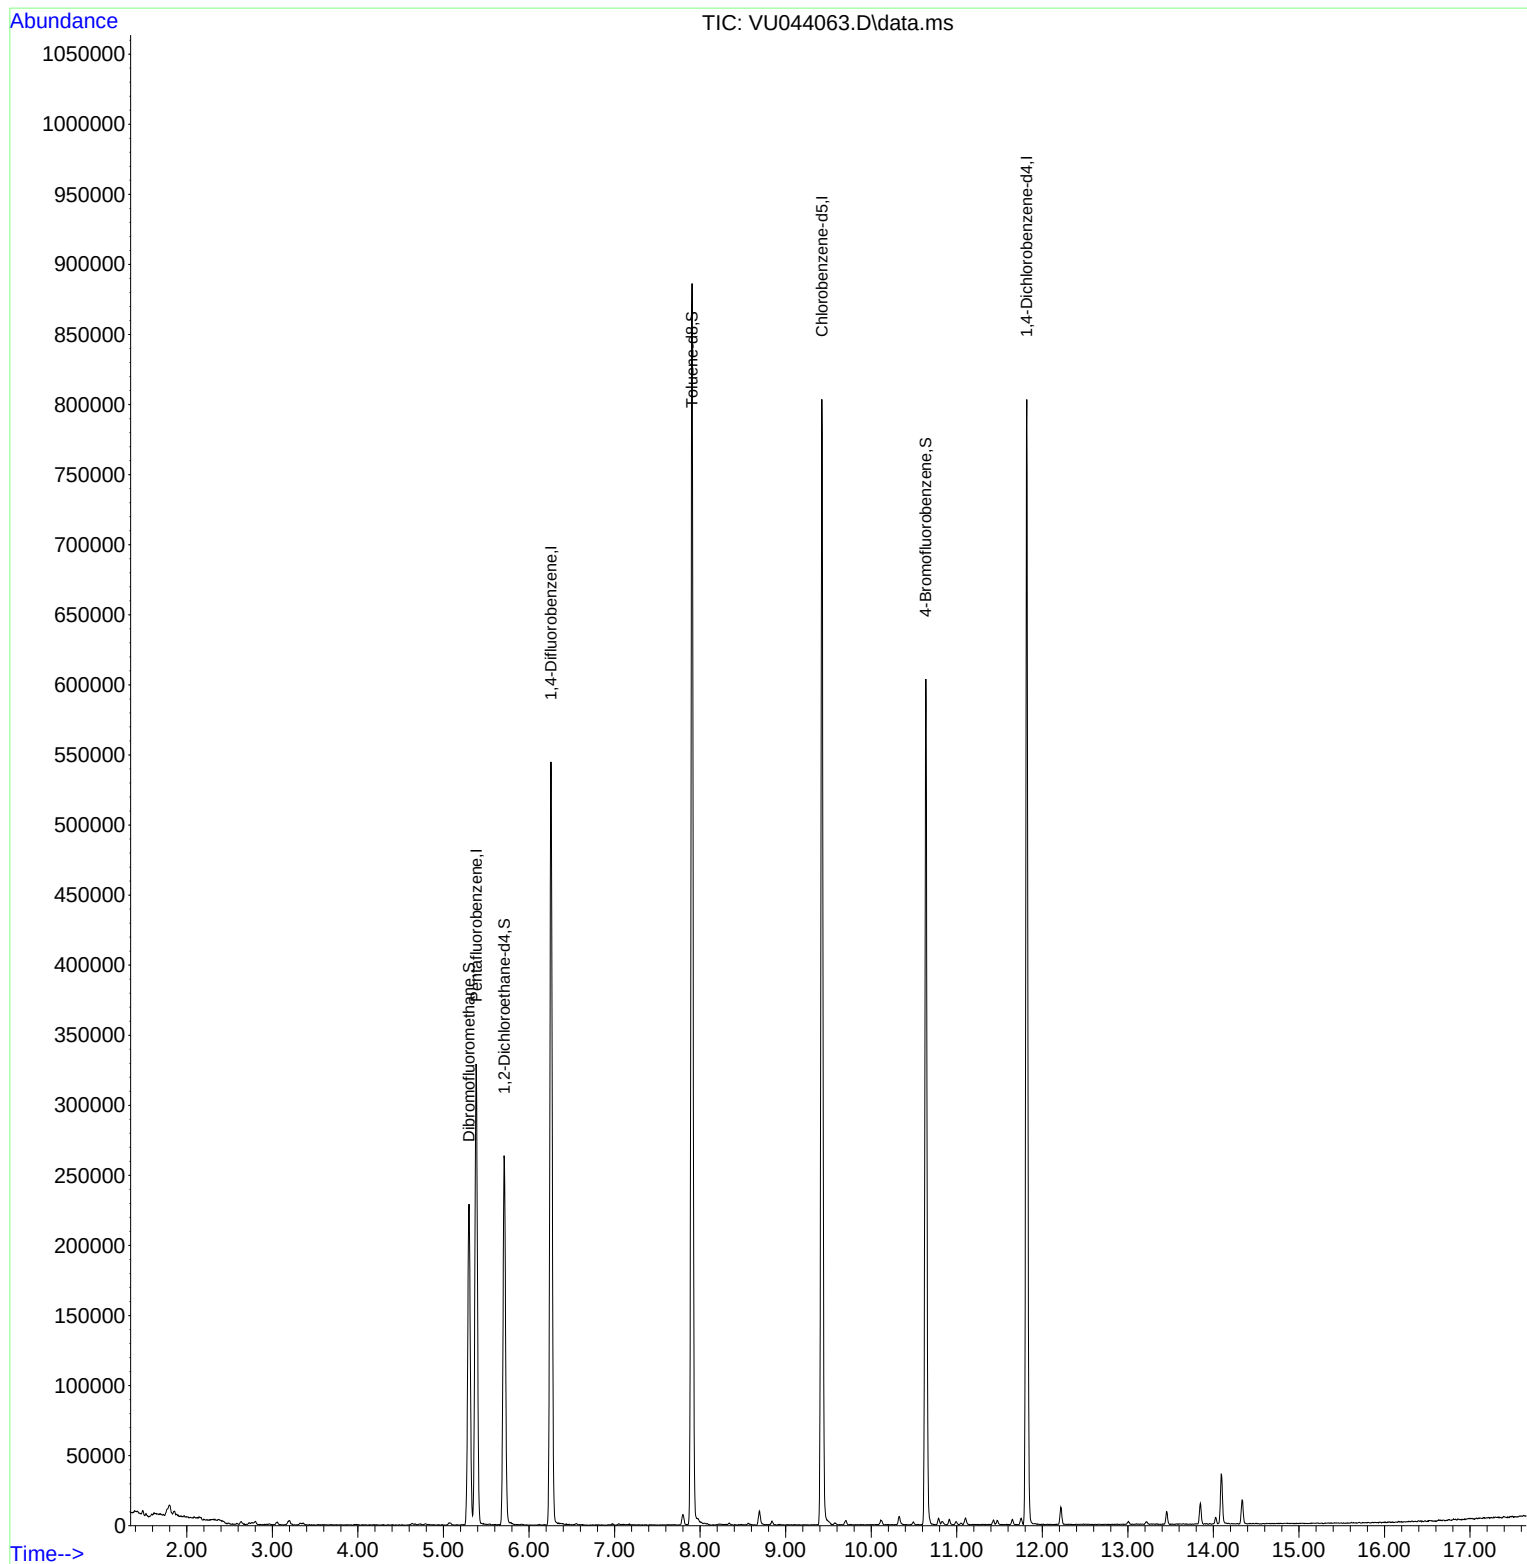


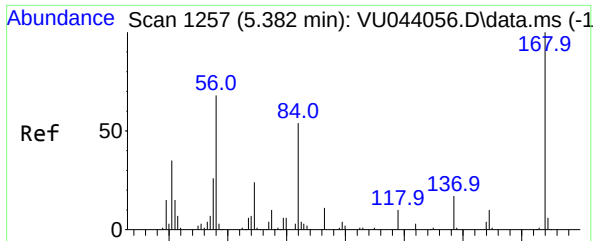

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.382 min Scan# 1257
Delta R.T. -0.000 min
Lab File: VU044063.D
Acq: 07 Jun 2021 18:19




Instrument :
MSVOA_U
ClientSampleId :
VU0607WBL01


Tgt Ion:168 Resp: 209778
Ion Ratio Lower Upper
168 100
99 66.1 52.6 78.8

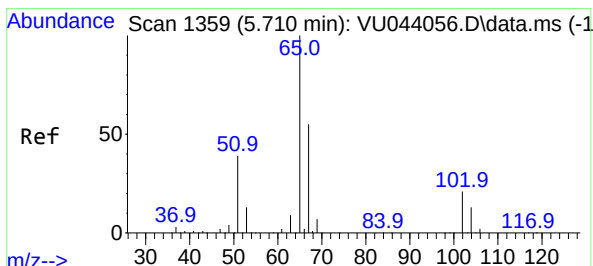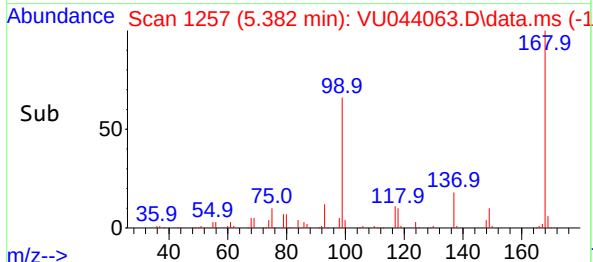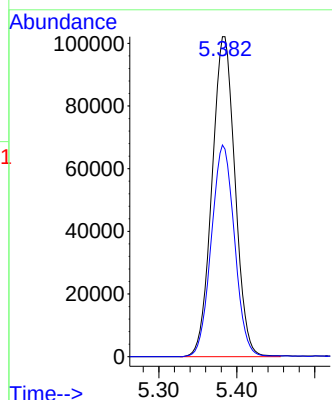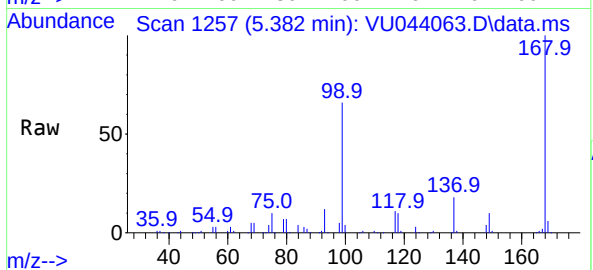

#33
1,2-Dichloroethane-d4
Concen: 52.764 ug/l
RT: 5.710 min Scan# 1359
Delta R.T. -0.000 min
Lab File: VU044063.D
Acq: 07 Jun 2021 18:19

Tgt Ion: 65 Resp: 192769
Ion Ratio Lower Upper
65 100
67 54.0 0.0 109.2


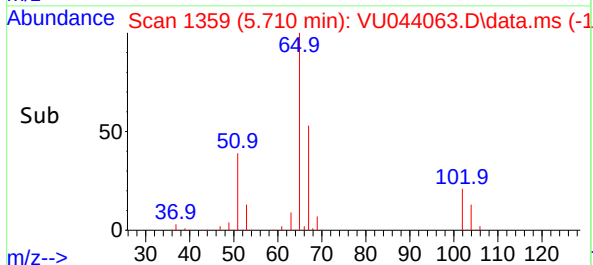
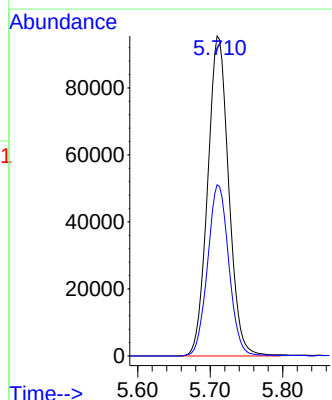
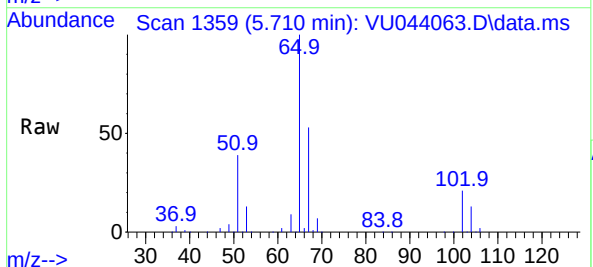


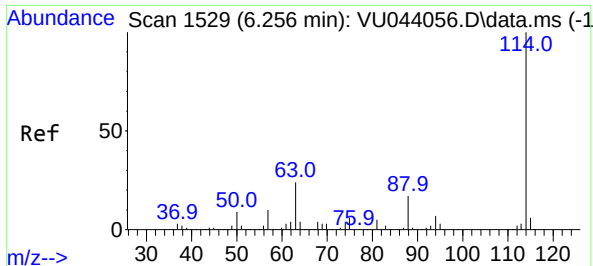

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.256 min Scan# 1529
Delta R.T. 0.000 min
Lab File: VU044063.D
Acq: 07 Jun 2021 18:19




Instrument :
MSVOA_U
ClientSampleId :
VU0607WBL01


Tgt Ion:114 Resp: 419057
Ion Ratio Lower Upper
114 100
63 23.9 0.0 48.4
88 17.5 0.0 34.4

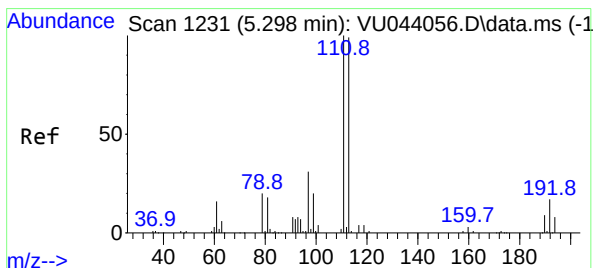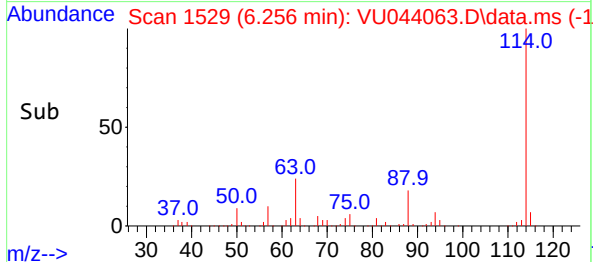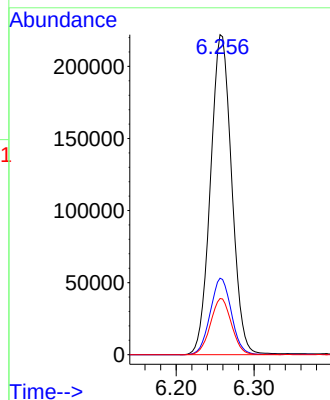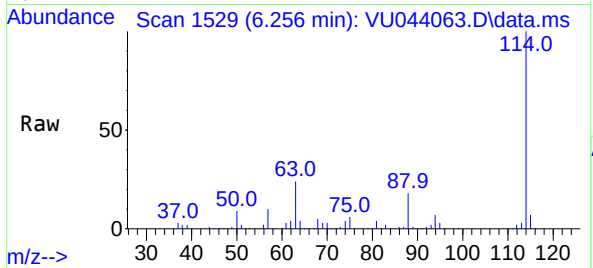

#35
Dibromofluoromethane
Concen: 49.954 ug/l
RT: 5.298 min Scan# 1231
Delta R.T. -0.000 min
Lab File: VU044063.D
Acq: 07 Jun 2021 18:19

Tgt Ion:113 Resp: 149386
Ion Ratio Lower Upper
113 100
111 102.3 82.1 123.1
192 17.6 13.8 20.8


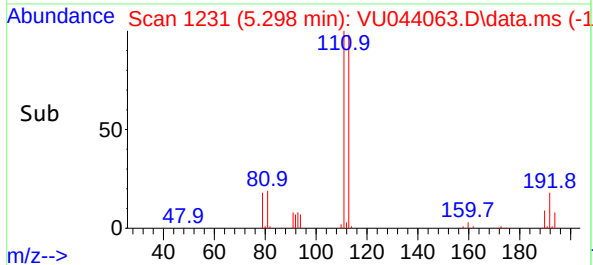
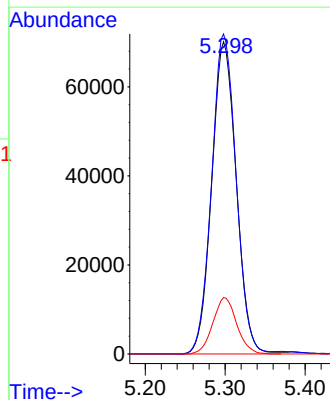
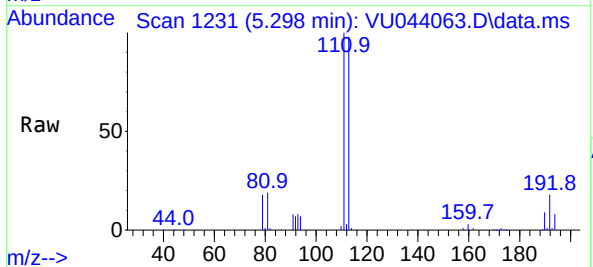


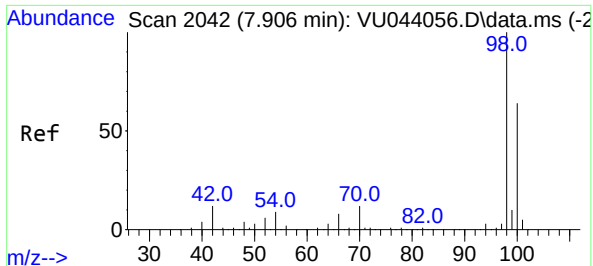

#50
Toluene-d8
Concen: 48.577 ug/l
RT: 7.906 min Scan# 2042
Delta R.T. -0.000 min
Lab File: VU044063.D
Acq: 07 Jun 2021 18:19




Instrument :
MSVOA_U
ClientSampleId :
VU0607WBL01


Tgt Ion: 98 Resp: 560335
Ion Ratio Lower Upper
98 100
100 64.5 51.6 77.4

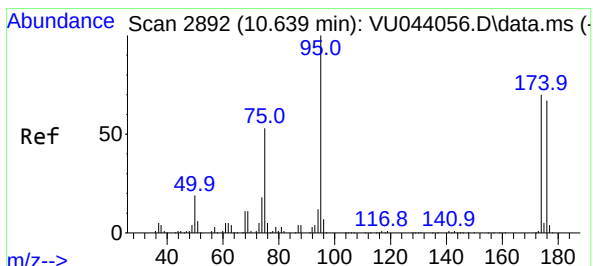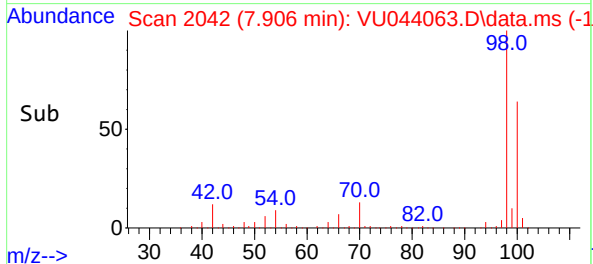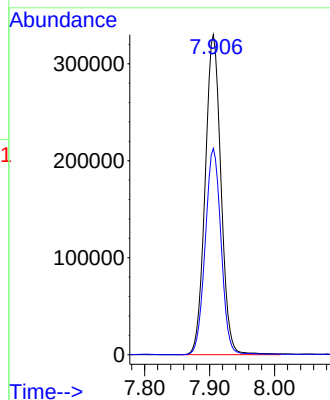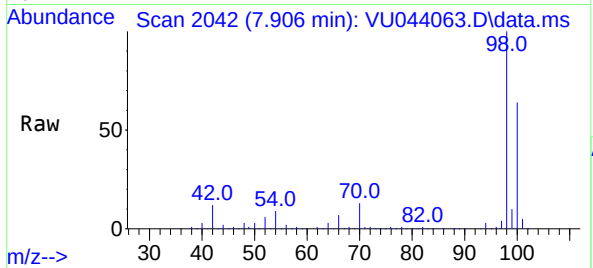

#62
4-Bromofluorobenzene
Concen: 45.069 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. -0.000 min
Lab File: VU044063.D
Acq: 07 Jun 2021 18:19

Tgt Ion: 95 Resp: 205826
Ion Ratio Lower Upper
95 100
174 71.2 0.0 141.0
176 67.3 0.0 135.2


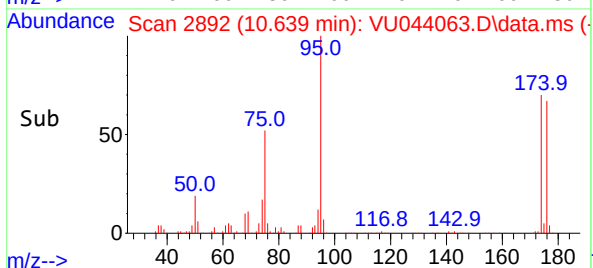
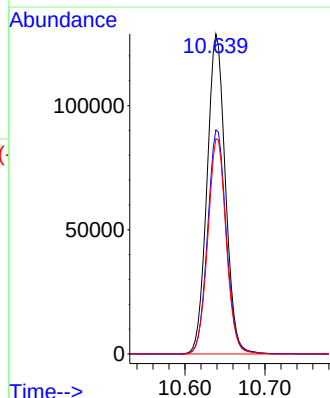
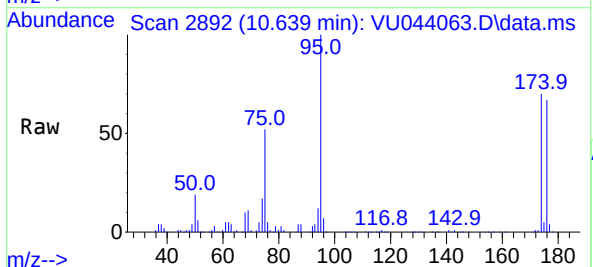


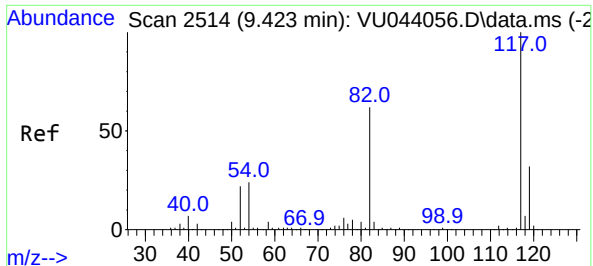

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.423 min Scan# 2514
Delta R.T. 0.000 min
Lab File: VU044063.D
Acq: 07 Jun 2021 18:19

Instrument :
MSVOA_U
ClientSampleId :
VU0607WBL01

Tgt Ion:117 Resp: 419474
Ion Ratio Lower Upper
117 100
82 61.4 50.0 75.0
119 31.2 25.9 38.9

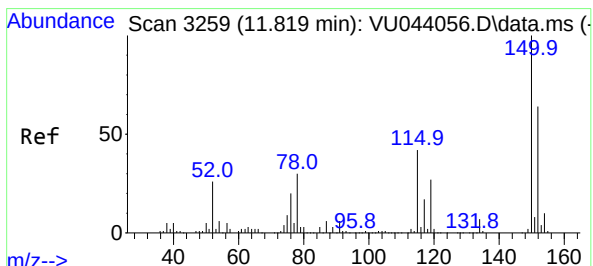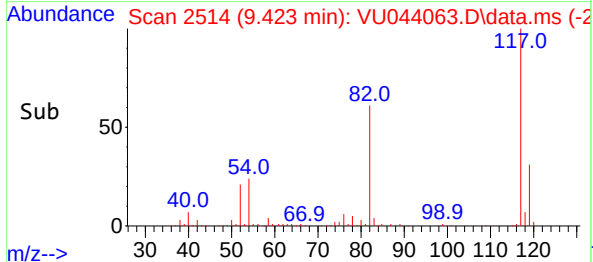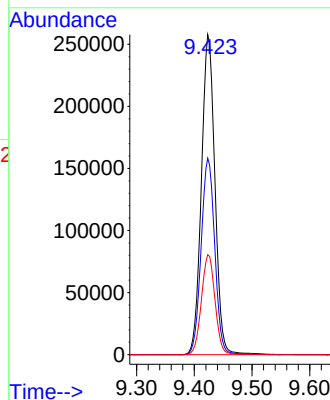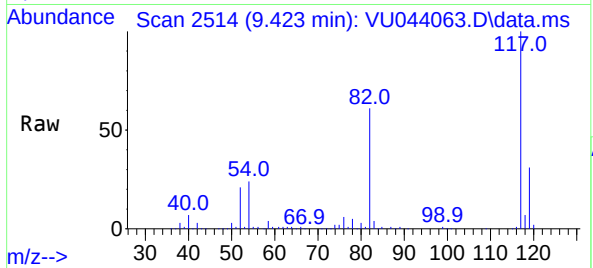

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.819 min Scan# 3259
Delta R.T. -0.000 min
Lab File: VU044063.D
Acq: 07 Jun 2021 18:19

Tgt Ion:152 Resp: 197304
Ion Ratio Lower Upper
152 100
115 62.8 44.6 134.0
150 156.5 0.0 347.8

