


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060721\
Data File : VU044052.D
Acq On : 07 Jun 2021 12:56
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U060721W.M
Title : SW846 8260
Last Update : Tue Jun 08 05:21:34 2021

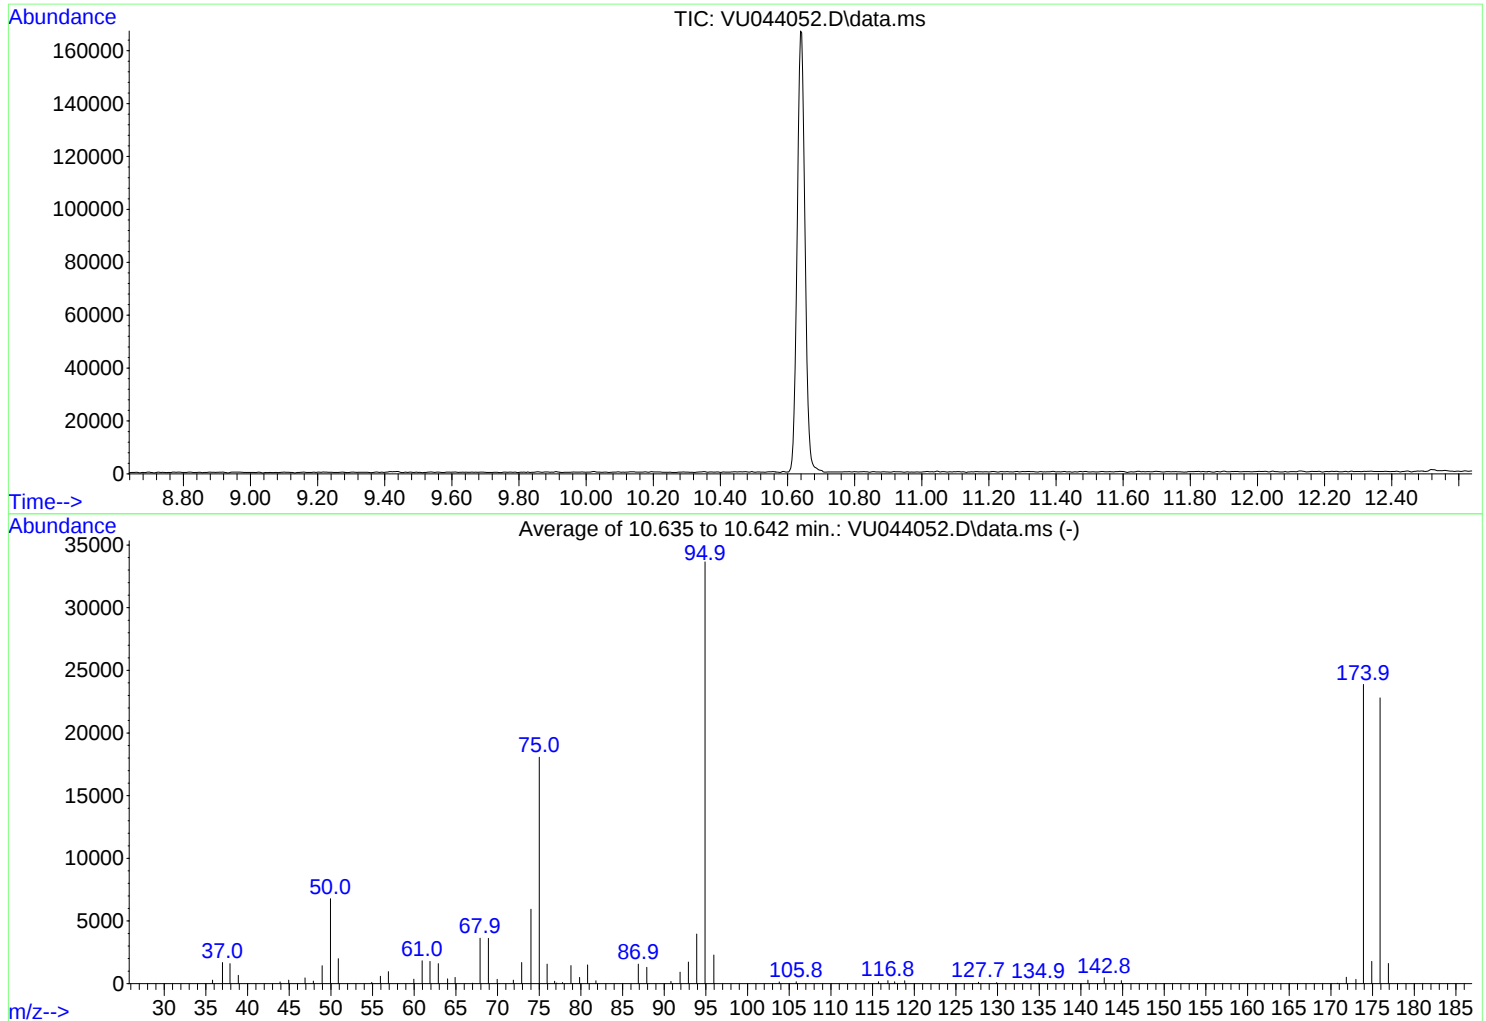

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2879

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.2	6785	PASS
75	95	30	60	53.7	18064	PASS
95	95	100	100	100.0	33659	PASS
96	95	5	9	6.8	2289	PASS
173	174	0.00	2	1.5	347	PASS
174	95	50	100	70.9	23875	PASS
175	174	5	9	7.4	1771	PASS
176	174	95	101	95.5	22800	PASS
177	176	5	9	7.1	1609	PASS