


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060721\
Data File : VU044061.D
Acq On : 07 Jun 2021 17:29
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U060721W.M
Title : SW846 8260
Last Update : Tue Jun 08 17:38:51 2021

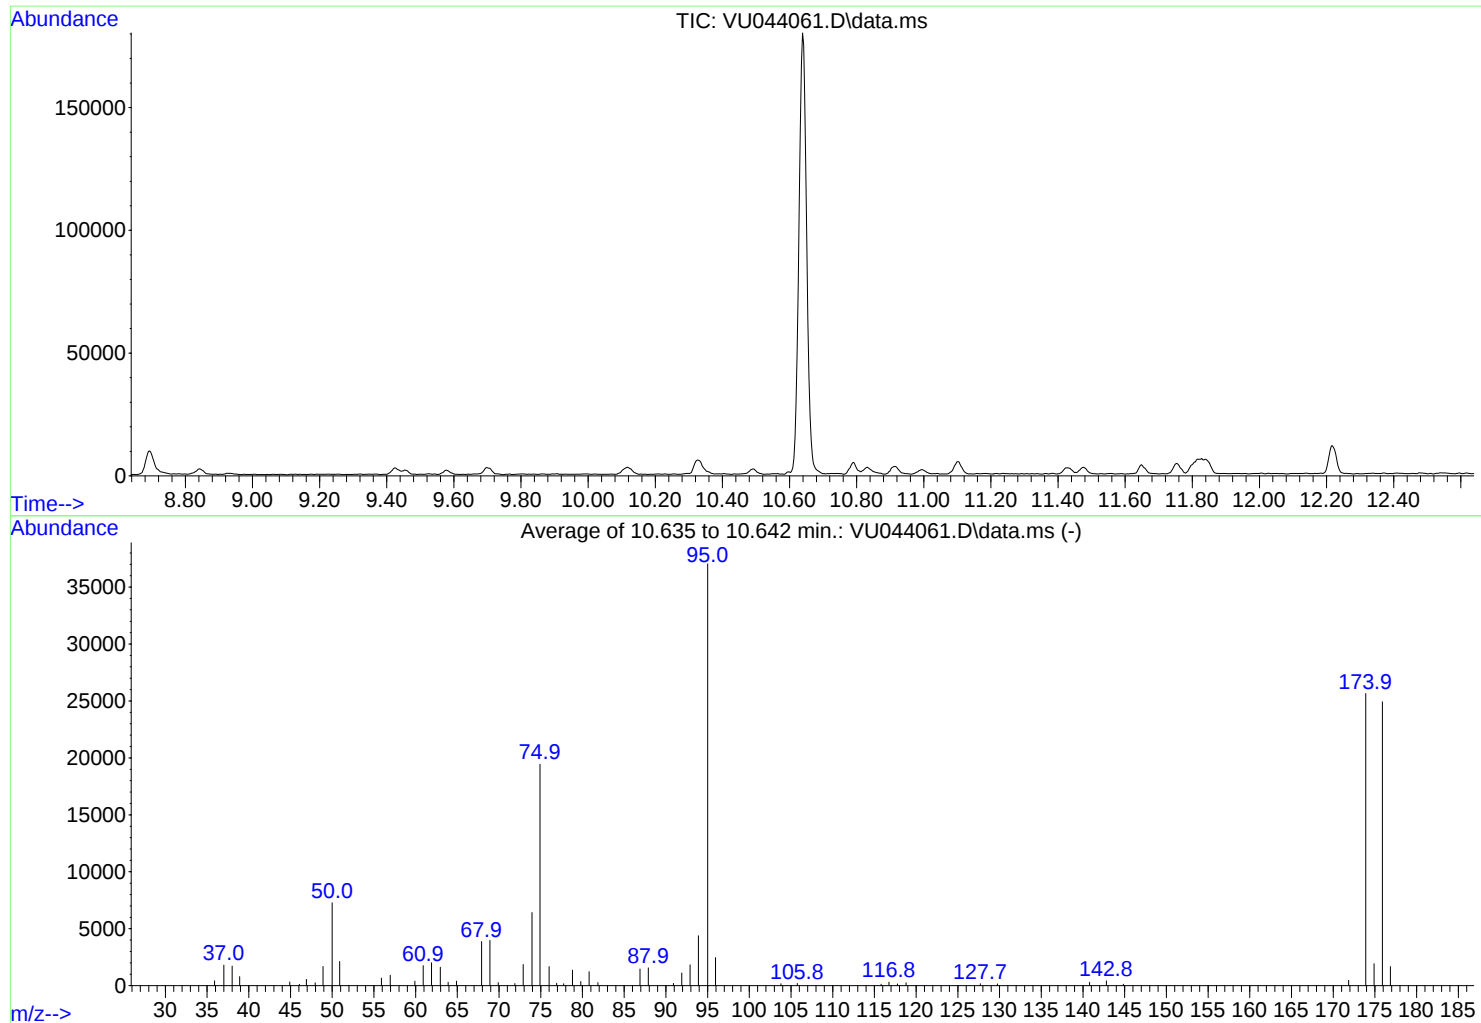

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	7279	PASS
75	95	30	60	52.5	19443	PASS
95	95	100	100	100.0	37043	PASS
96	95	5	9	6.6	2463	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	69.3	25659	PASS
175	174	5	9	7.5	1933	PASS
176	174	95	101	97.1	24923	PASS
177	176	5	9	6.7	1668	PASS