

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060722\
 Data File : VU048928.D
 Acq On : 07 Jun 2022 23:05
 Operator : SY/MD
 Sample : VU0607WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0607WBL02

Quant Time: Jun 08 04:58:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U052622W.M
 Quant Title : SW846 8260
 QLast Update : Fri May 27 06:42:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.372	168	245359	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.250	114	397510	50.000	ug/l	0.00
63) Chlorobenzene-d5	9.417	117	370187	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.812	152	164975	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.700	65	186468	50.604	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	101.200%
35) Dibromofluoromethane	5.288	113	138101	48.697	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	97.400%
50) Toluene-d8	7.896	98	474435	46.670	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	93.340%
62) 4-Bromofluorobenzene	10.632	95	173054	45.012	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	90.020%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060722\
Data File : VU048928.D
Acq On : 07 Jun 2022 23:05
Operator : SY/MD
Sample : VU0607WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0607WBL02

Quant Time: Jun 08 04:58:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U052622W.M
Quant Title : SW846 8260
QLast Update : Fri May 27 06:42:31 2022
Response via : Initial Calibration




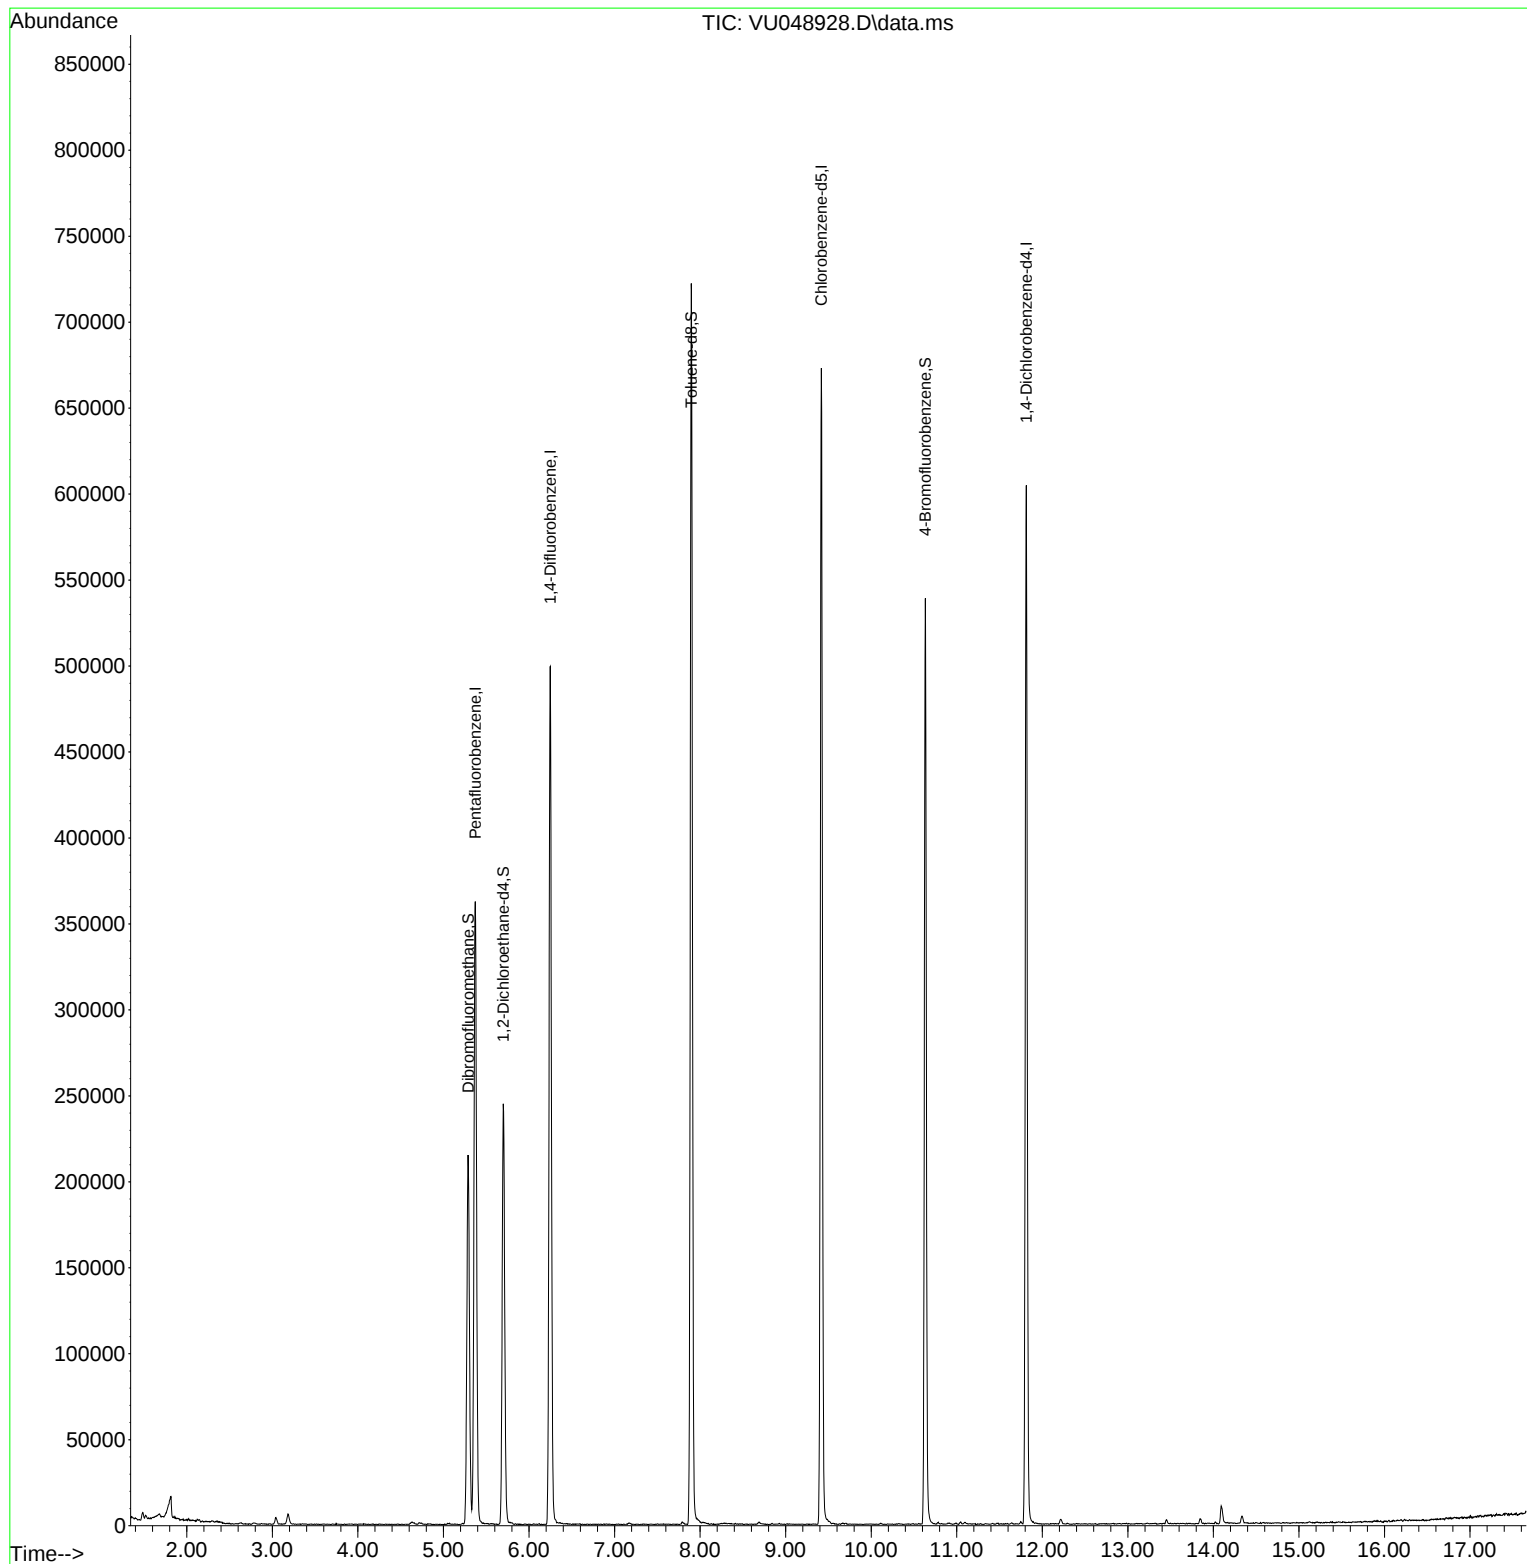




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.372 min Scan# 1254
Delta R.T. -0.003 min
Lab File: VU048928.D
Acq: 07 Jun 2022 23:05




Instrument :
MSVOA_U
ClientSampleId :
VU0607WBL02


Tgt Ion:168 Resp: 245359
Ion Ratio Lower Upper
168 100
99 59.8 49.3 73.9

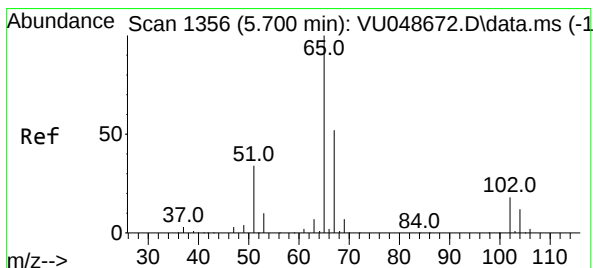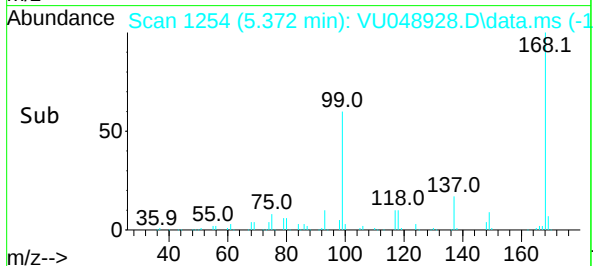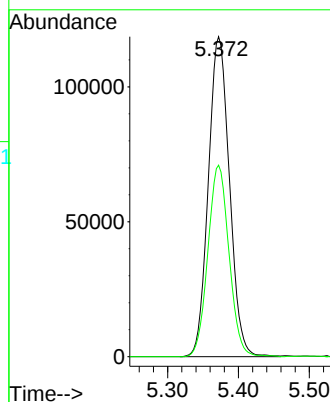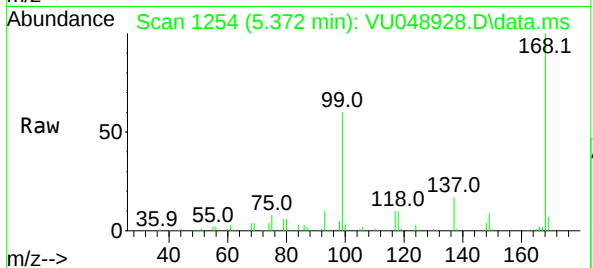

#33
1,2-Dichloroethane-d4
Concen: 50.604 ug/l
RT: 5.700 min Scan# 1356
Delta R.T. -0.000 min
Lab File: VU048928.D
Acq: 07 Jun 2022 23:05

Tgt Ion: 65 Resp: 186468
Ion Ratio Lower Upper
65 100
67 52.7 0.0 103.0

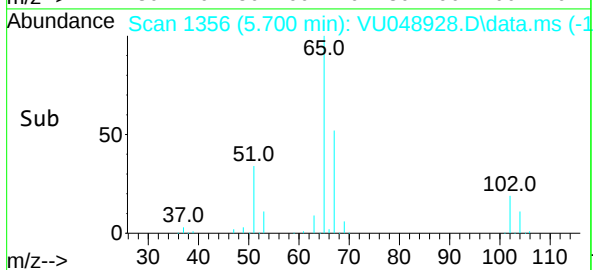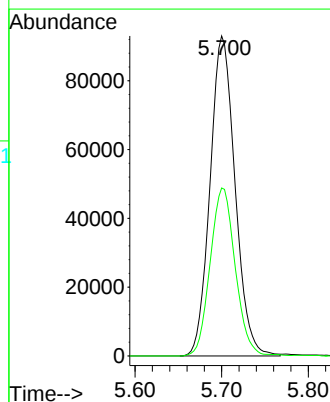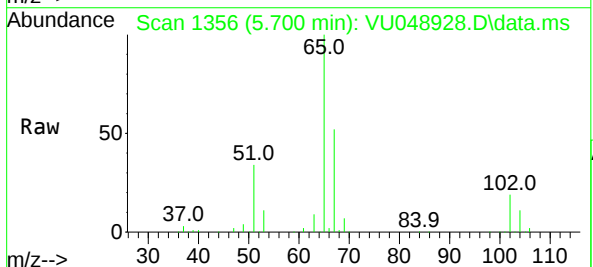

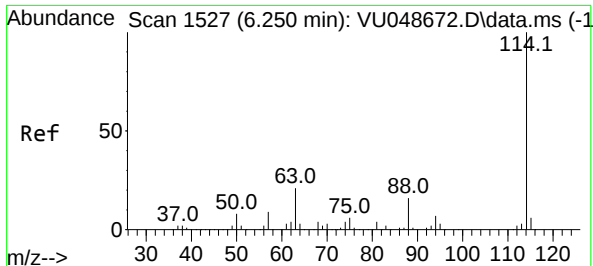

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.250 min Scan# 1

Delta R.T. -0.000 min

Lab File: VU048928.D

Acq: 07 Jun 2022 23:05

Instrument :

MSVOA_U

ClientSampleId :

VU0607WBL02





Tgt Ion:114 Resp: 397510

Ion Ratio Lower Upper

114 100

63 21.6 0.0 42.6

88 15.7 0.0 32.2

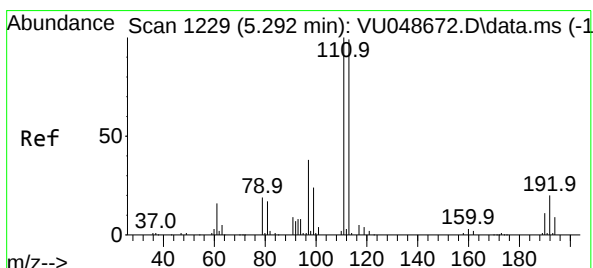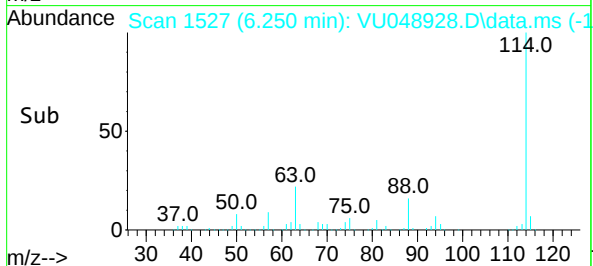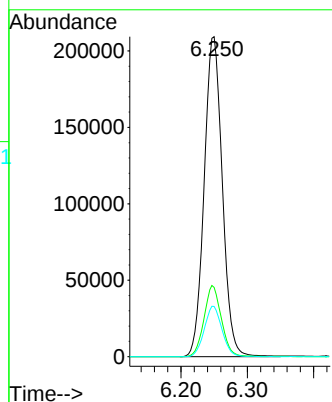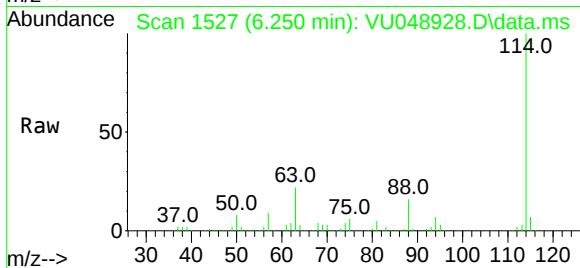

#35

Dibromofluoromethane

Concen: 48.697 ug/l

RT: 5.288 min Scan# 1228

Delta R.T. -0.003 min

Lab File: VU048928.D

Acq: 07 Jun 2022 23:05




Tgt Ion:113 Resp: 138101


Ion Ratio Lower Upper

113 100

111 102.6 80.7 121.1

192 19.4 15.9 23.9


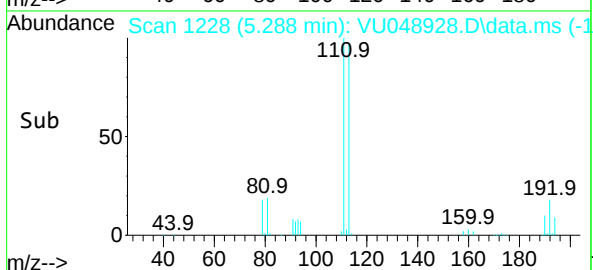
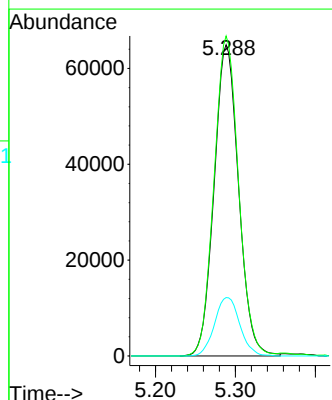
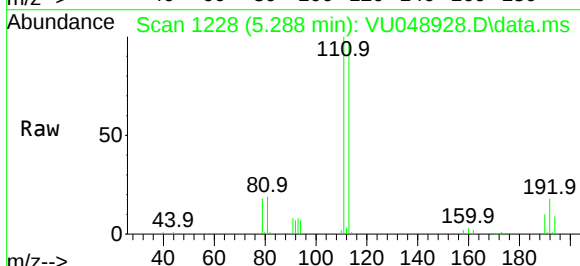


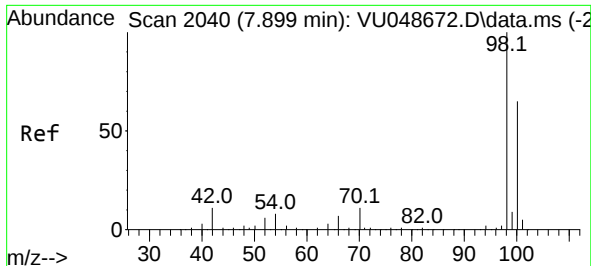

#50
Toluene-d8
Concen: 46.670 ug/l
RT: 7.896 min Scan# 2040
Delta R.T. -0.003 min
Lab File: VU048928.D
Acq: 07 Jun 2022 23:05




Instrument :
MSVOA_U
ClientSampleId :
VU0607WBL02


Tgt Ion: 98 Resp: 474435
Ion Ratio Lower Upper
98 100
100 65.4 52.2 78.4

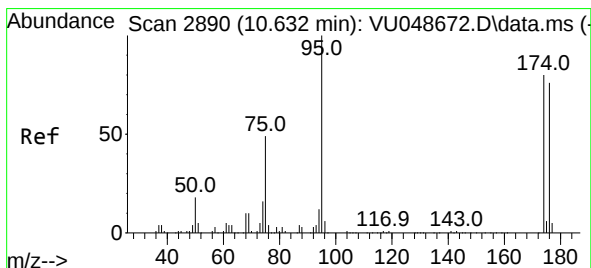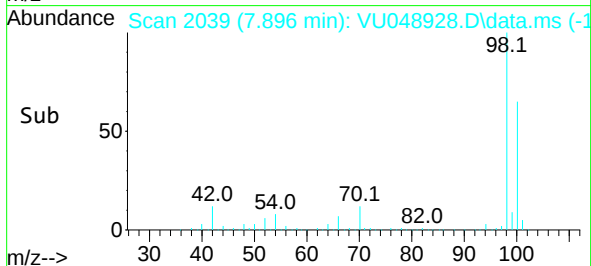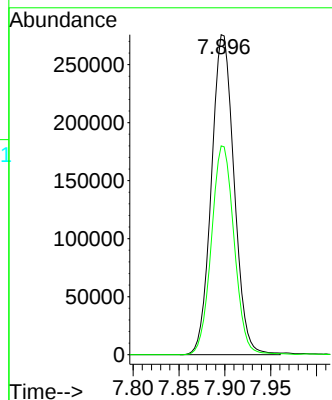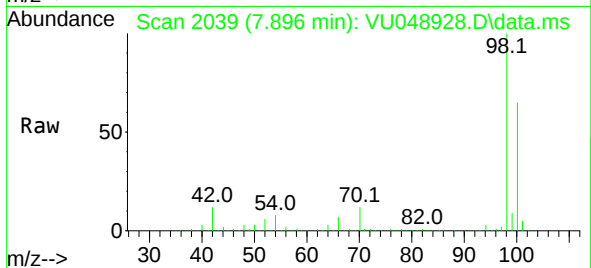

#62
4-Bromofluorobenzene
Concen: 45.012 ug/l
RT: 10.632 min Scan# 2890
Delta R.T. -0.000 min
Lab File: VU048928.D
Acq: 07 Jun 2022 23:05

Tgt Ion: 95 Resp: 173054
Ion Ratio Lower Upper
95 100
174 81.9 0.0 159.4
176 78.4 0.0 152.4


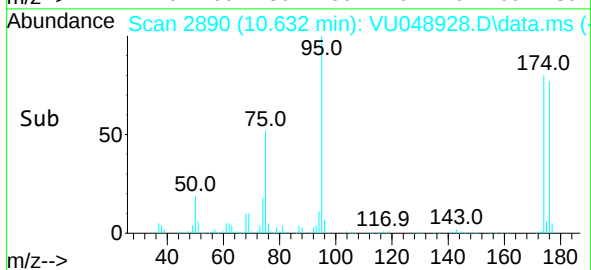
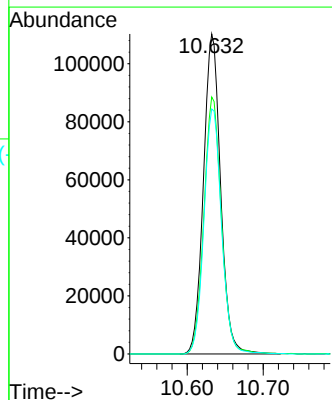
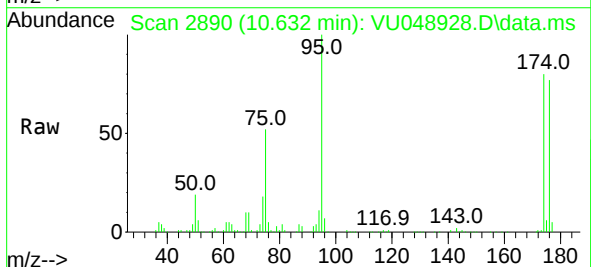


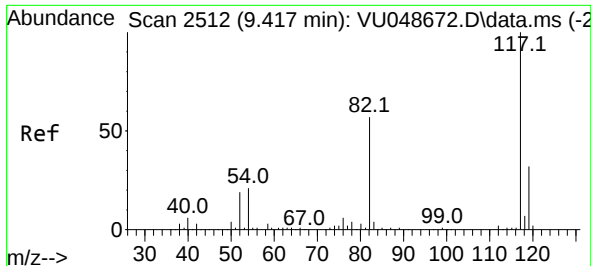

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.417 min Scan# 21
Delta R.T. -0.000 min
Lab File: VU048928.D
Acq: 07 Jun 2022 23:05

Instrument :
MSVOA_U
ClientSampleId :
VU0607WBL02

Tgt Ion:117 Resp: 370187
Ion Ratio Lower Upper
117 100
82 57.8 45.3 67.9
119 32.5 25.4 38.2

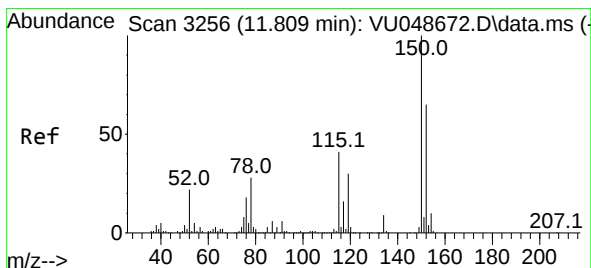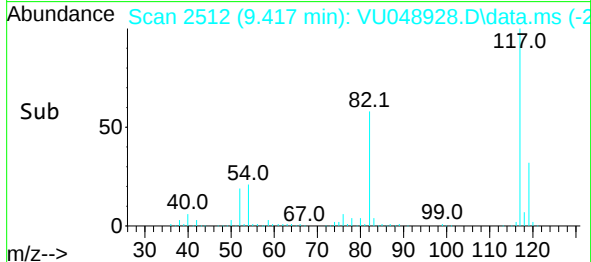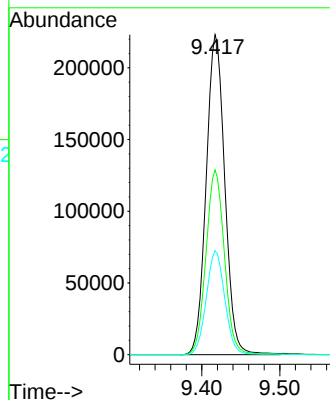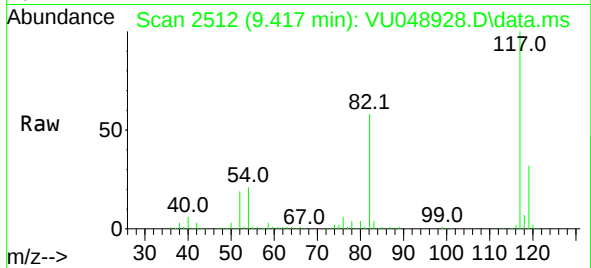

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.812 min Scan# 3257
Delta R.T. 0.003 min
Lab File: VU048928.D
Acq: 07 Jun 2022 23:05

Tgt Ion:152 Resp: 164975
Ion Ratio Lower Upper
152 100
115 58.8 41.8 125.4
150 154.7 0.0 341.0

