


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060722\
Data File : VU048900.D
Acq On : 07 Jun 2022 09:35
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : C:\Users\eUser\Desktop\Practice\8270-BF031022.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Mar 19 01:50:04 2022

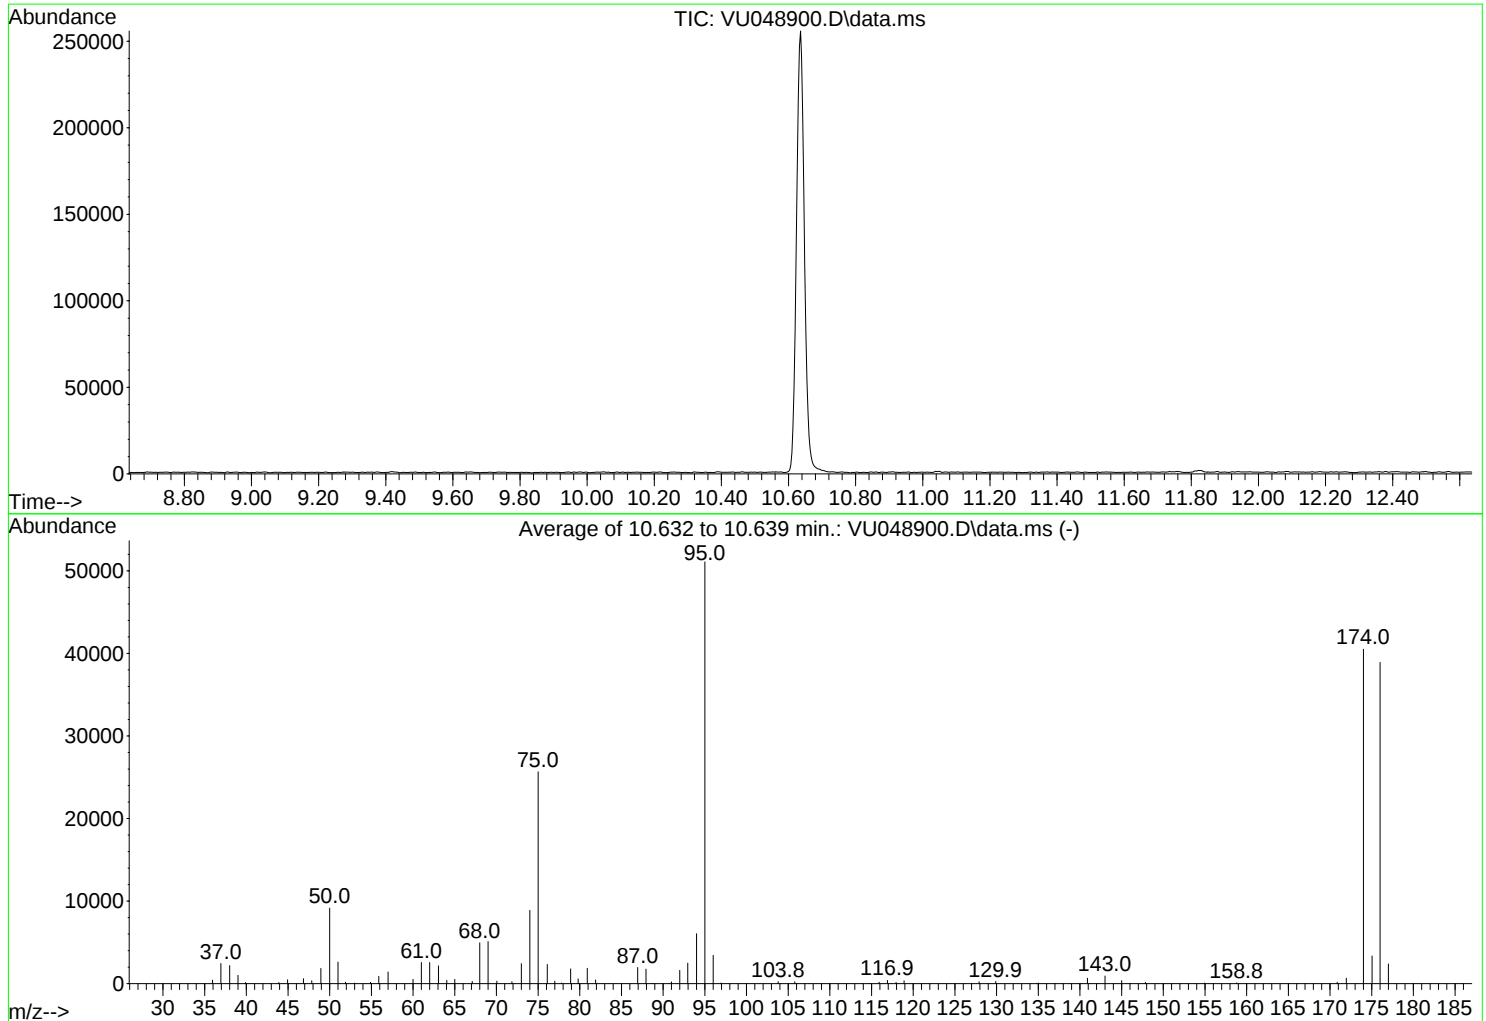

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	9156	PASS
75	95	30	60	50.2	25659	PASS
95	95	100	100	100.0	51096	PASS
96	95	5	9	6.7	3436	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	79.3	40507	PASS
175	174	5	9	8.3	3346	PASS
176	174	95	101	96.1	38923	PASS
177	176	5	9	6.1	2393	PASS