
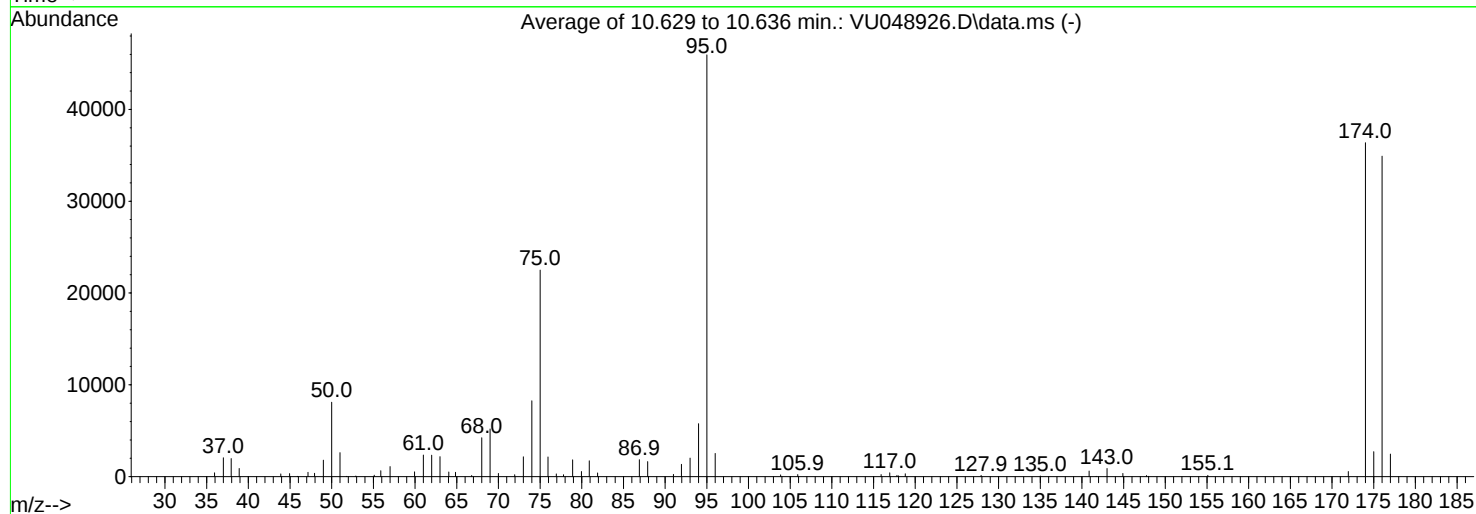


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060722\
 Data File : VU048926.D
 Acq On : 07 Jun 2022 21:48
 Operator : SY/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U052622W.M
 Title : SW846 8260
 Last Update : Fri May 27 06:42:31 2022

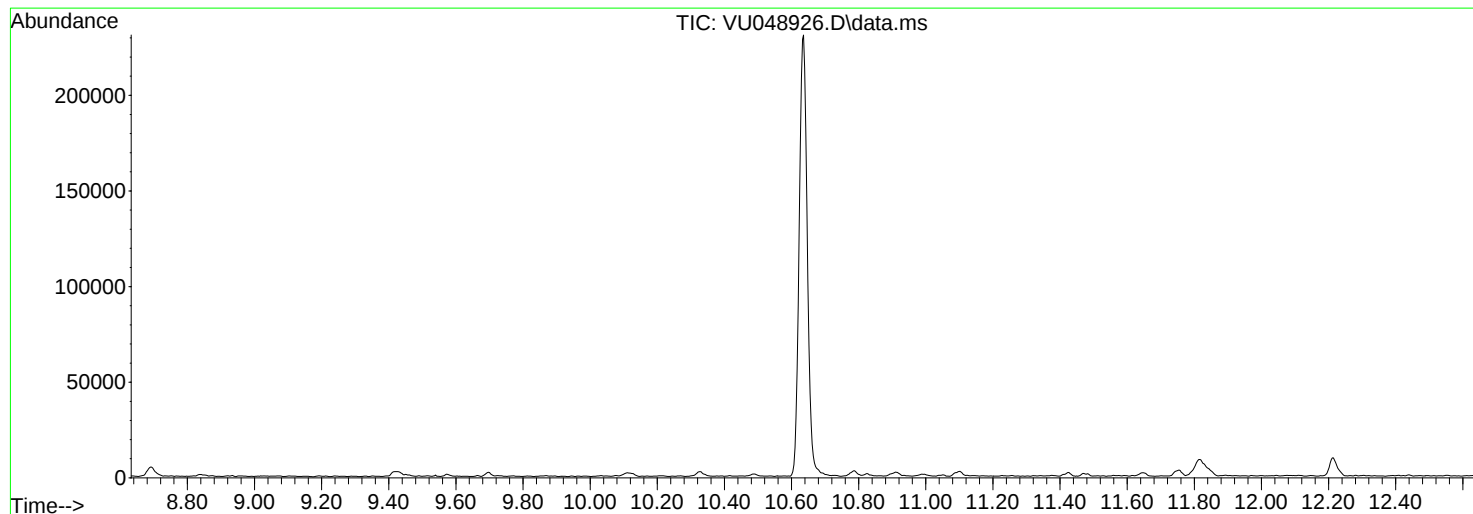

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	8113	PASS
75	95	30	60	49.0	22509	PASS
95	95	100	100	100.0	45944	PASS
96	95	5	9	5.5	2525	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	79.2	36376	PASS
175	174	5	9	7.5	2717	PASS
176	174	95	101	96.0	34904	PASS
177	176	5	9	7.0	2457	PASS