

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060723\
 Data File : VU054413.D
 Acq On : 07 Jun 2023 16:07
 Operator : MD/SY
 Sample : 03075-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0F81

Quant Time: Jun 08 01:21:43 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jun 08 01:20:50 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	323063	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	309565	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	150081	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.599	65	86664	4.215	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.400%
7) Chloroethane-d5	1.914	69	84433	4.386	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.800%
11) 1,1-Dichloroethene-d2	2.563	65	39922	4.348	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	87.000%
20) 2-Butanone-d5	4.631	46	286930	49.636	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.280%
24) Chloroform-d	5.059	84	195985	4.560	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.200%
26) 1,2-Dichloroethane-d4	5.698	65	99519	4.750	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.000%
32) Benzene-d6	5.724	84	388471	4.514	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.200%
36) 1,2-Dichloropropane-d6	6.685	67	135480	4.714	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.200%
41) Toluene-d8	7.894	98	335512	4.393	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.800%
43) trans-1,3-Dichloroprop...	8.177	79	45528	4.556	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.200%
46) 2-Hexanone-d5	8.631	63	190427	45.419	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.840%
56) 1,1,2,2-Tetrachloroeth...	10.750	84	98251	4.585	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.600%
66) 1,2-Dichlorobenzene-d4	12.187	152	123947	4.896	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.000%
Target Compounds						
					Qvalue	
13) Acetone	2.647	43	34847	6.393	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060723\
Data File : VU054413.D
Acq On : 07 Jun 2023 16:07
Operator : MD/SY
Sample : 03075-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0F81

Quant Time: Jun 08 01:21:43 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jun 08 01:20:50 2023
Response via : Initial Calibration

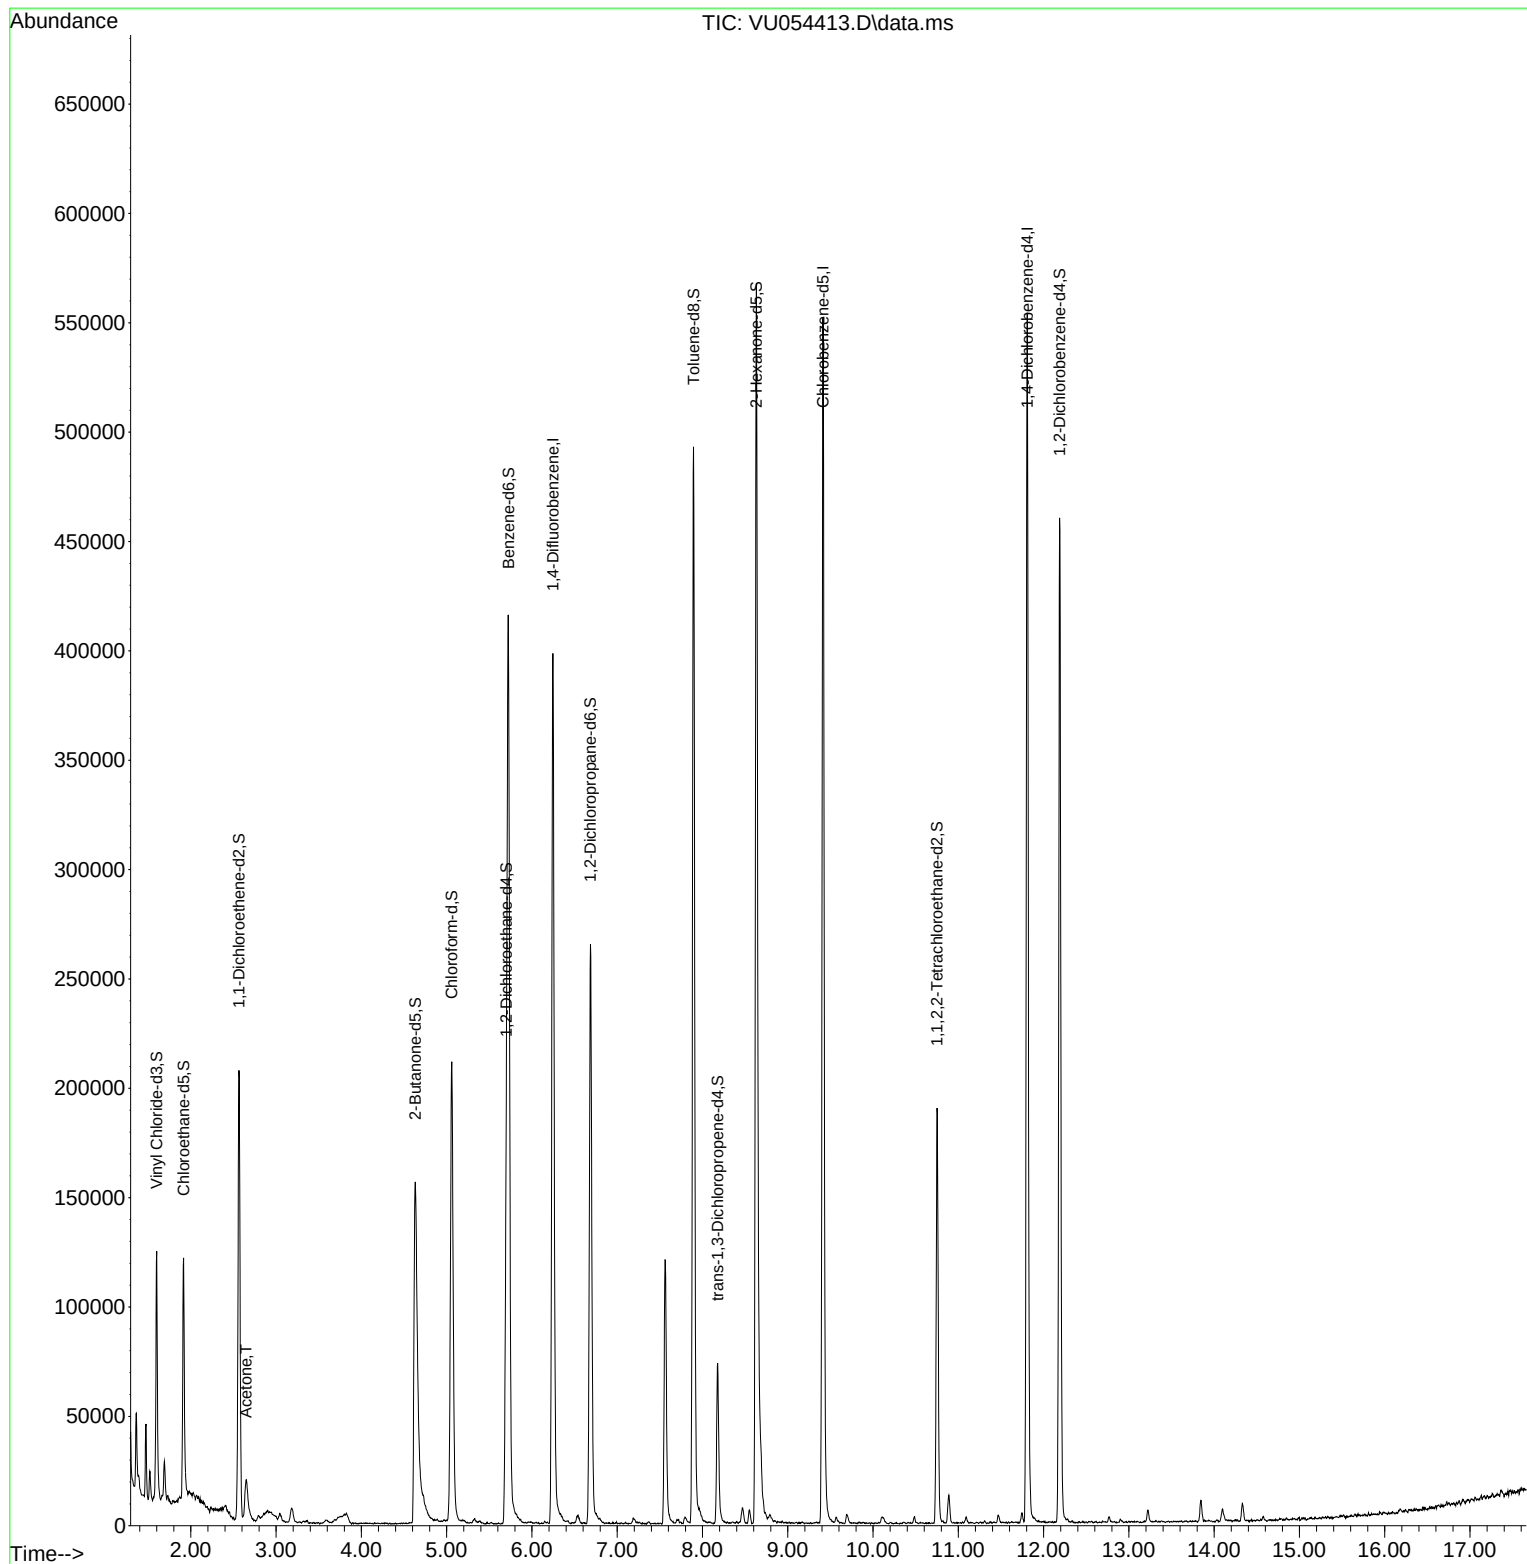

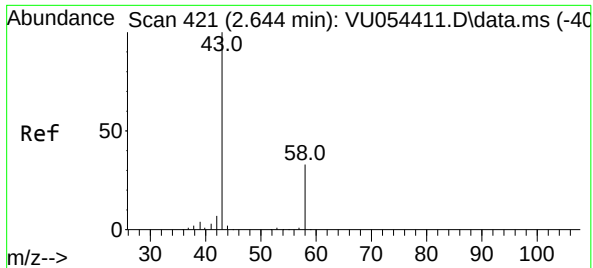

#13
 Acetone
 Concen: 6.393 ug/L
 RT: 2.647 min Scan# 41
 Delta R.T. 0.003 min
 Lab File: VU054413.D
 Acq: 07 Jun 2023 16:07

Instrument :
 MSVOA_U
 ClientSampleId :
 C0F81

Tgt Ion: 43 Resp: 34847
 Ion Ratio Lower Upper
 43 100
 58 30.6 0.0 67.2

