

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060723\
 Data File : VU054412.D
 Acq On : 07 Jun 2023 15:42
 Operator : MD/SY
 Sample : VU0607WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK196

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054412.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	111	rVB	126681	153111	12.71%	1.545%
2	1.914	185	194	210	rBV	120310	171092	14.21%	1.727%
3	2.563	384	396	412	rBV	228124	375440	31.17%	3.789%
4	4.631	1028	1039	1074	rBV2	172157	510523	42.39%	5.153%
5	5.058	1155	1172	1193	rBV	225086	505537	41.97%	5.102%
6	5.721	1358	1378	1417	rBV3	458468	1204386	100.00%	12.156%
7	6.245	1527	1541	1569	rBV	397416	785123	65.19%	7.924%
8	6.685	1664	1678	1697	rBV	287451	574998	47.74%	5.804%
9	6.840	1718	1726	1741	rVB2	12237	22950	1.91%	0.232%
10	7.563	1938	1951	1975	rBV	135465	247958	20.59%	2.503%
11	7.894	2041	2054	2072	rBV	549892	963411	79.99%	9.724%
12	8.177	2131	2142	2165	rBV2	81202	148405	12.32%	1.498%
13	8.630	2270	2283	2317	rBV2	602315	1195847	99.29%	12.070%
14	9.412	2513	2526	2551	rBV	538933	927414	77.00%	9.360%
15	10.753	2931	2943	2960	rBV	206472	339819	28.22%	3.430%
16	11.807	3259	3271	3290	rVV	534893	880967	73.15%	8.892%
17	12.190	3376	3390	3408	rBV	492490	828074	68.75%	8.358%
18	13.222	3698	3711	3725	rBV7	7012	13075	1.09%	0.132%
19	13.842	3895	3904	3916	rBV4	13513	22612	1.88%	0.228%
20	14.090	3974	3981	3992	rBV2	8565	15992	1.33%	0.161%
21	14.331	4047	4056	4069	rVB5	12141	21014	1.74%	0.212%




Sum of corrected areas: 9907748

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060723\
Data File : VU054412.D
Acq On : 07 Jun 2023 15:42
Operator : MD/SY
Sample : VU0607WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK196

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

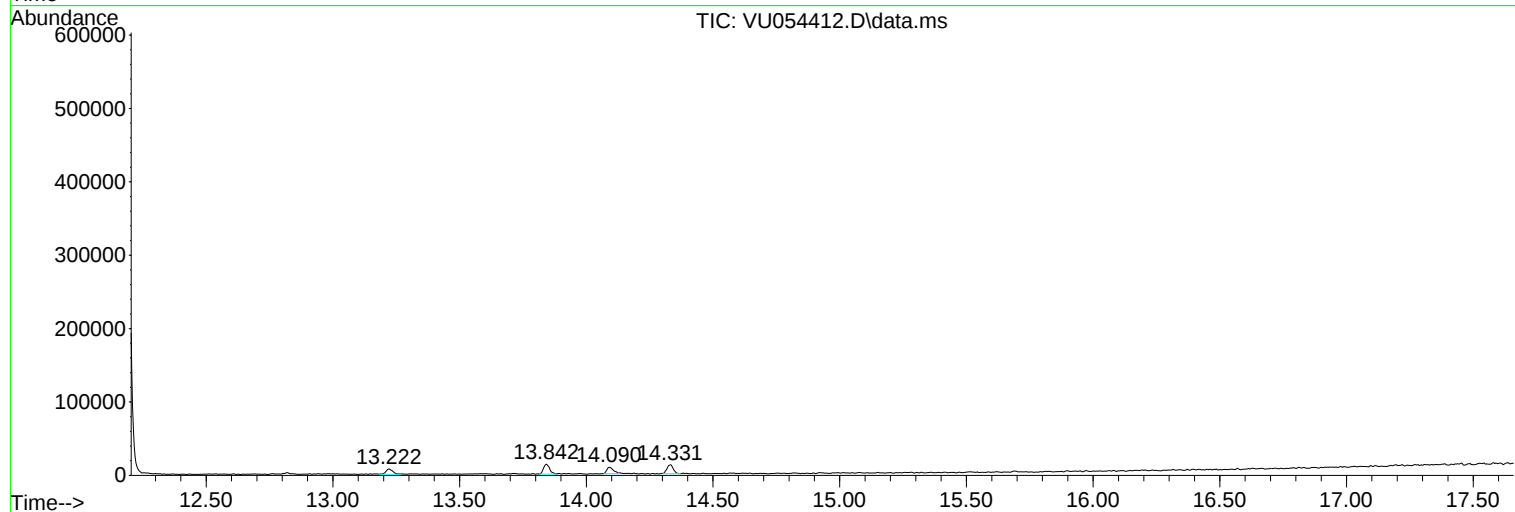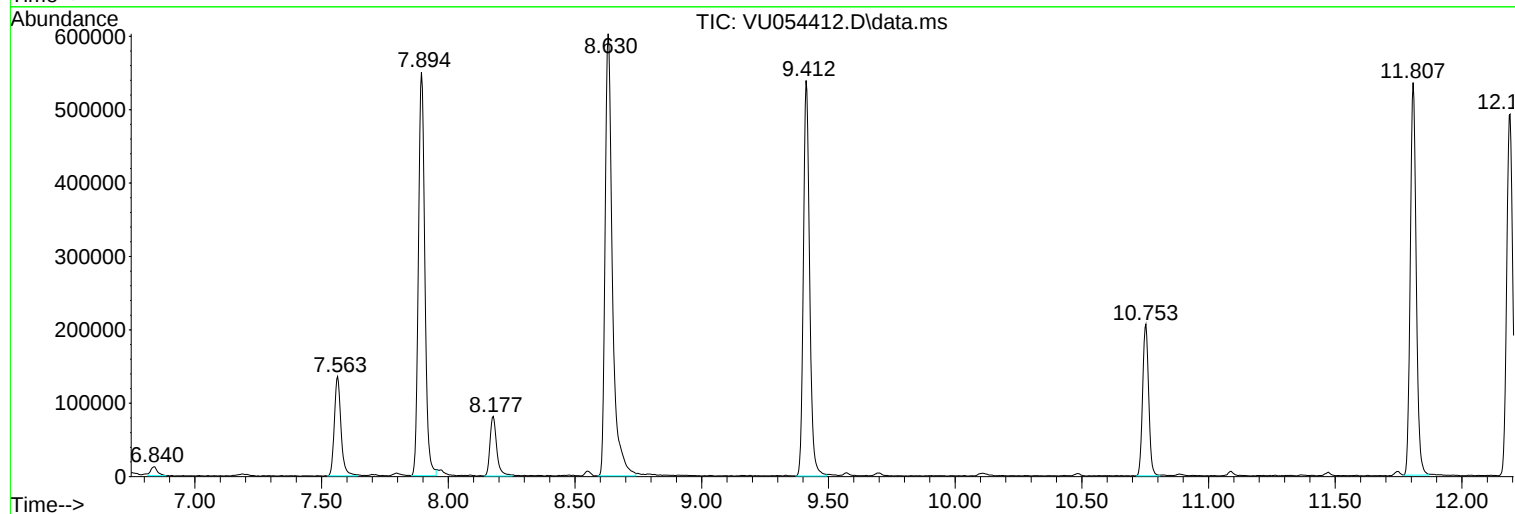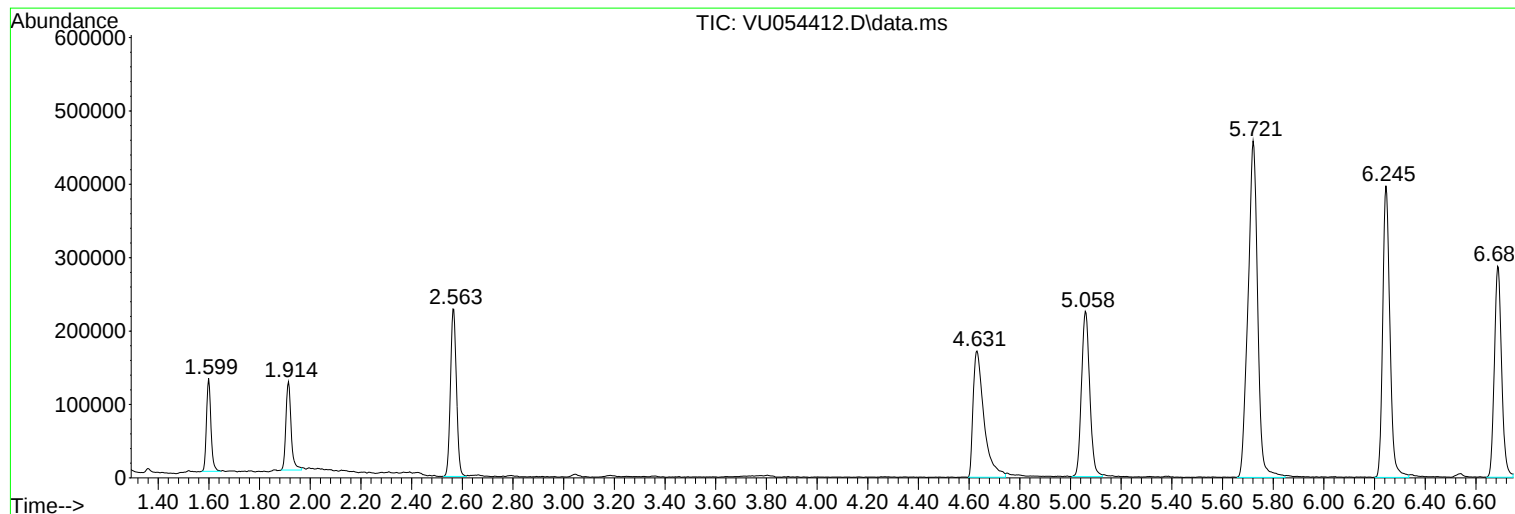

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060723\
Data File : VU054412.D
Acq On : 07 Jun 2023 15:42
Operator : MD/SY
Sample : VU0607WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK196

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060723\
Data File : VU054412.D
Acq On : 07 Jun 2023 15:42
Operator : MD/SY
Sample : VU0607WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK196

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc