

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060723\
 Data File : VU054422.D
 Acq On : 07 Jun 2023 19:45
 Operator : MD/SY
 Sample : 03075-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0FA8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054422.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.518	66	71	86	rVB	11257	13956	1.28%	0.152%
2	1.599	88	96	111	rVB	107326	133070	12.21%	1.453%
3	1.914	185	194	209	rBV	106016	149613	13.73%	1.633%
4	2.563	382	396	413	rBV	193634	322163	29.56%	3.517%
5	2.644	413	421	440	rVB2	8845	22131	2.03%	0.242%
6	3.184	575	589	602	rBV2	4790	12350	1.13%	0.135%
7	4.628	1027	1038	1071	rBV	154945	464318	42.60%	5.069%
8	5.058	1156	1172	1194	rBV	206677	475616	43.63%	5.192%
9	5.721	1356	1378	1409	rBV2	405066	1058084	97.07%	11.551%
10	6.245	1525	1541	1566	rBV	421281	816975	74.95%	8.919%
11	6.685	1664	1678	1697	rBV	261577	507665	46.57%	5.542%
12	7.563	1938	1951	1971	rBV	114609	210560	19.32%	2.299%
13	7.894	2039	2054	2074	rBV	467678	837898	76.87%	9.147%
14	8.177	2131	2142	2165	rBV2	68967	125835	11.54%	1.374%
15	8.631	2271	2283	2323	rBV2	534486	1090034	100.00%	11.899%
16	9.412	2513	2526	2557	rBV	556517	961633	88.22%	10.498%
17	10.753	2931	2943	2959	rBV	181115	297665	27.31%	3.249%
18	11.807	3259	3271	3296	rBV	567651	923845	84.75%	10.085%
19	12.187	3376	3389	3409	rBV	440130	737037	67.62%	8.046%




Sum of corrected areas: 9160448

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060723\
Data File : VU054422.D
Acq On : 07 Jun 2023 19:45
Operator : MD/SY
Sample : 03075-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FA8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

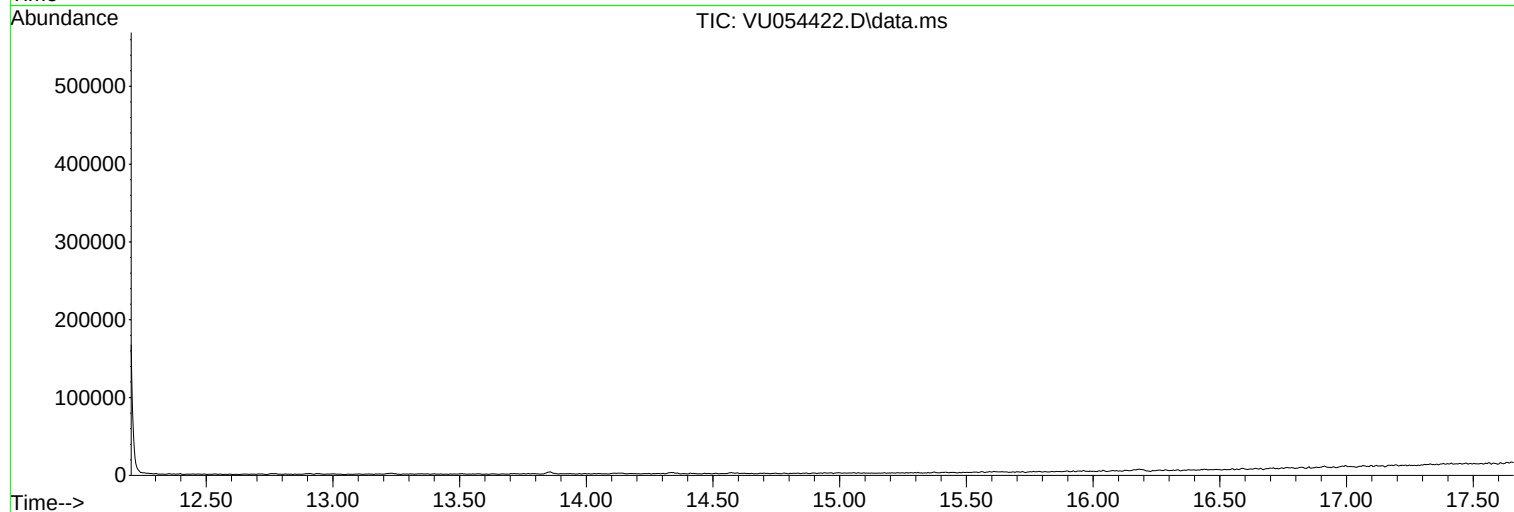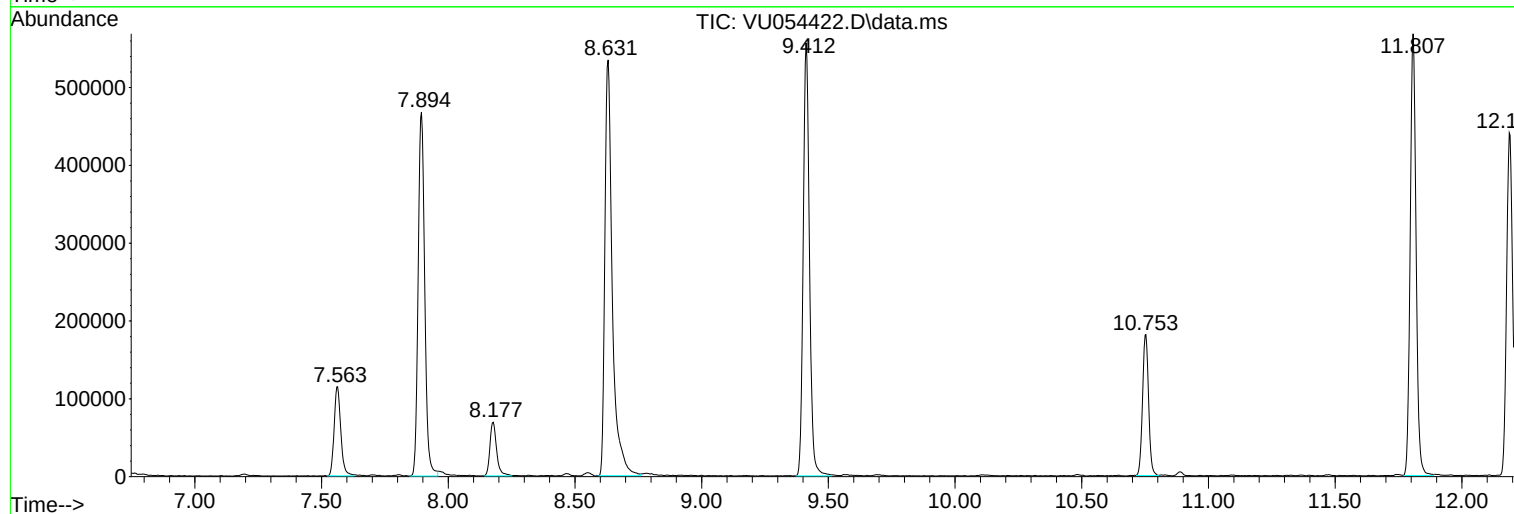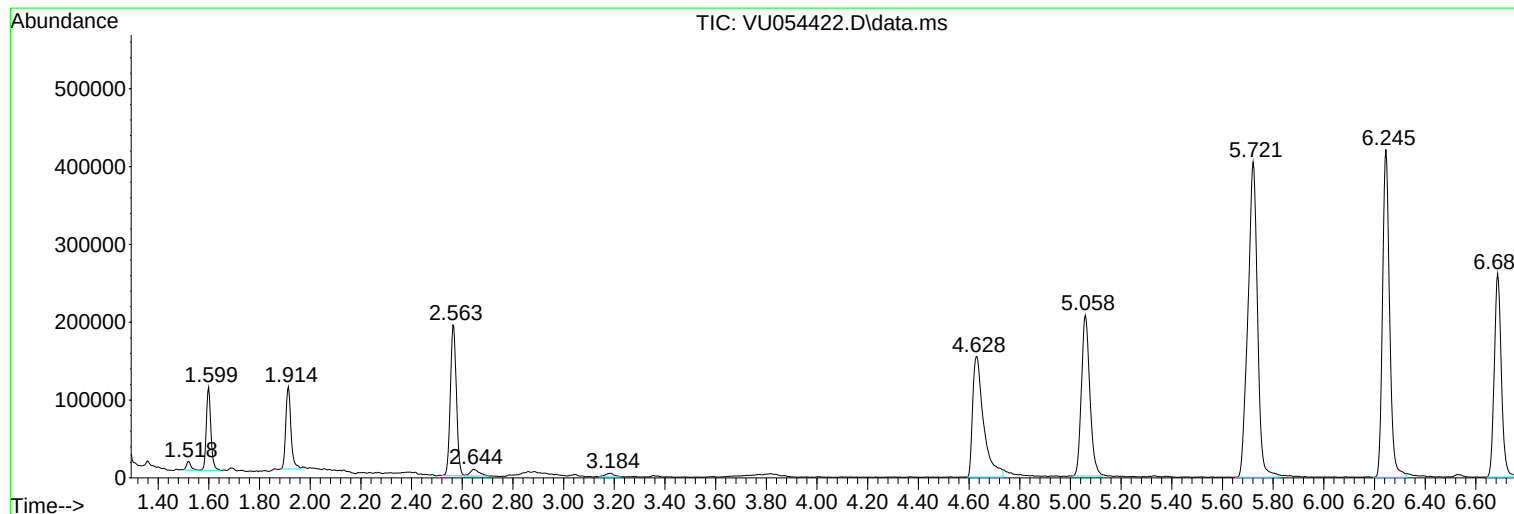

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060723\
Data File : VU054422.D
Acq On : 07 Jun 2023 19:45
Operator : MD/SY
Sample : 03075-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FA8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060723\
Data File : VU054422.D
Acq On : 07 Jun 2023 19:45
Operator : MD/SY
Sample : 03075-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FA8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------