

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060723\
 Data File : VU054426.D
 Acq On : 07 Jun 2023 21:22
 Operator : MD/SY
 Sample : 03075-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0FC1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054426.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.390	27	31	42	rVB2	9388	10907	1.00%	0.119%
2	1.599	88	96	116	rVB	109298	136252	12.55%	1.491%
3	1.914	185	194	210	rBV	110360	156745	14.44%	1.715%
4	2.567	384	397	411	rBV2	195105	321160	29.59%	3.515%
5	2.641	411	420	438	rVB2	7674	19349	1.78%	0.212%
6	4.631	1025	1039	1070	rBV	157006	466007	42.94%	5.100%
7	5.059	1156	1172	1199	rBV	215377	508276	46.83%	5.562%
8	5.522	1301	1316	1333	rBV4	32815	70450	6.49%	0.771%
9	5.721	1358	1378	1402	rBV2	403551	1056130	97.31%	11.558%
10	6.245	1527	1541	1564	rBV	394502	764340	70.42%	8.365%
11	6.685	1664	1678	1698	rBV	257529	517413	47.67%	5.662%
12	7.563	1938	1951	1972	rBV	113473	208990	19.26%	2.287%
13	7.894	2040	2054	2077	rBV	473368	843558	77.72%	9.232%
14	8.177	2131	2142	2160	rBV	68331	124029	11.43%	1.357%
15	8.631	2270	2283	2320	rBV2	522609	1085347	100.00%	11.878%
16	9.412	2513	2526	2555	rBV	540819	919668	84.73%	10.065%
17	10.750	2930	2942	2959	rBV	185092	306648	28.25%	3.356%
18	10.888	2975	2985	2998	rVB4	9010	14269	1.31%	0.156%
19	11.807	3259	3271	3295	rBV	530876	863782	79.59%	9.453%
20	12.187	3374	3389	3412	rBV	446571	744309	68.58%	8.146%




Sum of corrected areas: 9137629

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060723\
Data File : VU054426.D
Acq On : 07 Jun 2023 21:22
Operator : MD/SY
Sample : 03075-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FC1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

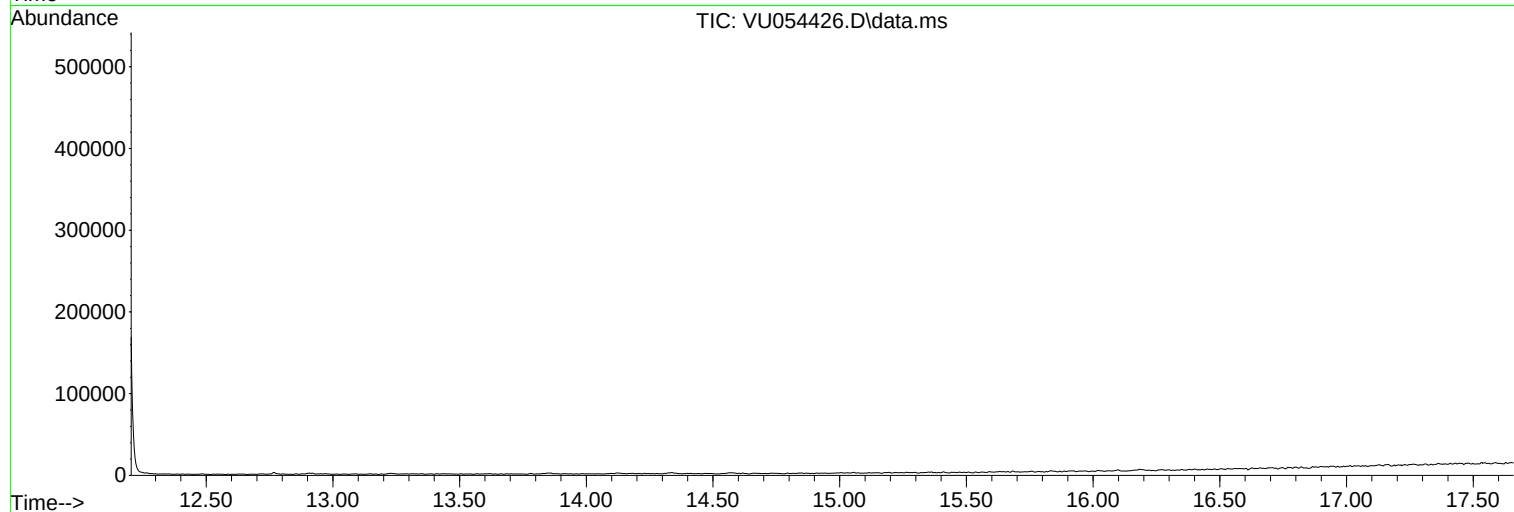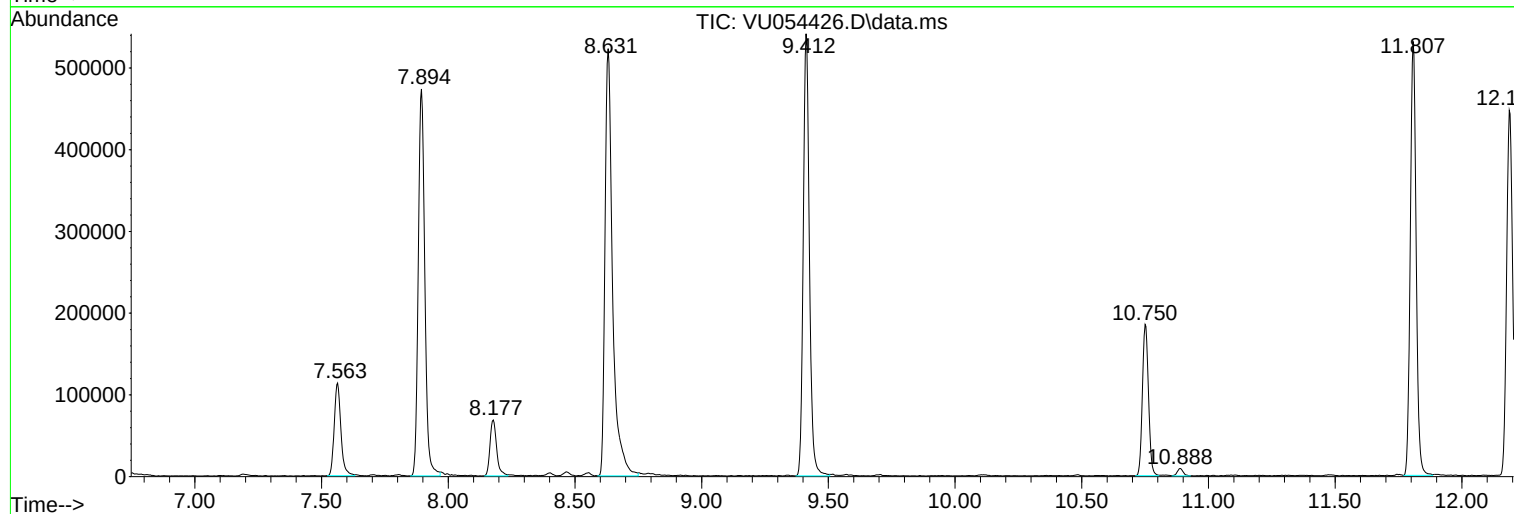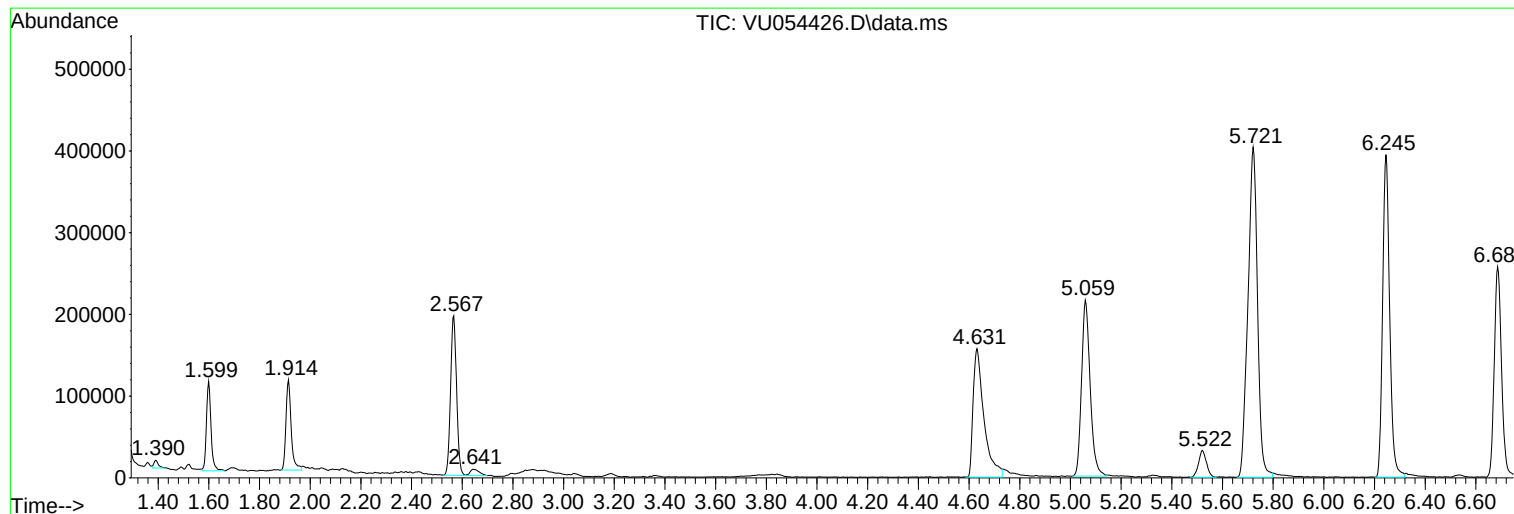

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060723\
Data File : VU054426.D
Acq On : 07 Jun 2023 21:22
Operator : MD/SY
Sample : 03075-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FC1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060723\
Data File : VU054426.D
Acq On : 07 Jun 2023 21:22
Operator : MD/SY
Sample : 03075-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FC1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc