
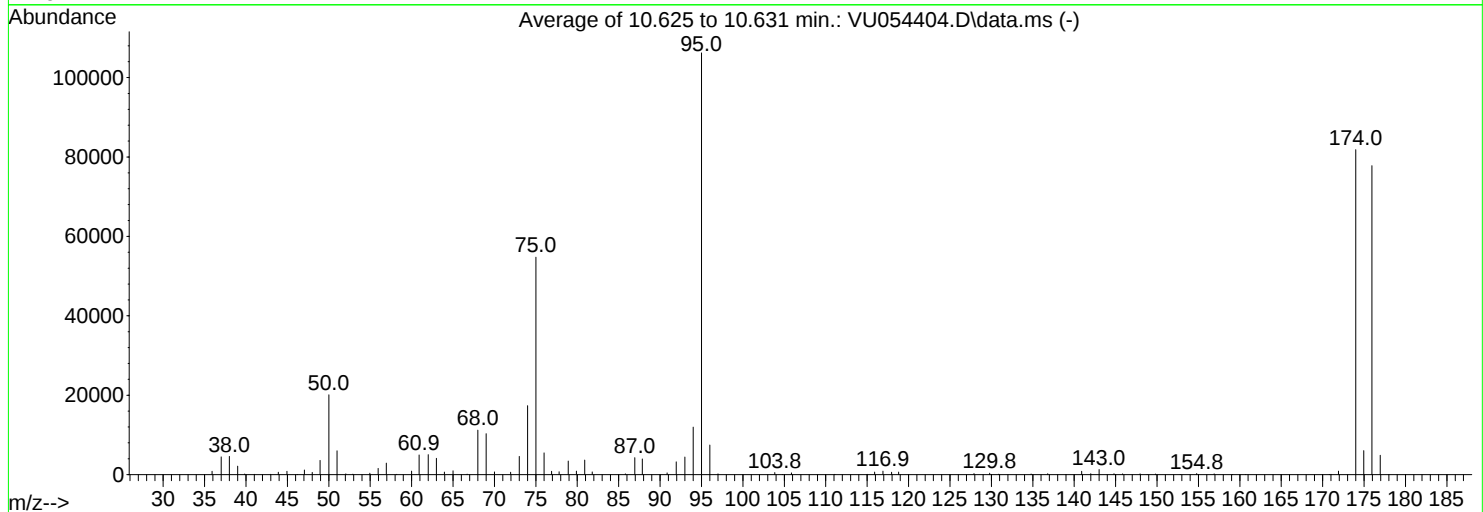


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060723\
Data File : VU054404.D
Acq On : 07 Jun 2023 09:07
Operator : MD/SY
Sample : BFB014
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB014

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Jun 08 01:20:50 2023

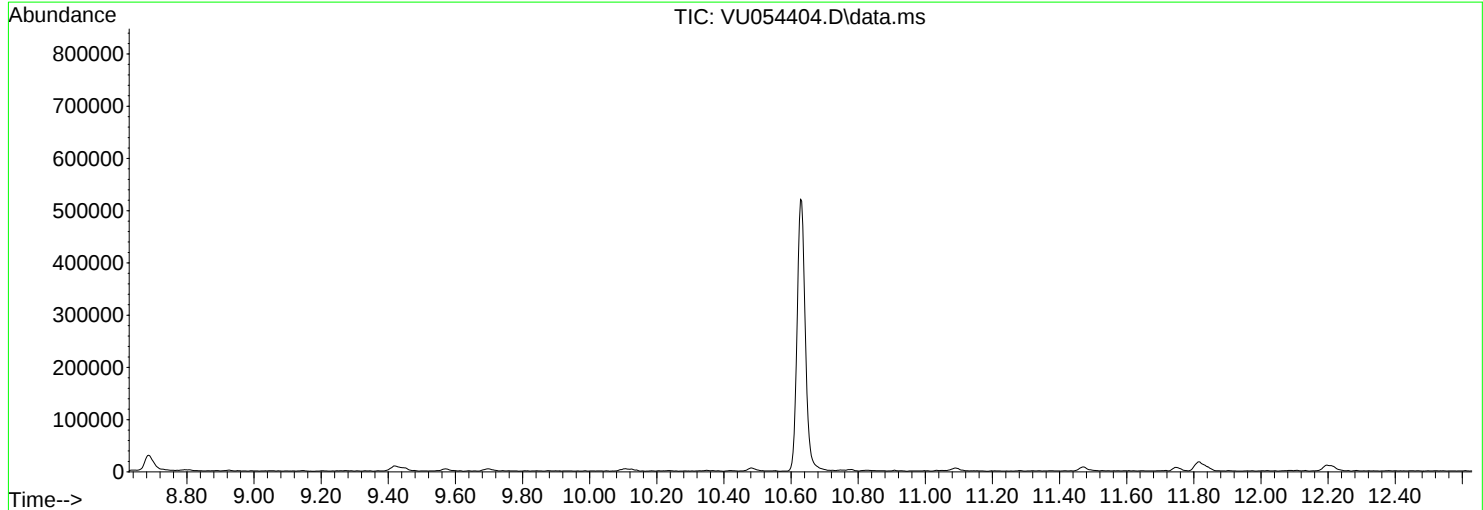

AutoFind: Scans 3121, 3122, 3123; Background Corrected with Scan 3107

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.9	20125	PASS
75	95	30	80	51.6	54773	PASS
95	95	100	100	100.0	106227	PASS
96	95	5	9	7.0	7449	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.1	81851	PASS
175	174	5	9	7.4	6064	PASS
176	174	95	101	95.1	77824	PASS
177	176	5	9	6.3	4868	PASS

m/z	Abundance
35.80	223.0
39.80	261.0
43.90	948.0

Instrument :
MSVOA_U
ClientSampleId :
BFB014

m/z	Abundance
36.00	1119.0
37.00	4392.0
38.00	4495.0
39.00	1837.0
39.90	367.0
41.00	119.0
44.00	1533.0
45.00	815.0
47.00	1011.0
48.00	705.0
48.90	3447.0
50.00	19280.0
51.00	6165.0
52.00	165.0
52.90	164.0
54.90	415.0
56.00	1566.0
56.90	2689.0
60.00	880.0
60.90	4624.0
62.00	4728.0
63.00	3816.0
64.00	591.0
65.00	884.0
66.70	212.0
68.00	10987.0
69.00	10197.0
70.10	747.0
71.90	637.0
73.00	4409.0
74.00	16664.0
75.00	52128.0
76.00	5423.0
76.90	773.0
77.80	586.0
78.90	3119.0
79.90	911.0
80.90	3424.0
81.70	700.0
85.80	198.0
86.90	4066.0
87.90	3825.0
90.90	423.0
92.00	3031.0
93.00	4190.0
94.00	11661.0
95.00	100184.0
96.00	7110.0
96.90	201.0
103.80	507.0
105.80	458.0
111.10	148.0
115.00	166.0
115.90	601.0
116.90	981.0
118.00	527.0
118.80	567.0
127.90	299.0
129.80	357.0
130.90	112.0
134.80	144.0
136.80	202.0
141.00	784.0
142.00	217.0
143.00	1196.0
144.80	260.0
145.90	187.0
147.90	183.0
148.80	121.0
149.80	175.0
154.80	230.0
156.90	209.0
159.10	125.0
170.80	107.0
171.90	823.0
174.00	76344.0
175.00	5514.0
176.00	73168.0
176.90	4365.0
178.00	126.0

Instrument :
MSVOA_U
ClientSampleId :
BFB014

m/z	Abundance
36.00	1073.0
37.00	4560.0
38.00	4708.0
39.00	2239.0
39.90	452.0
41.00	118.0
42.90	106.0
44.00	1575.0
45.00	853.0
46.20	119.0
47.10	1185.0
48.00	534.0
49.00	3659.0
50.00	20664.0
51.00	6196.0
52.10	201.0
52.90	135.0
55.00	350.0
56.00	1652.0
56.90	3039.0
58.20	108.0
60.00	945.0
60.90	5041.0
62.00	5134.0
63.00	4227.0
64.00	657.0
65.00	952.0
66.70	176.0
68.00	11390.0
69.00	10683.0
70.00	671.0
72.00	611.0
73.00	4710.0
74.00	17912.0
75.00	56704.0
76.00	5785.0
76.90	903.0
77.80	738.0
78.90	3544.0
79.90	927.0
80.90	3750.0
81.80	670.0
85.80	231.0
87.00	4322.0
87.90	3955.0
90.90	457.0
91.90	3404.0
93.00	4532.0
94.00	12250.0
95.00	109864.0
96.00	7761.0
97.00	189.0
103.90	541.0
105.90	437.0
111.10	112.0
115.00	118.0
115.90	719.0
116.90	898.0
117.90	611.0
118.80	671.0
127.90	299.0
129.80	358.0
130.90	146.0
134.80	159.0
136.80	276.0
140.90	829.0
142.00	299.0
143.00	1353.0
144.80	263.0
145.90	232.0
148.00	198.0
149.80	166.0
154.80	279.0
156.90	219.0
171.00	120.0
171.90	911.0
174.00	84208.0
174.90	6299.0
176.00	79992.0
177.00	5027.0

Instrument :
MSVOA_U
ClientSampleId :
BFB014

m/z	Abundance
35.90	973.0
37.00	4534.0
38.00	4545.0
39.00	2329.0
39.90	472.0
43.00	154.0
43.90	1550.0
44.90	848.0
47.00	1367.0
48.00	438.0
49.00	3681.0
50.00	20432.0
51.00	5685.0
52.10	194.0
52.90	104.0
55.00	279.0
55.90	1554.0
57.00	3033.0
58.20	107.0
60.00	880.0
60.90	5232.0
62.00	5218.0
63.00	4236.0
63.90	663.0
65.00	1029.0
68.00	11203.0
69.00	10132.0
69.90	627.0
72.00	546.0
73.00	4633.0
74.00	17576.0
75.00	55488.0
76.00	5294.0
76.90	841.0
77.80	829.0
78.90	3590.0
79.90	854.0
80.90	3788.0
81.90	659.0
85.80	220.0
87.00	4420.0
87.80	4084.0
90.80	430.0
91.90	3256.0
93.00	4568.0
94.00	11984.0
95.00	108632.0
96.00	7476.0
97.10	188.0
103.90	546.0
104.80	154.0
105.90	412.0
115.90	676.0
116.90	750.0
117.90	715.0
118.80	751.0
127.90	306.0
129.80	332.0
130.90	169.0
134.80	144.0
136.80	286.0
139.00	106.0
140.80	945.0
142.00	256.0
143.00	1297.0
144.80	210.0
145.80	206.0
148.00	200.0
149.80	106.0
152.80	113.0
154.80	303.0
156.90	198.0
160.70	182.0
171.00	125.0
171.90	960.0
174.00	85000.0
174.90	6379.0
175.90	80312.0
177.00	5213.0

Instrument :
MSVOA_U
ClientSampleId :
BFB014