

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
 Data File : VU059179.D
 Acq On : 07 Jun 2024 12:03
 Operator : MD/SY
 Sample : VU0607WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jun 08 03:16:17 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 08 01:56:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	210963	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	209564	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.810	152	87140	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	71504	56.609	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 113.220%			
7) Chloroethane-d5	1.907	69	60778	56.171	ug/L	0.04
Spiked Amount 50.000	Range 70 - 130		Recovery = 112.340%			
11) 1,1-Dichloroethene-d2	2.560	63	90047	36.116	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 72.240%			
21) 2-Butanone-d5	4.615	46	92444	77.646	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 77.650%			
24) Chloroform-d	5.055	84	121403	48.280	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 96.560%			
26) 1,2-Dichloroethane-d4	5.695	65	81287	52.743	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 105.480%			
32) Benzene-d6	5.721	84	254211	52.853	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 105.700%			
36) 1,2-Dichloropropane-d6	6.685	67	84162	50.749	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 101.500%			
41) Toluene-d8	7.894	98	211148	51.713	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 103.420%			
43) trans-1,3-Dichloroprop...	8.177	79	31712	47.306	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 94.620%			
47) 2-Hexanone-d5	8.627	63	50738	66.160	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 66.160%			
56) 1,1,2,2-Tetrachloroeth...	10.749	84	115278	41.072	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 82.140%			
66) 1,2-Dichlorobenzene-d4	12.190	152	69473	53.423	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 106.840%			
Target Compounds						Qvalue
37) 1,2-Dichloropropane	6.685	63	8849	4.118	ug/L	# 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
Data File : VU059179.D
Acq On : 07 Jun 2024 12:03
Operator : MD/SY
Sample : VU0607WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Jun 08 03:16:17 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 08 01:56:01 2024
Response via : Initial Calibration

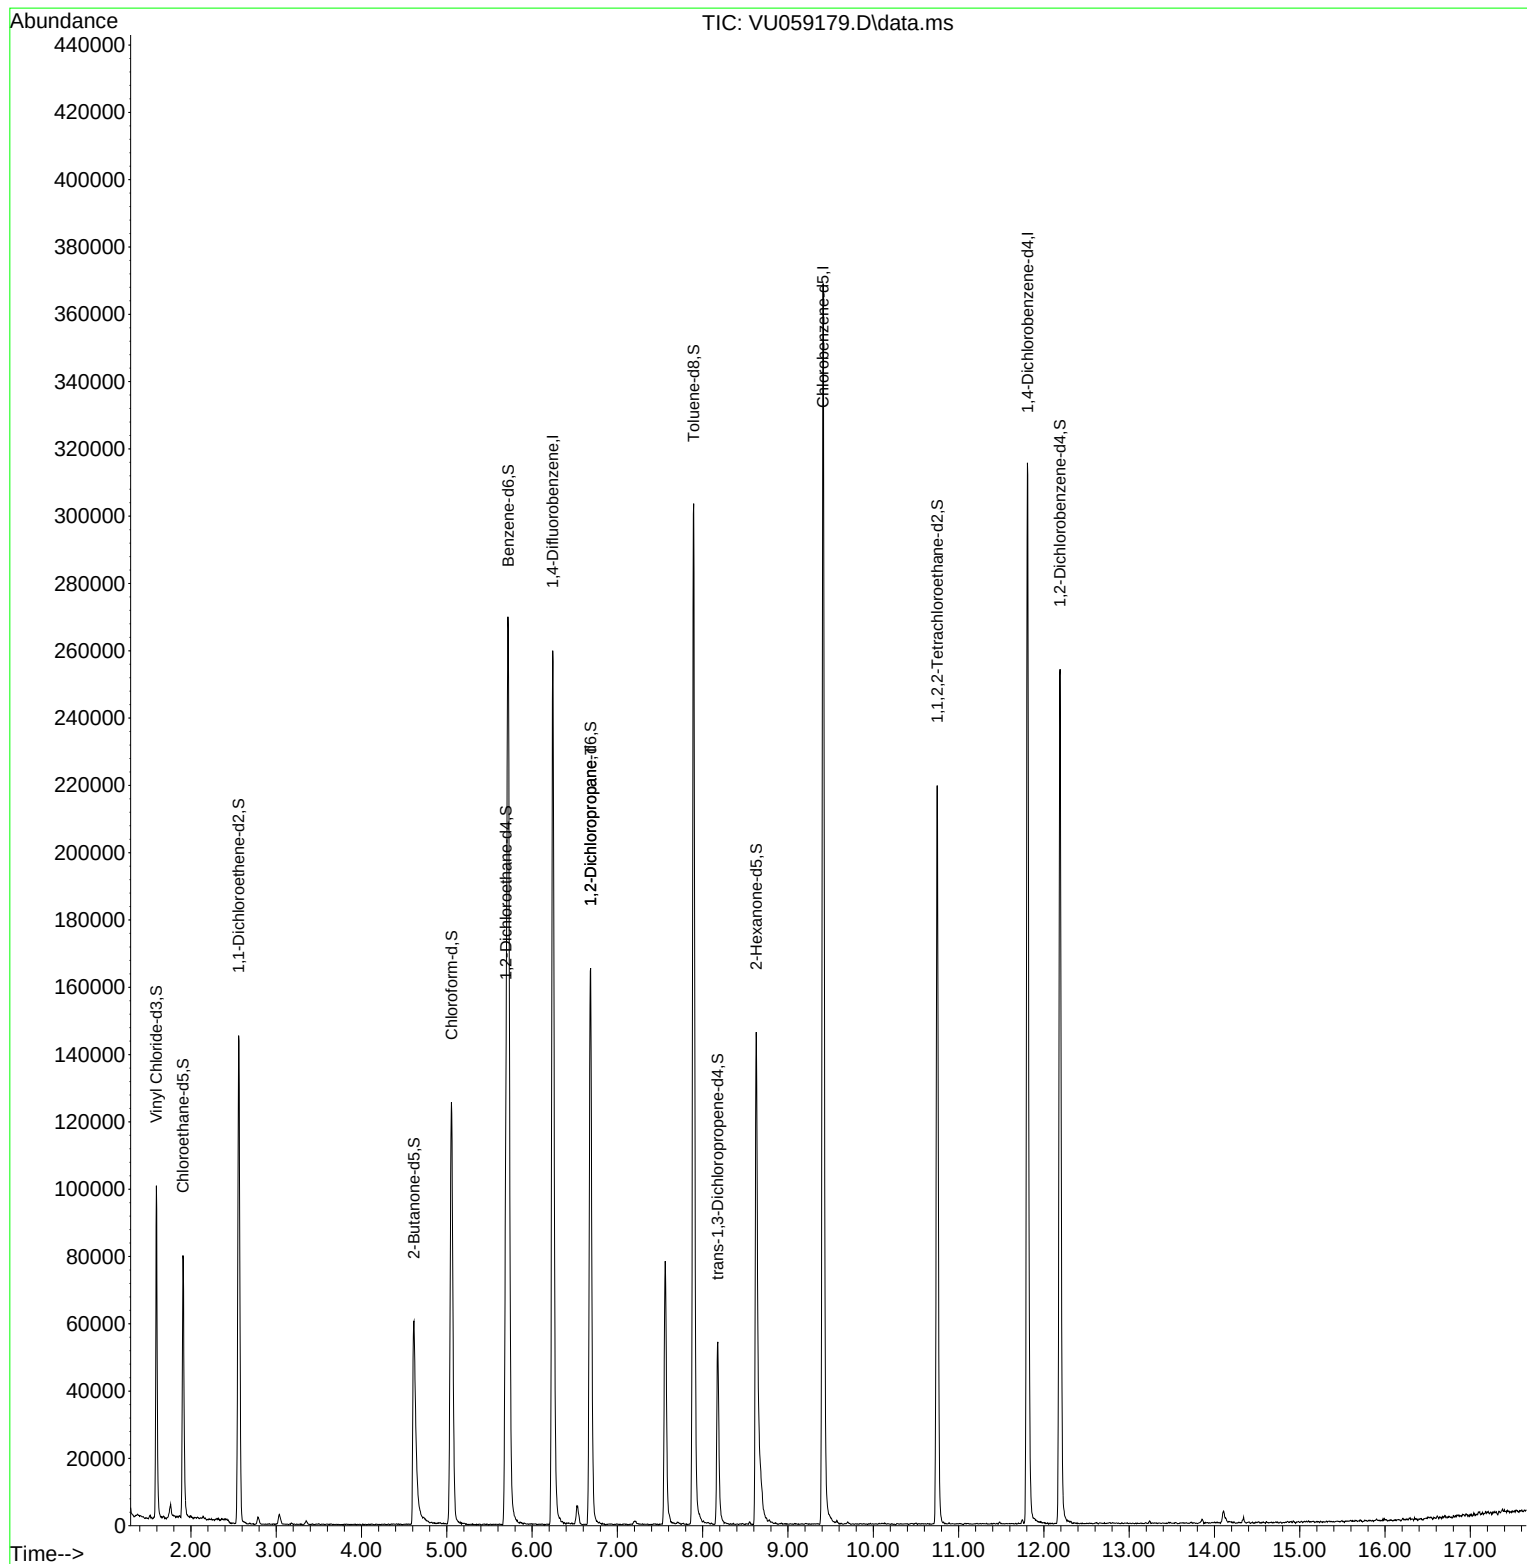

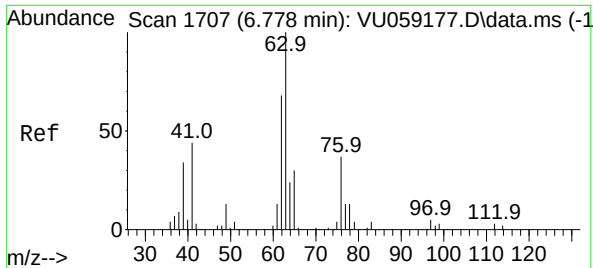

#37
1,2-Dichloropropane
Concen: 4.118 ug/L
RT: 6.685 min Scan# 1
Delta R.T. -0.093 min
Lab File: VU059179.D
Acq: 07 Jun 2024 12:03

Instrument :
MSVOA_U
ClientSampleId :

Tgt Ion: 63 Resp: 8849
Ion Ratio Lower Upper
63 100
112 0.0 2.6 4.0#

