

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
 Data File : VU059180.D
 Acq On : 07 Jun 2024 12:26
 Operator : MD/SY
 Sample : P2738-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jun 08 03:16:31 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 08 01:56:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	197719	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	201356	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	84088	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	67197	56.762	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	113.520%
7) Chloroethane-d5	1.907	69	59273	58.450	ug/L	0.04
Spiked Amount	50.000	Range	70 - 130	Recovery	=	116.900%
11) 1,1-Dichloroethene-d2	2.560	63	84403	36.120	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	72.240%
21) 2-Butanone-d5	4.612	46	92232	82.658	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	82.660%
24) Chloroform-d	5.055	84	118584	50.318	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.640%
26) 1,2-Dichloroethane-d4	5.695	65	76754	53.138	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	106.280%
32) Benzene-d6	5.721	84	241654	52.290	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.580%
36) 1,2-Dichloropropane-d6	6.682	67	81430	51.103	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	102.200%
41) Toluene-d8	7.894	98	203139	51.779	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.560%
43) trans-1,3-Dichloroprop...	8.174	79	31314	48.616	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	97.240%
47) 2-Hexanone-d5	8.627	63	49878	67.690	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	67.690%
56) 1,1,2,2-Tetrachloroeth...	10.750	84	114730	42.543	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	85.080%
66) 1,2-Dichlorobenzene-d4	12.190	152	66742	53.186	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	106.380%
Target Compounds						
37) 1,2-Dichloropropane	6.685	63	8370	4.054	ug/L	Qvalue # 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
Data File : VU059180.D
Acq On : 07 Jun 2024 12:26
Operator : MD/SY
Sample : P2738-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: Jun 08 03:16:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 08 01:56:01 2024
Response via : Initial Calibration

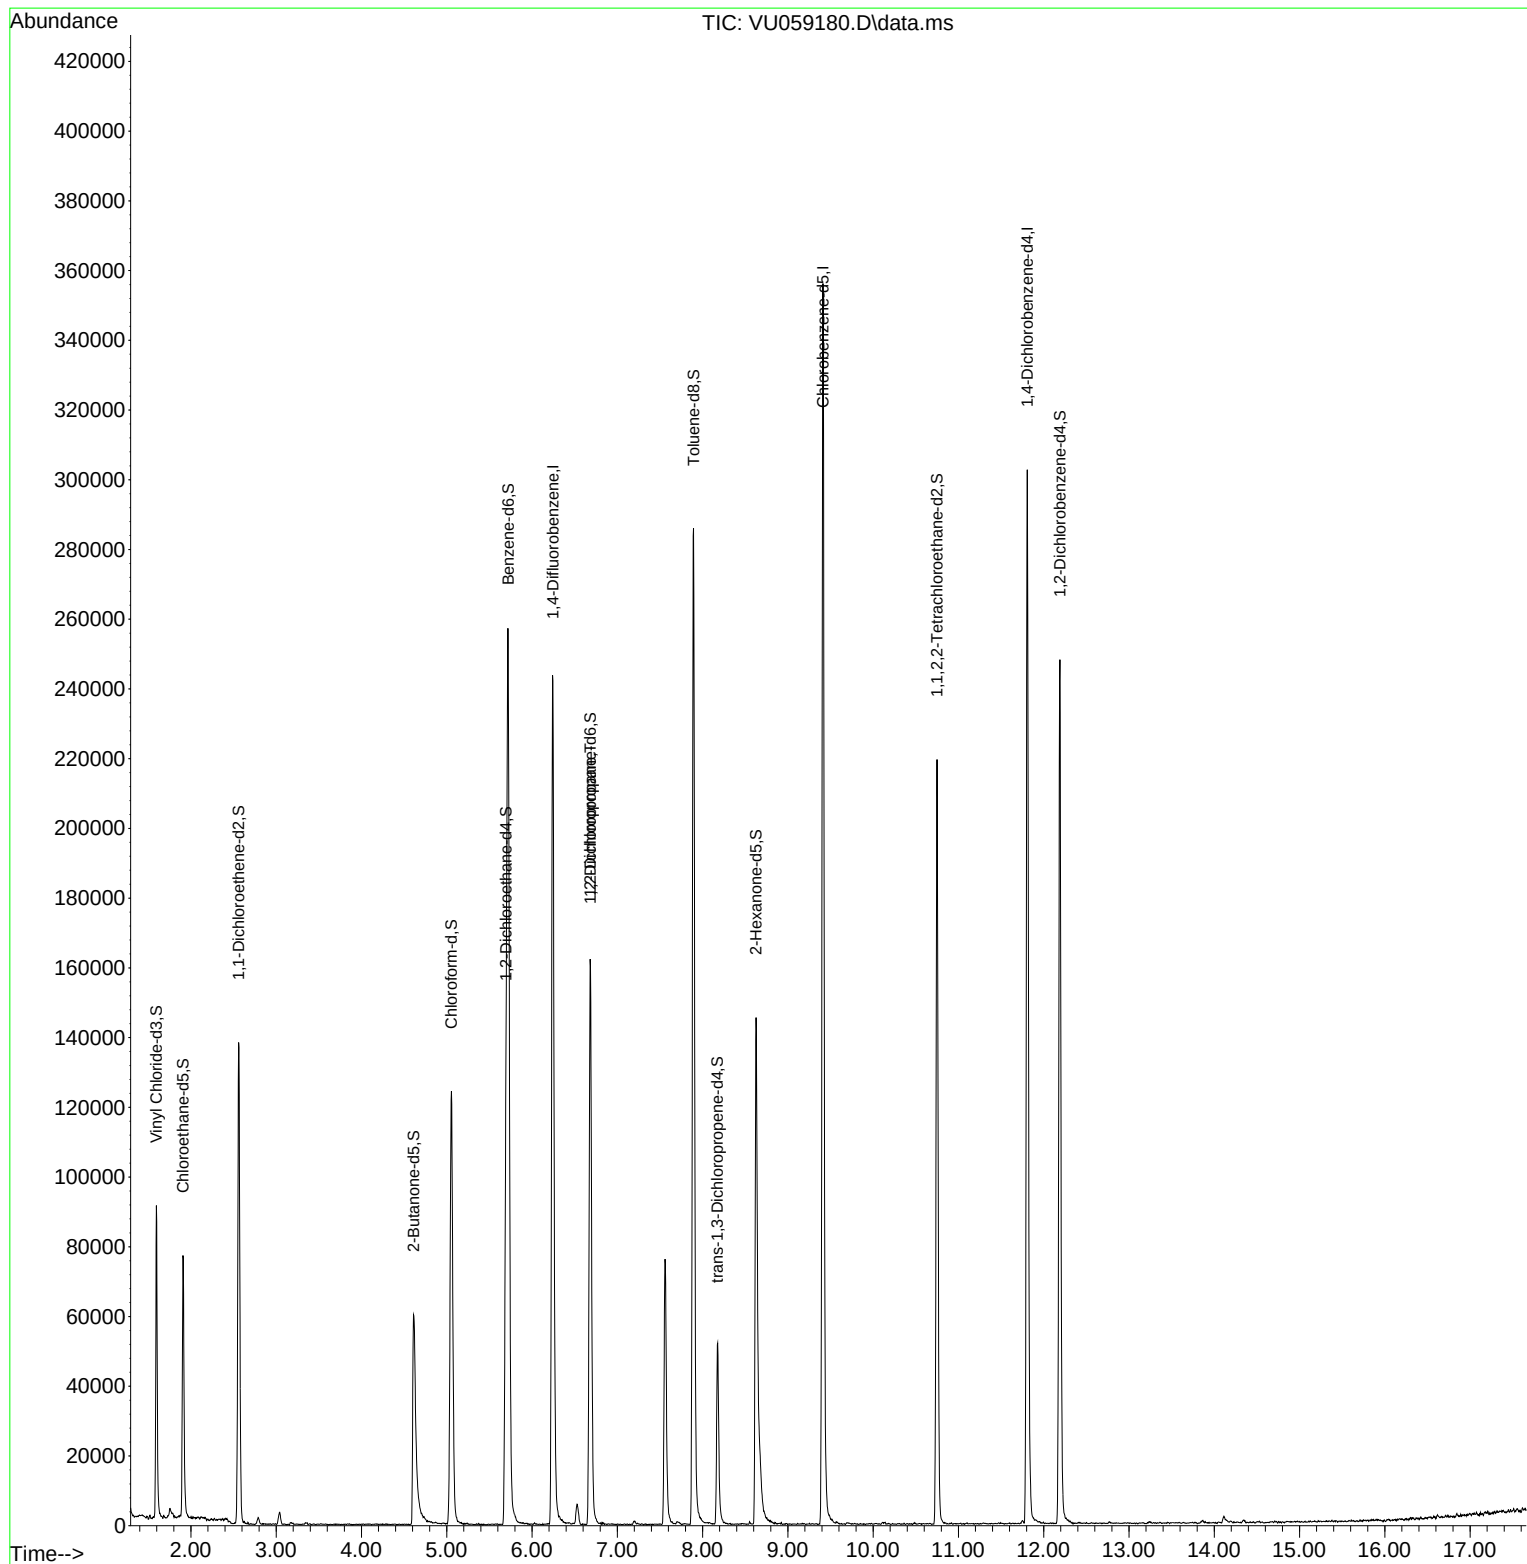

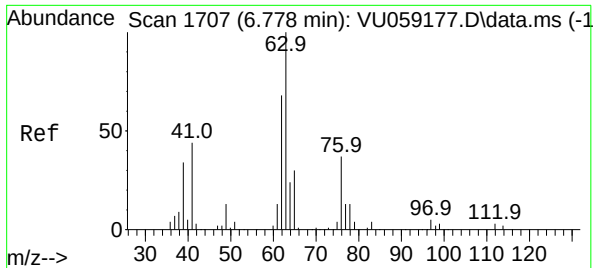

#37
1,2-Dichloropropane
Concen: 4.054 ug/L
RT: 6.685 min Scan# 1
Delta R.T. -0.093 min
Lab File: VU059180.D
Acq: 07 Jun 2024 12:26

Instrument :
MSVOA_U
ClientSampleId :

Tgt Ion: 63 Resp: 8370
Ion Ratio Lower Upper
63 100
112 0.0 2.6 4.0#

