

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
 Data File : VU059187.D
 Acq On : 07 Jun 2024 15:18
 Operator : MD/SY
 Sample : P2710-13ME
 Misc : 4.34g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Jun 08 03:18:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 08 01:56:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	195813	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	197851	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	85216	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	67413	57.499	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 115.000%			
7) Chloroethane-d5	1.907	69	57632	57.385	ug/L	0.04
Spiked Amount 50.000	Range 70 - 130		Recovery = 114.760%			
11) 1,1-Dichloroethene-d2	2.560	63	83735	36.183	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 72.360%			
21) 2-Butanone-d5	4.615	46	100381	90.836	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 90.840%			
24) Chloroform-d	5.055	84	115834	49.630	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 99.260%			
26) 1,2-Dichloroethane-d4	5.695	65	77155	53.935	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 107.880%			
32) Benzene-d6	5.721	84	240160	52.887	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 105.780%			
36) 1,2-Dichloropropane-d6	6.682	67	79804	50.970	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 101.940%			
41) Toluene-d8	7.894	98	196353	50.936	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 101.880%			
43) trans-1,3-Dichloroprop...	8.174	79	31996	50.555	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 101.120%			
47) 2-Hexanone-d5	8.627	63	56506	78.043	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 78.040%			
56) 1,1,2,2-Tetrachloroeth...	10.750	84	115360	43.534	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 87.060%			
66) 1,2-Dichlorobenzene-d4	12.190	152	68857	54.145	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 108.300%			
Target Compounds						Qvalue
60) 1,2,3-Trichloropropane	11.811	75	11327	4.780	ug/L	# 67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
Data File : VU059187.D
Acq On : 07 Jun 2024 15:18
Operator : MD/SY
Sample : P2710-13ME
Misc : 4.34g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Jun 08 03:18:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 08 01:56:01 2024
Response via : Initial Calibration

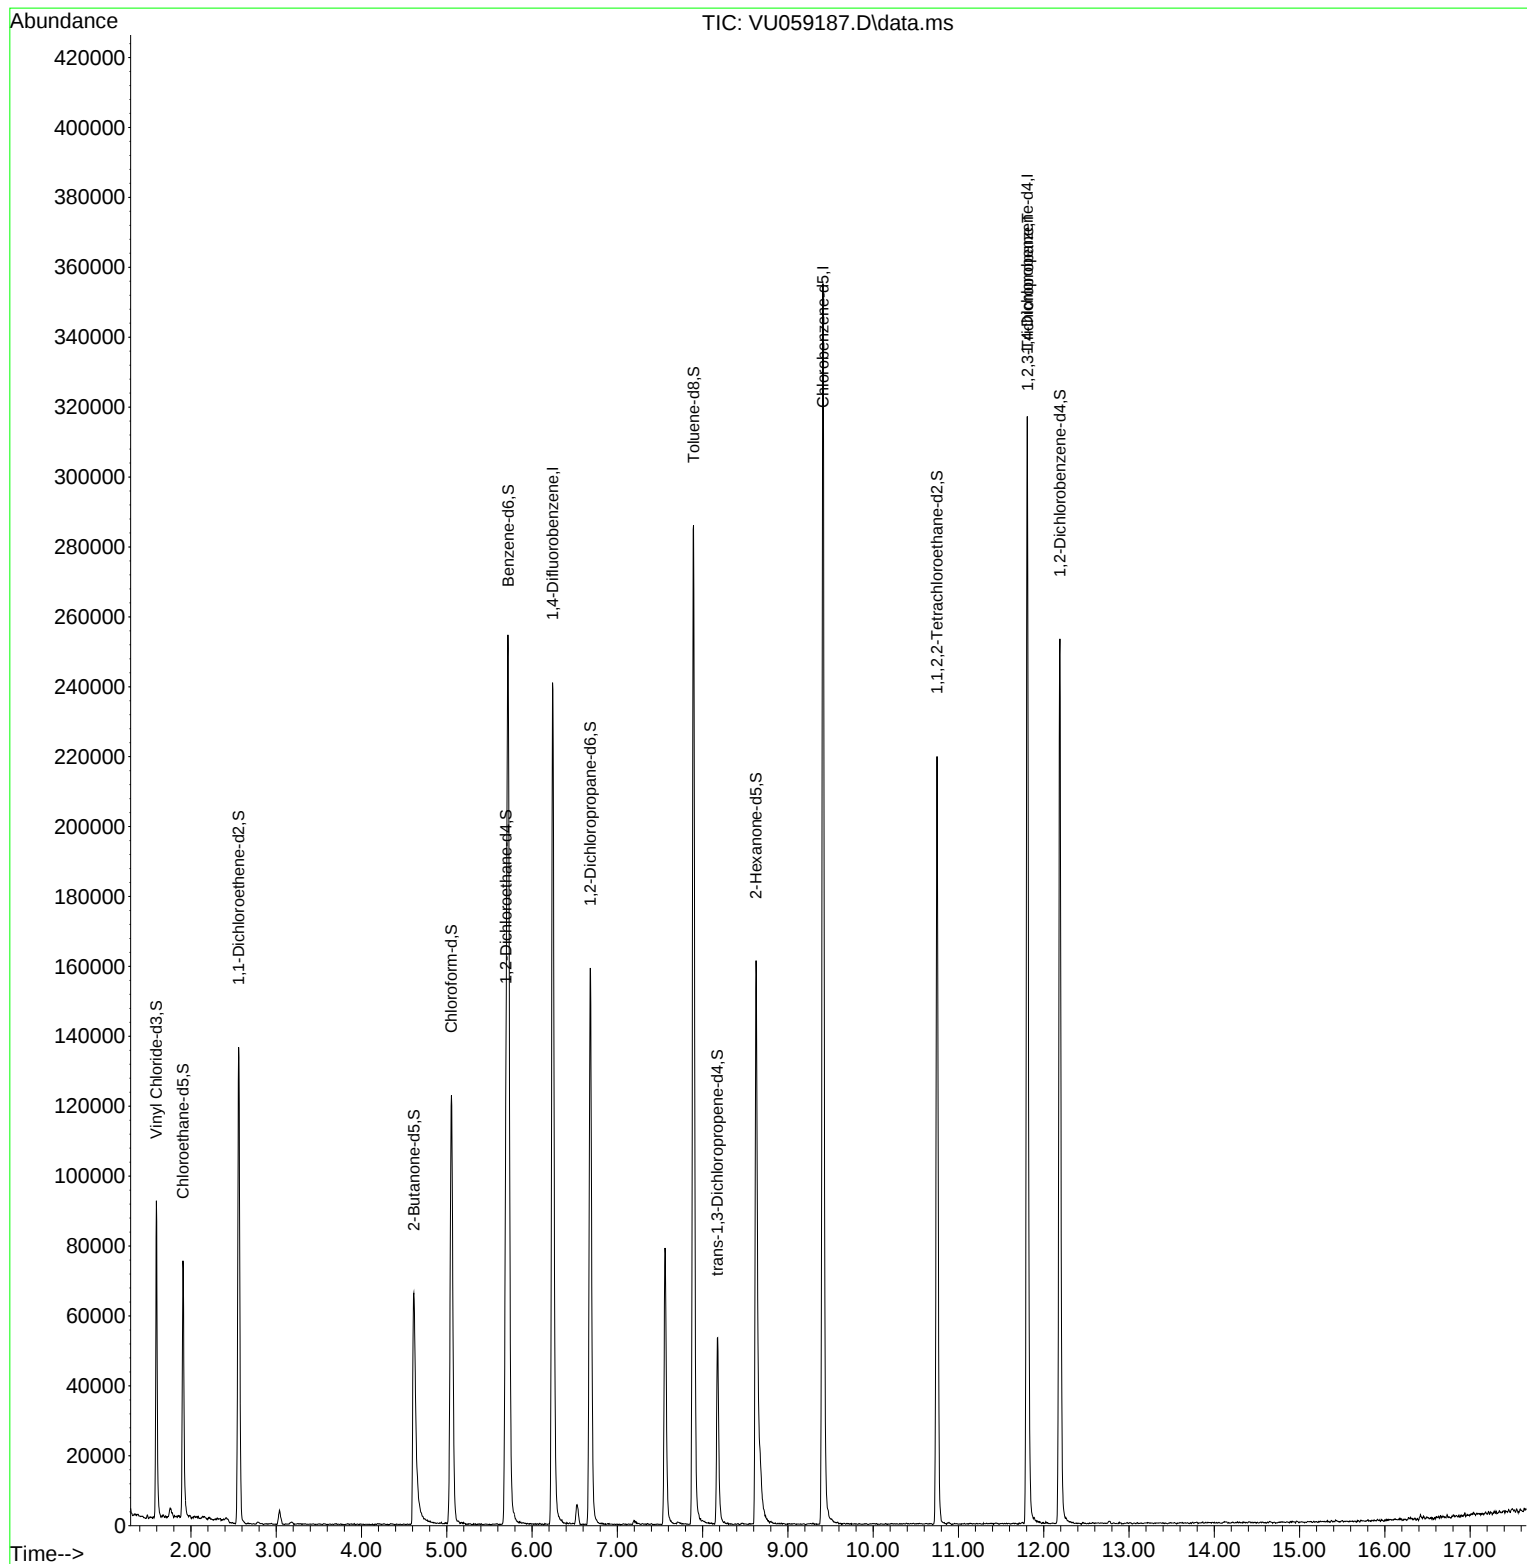

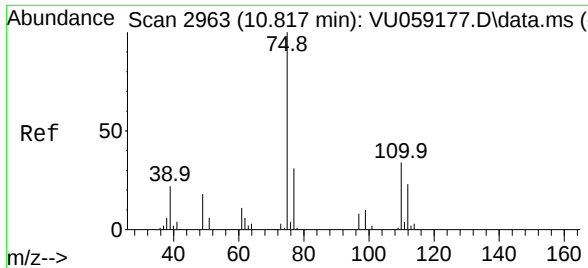

#60
 1,2,3-Trichloropropane
 Concen: 4.780 ug/L
 RT: 11.811 min Scan# 31
 Delta R.T. 0.994 min
 Lab File: VU059187.D
 Acq: 07 Jun 2024 15:18

Instrument :
 MSVOA_U
 ClientSampleId :

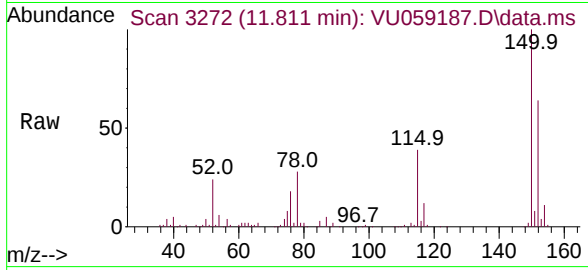

Tgt Ion: 75 Resp: 11327

Ion	Ratio	Lower	Upper
75	100		
77	30.9	26.2	39.2
110	0.0	28.4	42.6#

