

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
 Data File : VU059184.D
 Acq On : 07 Jun 2024 14:08
 Operator : MD/SY
 Sample : P2695-22
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A4DB5

Quant Time: Jun 08 03:17:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 08 01:56:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	221782	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	221390	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	100142	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	44253	33.325	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	66.660%	
7) Chloroethane-d5	1.907	69	42697	37.536	ug/L	0.04
Spiked Amount	50.000	Range 70 - 130	Recovery	=	75.080%	
11) 1,1-Dichloroethene-d2	2.560	63	62775	23.950	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	47.900%#	
21) 2-Butanone-d5	4.611	46	125206	100.034	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	100.030%	
24) Chloroform-d	5.055	84	115612	43.735	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	87.460%	
26) 1,2-Dichloroethane-d4	5.695	65	72976	45.041	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	90.080%	
32) Benzene-d6	5.721	84	209790	41.287	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	82.580%	
36) 1,2-Dichloropropane-d6	6.682	67	78089	44.571	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	89.140%	
41) Toluene-d8	7.891	98	170961	39.634	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	79.260%#	
43) trans-1,3-Dichloroprop...	8.174	79	29997	42.357	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	84.720%	
47) 2-Hexanone-d5	8.624	63	67357	83.139	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	83.140%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84	134628	45.404	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	90.800%	
66) 1,2-Dichlorobenzene-d4	12.190	152	68708	45.975	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	91.960%	
Target Compounds						
13) Acetone	2.618	43	35983	24.459	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
Data File : VU059184.D
Acq On : 07 Jun 2024 14:08
Operator : MD/SY
Sample : P2695-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A4DB5

Quant Time: Jun 08 03:17:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 08 01:56:01 2024
Response via : Initial Calibration

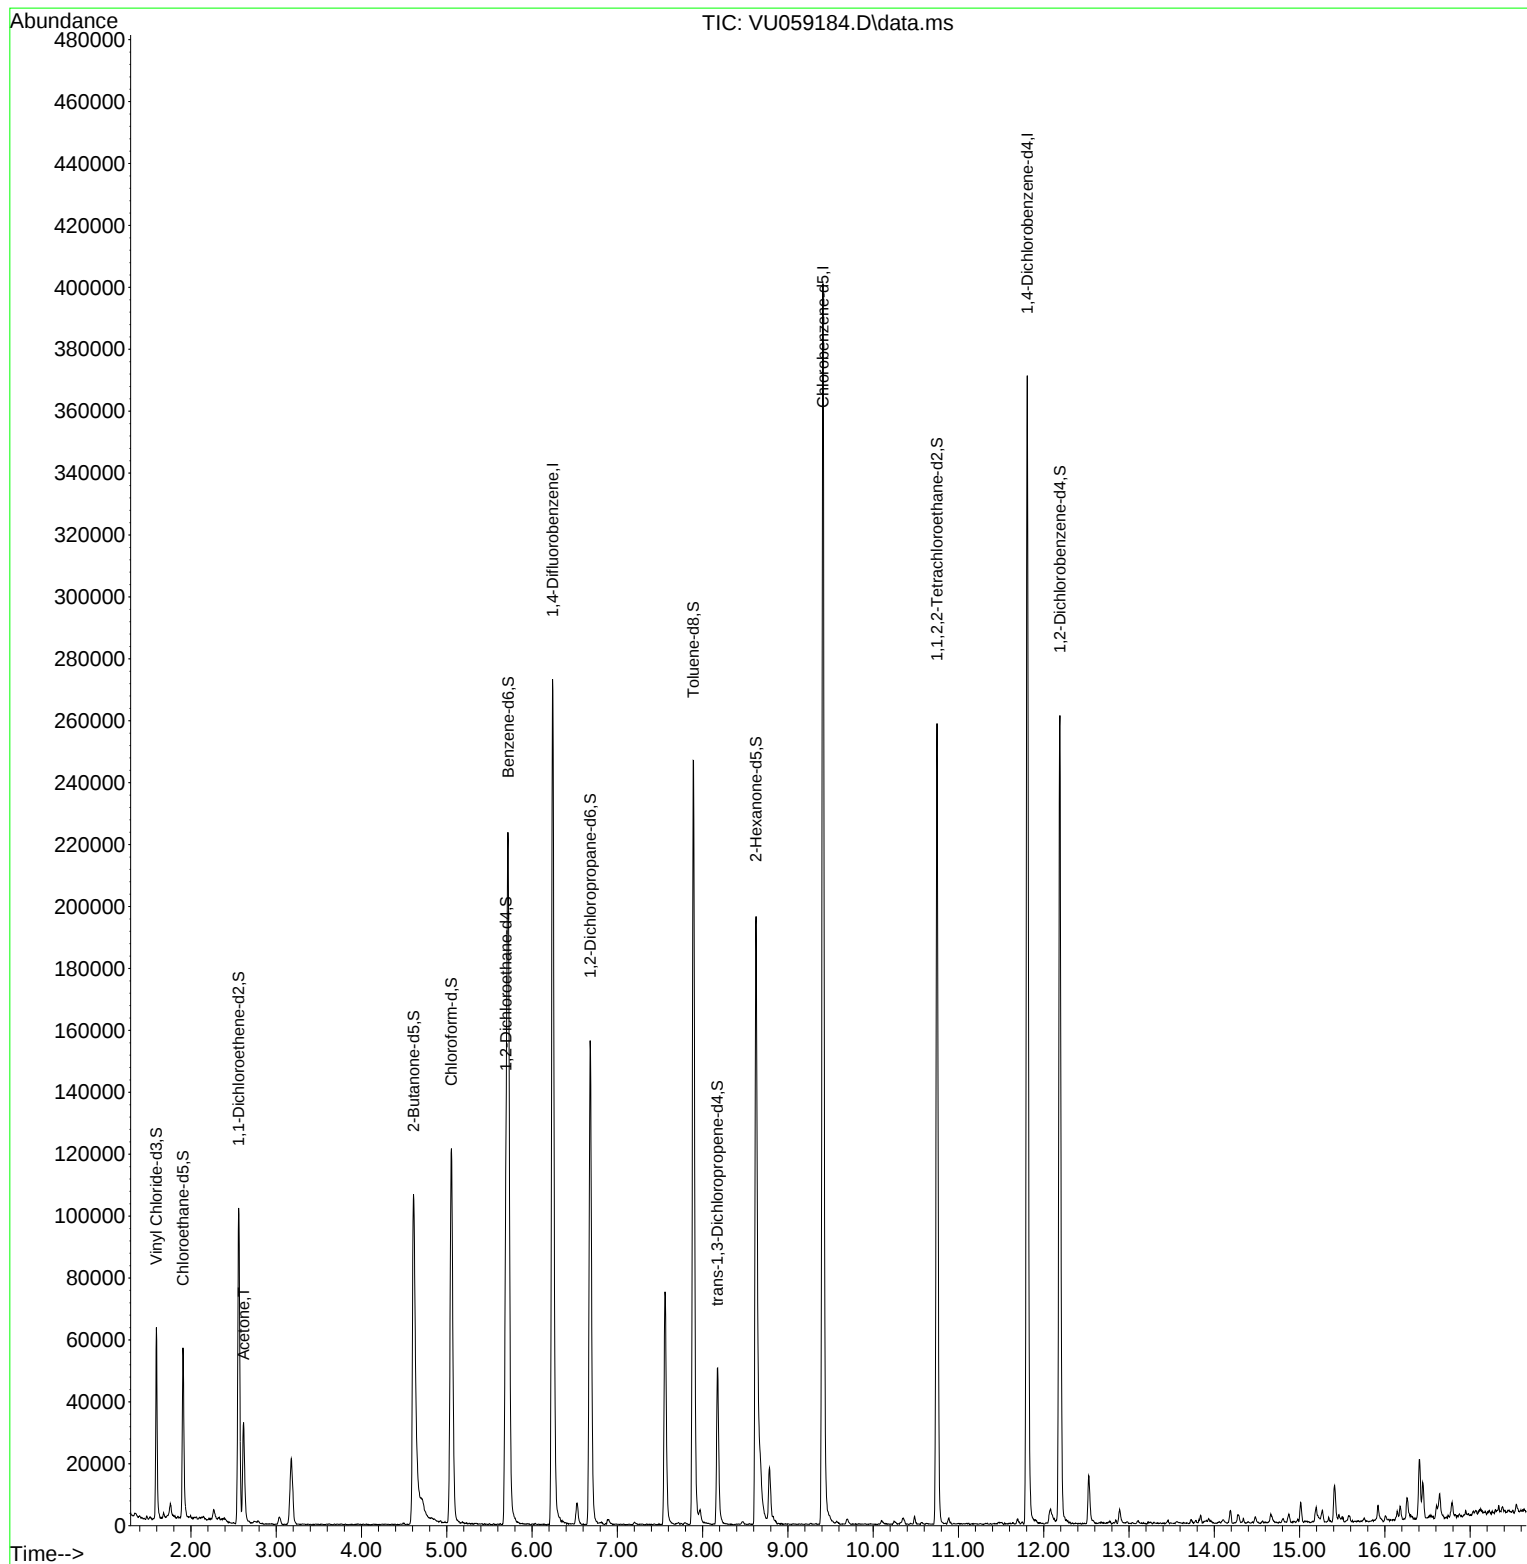

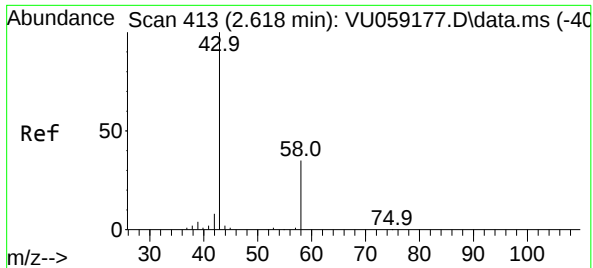

#13
 Acetone
 Concen: 24.459 ug/L
 RT: 2.618 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: VU059184.D
 Acq: 07 Jun 2024 14:08

Instrument :
 MSVOA_U
 ClientSampleId :
 A4DB5

Tgt Ion: 43 Resp: 35983
 Ion Ratio Lower Upper
 43 100
 58 34.9 0.0 68.8

