

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
 Data File : VU059180.D
 Acq On : 07 Jun 2024 12:26
 Operator : MD/SY
 Sample : P2738-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M

Title : VOC Analysis

Signal : TIC: VU059180.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	112	rBV	89423	106855	15.15%	1.979%
2	1.756	141	145	152	rBV6	1594	1872	0.27%	0.035%
3	1.907	184	192	214	rVB	75197	105949	15.02%	1.962%
4	2.560	383	395	412	rVV	137961	226579	32.13%	4.197%
5	2.621	412	414	419	rVB3	575	449	0.06%	0.008%
6	2.669	427	429	433	rVB	554	270	0.04%	0.005%
7	2.702	437	439	444	rVB2	205	166	0.02%	0.003%
8	2.788	454	466	478	rBV3	2008	3694	0.52%	0.068%
9	3.042	535	545	555	rVB4	3455	6055	0.86%	0.112%
10	3.171	580	585	588	rBV2	752	894	0.13%	0.017%
11	3.341	634	638	644	rBV4	432	581	0.08%	0.011%
12	3.396	649	655	659	rVB	273	294	0.04%	0.005%
13	3.486	677	683	685	rBV3	205	245	0.03%	0.005%
14	3.637	723	730	733	rBV2	228	302	0.04%	0.006%
15	3.679	740	743	747	rVB2	226	178	0.03%	0.003%
16	3.702	747	750	754	rBV2	284	206	0.03%	0.004%
17	3.763	767	769	774	rBV2	176	200	0.03%	0.004%
18	3.859	797	799	805	rVB2	278	236	0.03%	0.004%
19	3.911	812	815	818	rBV2	149	155	0.02%	0.003%
20	4.020	846	849	854	rVB2	183	168	0.02%	0.003%
21	4.612	1023	1033	1061	rBV	60099	156519	22.19%	2.899%
22	4.775	1082	1084	1088	rBV3	379	210	0.03%	0.004%
23	4.949	1135	1138	1140	rBV2	223	177	0.03%	0.003%
24	4.997	1149	1153	1156	rVB3	222	147	0.02%	0.003%
25	5.055	1156	1171	1194	rBV	124203	275732	39.10%	5.107%
26	5.203	1215	1217	1220	rVB2	324	206	0.03%	0.004%
27	5.229	1220	1225	1227	rBV2	290	281	0.04%	0.005%
28	5.245	1227	1230	1233	rVB	297	179	0.03%	0.003%
29	5.348	1257	1262	1265	rBV2	244	202	0.03%	0.004%
30	5.377	1268	1271	1275	rVB2	400	278	0.04%	0.005%
31	5.486	1300	1305	1312	rBV2	182	210	0.03%	0.004%
32	5.566	1326	1330	1332	rBV2	200	165	0.02%	0.003%
33	5.595	1336	1339	1344	rVB	227	154	0.02%	0.003%
34	5.718	1357	1377	1415	rBV2	257054	705223	100.00%	13.063%
35	6.029	1469	1474	1478	rBV	490	450	0.06%	0.008%
36	6.242	1528	1540	1562	rBV	243519	475976	67.49%	8.816%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
 Data File : VU059180.D
 Acq On : 07 Jun 2024 12:26
 Operator : MD/SY
 Sample : P2738-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	6.480	1611	1614	1619	rVV3	284	313	0.04%	0.006%
38	6.528	1619	1629	1641	rVB6	5772	11814	1.68%	0.219%
39	6.682	1663	1677	1709	rBV	162149	322765	45.77%	5.979%
40	6.820	1717	1720	1722	rBV3	617	346	0.05%	0.006%
41	6.836	1722	1725	1728	rVB2	474	329	0.05%	0.006%
42	6.894	1738	1743	1747	rBV2	215	235	0.03%	0.004%
43	7.193	1830	1836	1838	rBV3	865	800	0.11%	0.015%
44	7.283	1860	1864	1866	rBV	225	194	0.03%	0.004%
45	7.316	1872	1874	1877	rBV	272	212	0.03%	0.004%
46	7.335	1877	1880	1883	rVB	327	232	0.03%	0.004%
47	7.438	1907	1912	1917	rVV2	147	195	0.03%	0.004%
48	7.560	1938	1950	1973	rBV2	76071	141334	20.04%	2.618%
49	7.698	1989	1993	1995	rBV2	644	534	0.08%	0.010%
50	7.769	2011	2015	2017	rBV	252	217	0.03%	0.004%
51	7.894	2041	2054	2080	rBV	285770	516206	73.20%	9.562%
52	8.177	2130	2142	2164	rBV2	51833	92843	13.17%	1.720%
53	8.550	2255	2258	2264	rBV3	679	527	0.07%	0.010%
54	8.627	2271	2282	2320	rBV2	145224	318382	45.15%	5.897%
55	8.849	2348	2351	2356	rBV4	473	380	0.05%	0.007%
56	8.923	2371	2374	2377	rVB	580	373	0.05%	0.007%
57	8.978	2389	2391	2398	rVB2	397	445	0.06%	0.008%
58	9.116	2430	2434	2439	rBV	335	306	0.04%	0.006%
59	9.190	2454	2457	2462	rVB2	249	223	0.03%	0.004%
60	9.412	2514	2526	2548	rBV	355839	611934	86.77%	11.335%
61	9.566	2572	2574	2577	rBV2	414	306	0.04%	0.006%
62	9.663	2601	2604	2607	rVB2	252	171	0.02%	0.003%
63	9.695	2607	2614	2618	rBV3	545	744	0.11%	0.014%
64	9.894	2673	2676	2679	rBV	232	159	0.02%	0.003%
65	9.930	2682	2687	2690	rBV	257	312	0.04%	0.006%
66	9.978	2699	2702	2708	rVB2	246	212	0.03%	0.004%
67	10.113	2738	2744	2747	rBV	561	681	0.10%	0.013%
68	10.164	2756	2760	2763	rBV2	155	156	0.02%	0.003%
69	10.184	2763	2766	2772	rVB2	308	290	0.04%	0.005%
70	10.229	2777	2780	2785	rBV	208	157	0.02%	0.003%
71	10.364	2819	2822	2826	rVB2	352	236	0.03%	0.004%
72	10.399	2827	2833	2838	rBV2	240	284	0.04%	0.005%
73	10.425	2838	2841	2846	rBV2	196	193	0.03%	0.004%
74	10.450	2846	2849	2852	rVB2	259	164	0.02%	0.003%
75	10.589	2886	2892	2895	rBV2	247	289	0.04%	0.005%
76	10.750	2929	2942	2967	rVV	219323	358137	50.78%	6.634%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
 Data File : VU059180.D
 Acq On : 07 Jun 2024 12:26
 Operator : MD/SY
 Sample : P2738-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	10.901	2987	2989	2992	rBV2	252	146	0.02%	0.003%
78	10.920	2992	2995	3000	rVB2	450	360	0.05%	0.007%
79	10.946	3000	3003	3007	rBV2	254	279	0.04%	0.005%
80	11.081	3042	3045	3047	rBV	251	190	0.03%	0.004%
81	11.200	3078	3082	3085	rBV2	205	197	0.03%	0.004%
82	11.470	3163	3166	3171	rBV2	280	251	0.04%	0.005%
83	11.602	3205	3207	3211	rVB2	300	178	0.03%	0.003%
84	11.753	3248	3254	3260	rBV4	777	1042	0.15%	0.019%
85	11.807	3260	3271	3293	rBV	302127	511533	72.53%	9.475%
86	12.106	3361	3364	3368	rVB	279	214	0.03%	0.004%
87	12.190	3377	3390	3411	rBV	247752	422032	59.84%	7.817%
88	12.502	3484	3487	3489	rBV2	301	150	0.02%	0.003%
89	13.087	3666	3669	3674	rVB2	268	252	0.04%	0.005%
90	13.126	3675	3681	3684	rBV2	273	347	0.05%	0.006%
91	13.222	3707	3711	3712	rBV	333	209	0.03%	0.004%
92	13.486	3790	3793	3796	rBV2	260	213	0.03%	0.004%
93	14.052	3964	3969	3973	rBV3	365	486	0.07%	0.009%
94	14.113	3980	3988	3994	rBV4	1856	3207	0.45%	0.059%
95	14.232	4022	4025	4027	rBV	410	213	0.03%	0.004%
96	14.341	4052	4059	4060	rBV2	778	826	0.12%	0.015%
97	14.711	4171	4174	4177	rBV	417	297	0.04%	0.006%
98	14.756	4185	4188	4192	rBV2	458	382	0.05%	0.007%
99	14.798	4198	4201	4206	rBV2	366	360	0.05%	0.007%
100	16.145	4618	4620	4622	rBV2	521	269	0.04%	0.005%




Sum of corrected areas: 5398720

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
Data File : VU059180.D
Acq On : 07 Jun 2024 12:26
Operator : MD/SY
Sample : P2738-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

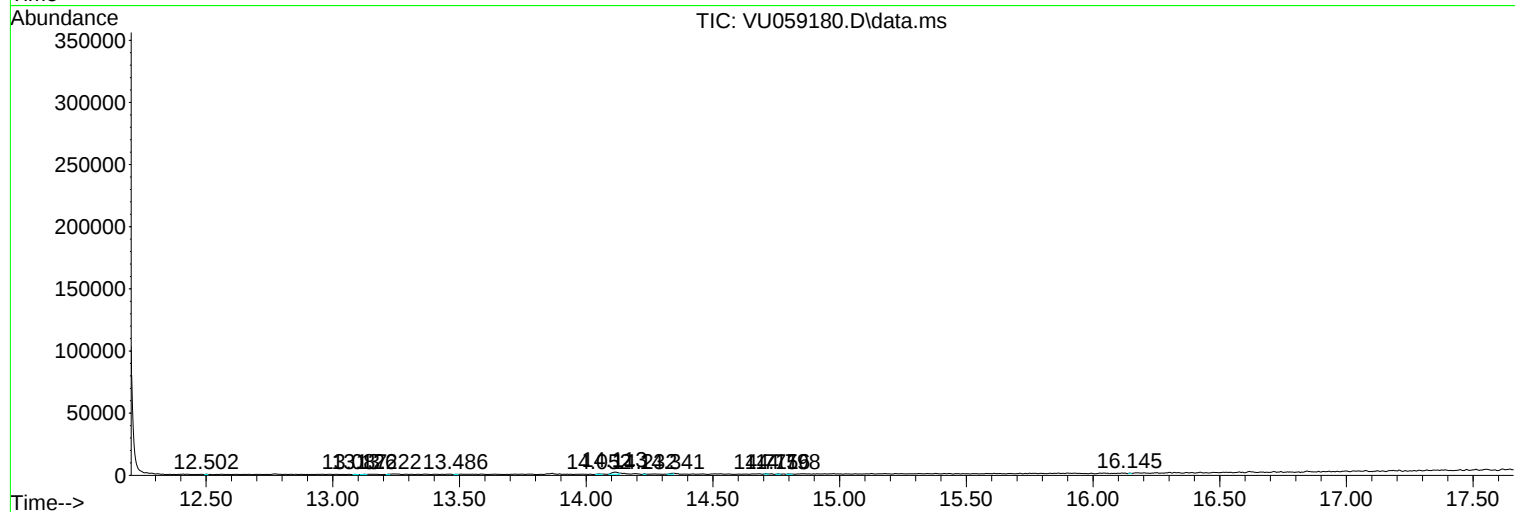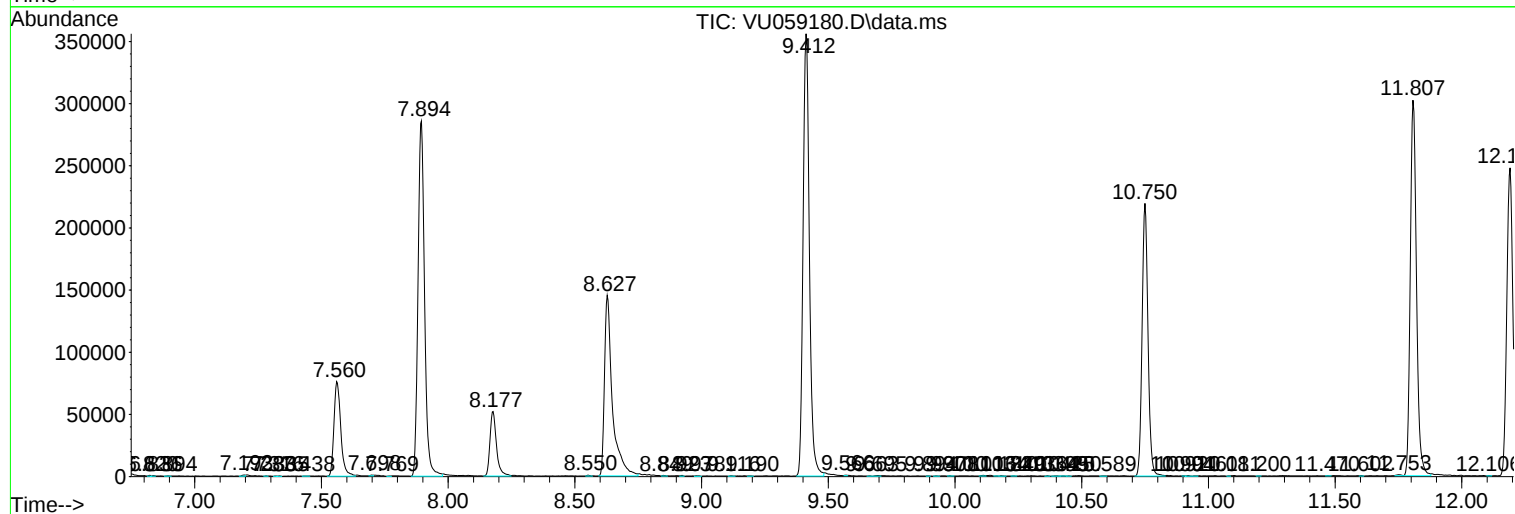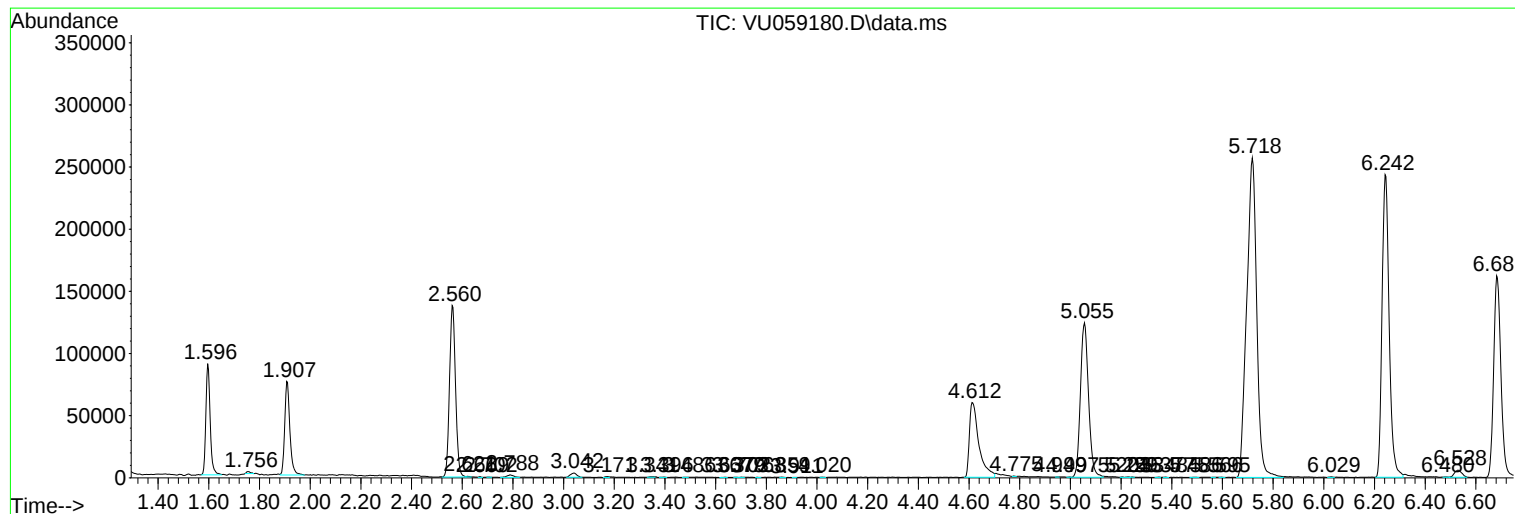

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
Data File : VU059180.D
Acq On : 07 Jun 2024 12:26
Operator : MD/SY
Sample : P2738-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
Data File : VU059180.D
Acq On : 07 Jun 2024 12:26
Operator : MD/SY
Sample : P2738-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------