

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
 Data File : VU059181.D
 Acq On : 07 Jun 2024 12:59
 Operator : MD/SY
 Sample : P2693-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHT1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

Signal : TIC: VU059181.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.357	18	21	28	rVB3	2603	2052	0.30%	0.036%
2	1.595	88	95	110	rVB	67600	79709	11.81%	1.404%
3	1.682	118	122	127	rBV2	2539	2431	0.36%	0.043%
4	1.759	138	146	161	rVB5	4333	8418	1.25%	0.148%
5	1.907	184	192	210	rVB	59091	81355	12.05%	1.433%
6	2.560	384	395	409	rBV	111179	183627	27.21%	3.234%
7	2.695	434	437	441	rBV	207	217	0.03%	0.004%
8	2.785	458	465	478	rVB2	1658	3122	0.46%	0.055%
9	2.878	489	494	498	rBV2	237	275	0.04%	0.005%
10	3.010	530	535	536	rBV	219	207	0.03%	0.004%
11	3.039	536	544	555	rVV3	3220	6246	0.93%	0.110%
12	3.171	578	585	587	rBV3	713	905	0.13%	0.016%
13	3.348	636	640	641	rBV	390	199	0.03%	0.004%
14	3.361	641	644	650	rVB3	549	512	0.08%	0.009%
15	3.470	675	678	684	rVB2	270	290	0.04%	0.005%
16	3.554	696	704	707	rBV2	309	380	0.06%	0.007%
17	3.679	739	743	746	rBV	289	232	0.03%	0.004%
18	3.791	772	778	782	rVB2	229	267	0.04%	0.005%
19	3.817	782	786	790	rBV2	286	304	0.05%	0.005%
20	4.161	888	893	896	rBV2	199	241	0.04%	0.004%
21	4.396	960	966	972	rBV2	120	212	0.03%	0.004%
22	4.496	994	997	1002	rVB	248	209	0.03%	0.004%
23	4.611	1023	1033	1074	rBV	83836	218213	32.33%	3.843%
24	4.959	1135	1141	1145	rBV3	364	484	0.07%	0.009%
25	5.055	1154	1171	1194	rBV2	130063	301888	44.73%	5.316%
26	5.193	1209	1214	1217	rVV3	334	401	0.06%	0.007%
27	5.293	1241	1245	1247	rBV2	442	364	0.05%	0.006%
28	5.354	1252	1264	1268	rBV2	475	676	0.10%	0.012%
29	5.434	1286	1289	1292	rVV2	259	196	0.03%	0.003%
30	5.553	1323	1326	1330	rBV2	222	234	0.03%	0.004%
31	5.717	1357	1377	1410	rBV2	242529	674872	100.00%	11.884%
32	5.936	1438	1445	1448	rBV2	374	362	0.05%	0.006%
33	6.177	1517	1520	1525	rBV2	185	210	0.03%	0.004%
34	6.245	1527	1541	1570	rBV	265577	519580	76.99%	9.150%
35	6.534	1619	1631	1643	rVB8	7896	16784	2.49%	0.296%
36	6.579	1643	1645	1647	rVB	495	224	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
 Data File : VU059181.D
 Acq On : 07 Jun 2024 12:59
 Operator : MD/SY
 Sample : P2693-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHT1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	6.595	1647	1650	1653	rBV	311	220	0.03%	0.004%
38	6.685	1664	1678	1701	rBV	165473	330333	48.95%	5.817%
39	6.807	1714	1716	1719	rBV2	554	346	0.05%	0.006%
40	6.846	1726	1728	1735	rVB2	312	308	0.05%	0.005%
41	6.885	1735	1740	1742	rBV2	278	221	0.03%	0.004%
42	7.068	1795	1797	1801	rVB	269	205	0.03%	0.004%
43	7.139	1813	1819	1829	rVB2	300	504	0.07%	0.009%
44	7.196	1829	1837	1843	rBV4	818	1306	0.19%	0.023%
45	7.306	1868	1871	1876	rVB2	304	310	0.05%	0.005%
46	7.563	1938	1951	1975	rBV	78631	145884	21.62%	2.569%
47	7.647	1975	1977	1980	rBV2	407	217	0.03%	0.004%
48	7.701	1991	1994	1999	rVB2	356	300	0.04%	0.005%
49	7.894	2040	2054	2071	rBV	265588	460256	68.20%	8.105%
50	8.177	2132	2142	2167	rVV2	53283	94965	14.07%	1.672%
51	8.470	2223	2233	2244	rVB3	2190	3931	0.58%	0.069%
52	8.557	2253	2260	2265	rVB4	1387	1724	0.26%	0.030%
53	8.627	2271	2282	2317	rBV3	195778	414165	61.37%	7.293%
54	8.762	2322	2324	2330	rVB5	1060	960	0.14%	0.017%
55	8.833	2343	2346	2350	rVB3	404	325	0.05%	0.006%
56	8.952	2379	2383	2386	rBV3	293	280	0.04%	0.005%
57	8.991	2392	2395	2400	rBV2	430	389	0.06%	0.007%
58	9.036	2407	2409	2416	rVB2	369	330	0.05%	0.006%
59	9.209	2460	2463	2472	rVV2	138	223	0.03%	0.004%
60	9.412	2514	2526	2553	rBV	387340	657511	97.43%	11.579%
61	9.569	2573	2575	2576	rBV	410	197	0.03%	0.003%
62	9.621	2587	2591	2595	rVB3	251	207	0.03%	0.004%
63	9.704	2611	2617	2625	rVB3	667	982	0.15%	0.017%
64	9.791	2641	2644	2648	rBV2	197	205	0.03%	0.004%
65	9.814	2648	2651	2657	rVB2	273	221	0.03%	0.004%
66	9.958	2691	2696	2697	rBV	242	203	0.03%	0.004%
67	10.161	2756	2759	2763	rVB2	246	190	0.03%	0.003%
68	10.206	2770	2773	2775	rVB	368	205	0.03%	0.004%
69	10.248	2775	2786	2789	rBV2	339	526	0.08%	0.009%
70	10.351	2814	2818	2820	rBV	347	271	0.04%	0.005%
71	10.749	2929	2942	2969	rVB	272619	439255	65.09%	7.735%
72	10.846	2969	2972	2975	rVV3	473	305	0.05%	0.005%
73	10.888	2976	2985	2997	rVB3	2995	4855	0.72%	0.085%
74	10.965	3004	3009	3013	rBV2	297	321	0.05%	0.006%
75	10.994	3015	3018	3024	rVB	379	388	0.06%	0.007%
76	11.036	3024	3031	3034	rBV2	251	356	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
 Data File : VU059181.D
 Acq On : 07 Jun 2024 12:59
 Operator : MD/SY
 Sample : P2693-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHT1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	11.084	3042	3046	3048	rBV2	475	330	0.05%	0.006%
78	11.122	3055	3058	3062	rBV	230	236	0.03%	0.004%
79	11.190	3072	3079	3081	rBV	385	477	0.07%	0.008%
80	11.476	3165	3168	3170	rBV2	376	228	0.03%	0.004%
81	11.749	3249	3253	3255	rBV3	755	574	0.09%	0.010%
82	11.807	3260	3271	3292	rBV	326722	554817	82.21%	9.770%
83	12.077	3353	3355	3360	rVB2	403	258	0.04%	0.005%
84	12.190	3377	3390	3413	rBV	252722	442652	65.59%	7.795%
85	12.370	3439	3446	3449	rBV2	351	432	0.06%	0.008%
86	12.482	3478	3481	3485	rBV2	324	266	0.04%	0.005%
87	12.691	3543	3546	3551	rVV2	249	261	0.04%	0.005%
88	12.736	3557	3560	3562	rBV	319	222	0.03%	0.004%
89	12.769	3562	3570	3579	rVV2	1415	2398	0.36%	0.042%
90	12.916	3612	3616	3618	rBV	402	244	0.04%	0.004%
91	13.309	3732	3738	3740	rBV2	375	420	0.06%	0.007%
92	13.855	3905	3908	3915	rVB4	931	1044	0.15%	0.018%
93	13.958	3937	3940	3943	rBV	355	194	0.03%	0.003%
94	14.003	3951	3954	3957	rBV3	298	225	0.03%	0.004%
95	14.113	3980	3988	3991	rBV2	1112	1362	0.20%	0.024%
96	14.334	4054	4057	4060	rBV2	672	583	0.09%	0.010%
97	14.514	4110	4113	4116	rBV	492	336	0.05%	0.006%
98	14.569	4127	4130	4134	rBV	482	458	0.07%	0.008%
99	14.756	4185	4188	4193	rBV	471	411	0.06%	0.007%
100	16.730	4800	4802	4804	rBV2	765	422	0.06%	0.007%




Sum of corrected areas: 5678648

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
Data File : VU059181.D
Acq On : 07 Jun 2024 12:59
Operator : MD/SY
Sample : P2693-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHT1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

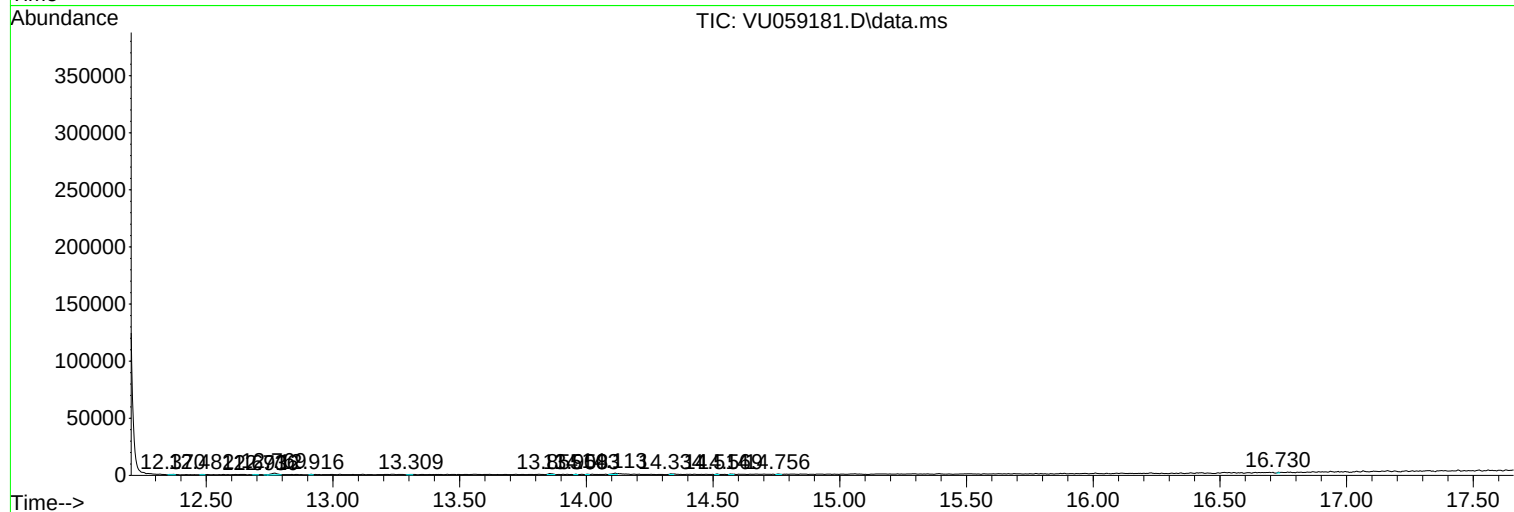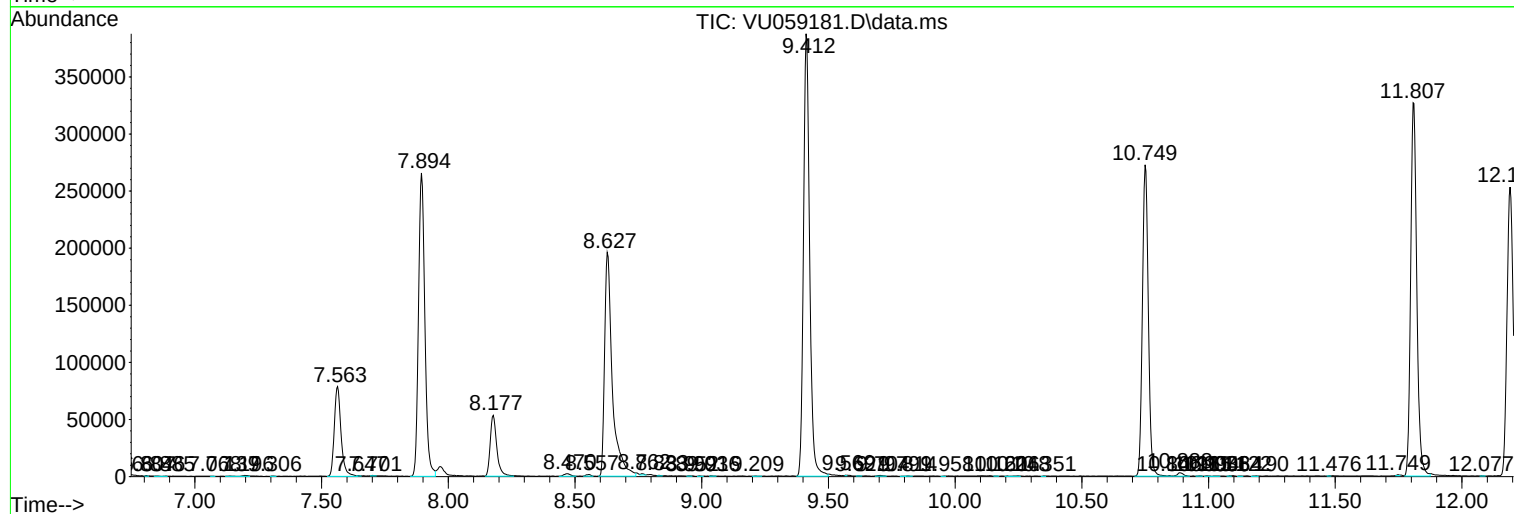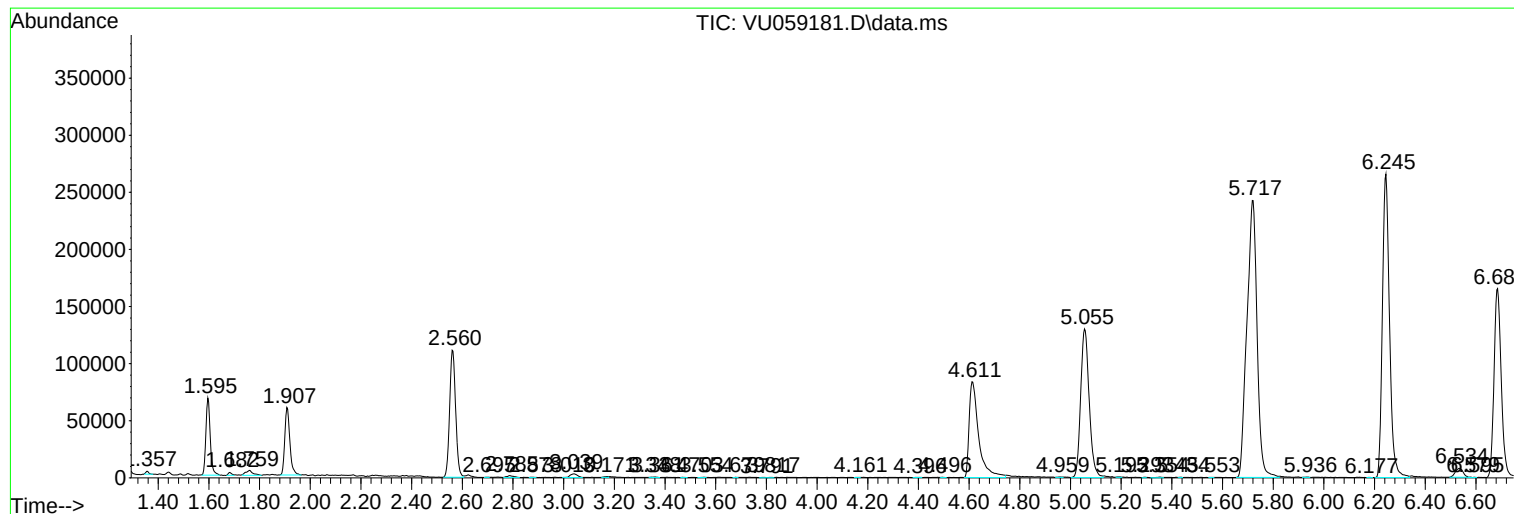

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
Data File : VU059181.D
Acq On : 07 Jun 2024 12:59
Operator : MD/SY
Sample : P2693-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHT1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
Data File : VU059181.D
Acq On : 07 Jun 2024 12:59
Operator : MD/SY
Sample : P2693-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHT1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc