

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
 Data File : VU059182.D
 Acq On : 07 Jun 2024 13:23
 Operator : MD/SY
 Sample : P2693-02 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHT2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

Signal : TIC: VU059182.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	88	95	111	rVB	56766	67192	10.12%	1.253%
2	1.907	184	192	209	rVB	52948	71351	10.75%	1.331%
3	2.193	279	281	284	rBV2	533	332	0.05%	0.006%
4	2.476	365	369	370	rBV2	413	288	0.04%	0.005%
5	2.560	384	395	416	rBV	100369	164788	24.82%	3.074%
6	2.759	454	457	459	rVV3	316	259	0.04%	0.005%
7	2.785	459	465	476	rVB2	1171	1926	0.29%	0.036%
8	3.039	536	544	557	rBV4	2963	5777	0.87%	0.108%
9	3.447	666	671	675	rBV	257	301	0.05%	0.006%
10	3.801	773	781	787	rVB2	384	591	0.09%	0.011%
11	3.830	787	790	793	rBV2	273	277	0.04%	0.005%
12	4.296	930	935	941	rVB2	323	417	0.06%	0.008%
13	4.341	941	949	958	rVB2	366	685	0.10%	0.013%
14	4.611	1022	1033	1070	rBV	79686	206014	31.03%	3.843%
15	4.984	1144	1149	1152	rBV2	287	278	0.04%	0.005%
16	5.055	1155	1171	1192	rBV2	115892	262139	39.49%	4.889%
17	5.209	1215	1219	1222	rBV2	368	301	0.05%	0.006%
18	5.647	1351	1355	1358	rBV	333	242	0.04%	0.005%
19	5.717	1358	1377	1409	rVV2	216562	609277	91.78%	11.364%
20	5.840	1413	1415	1418	rVB2	573	347	0.05%	0.006%
21	5.904	1433	1435	1441	rVB	402	314	0.05%	0.006%
22	6.007	1463	1467	1471	rBV3	384	300	0.05%	0.006%
23	6.171	1513	1518	1520	rBV2	266	277	0.04%	0.005%
24	6.242	1528	1540	1571	rBV	264246	515637	77.68%	9.618%
25	6.373	1579	1581	1583	rBV2	378	242	0.04%	0.005%
26	6.528	1620	1629	1644	rVB6	6382	13318	2.01%	0.248%
27	6.589	1644	1648	1653	rVB2	226	256	0.04%	0.005%
28	6.621	1653	1658	1659	rBV	380	317	0.05%	0.006%
29	6.685	1665	1678	1698	rBV	150029	298195	44.92%	5.562%
30	6.830	1719	1723	1726	rVB3	687	555	0.08%	0.010%
31	6.856	1726	1731	1734	rBV2	247	298	0.04%	0.006%
32	7.206	1831	1840	1844	rBV4	751	1124	0.17%	0.021%
33	7.306	1865	1871	1873	rBV2	260	316	0.05%	0.006%
34	7.467	1918	1921	1928	rVB	234	249	0.04%	0.005%
35	7.560	1936	1950	1970	rBV	70427	128298	19.33%	2.393%
36	7.679	1984	1987	1991	rBV2	499	366	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
 Data File : VU059182.D
 Acq On : 07 Jun 2024 13:23
 Operator : MD/SY
 Sample : P2693-02 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHT2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	7.717	1996	1999	2008	rVB3	682	864	0.13%	0.016%
38	7.791	2018	2022	2026	rBV2	264	239	0.04%	0.004%
39	7.894	2041	2054	2077	rBV	232222	415744	62.63%	7.755%
40	8.052	2099	2103	2106	rBV2	348	324	0.05%	0.006%
41	8.177	2132	2142	2159	rBV2	47923	84733	12.76%	1.580%
42	8.544	2251	2256	2262	rBV4	510	529	0.08%	0.010%
43	8.627	2271	2282	2316	rBV2	184868	397569	59.89%	7.416%
44	9.315	2493	2496	2498	rBV	339	272	0.04%	0.005%
45	9.412	2513	2526	2553	rBV	391390	663829	100.00%	12.382%
46	9.701	2613	2616	2622	rVB2	743	719	0.11%	0.013%
47	10.142	2748	2753	2759	rVB2	503	606	0.09%	0.011%
48	10.180	2759	2765	2767	rBV	281	291	0.04%	0.005%
49	10.290	2794	2799	2802	rBV2	296	266	0.04%	0.005%
50	10.483	2855	2859	2864	rBV2	547	496	0.07%	0.009%
51	10.653	2909	2912	2920	rVB2	196	262	0.04%	0.005%
52	10.749	2930	2942	2969	rVV	244450	399652	60.20%	7.454%
53	10.875	2975	2981	2983	rBV2	302	374	0.06%	0.007%
54	11.039	3028	3032	3036	rVV2	265	262	0.04%	0.005%
55	11.064	3036	3040	3044	rVV2	376	293	0.04%	0.005%
56	11.595	3198	3205	3211	rBV2	300	550	0.08%	0.010%
57	11.634	3212	3217	3218	rVV3	728	692	0.10%	0.013%
58	11.643	3218	3220	3229	rVB2	926	842	0.13%	0.016%
59	11.753	3247	3254	3259	rBV4	957	1070	0.16%	0.020%
60	11.807	3259	3271	3294	rBV	337844	568173	85.59%	10.598%
61	12.097	3353	3361	3368	rBV4	1411	1858	0.28%	0.035%
62	12.190	3377	3390	3410	rBV	242157	414530	62.45%	7.732%
63	12.309	3425	3427	3435	rVB4	791	866	0.13%	0.016%
64	12.344	3435	3438	3443	rVB2	411	306	0.05%	0.006%
65	12.572	3504	3509	3518	rVB3	617	973	0.15%	0.018%
66	12.682	3538	3543	3549	rBV4	1293	1415	0.21%	0.026%
67	12.765	3566	3569	3579	rVB2	610	662	0.10%	0.012%
68	12.820	3581	3586	3588	rBV2	726	558	0.08%	0.010%
69	12.833	3588	3590	3595	rVV3	393	273	0.04%	0.005%
70	12.978	3628	3635	3645	rVB4	1021	1791	0.27%	0.033%
71	13.293	3730	3733	3736	rBV3	373	254	0.04%	0.005%
72	13.453	3777	3783	3792	rVB6	2838	4024	0.61%	0.075%
73	13.524	3801	3805	3808	rBV2	474	361	0.05%	0.007%
74	13.736	3869	3871	3875	rVB	445	266	0.04%	0.005%
75	13.778	3879	3884	3885	rBV	737	535	0.08%	0.010%
76	13.785	3885	3886	3891	rVB2	1073	655	0.10%	0.012%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
 Data File : VU059182.D
 Acq On : 07 Jun 2024 13:23
 Operator : MD/SY
 Sample : P2693-02 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHT2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	13.833	3895	3901	3902	rBV4	1413	1023	0.15%	0.019%
78	14.000	3947	3953	3957	rBV4	647	608	0.09%	0.011%
79	14.048	3960	3968	3970	rBV3	944	1152	0.17%	0.021%
80	14.116	3978	3989	3994	rBV4	1968	3480	0.52%	0.065%
81	14.187	4005	4011	4018	rVB7	4060	5639	0.85%	0.105%
82	14.286	4032	4042	4049	rBV10	2251	4092	0.62%	0.076%
83	14.341	4053	4059	4061	rVV5	1038	1035	0.16%	0.019%
84	14.447	4090	4092	4094	rBV2	484	348	0.05%	0.006%
85	14.518	4112	4114	4116	rBV2	524	280	0.04%	0.005%
86	14.566	4125	4129	4133	rBV6	784	813	0.12%	0.015%
87	14.662	4152	4159	4170	rBV6	2173	3612	0.54%	0.067%
88	14.807	4197	4204	4207	rBV4	940	1059	0.16%	0.020%
89	14.868	4218	4223	4224	rBV3	1609	1146	0.17%	0.021%
90	15.013	4263	4268	4270	rBV4	1488	1478	0.22%	0.028%
91	15.074	4283	4287	4291	rBV4	827	806	0.12%	0.015%
92	15.206	4320	4328	4335	rBV6	4049	6149	0.93%	0.115%
93	15.254	4341	4343	4344	rBV	1039	470	0.07%	0.009%
94	15.421	4391	4395	4401	rVB5	2177	2069	0.31%	0.039%
95	15.646	4461	4465	4468	rBV3	914	651	0.10%	0.012%
96	15.920	4547	4550	4556	rBV7	1342	1342	0.20%	0.025%
97	15.968	4562	4565	4569	rBV4	1427	1230	0.19%	0.023%
98	16.035	4584	4586	4591	rBV6	819	520	0.08%	0.010%
99	16.186	4630	4633	4636	rBV4	829	666	0.10%	0.012%
100	16.482	4723	4725	4729	rVB4	1267	828	0.12%	0.015%




Sum of corrected areas: 5361318

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
Data File : VU059182.D
Acq On : 07 Jun 2024 13:23
Operator : MD/SY
Sample : P2693-02 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

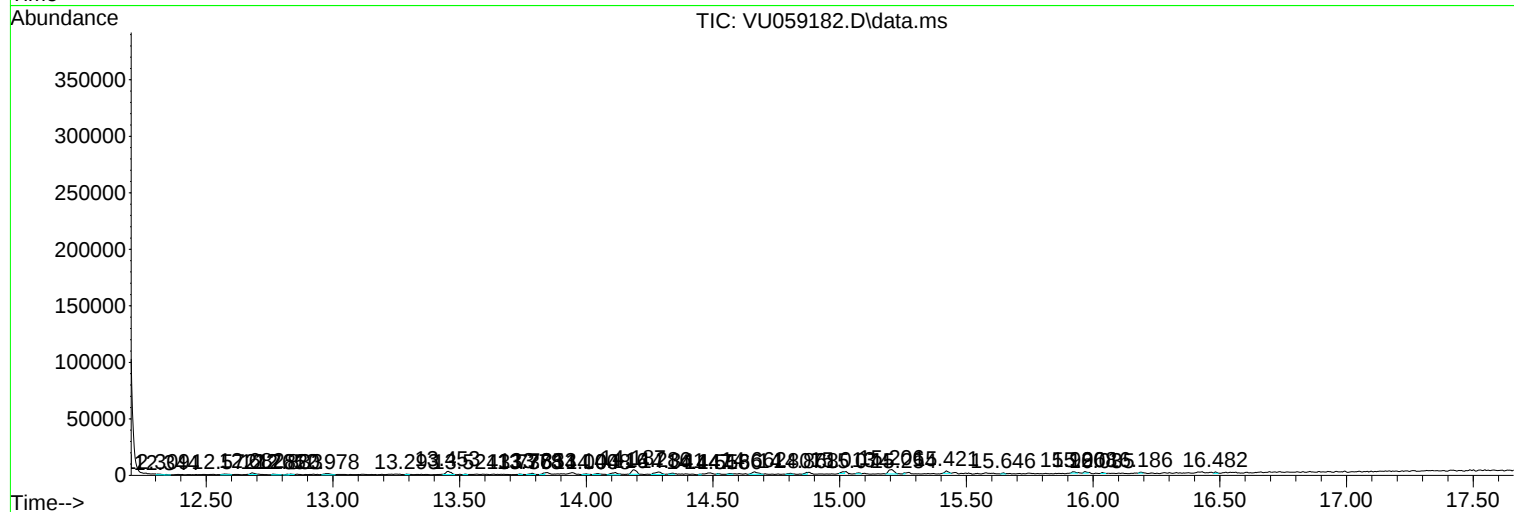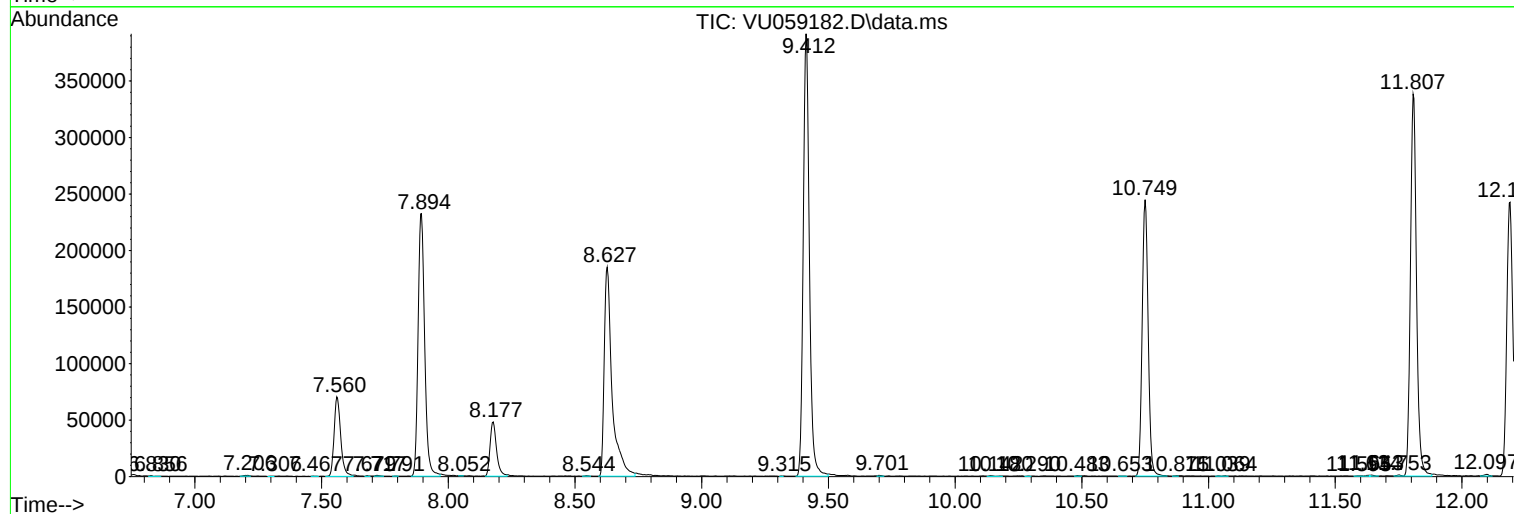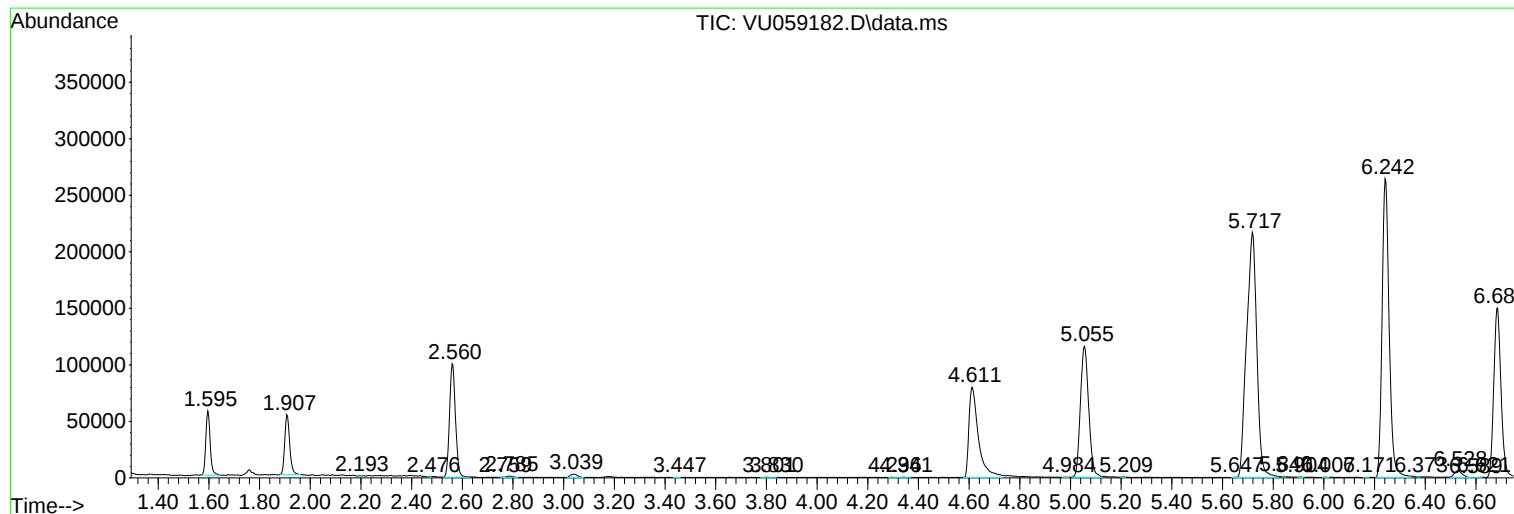

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
Data File : VU059182.D
Acq On : 07 Jun 2024 13:23
Operator : MD/SY
Sample : P2693-02 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
Data File : VU059182.D
Acq On : 07 Jun 2024 13:23
Operator : MD/SY
Sample : P2693-02 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------