

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
 Data File : VU059185.D
 Acq On : 07 Jun 2024 14:31
 Operator : MD/SY
 Sample : P2695-24
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

Signal : TIC: VU059185.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	111	rBV	100294	116716	15.68%	2.005%
2	1.907	184	192	211	rBV	81339	112299	15.09%	1.929%
3	2.560	382	395	414	rBV	152707	249075	33.47%	4.280%
4	2.785	459	465	473	rBV2	785	1174	0.16%	0.020%
5	2.891	494	498	503	rBV2	151	191	0.03%	0.003%
6	2.943	509	514	520	rVB	295	386	0.05%	0.007%
7	3.039	535	544	555	rVB3	3241	5929	0.80%	0.102%
8	3.174	580	586	589	rBV3	486	552	0.07%	0.009%
9	3.451	665	672	674	rBV2	204	224	0.03%	0.004%
10	3.489	679	684	688	rBV	258	274	0.04%	0.005%
11	3.676	737	742	745	rBV2	185	185	0.02%	0.003%
12	3.702	745	750	752	rVV2	201	215	0.03%	0.004%
13	3.714	752	754	759	rVB	225	166	0.02%	0.003%
14	3.808	780	783	789	rVB2	234	317	0.04%	0.005%
15	3.840	789	793	795	rBV2	244	238	0.03%	0.004%
16	3.939	820	824	832	rVB2	329	479	0.06%	0.008%
17	3.985	832	838	845	rBV2	265	370	0.05%	0.006%
18	4.177	894	898	900	rBV2	289	185	0.02%	0.003%
19	4.258	920	923	925	rBV2	243	190	0.03%	0.003%
20	4.615	1023	1034	1078	rBV	66287	177434	23.84%	3.049%
21	4.943	1133	1136	1139	rVB2	335	230	0.03%	0.004%
22	5.055	1155	1171	1190	rBV	131545	291209	39.13%	5.003%
23	5.181	1207	1210	1213	rBV2	443	354	0.05%	0.006%
24	5.296	1243	1246	1250	rBV2	227	206	0.03%	0.004%
25	5.361	1262	1266	1268	rBV	318	284	0.04%	0.005%
26	5.390	1272	1275	1278	rBV	249	166	0.02%	0.003%
27	5.473	1298	1301	1304	rBV2	253	156	0.02%	0.003%
28	5.525	1311	1317	1325	rVB2	306	498	0.07%	0.009%
29	5.566	1325	1330	1333	rBV2	250	288	0.04%	0.005%
30	5.718	1357	1377	1410	rBV2	273223	744126	100.00%	12.785%
31	6.007	1464	1467	1469	rBV3	233	172	0.02%	0.003%
32	6.107	1495	1498	1502	rBV2	258	267	0.04%	0.005%
33	6.161	1508	1515	1517	rBV	215	219	0.03%	0.004%
34	6.242	1527	1540	1562	rBV	263009	513173	68.96%	8.817%
35	6.431	1596	1599	1604	rBV3	355	289	0.04%	0.005%
36	6.467	1607	1610	1612	rBV	281	161	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
 Data File : VU059185.D
 Acq On : 07 Jun 2024 14:31
 Operator : MD/SY
 Sample : P2695-24
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

37	6.525	1621	1628	1630	rBV3	4460	5135	0.69%	0.088%
38	6.605	1650	1653	1656	rVB	388	256	0.03%	0.004%
39	6.682	1664	1677	1701	rBV	171664	336840	45.27%	5.788%
40	6.811	1713	1717	1720	rVB3	544	380	0.05%	0.007%
41	6.869	1731	1735	1739	rVB	430	329	0.04%	0.006%
42	6.898	1739	1744	1745	rBV	428	322	0.04%	0.006%
43	7.013	1775	1780	1782	rVB2	182	181	0.02%	0.003%
44	7.142	1817	1820	1825	rVB2	245	192	0.03%	0.003%
45	7.203	1831	1839	1851	rBV3	1169	2222	0.30%	0.038%
46	7.335	1874	1880	1884	rBV2	173	230	0.03%	0.004%
47	7.393	1894	1898	1903	rBV2	263	348	0.05%	0.006%
48	7.463	1917	1920	1924	rBV	162	160	0.02%	0.003%
49	7.502	1928	1932	1935	rBV	281	246	0.03%	0.004%
50	7.560	1939	1950	1968	rBV	81237	148936	20.01%	2.559%
51	7.701	1989	1994	1995	rBV3	753	607	0.08%	0.010%
52	7.785	2013	2020	2022	rBV2	245	336	0.05%	0.006%
53	7.891	2041	2053	2076	rBV	310603	553857	74.43%	9.516%
54	8.123	2122	2125	2127	rBV2	177	157	0.02%	0.003%
55	8.174	2131	2141	2160	rVV	55064	97677	13.13%	1.678%
56	8.312	2178	2184	2189	rBV2	402	516	0.07%	0.009%
57	8.544	2253	2256	2261	rVB3	507	442	0.06%	0.008%
58	8.586	2261	2269	2271	rBV	234	338	0.05%	0.006%
59	8.627	2271	2282	2321	rBV2	162194	350274	47.07%	6.018%
60	8.897	2364	2366	2372	rVB2	316	301	0.04%	0.005%
61	8.968	2385	2388	2390	rBV2	240	171	0.02%	0.003%
62	9.412	2514	2526	2557	rBV	382208	657413	88.35%	11.296%
63	9.573	2574	2576	2579	rVB3	607	289	0.04%	0.005%
64	9.705	2614	2617	2623	rVB2	333	314	0.04%	0.005%
65	10.032	2713	2719	2723	rVB2	350	446	0.06%	0.008%
66	10.061	2723	2728	2730	rBV2	286	267	0.04%	0.005%
67	10.097	2736	2739	2740	rBV	289	151	0.02%	0.003%
68	10.483	2856	2859	2862	rBV3	218	175	0.02%	0.003%
69	10.569	2883	2886	2891	rBV2	278	240	0.03%	0.004%
70	10.750	2925	2942	2966	rBV	227615	374065	50.27%	6.427%
71	10.888	2981	2985	2995	rVB3	1150	1193	0.16%	0.020%
72	10.946	2999	3003	3007	rBV2	334	350	0.05%	0.006%
73	10.975	3007	3012	3014	rBV	229	196	0.03%	0.003%
74	11.081	3041	3045	3048	rBV2	282	212	0.03%	0.004%
75	11.100	3048	3051	3056	rVB3	336	291	0.04%	0.005%
76	11.142	3060	3064	3066	rBV2	333	256	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
 Data File : VU059185.D
 Acq On : 07 Jun 2024 14:31
 Operator : MD/SY
 Sample : P2695-24
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
 Title : VOC Analysis

77	11.357	3127	3131	3137	rBV	371	314	0.04%	0.005%
78	11.505	3172	3177	3179	rBV	319	278	0.04%	0.005%
79	11.746	3248	3252	3259	rVB3	722	694	0.09%	0.012%
80	11.807	3259	3271	3293	rBV	350027	579470	77.87%	9.956%
81	11.987	3324	3327	3329	rBV2	266	169	0.02%	0.003%
82	12.097	3356	3361	3368	rVB3	510	770	0.10%	0.013%
83	12.145	3373	3376	3377	rBV	317	176	0.02%	0.003%
84	12.190	3377	3390	3407	rBV	274241	458328	61.59%	7.875%
85	12.354	3439	3441	3443	rBV2	313	157	0.02%	0.003%
86	12.425	3459	3463	3465	rBV2	344	251	0.03%	0.004%
87	12.534	3494	3497	3500	rBV3	497	378	0.05%	0.006%
88	12.685	3541	3544	3547	rVB2	320	199	0.03%	0.003%
89	12.756	3563	3566	3567	rBV	334	204	0.03%	0.004%
90	13.000	3639	3642	3645	rBV2	311	261	0.04%	0.004%
91	13.315	3737	3740	3745	rBV	302	371	0.05%	0.006%
92	13.463	3784	3786	3789	rBV2	265	196	0.03%	0.003%
93	13.904	3921	3923	3927	rBV2	292	207	0.03%	0.004%
94	14.820	4206	4208	4213	rBV3	508	449	0.06%	0.008%
95	15.010	4263	4267	4270	rBV3	603	569	0.08%	0.010%
96	15.267	4343	4347	4353	rBV4	669	817	0.11%	0.014%
97	15.415	4386	4393	4403	rBV4	3166	5263	0.71%	0.090%
98	16.125	4612	4614	4616	rBV2	631	358	0.05%	0.006%
99	16.412	4694	4703	4710	rBV5	6894	10892	1.46%	0.187%
100	16.447	4711	4714	4723	rVB6	3366	4632	0.62%	0.080%




Sum of corrected areas: 5820111

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
Data File : VU059185.D
Acq On : 07 Jun 2024 14:31
Operator : MD/SY
Sample : P2695-24
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

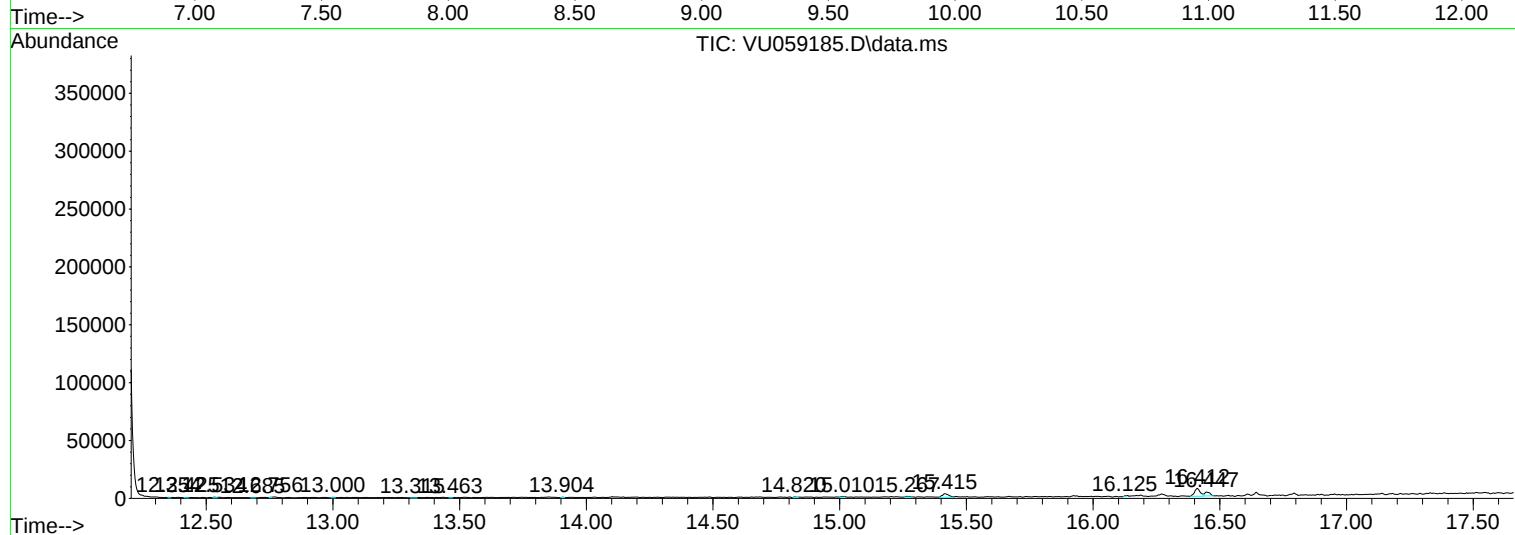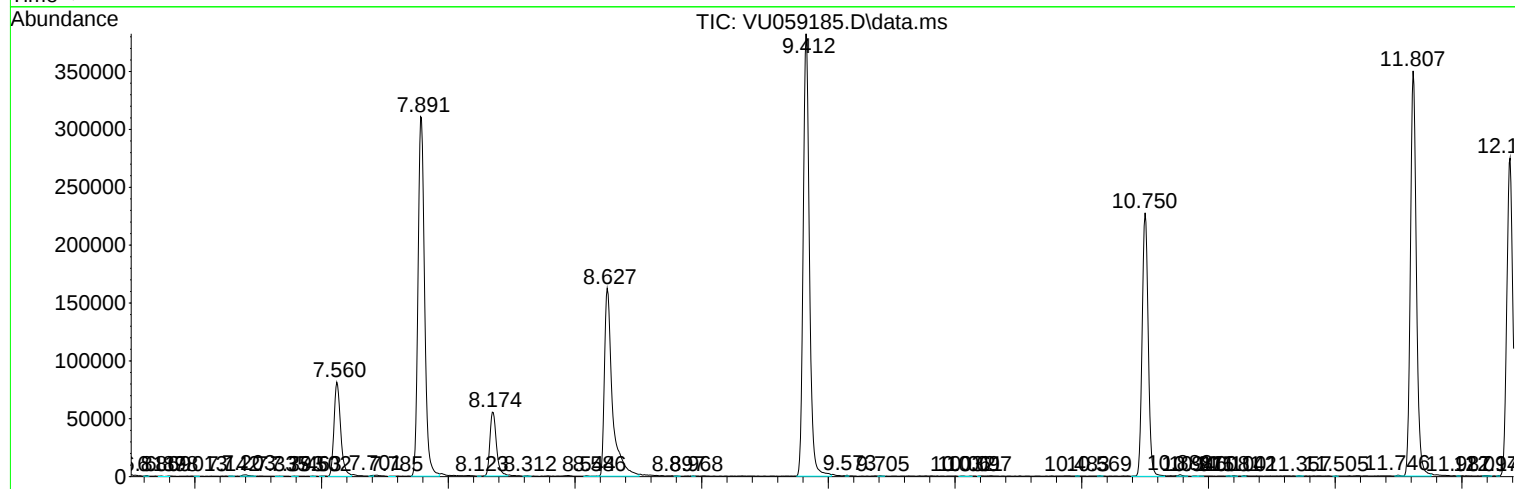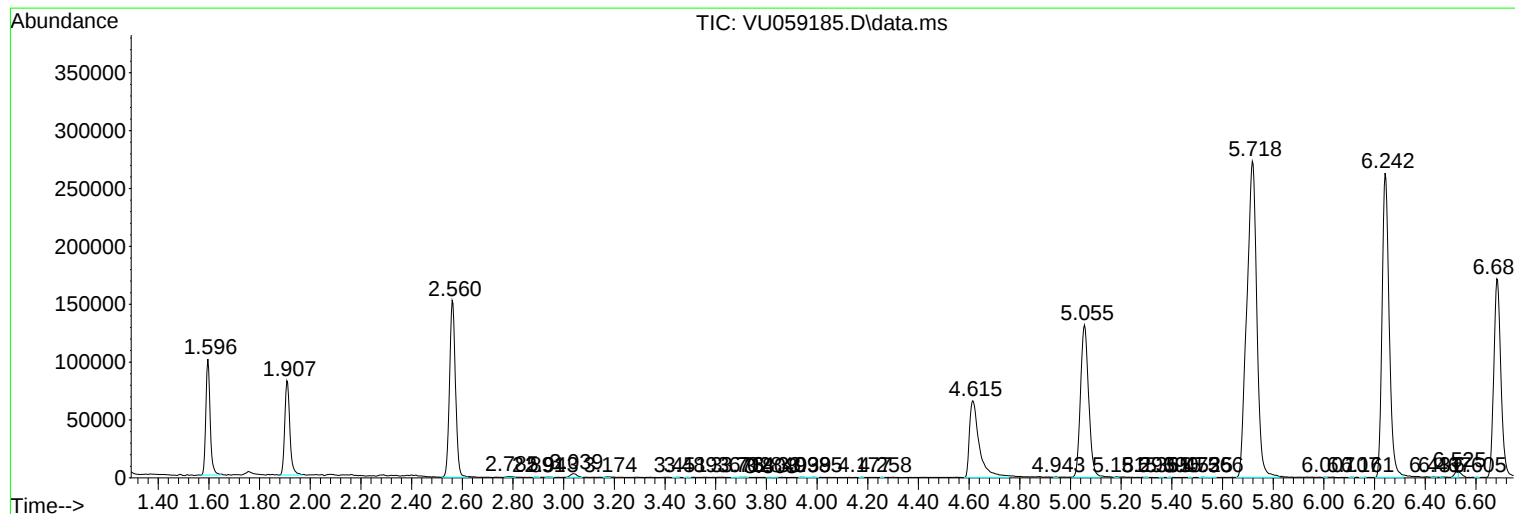

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
Data File : VU059185.D
Acq On : 07 Jun 2024 14:31
Operator : MD/SY
Sample : P2695-24
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
Data File : VU059185.D
Acq On : 07 Jun 2024 14:31
Operator : MD/SY
Sample : P2695-24
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------