


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060724\
Data File : VU059176.D
Acq On : 07 Jun 2024 09:18
Operator : MD/SY
Sample : BFB061
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB061

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052924WMA.M
Title : VOC Analysis
Last Update : Sat Jun 08 01:56:01 2024

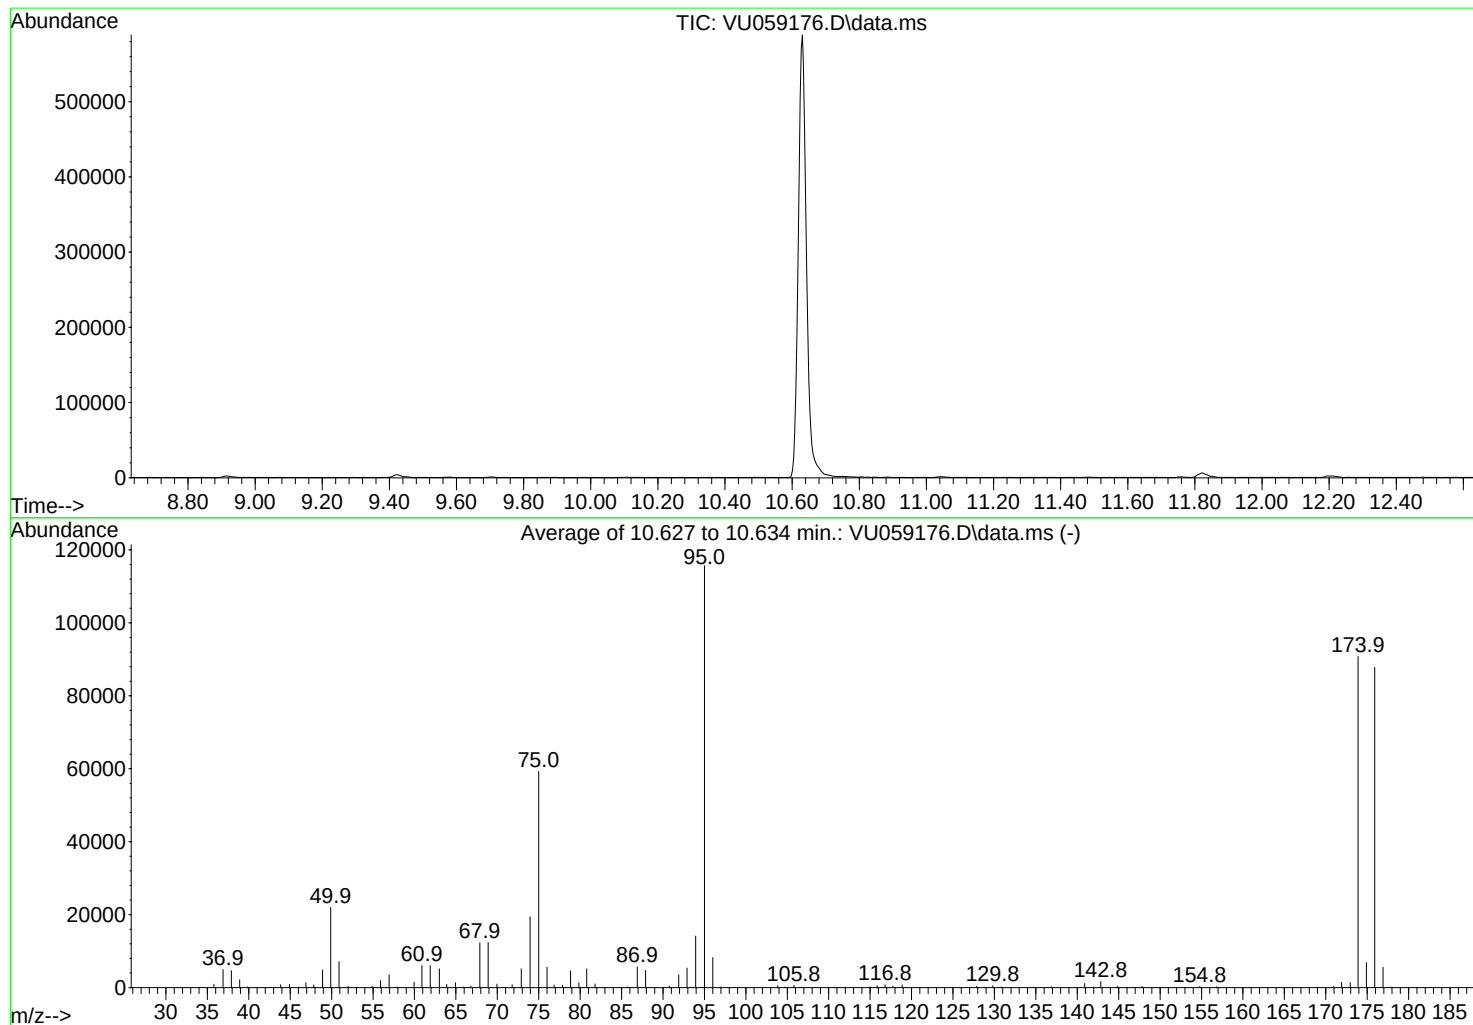

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.0	21955	PASS
75	95	30	80	51.2	59240	PASS
95	95	100	100	100.0	115664	PASS
96	95	5	9	7.1	8243	PASS
173	174	0.00	2	1.5	1370	PASS
174	95	50	120	78.5	90792	PASS
175	174	5	9	7.5	6844	PASS
176	174	95	101	96.7	87784	PASS
177	176	5	9	6.3	5562	PASS

m/z	Abundance
43.80	299.0

Instrument :
MSVOA_U
ClientSampleId :
BFB061

m/z	Abundance
35.80	960.0
36.90	5099.0
37.90	4662.0
38.90	2060.0
39.90	219.0
43.90	964.0
44.90	839.0
45.90	135.0
46.90	1355.0
47.80	751.0
48.90	4715.0
49.90	22376.0
50.90	7218.0
52.00	323.0
53.10	116.0
54.90	403.0
55.90	1962.0
57.00	3505.0
58.00	206.0
59.90	1470.0
60.90	6068.0
61.90	6296.0
63.00	5550.0
63.90	946.0
65.00	1332.0
65.90	152.0
66.80	382.0
67.90	12500.0
68.90	12389.0
69.90	998.0
71.80	845.0
72.90	5127.0
74.00	19440.0
75.00	60376.0
76.00	5617.0
76.80	727.0
77.90	666.0
78.80	4644.0
79.80	1330.0
80.80	5387.0
81.80	1088.0
82.90	124.0
85.80	209.0
86.90	5975.0
87.90	4656.0
90.70	430.0
91.90	3552.0
92.90	5475.0
93.90	14589.0
95.00	115736.0
96.00	8246.0
96.90	207.0
103.80	516.0
104.70	185.0
105.80	534.0
106.70	167.0
110.70	199.0
112.00	143.0
114.90	141.0
115.90	483.0
116.80	774.0
117.80	349.0
118.90	650.0
127.80	310.0
128.80	123.0
129.80	515.0
130.80	173.0
134.70	167.0
136.90	230.0
140.90	1152.0
141.90	186.0
142.80	1629.0
144.80	418.0
145.90	104.0
146.80	130.0
147.80	289.0
154.80	257.0
156.80	216.0
170.90	319.0
171.90	1312.0
172.90	1383.0
173.90	88944.0
174.90	6712.0
175.90	86472.0
176.90	5459.0
177.90	142.0

Instrument :
MSVOA_U
ClientSampleId :
BFB061

m/z	Abundance
35.80	958.0
36.90	5147.0
37.90	4763.0
38.90	2225.0
39.90	203.0
43.90	1092.0
44.90	866.0
46.00	146.0
46.90	1380.0
47.90	741.0
48.90	4999.0
49.90	22448.0
50.90	7348.0
52.00	348.0
53.10	121.0
54.90	419.0
55.90	1985.0
56.90	3666.0
57.90	163.0
60.00	1476.0
60.90	6217.0
61.90	6212.0
63.00	5205.0
63.90	886.0
64.90	1361.0
65.90	167.0
66.80	360.0
67.90	12681.0
68.90	12705.0
69.90	1032.0
71.80	807.0
72.90	5293.0
73.90	19920.0
75.00	61312.0
76.00	5757.0
76.80	757.0
77.90	728.0
78.80	4679.0
79.80	1429.0
80.80	5251.0
81.80	957.0
82.90	125.0
85.70	208.0
86.90	5792.0
87.90	4862.0
90.70	418.0
91.90	3571.0
92.90	5531.0
94.00	14424.0
95.00	119640.0
96.00	8676.0
96.90	224.0
103.80	550.0
104.70	179.0
105.80	592.0
106.70	200.0
110.70	153.0
112.00	175.0
114.90	147.0
115.90	506.0
116.80	835.0
117.80	365.0
118.80	735.0
127.90	318.0
128.70	144.0
129.80	534.0
130.90	158.0
134.70	177.0
136.80	231.0
140.90	1106.0
142.00	172.0
142.90	1680.0
144.90	425.0
145.90	125.0
147.80	351.0
154.80	285.0
156.80	227.0
158.80	104.0
160.70	118.0
170.90	314.0
171.90	1459.0
172.90	1361.0
173.90	93560.0
174.90	7068.0
175.90	90904.0
176.90	5765.0
177.90	140.0

Instrument :
MSVOA_U
ClientSampleId :
BFB061

m/z	Abundance
35.80	825.0
36.90	4613.0
37.90	4436.0
38.90	2090.0
39.80	191.0
43.90	1120.0
44.90	923.0
46.10	190.0
46.90	1351.0
47.90	670.0
48.90	4723.0
49.90	21040.0
50.90	6876.0
52.00	325.0
53.00	133.0
54.90	376.0
55.90	1744.0
56.90	3416.0
57.80	115.0
59.90	1334.0
60.90	5829.0
61.90	5649.0
63.00	4596.0
63.90	770.0
64.90	1189.0
65.90	136.0
66.80	326.0
67.90	11663.0
68.90	11906.0
70.00	861.0
71.80	713.0
72.90	5048.0
73.90	18856.0
75.00	56032.0
76.00	5272.0
76.90	679.0
77.80	667.0
78.90	4470.0
79.90	1286.0
80.80	4684.0
81.80	859.0
82.80	105.0
85.70	204.0
86.90	5324.0
87.90	4577.0
90.80	409.0
91.90	3323.0
92.90	5005.0
94.00	13373.0
95.00	111616.0
96.00	7807.0
96.90	181.0
103.90	550.0
104.70	149.0
105.80	638.0
106.70	162.0
110.70	110.0
112.00	158.0
114.90	125.0
115.80	502.0
116.80	755.0
117.70	370.0
118.80	741.0
127.90	351.0
128.80	151.0
129.80	470.0
130.90	138.0
134.80	185.0
136.80	210.0
140.90	1054.0
141.90	133.0
142.90	1646.0
144.90	421.0
145.90	131.0
147.80	347.0
149.60	101.0
154.80	267.0
156.80	203.0
160.80	150.0
170.90	254.0
171.90	1534.0
173.00	1367.0
173.90	89872.0
174.90	6753.0
175.90	85976.0
176.90	5461.0
177.80	138.0

Instrument :
MSVOA_U
ClientSampleId :
BFB061