

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060819\
 Data File : VU032545.D
 Acq On : 08 Jun 2019 16:12
 Operator : JC/SP
 Sample : K3276-15
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB8F1

Quant Time: Jun 08 23:39:49 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 08 23:12:44 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	208502	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.08	117	192055	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	99822	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	73644	54.44	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	108.88%
7) Chloroethane-d5	1.68	69	57773	53.15	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	106.30%
11) 1,1-Dichloroethene-d2	2.27	63	106948	40.38	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.76%
21) 2-Butanone-d5	4.17	46	120906	106.80	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	106.80%
24) Chloroform-d	4.64	84	126989	50.33	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.66%
26) 1,2-Dichloroethane-d4	5.30	65	84110	52.92	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	105.84%
32) Benzene-d6	5.33	84	269961	54.14	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	108.28%
36) 1,2-Dichloropropane-d6	6.32	67	84330	53.94	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	107.88%
41) Toluene-d8	7.56	98	253831	53.69	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	107.38%
43) trans-1,3-Dichloropropene-	7.85	79	40231	53.77	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	107.54%
47) 2-Hexanone-d5	8.31	63	79727	105.13	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	105.13%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	114331	50.47	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	100.94%
64) 1,2-Dichlorobenzene-d4	11.85	152	103239	54.00	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	108.00%


Target Compounds					Ovalue
13) Acetone	2.32	43	5034	4.310 ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU060819\
Data File : VU032545.D
Acq On : 08 Jun 2019 16:12
Operator : JC/SP
Sample : K3276-15
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB8F1

Quant Time: Jun 08 23:39:49 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Jun 08 23:12:44 2019
Response via : Initial Calibration

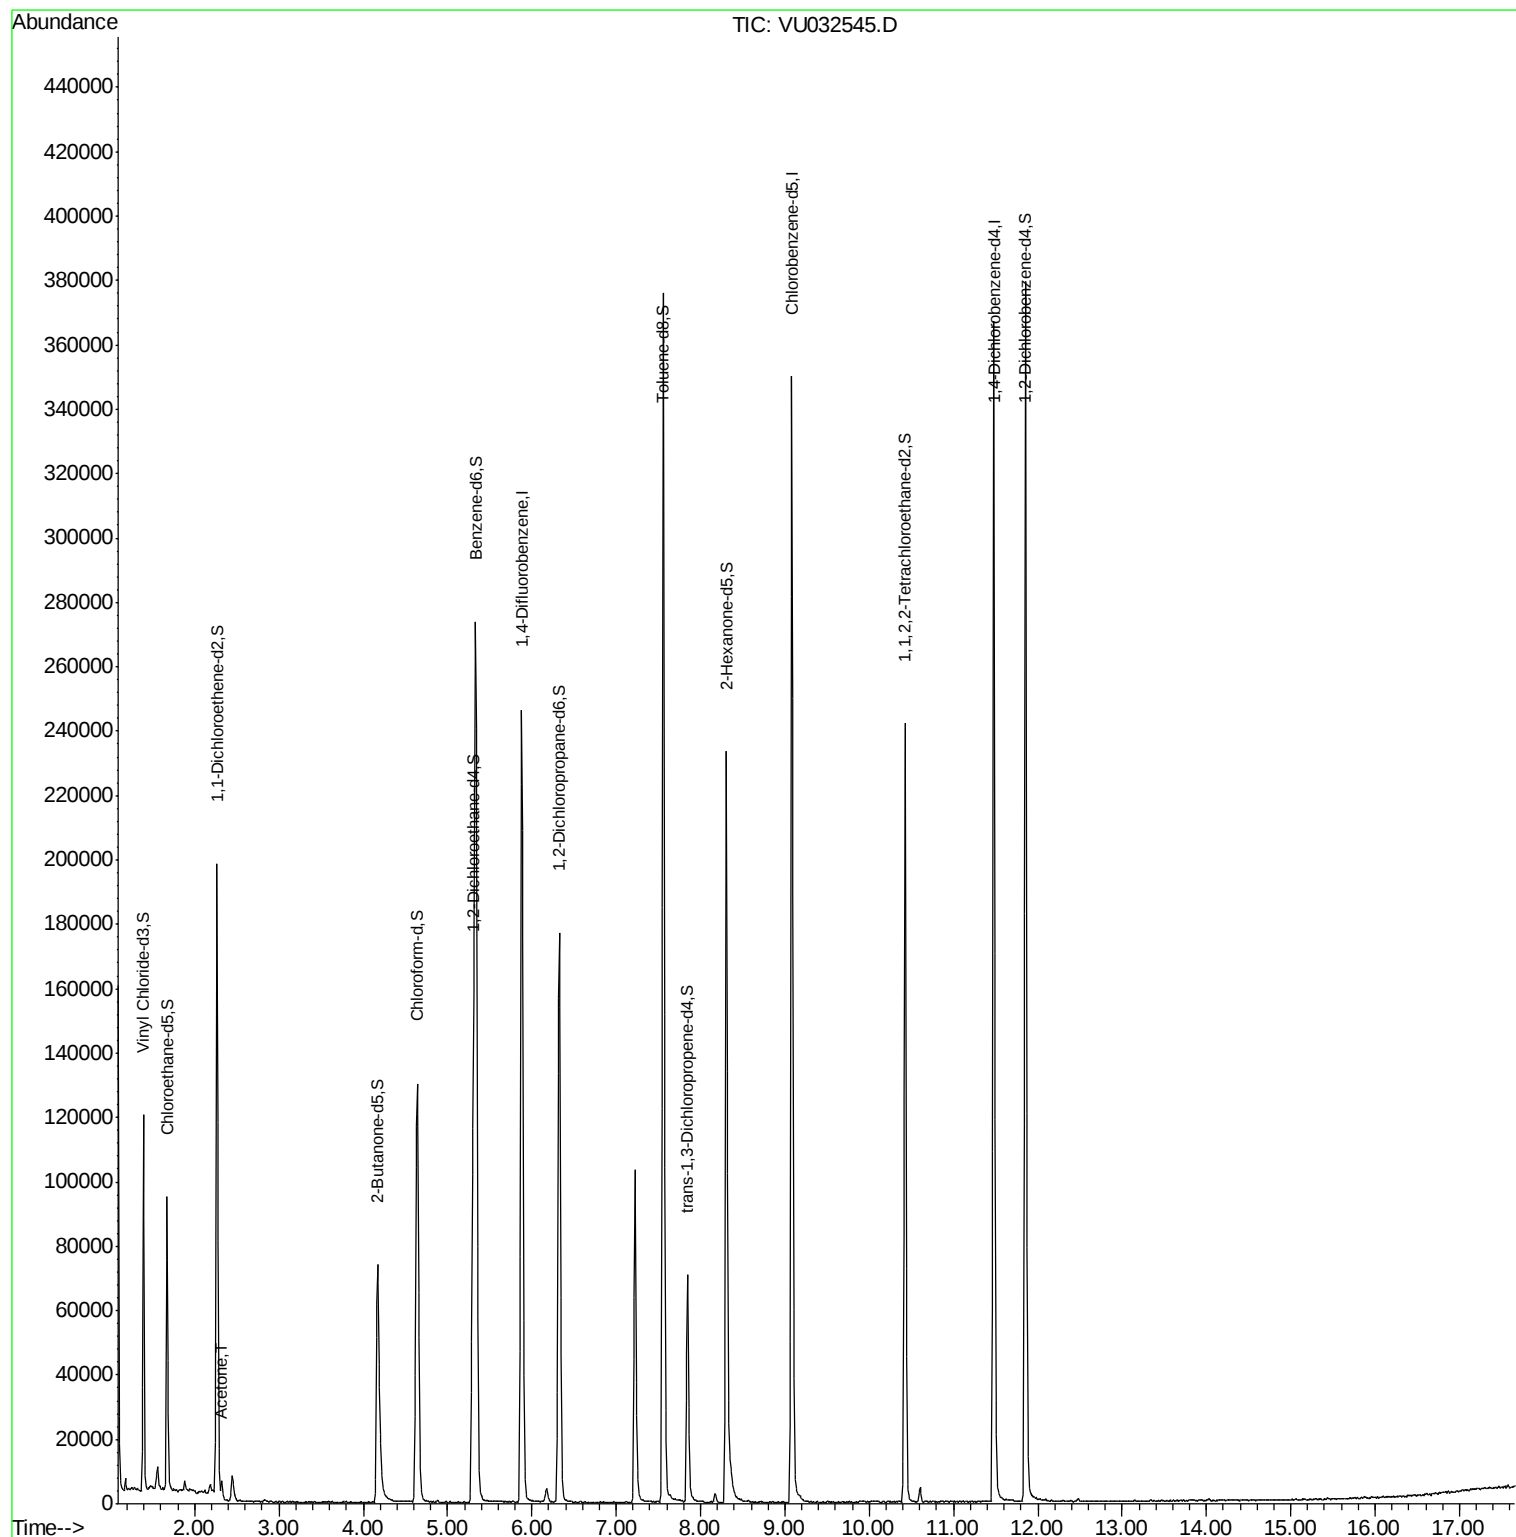

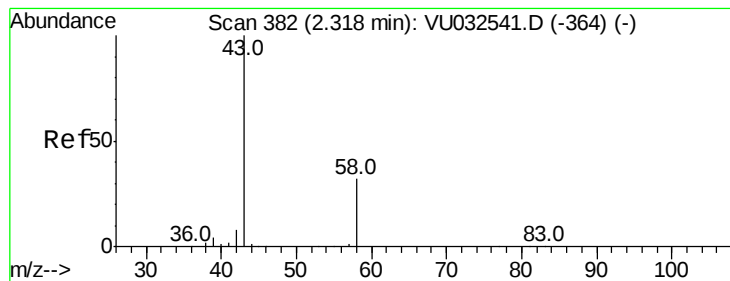

#13
 Acetone
 Concen: 4.310 ug/L
 RT: 2.32 min Scan# 382
 Delta R.T. -0.00 min
 Lab File: VU032545.D
 Acq: 08 Jun 2019 16:12

Instrument :
 MSVOA_U
 ClientSampleId :
 DB8F1

Tot Ion: 43 Resp: 5034
 Ion Ratio Lower Upper
 43 100
 58 24.4 0.0 64.0

