


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU060819\
 Data File : VU032540.D
 Acq On : 08 Jun 2019 14:00
 Operator : JC/SP
 Sample : BFB41
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB41

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060619WMA.M
 Title : VOC Analysis
 Last Update : Sat Jun 08 23:12:44 2019

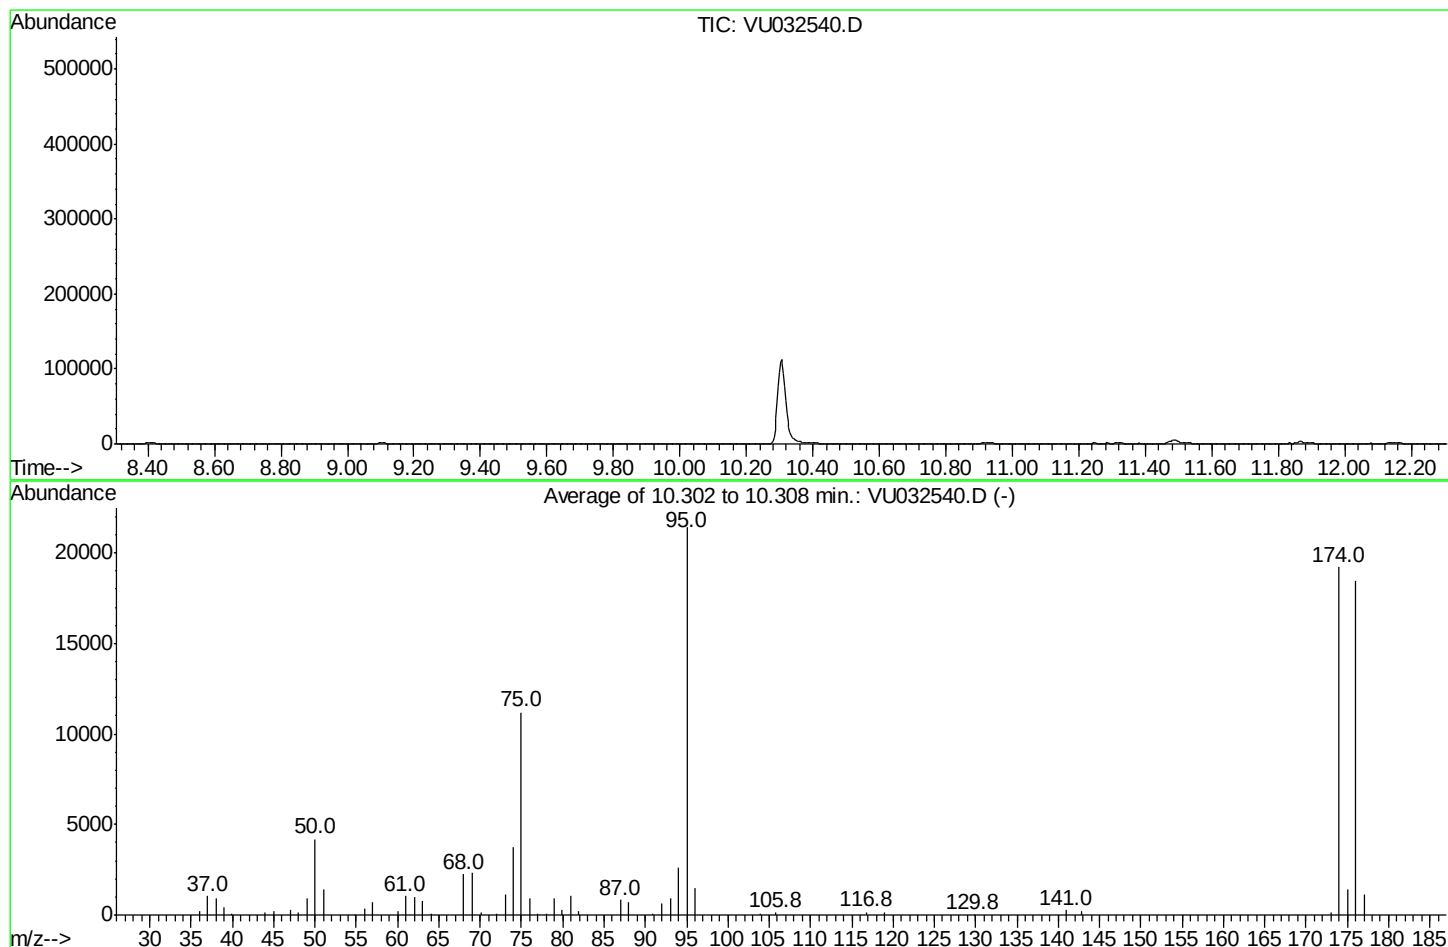

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	4207	PASS
75	95	30	80	52.2	11184	PASS
95	95	100	100	100.0	21408	PASS
96	95	5	9	7.0	1507	PASS
173	174	0.00	2	0.7	125	PASS
174	95	50	120	89.7	19213	PASS
175	174	5	9	7.4	1429	PASS
176	174	95	101	96.0	18445	PASS
177	176	5	9	6.3	1156	PASS

Scan 2854 (10.266 min): VU032540.D
BFB41

m/z	Abundance
39.90	224.0
43.90	271.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
36.00	229.0
37.00	1126.0
38.00	933.0
39.00	419.0
39.90	305.0
44.00	409.0
45.00	236.0
47.00	294.0
48.00	188.0
49.00	924.0
50.00	4310.0
51.00	1427.0
55.90	421.0
57.00	676.0
60.00	239.0
60.90	1073.0
62.00	1047.0
63.00	756.0
68.00	2262.0
69.00	2315.0
70.10	156.0
73.00	1062.0
74.00	3837.0
75.00	11413.0
76.00	963.0
76.90	170.0
77.90	112.0
78.90	877.0
79.90	266.0
80.90	1074.0
81.80	187.0
86.90	802.0
87.90	579.0
90.90	113.0
91.90	664.0
93.00	966.0
94.00	2723.0
95.00	21352.0
96.00	1581.0
103.90	113.0
105.80	125.0
116.90	168.0
118.90	145.0
129.80	101.0
141.00	268.0
142.90	242.0
174.00	18640.0
175.00	1466.0
176.00	17856.0
177.00	1138.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
35.90	245.0
37.00	1081.0
38.00	971.0
39.00	413.0
39.90	277.0
44.00	401.0
45.00	255.0
47.00	294.0
47.90	178.0
49.00	908.0
50.00	4275.0
51.00	1503.0
56.00	405.0
57.00	693.0
60.10	239.0
61.00	1076.0
62.00	1035.0
63.00	842.0
68.00	2338.0
69.00	2394.0
70.10	170.0
71.90	106.0
73.00	1134.0
74.00	3867.0
75.00	11541.0
76.00	956.0
78.00	105.0
78.90	939.0
79.90	260.0
80.90	1125.0
81.80	185.0
86.90	836.0
88.00	687.0
90.80	111.0
91.90	663.0
93.00	912.0
94.00	2692.0
95.00	22016.0
96.00	1548.0
104.00	115.0
105.80	133.0
116.80	159.0
118.90	171.0
141.00	275.0
142.80	253.0
173.10	188.0
174.00	19872.0
175.00	1451.0
176.00	18912.0
177.00	1159.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
35.00	270.0
37.00	921.0
38.00	893.0
39.00	383.0
39.00	250.0
44.00	392.0
45.00	245.0
47.00	273.0
47.00	170.0
49.00	864.0
50.00	4038.0
51.00	1405.0
54.80	105.0
56.00	346.0
57.00	661.0
60.00	229.0
61.00	1007.0
62.00	949.0
63.00	820.0
64.10	117.0
68.00	2169.0
69.00	2272.0
70.10	197.0
72.00	122.0
73.00	1122.0
74.00	3632.0
75.00	10600.0
76.00	898.0
78.00	100.0
78.90	938.0
80.00	233.0
80.90	1028.0
81.90	180.0
87.00	846.0
87.90	806.0
90.80	100.0
92.00	635.0
93.00	836.0
94.00	2495.0
95.00	20856.0
96.00	1394.0
105.80	130.0
116.80	168.0
118.90	171.0
141.00	240.0
142.80	251.0
173.00	189.0
174.00	19128.0
175.00	1372.0
176.00	18568.0
177.00	1173.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41