


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU060820\
 Data File : VU038658.D
 Acq On : 08 Jun 2020 09:12
 Operator : SY/MD
 Sample : BFB10
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB10

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR053120WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Jun 09 05:36:10 2020

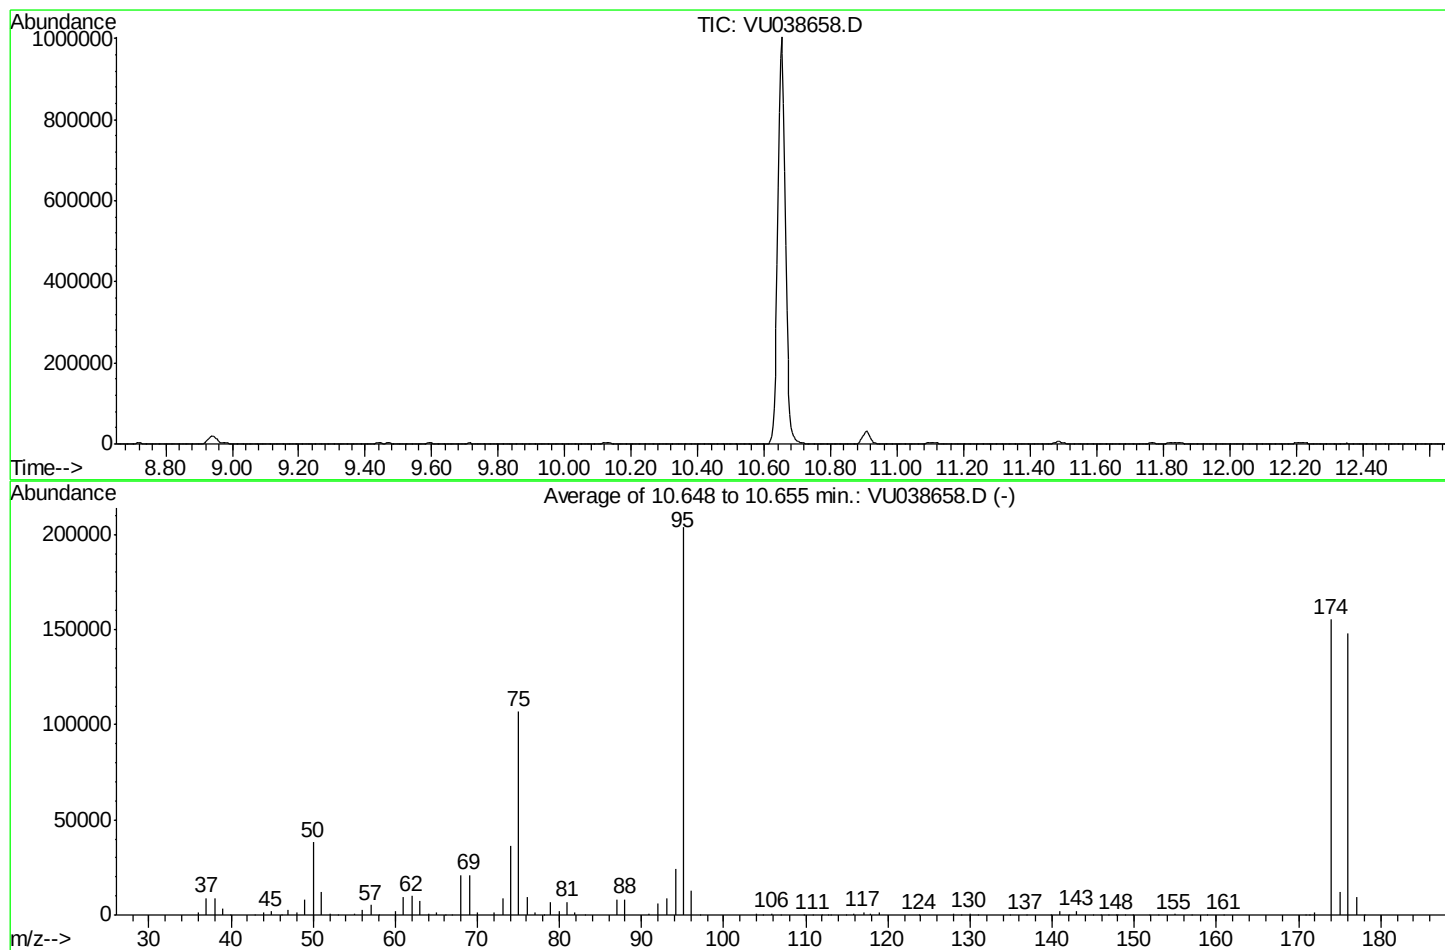

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2881

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	38274	PASS
75	95	30	80	52.4	106773	PASS
95	95	100	100	100.0	203754	PASS
96	95	5	9	6.4	13117	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.3	155392	PASS
175	174	5	9	7.7	12025	PASS
176	174	95	101	95.3	148117	PASS
177	176	5	9	6.5	9646	PASS

m/z	Abundance
36.00	1594.0
37.00	9255.0
38.00	8730.0
39.10	3446.0
39.90	321.0
43.00	133.0
44.00	1789.0
44.90	1945.0
46.10	194.0
47.00	2534.0
48.00	1130.0
49.00	7784.0
50.00	38064.0
51.00	12065.0
52.00	483.0
53.00	149.0
55.10	432.0
56.00	3053.0
57.00	5332.0
58.00	169.0
60.00	2032.0
61.00	10111.0
62.00	10075.0
63.00	7611.0
64.00	1032.0
65.10	1126.0
66.10	196.0
66.90	470.0
68.00	20552.0
69.00	21328.0
70.00	1603.0
72.00	1209.0
73.00	9077.0
74.00	35592.0
75.00	105472.0
76.10	9248.0
77.00	1375.0
78.90	6700.0
80.00	2073.0
80.90	6614.0
81.90	1523.0
83.10	224.0
87.00	7342.0
88.00	8308.0
90.90	749.0
92.00	6179.0
93.00	8974.0
94.10	23896.0
95.10	199552.0
96.00	13273.0
97.10	386.0
104.00	833.0
104.80	371.0
105.90	848.0
106.90	191.0
110.90	183.0
112.70	145.0
114.90	298.0
115.90	734.0
117.00	1244.0
117.90	758.0
119.00	1118.0
123.80	136.0
127.90	732.0
128.80	351.0
130.00	893.0
130.90	208.0
134.90	321.0
136.90	296.0
139.80	190.0
141.00	2025.0
142.00	136.0
143.00	2081.0
145.10	306.0
146.00	224.0
146.90	170.0
147.80	331.0
149.90	194.0
155.00	344.0
157.00	327.0
158.80	205.0
160.90	152.0
170.90	202.0
172.00	1367.0
174.00	148736.0
175.10	11825.0
176.00	141056.0
177.00	9292.0
178.00	255.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

m/z	Abundance
36.00	1697.0
37.00	9049.0
38.00	9181.0
39.00	3379.0
40.00	257.0
43.00	127.0
44.00	1816.0
44.90	2003.0
46.10	194.0
47.00	2687.0
47.90	1151.0
49.00	8296.0
50.00	39512.0
51.00	12245.0
52.10	443.0
53.00	168.0
55.10	388.0
56.10	3055.0
57.00	5405.0
58.00	204.0
60.00	1900.0
61.00	9909.0
62.00	10318.0
63.10	7491.0
64.00	963.0
65.00	1110.0
66.10	154.0
66.90	454.0
68.00	21464.0
69.00	21920.0
70.00	1692.0
72.00	1124.0
73.00	9256.0
74.00	37608.0
75.00	110168.0
76.10	9696.0
77.00	1282.0
78.90	7274.0
80.00	2126.0
81.00	7171.0
81.90	1589.0
83.10	263.0
87.00	8146.0
88.00	8634.0
90.90	840.0
92.00	6401.0
93.10	9148.0
94.10	25320.0
95.10	210176.0
96.00	13506.0
97.10	329.0
104.00	785.0
104.80	357.0
105.90	872.0
106.90	229.0
109.80	117.0
110.90	202.0
112.00	115.0
112.60	124.0
113.00	114.0
114.90	362.0
115.90	766.0
117.00	1390.0
117.90	781.0
118.90	1108.0
123.90	151.0
128.00	791.0
128.80	328.0
130.00	884.0
131.00	241.0
134.90	331.0
136.80	374.0
139.90	240.0
141.00	2068.0
142.00	259.0
143.00	2103.0
145.10	361.0
145.90	238.0
146.90	208.0
147.80	354.0
149.90	175.0
151.90	116.0
152.90	127.0
154.90	432.0
157.00	300.0
158.80	205.0
160.90	140.0
170.90	166.0
172.00	1318.0
174.00	160768.0
175.10	12386.0
176.00	152832.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

177.1010071.0

178.00255.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

m/z	Abundance
36.10	1627.0
37.00	8003.0
38.00	8335.0
39.00	3249.0
40.10	257.0
42.90	154.0
44.00	1751.0
44.90	1782.0
46.10	197.0
47.00	2486.0
47.90	1141.0
49.00	7888.0
50.00	37248.0
51.00	11382.0
52.10	387.0
52.90	151.0
55.00	378.0
56.10	2886.0
57.10	5129.0
58.00	233.0
60.00	1666.0
61.00	9031.0
62.00	9761.0
63.10	7065.0
64.00	743.0
65.00	1060.0
66.00	115.0
68.00	20112.0
69.00	20184.0
70.00	1676.0
71.90	978.0
73.10	8772.0
74.00	35552.0
75.00	104680.0
76.10	9122.0
77.10	1142.0
78.10	795.0
78.90	6898.0
80.00	1994.0
81.00	6773.0
81.90	1593.0
83.00	261.0
87.00	8328.0
88.00	8240.0
90.90	816.0
92.00	6084.0
93.10	8418.0
94.10	24520.0
95.10	201536.0
96.00	12574.0
97.10	304.0
103.90	692.0
104.80	299.0
105.90	834.0
106.90	255.0
109.80	110.0
110.90	215.0
112.00	122.0
113.00	143.0
114.90	341.0
115.90	761.0
117.00	1454.0
117.90	658.0
118.90	1122.0
123.90	124.0
128.00	805.0
128.90	317.0
130.00	830.0
131.00	260.0
134.90	277.0
136.80	399.0
139.90	219.0
141.00	1917.0
142.00	323.0
143.00	2105.0
145.00	336.0
145.90	286.0
146.90	161.0
148.00	373.0
148.90	105.0
149.80	210.0
151.90	145.0
152.90	138.0
154.90	489.0
157.00	274.0
158.90	198.0
161.00	163.0
171.30	160.0
172.00	1165.0
174.00	156672.0
175.10	11864.0
176.00	150464.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10

177.10

178.00

9576.0

202.0

Instrument :

MSVOA_U

ClientSampleId :

BFB10

Scan 2881 (10.603 min): VU038658.D
BFB10

m/z	Abundance
39.80	215.0
43.90	715.0

Instrument :
MSVOA_U
ClientSampleId :
BFB10