

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060821\
 Data File : VU044101.D
 Acq On : 08 Jun 2021 09:33
 Operator : SY/MD
 Sample : M2613-24
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 18-B12(126-130)

Quant Time: Jun 08 23:11:04 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U060721W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 08 17:38:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.382	168	205959	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.256	114	412467	50.000	ug/l	0.00
63) Chlorobenzene-d5	9.423	117	447682	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.819	152	210154	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.710	65	187432	52.254	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.500%	
35) Dibromofluoromethane	5.298	113	145485	49.427	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.860%	
50) Toluene-d8	7.906	98	575215	50.664	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.320%	
62) 4-Bromofluorobenzene	10.639	95	221328	49.238	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.480%	
Target Compounds						
					Qvalue	
16) Acetone	2.636	43	12632	6.102	ug/l	95
20) Methylene Chloride	3.051	84	26576	7.102	ug/l	97
43) Isopropyl Acetate	5.919	43	26232	3.169	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060821\
Data File : VU044101.D
Acq On : 08 Jun 2021 09:33
Operator : SY/MD
Sample : M2613-24
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
18-B12(126-130)

Quant Time: Jun 08 23:11:04 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U060721W.M
Quant Title : SW846 8260
QLast Update : Tue Jun 08 17:38:51 2021
Response via : Initial Calibration




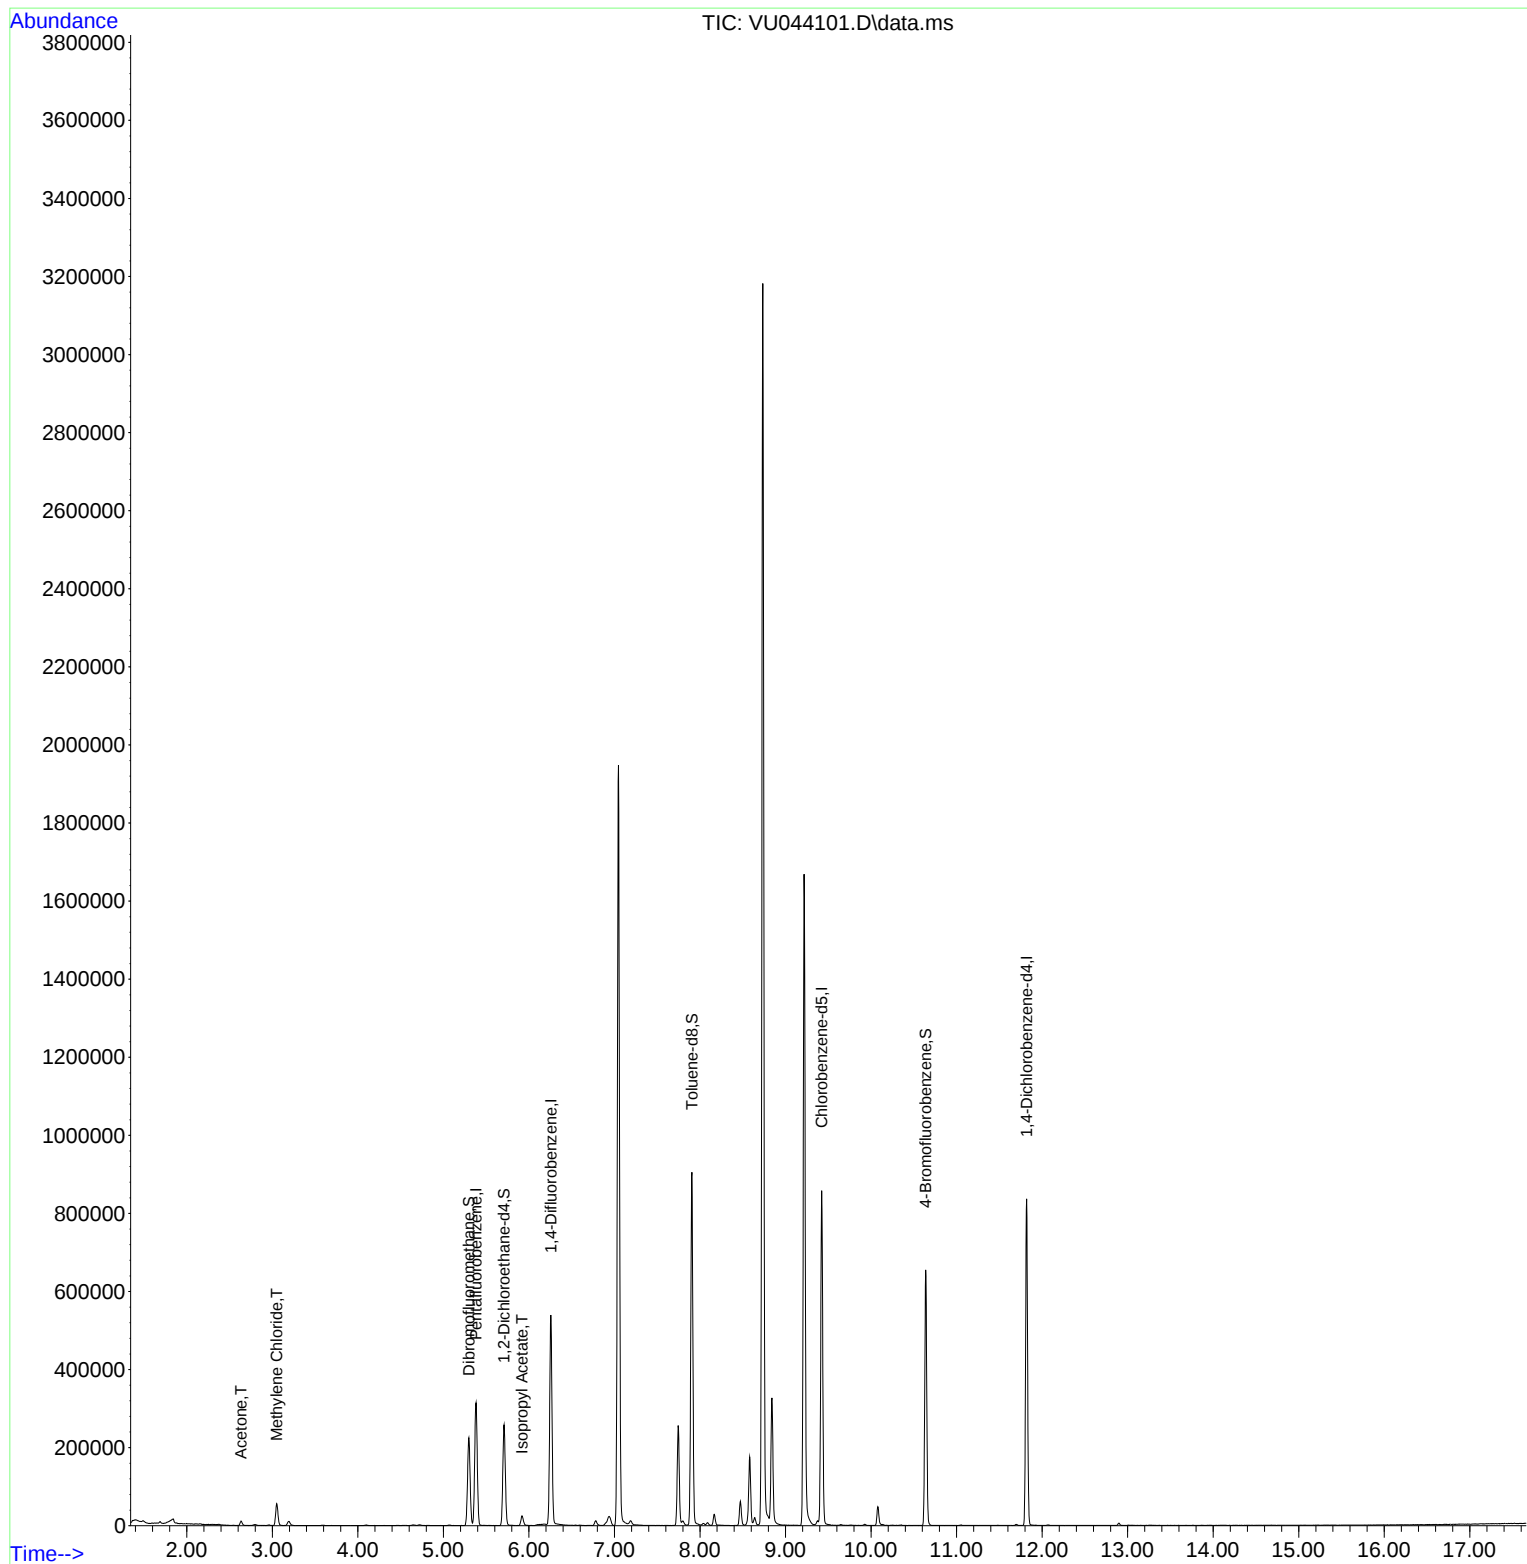


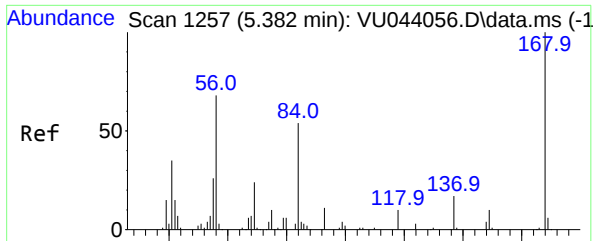

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.382 min Scan# 1257
Delta R.T. -0.000 min
Lab File: VU044101.D
Acq: 08 Jun 2021 09:33




Instrument :
MSVOA_U
ClientSampleId :
18-B12(126-130)


Tgt Ion:168 Resp: 205959
Ion Ratio Lower Upper
168 100
99 64.6 52.6 78.8

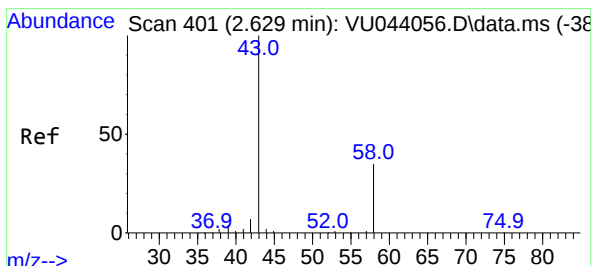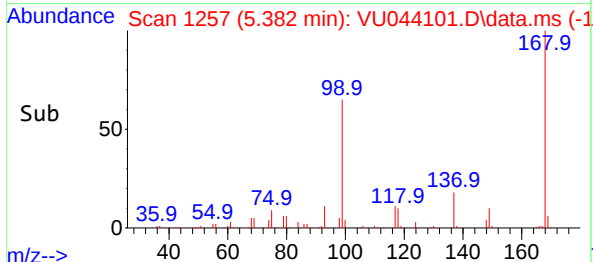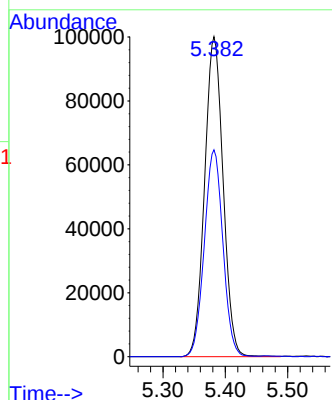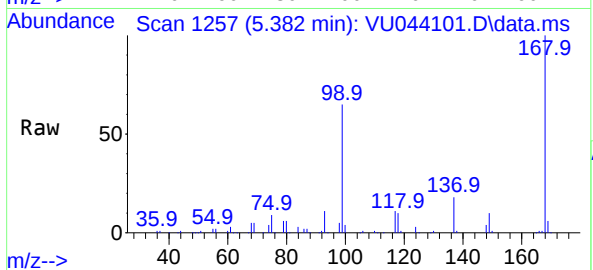

#16
Acetone
Concen: 6.102 ug/l
RT: 2.636 min Scan# 403
Delta R.T. 0.007 min
Lab File: VU044101.D
Acq: 08 Jun 2021 09:33


Tgt Ion: 43 Resp: 12632
Ion Ratio Lower Upper
43 100
58 37.5 27.7 41.5

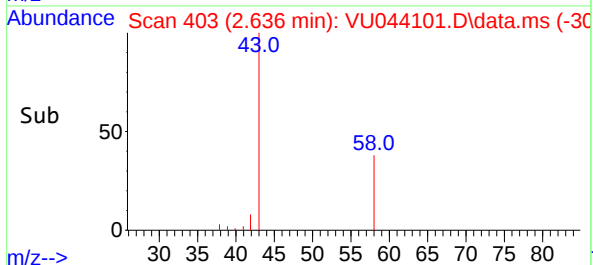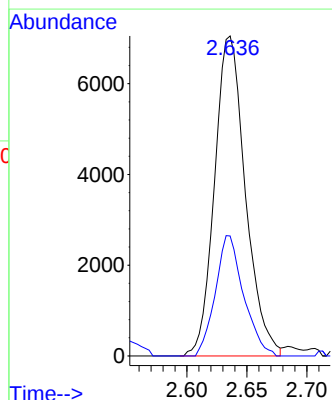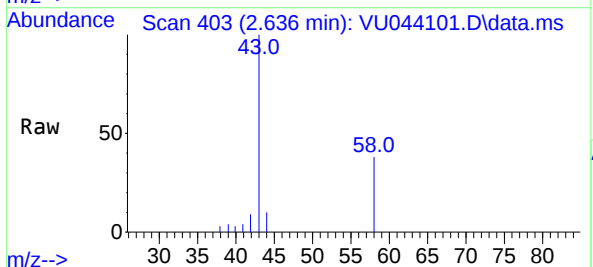



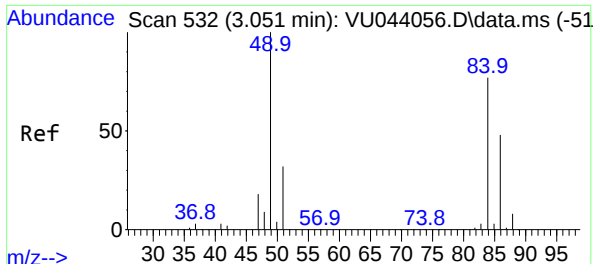


#20
Methylene Chloride
Concen: 7.102 ug/l
RT: 3.051 min Scan# 532
Delta R.T. -0.000 min
Lab File: VU044101.D
Acq: 08 Jun 2021 09:33

Instrument :
MSVOA_U
ClientSampleId :
18-B12(126-130)



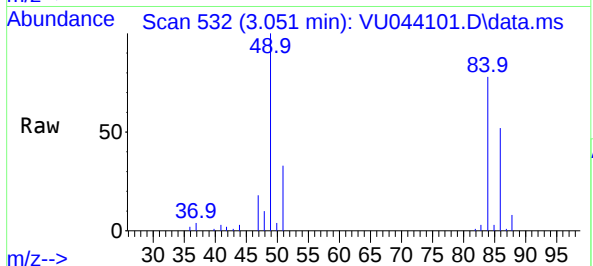



Tgt Ion:	84	Resp:	26576
Ion	Ratio	Lower	Upper
84	100		
49	127.7	103.6	155.4
51	42.7	32.8	49.2
86	66.3	49.9	74.9

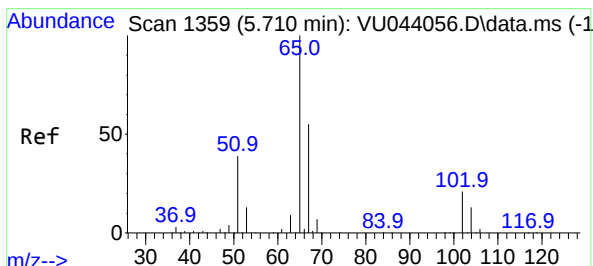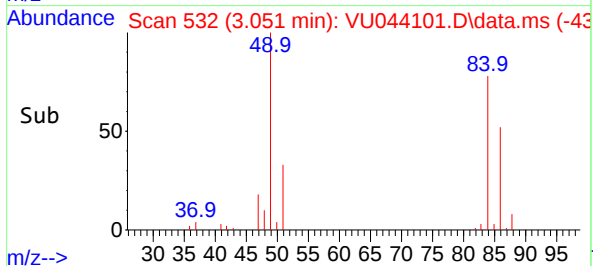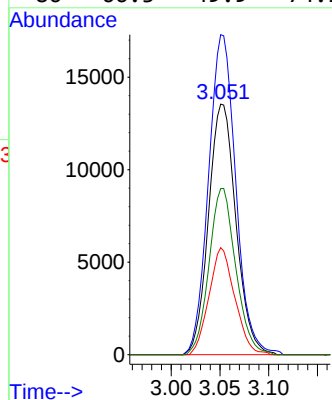

#33
1,2-Dichloroethane-d4
Concen: 52.254 ug/l
RT: 5.710 min Scan# 1359
Delta R.T. -0.000 min
Lab File: VU044101.D
Acq: 08 Jun 2021 09:33

Tgt Ion:	65	Resp:	187432
Ion	Ratio	Lower	Upper
65	100		
67	53.9	0.0	109.2

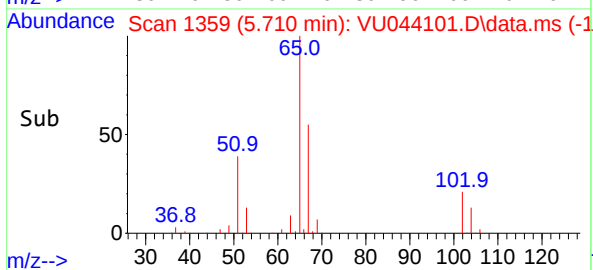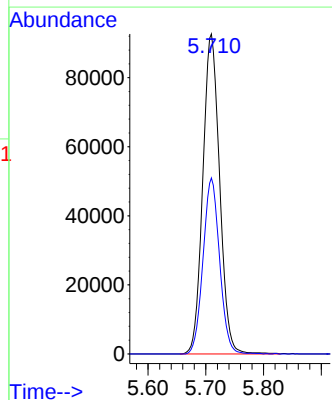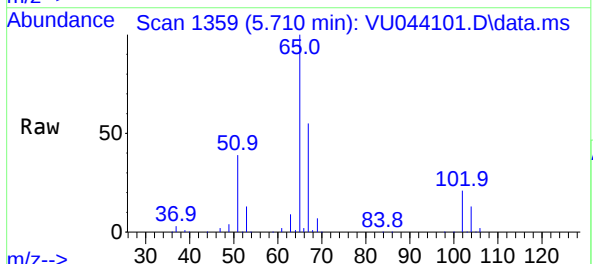




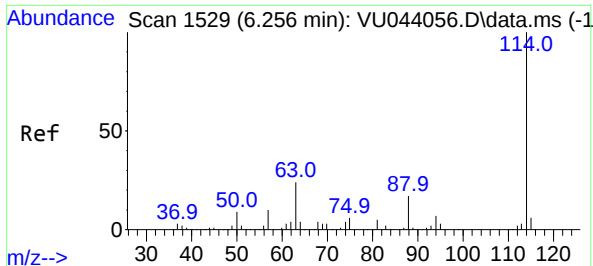


#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.256 min Scan# 1529
Delta R.T. 0.000 min
Lab File: VU044101.D
Acq: 08 Jun 2021 09:33

Instrument :
MSVOA_U
ClientSampleId :
18-B12(126-130)




Tgt Ion:114 Resp: 412467
Ion Ratio Lower Upper
114 100
63 23.3 0.0 48.4
88 16.8 0.0 34.4

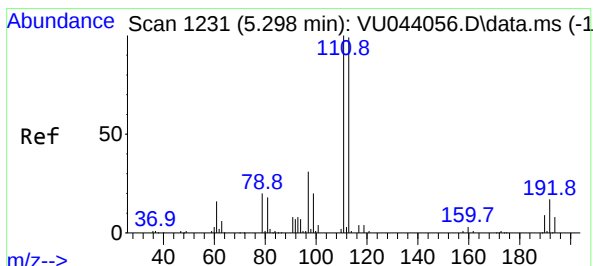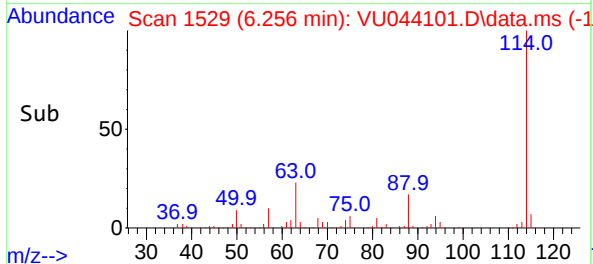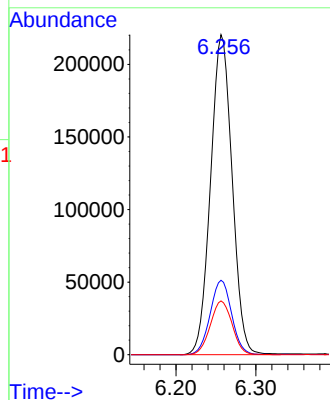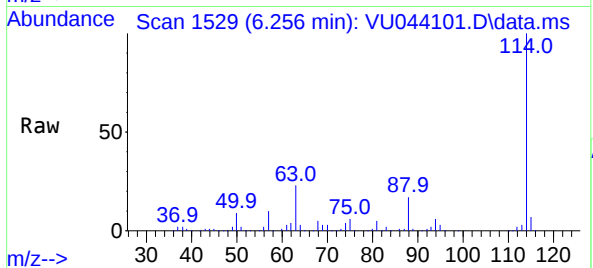


#35

Dibromofluoromethane
Concen: 49.427 ug/l
RT: 5.298 min Scan# 1231
Delta R.T. 0.000 min
Lab File: VU044101.D
Acq: 08 Jun 2021 09:33

Tgt Ion:113 Resp: 145485
Ion Ratio Lower Upper
113 100
111 103.0 82.1 123.1
192 17.9 13.8 20.8


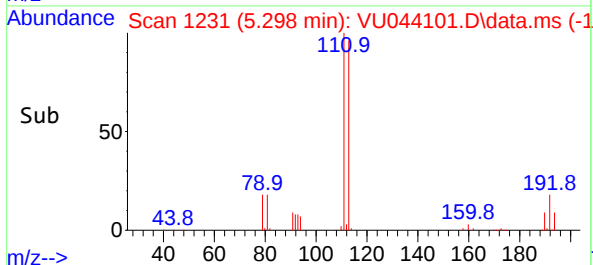
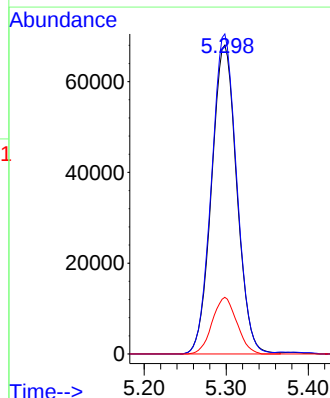
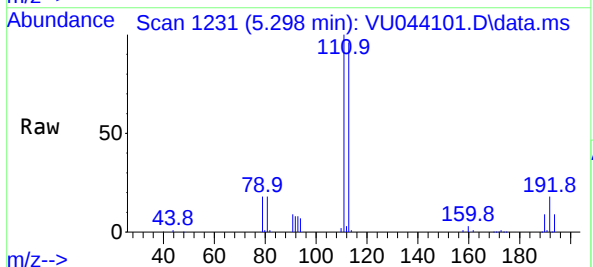


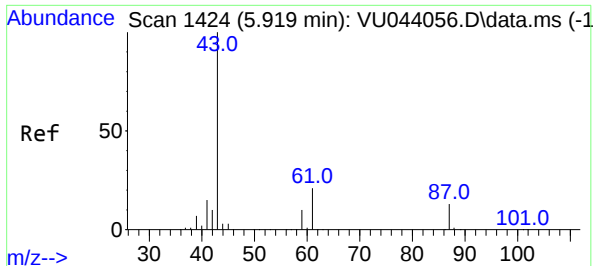

#43
Isopropyl Acetate
Concen: 3.169 ug/l
RT: 5.919 min Scan# 1424
Delta R.T. -0.000 min
Lab File: VU044101.D
Acq: 08 Jun 2021 09:33




Instrument :
MSVOA_U
ClientSampleId :
18-B12(126-130)


Tgt Ion: 43	Resp: 26232
Ion Ratio	Lower Upper
43	100
61	19.5 16.8 25.2
87	13.4 10.2 15.2

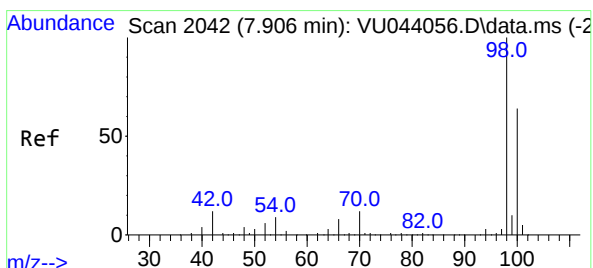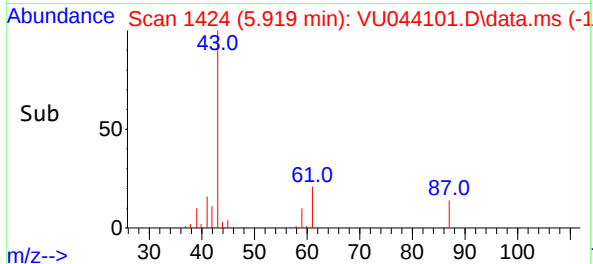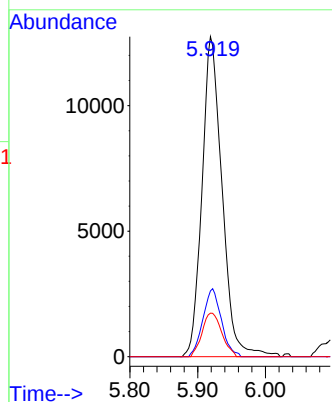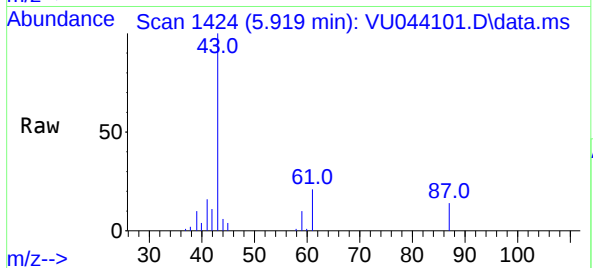

#50
Toluene-d8
Concen: 50.664 ug/l
RT: 7.906 min Scan# 2042
Delta R.T. -0.000 min
Lab File: VU044101.D
Acq: 08 Jun 2021 09:33

Tgt Ion: 98	Resp: 575215
Ion Ratio	Lower Upper
98	100
100	64.6 51.6 77.4

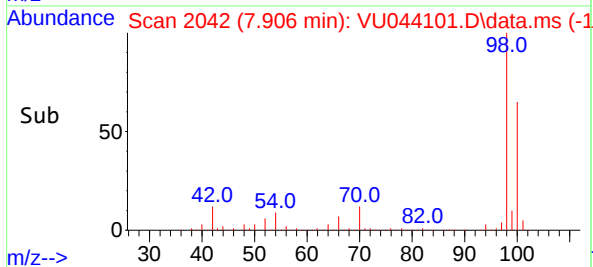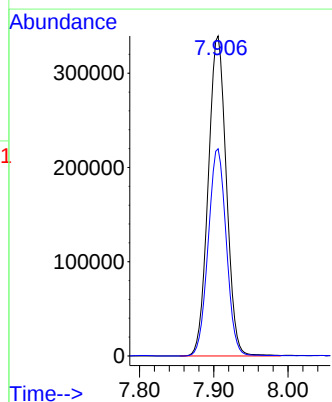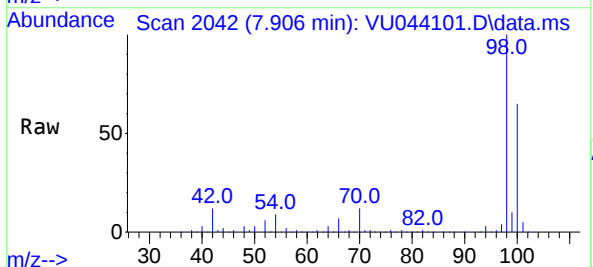




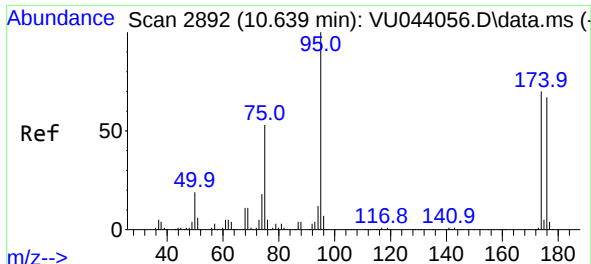


#62
4-Bromofluorobenzene
Concen: 49.238 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. -0.000 min
Lab File: VU044101.D
Acq: 08 Jun 2021 09:33

Instrument :
MSVOA_U
ClientSampleId :
18-B12(126-130)

Tgt Ion: 95 Resp: 221328




Ion	Ratio	Lower	Upper
95	100		
174	71.8	0.0	141.0
176	69.1	0.0	135.2

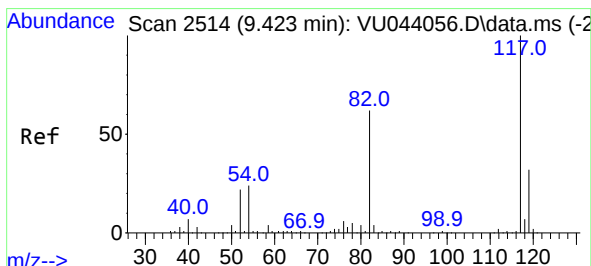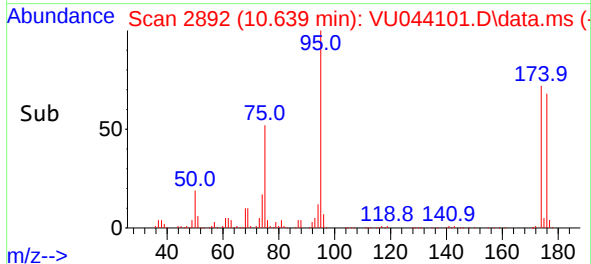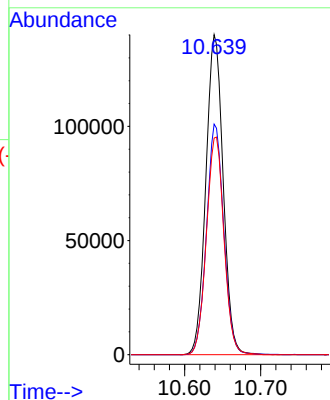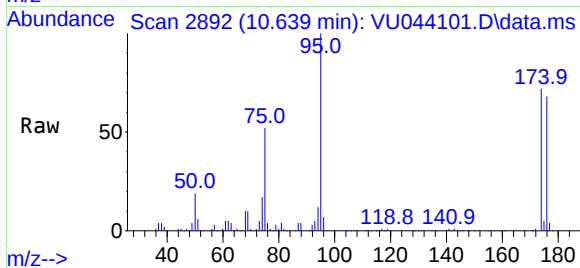


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.423 min Scan# 2514
Delta R.T. 0.000 min
Lab File: VU044101.D
Acq: 08 Jun 2021 09:33

Tgt Ion: 117 Resp: 447682

Ion	Ratio	Lower	Upper
117	100		
82	62.2	50.0	75.0
119	32.3	25.9	38.9

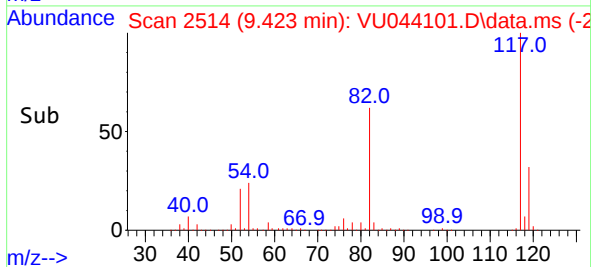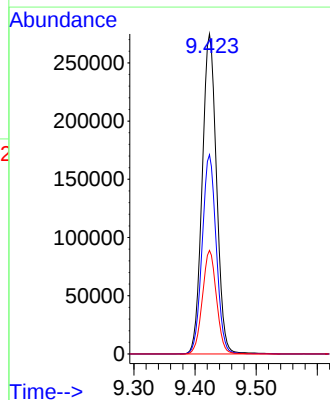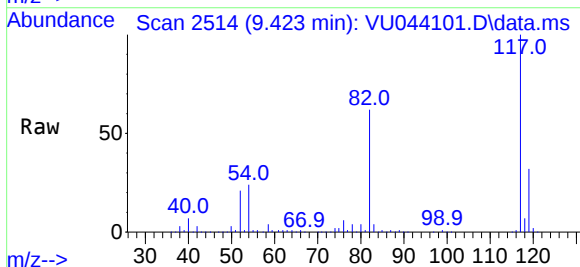

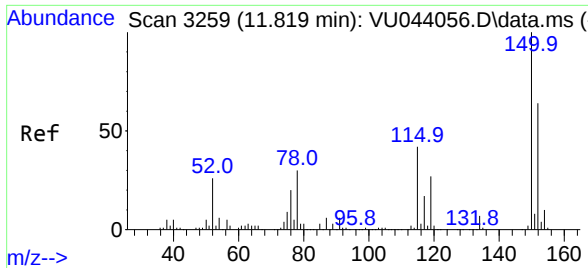

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 11.819 min Scan# 3259
 Delta R.T. -0.000 min
 Lab File: VU044101.D
 Acq: 08 Jun 2021 09:33

Instrument :
 MSVOA_U
 ClientSampleId :
 18-B12(126-130)

Tgt Ion:152 Resp: 210154
 Ion Ratio Lower Upper
 152 100
 115 62.1 44.6 134.0
 150 157.0 0.0 347.8

