

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060821\
 Data File : VU044103.D
 Acq On : 08 Jun 2021 10:20
 Operator : SY/MD
 Sample : M2613-26
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 18-B12(134-138)

Quant Time: Jun 08 23:11:24 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U060721W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 08 17:38:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.382	168	214453	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.256	114	435996	50.000	ug/l	0.00
63) Chlorobenzene-d5	9.423	117	460544	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.819	152	214581	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.710	65	197681	52.929	ug/l	0.00
Spiked Amount	50.000		Recovery	=	105.860%	
35) Dibromofluoromethane	5.298	113	151506	48.695	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.380%	
50) Toluene-d8	7.906	98	603737	50.307	ug/l	0.00
Spiked Amount	50.000		Recovery	=	100.620%	
62) 4-Bromofluorobenzene	10.639	95	224254	47.197	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.400%	
Target Compounds						
						Qvalue
16) Acetone	2.633	43	15981	7.414	ug/l	96
20) Methylene Chloride	3.054	84	26229	6.640	ug/l	95
43) Isopropyl Acetate	5.919	43	26692	3.050	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060821\
Data File : VU044103.D
Acq On : 08 Jun 2021 10:20
Operator : SY/MD
Sample : M2613-26
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
18-B12(134-138)

Quant Time: Jun 08 23:11:24 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U060721W.M
Quant Title : SW846 8260
QLast Update : Tue Jun 08 17:38:51 2021
Response via : Initial Calibration




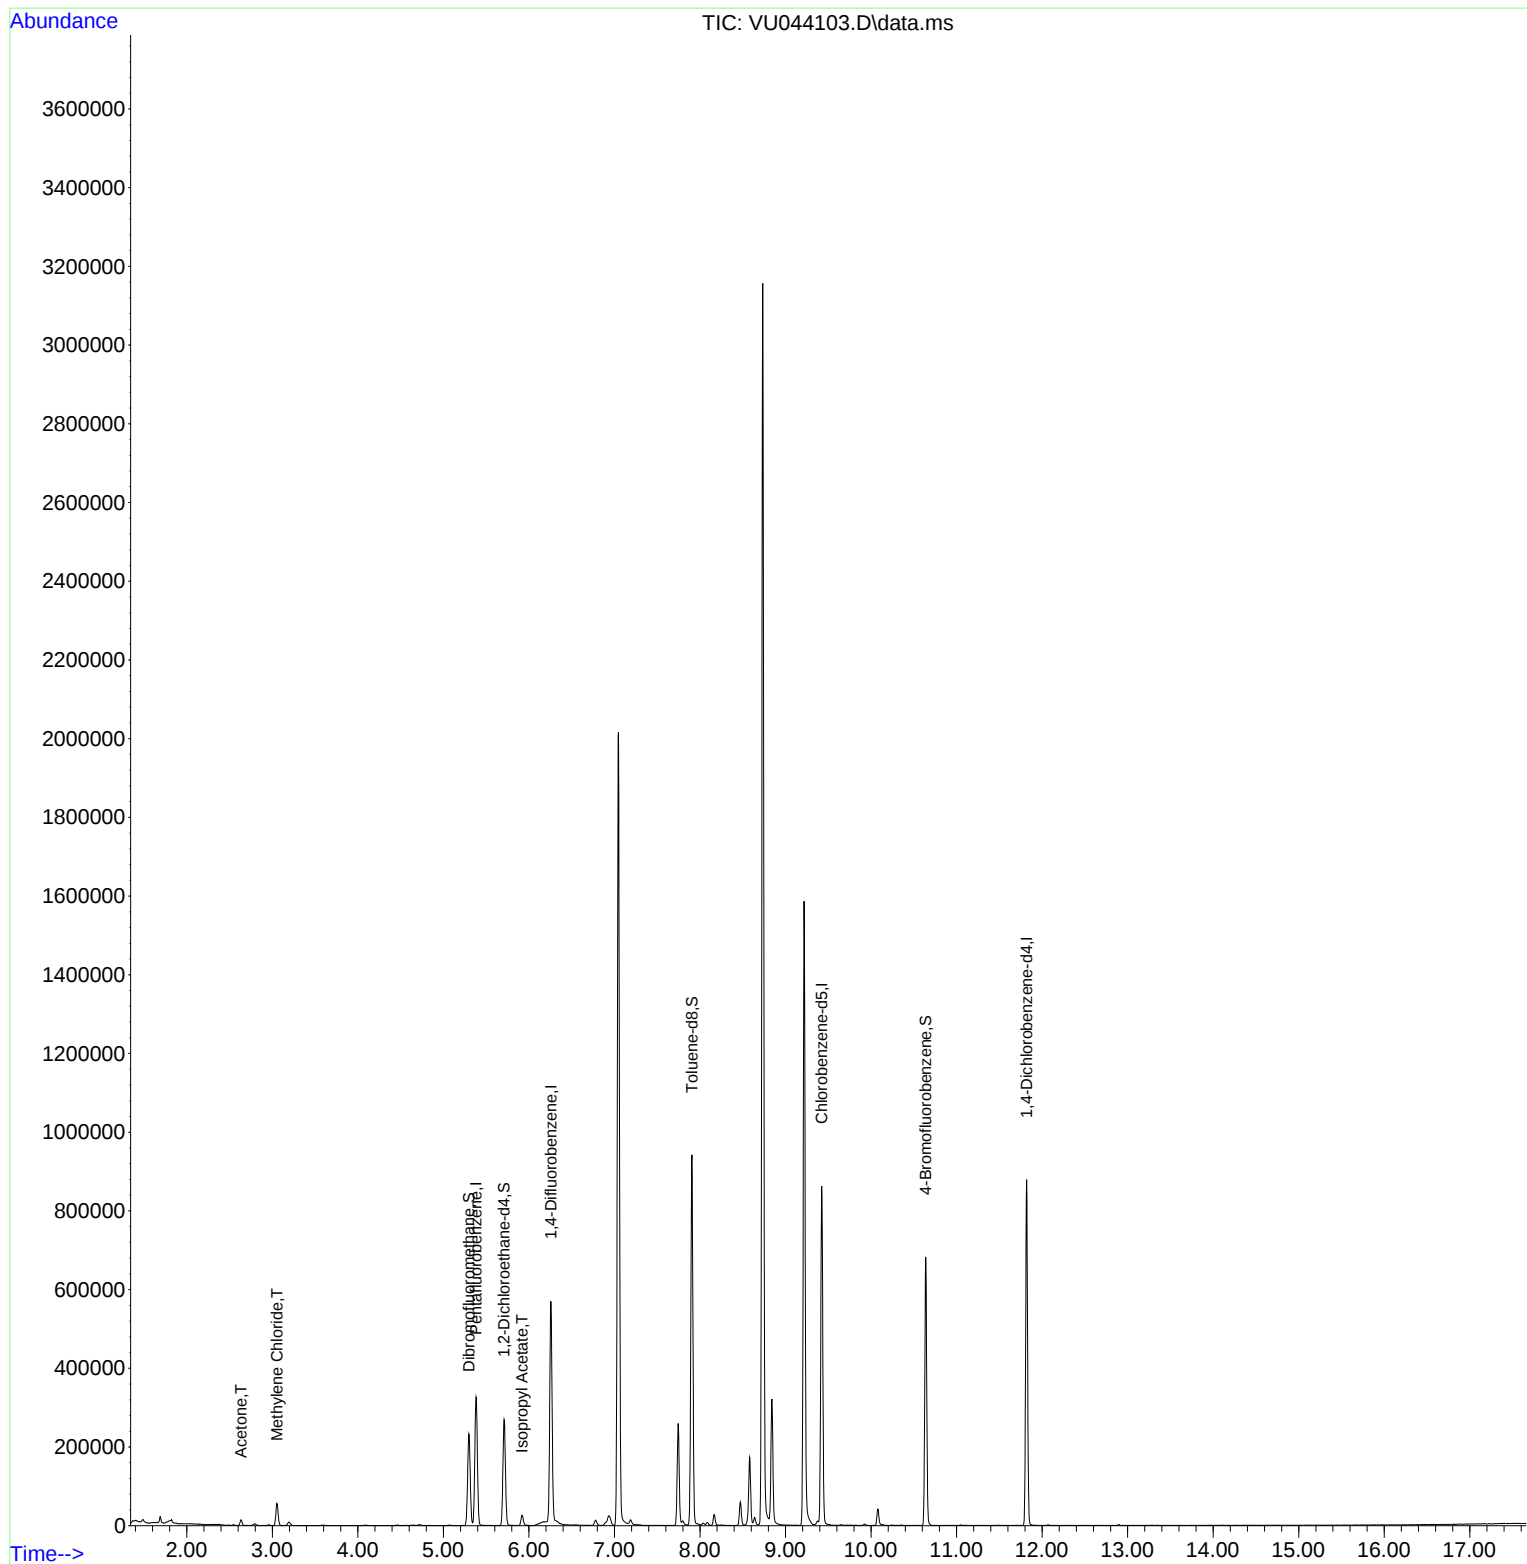


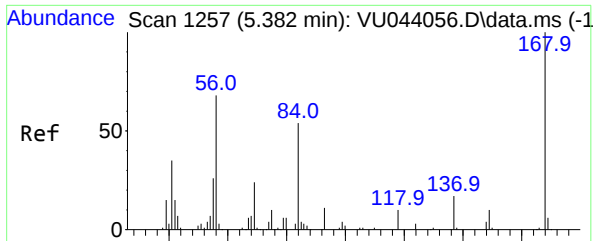

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.382 min Scan# 1257
Delta R.T. -0.000 min
Lab File: VU044103.D
Acq: 08 Jun 2021 10:20




Instrument :
MSVOA_U
ClientSampleId :
18-B12(134-138)


Tgt Ion:168 Resp: 214453
Ion Ratio Lower Upper
168 100
99 64.5 52.6 78.8

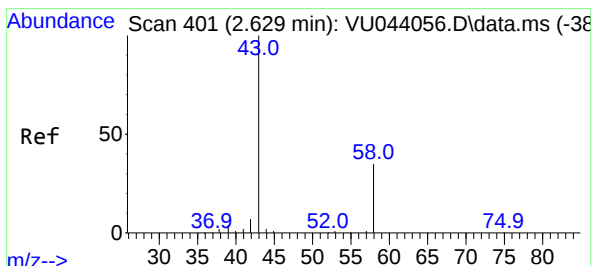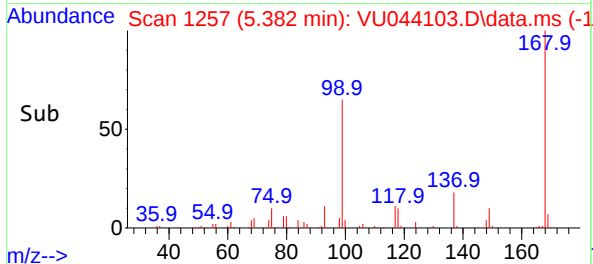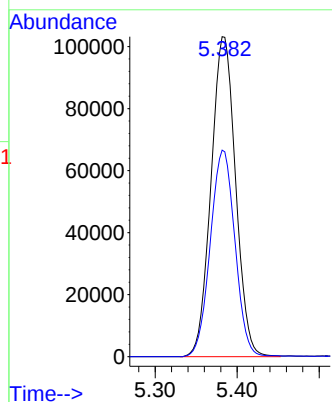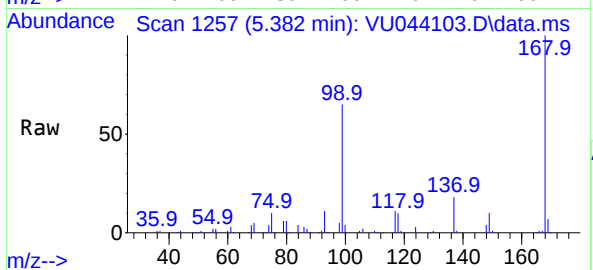

#16
Acetone
Concen: 7.414 ug/l
RT: 2.633 min Scan# 402
Delta R.T. 0.004 min
Lab File: VU044103.D
Acq: 08 Jun 2021 10:20


Tgt Ion: 43 Resp: 15981
Ion Ratio Lower Upper
43 100
58 36.8 27.7 41.5

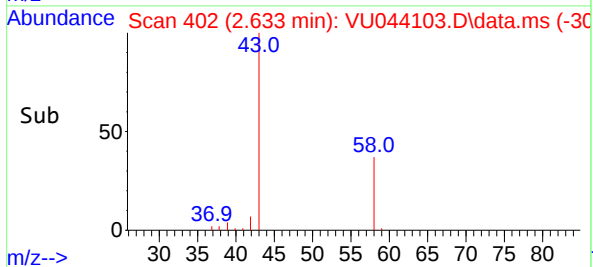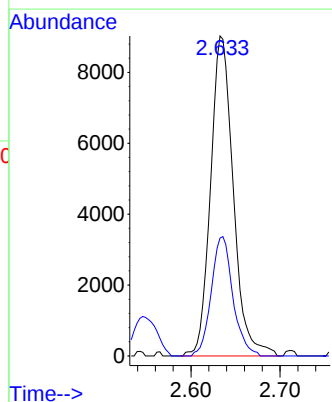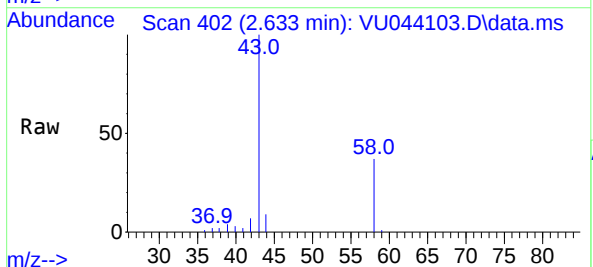



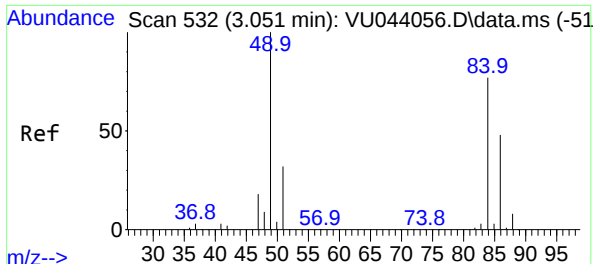


#20
Methylene Chloride
Concen: 6.640 ug/l
RT: 3.054 min Scan# 533
Delta R.T. 0.003 min
Lab File: VU044103.D
Acq: 08 Jun 2021 10:20

Instrument :
MSVOA_U
ClientSampleId :
18-B12(134-138)



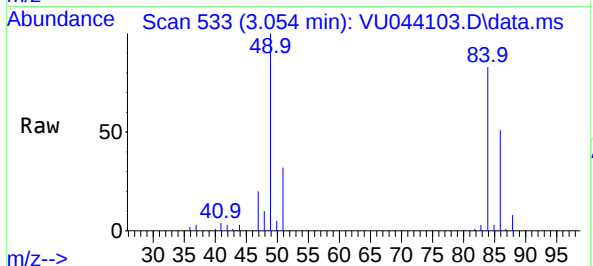



Tgt Ion:	84	Resp:	26229
Ion	Ratio	Lower	Upper
84	100		
49	120.8	103.6	155.4
51	38.2	32.8	49.2
86	62.1	49.9	74.9

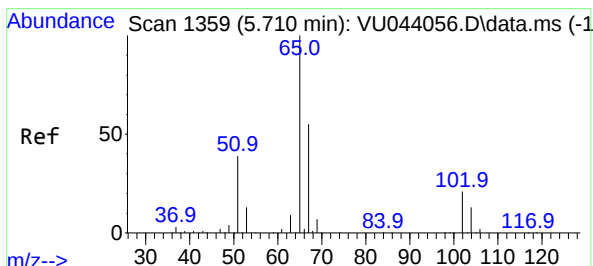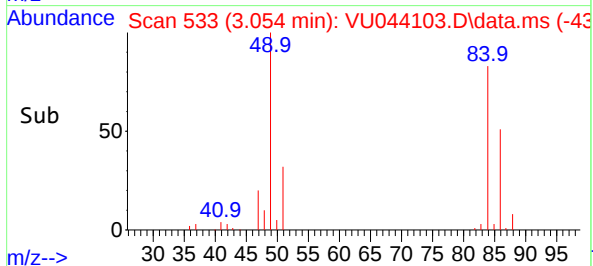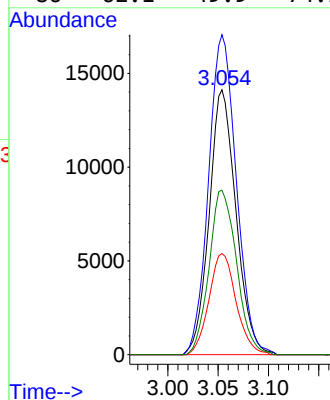

#33
1,2-Dichloroethane-d4
Concen: 52.929 ug/l
RT: 5.710 min Scan# 1359
Delta R.T. -0.000 min
Lab File: VU044103.D
Acq: 08 Jun 2021 10:20

Tgt Ion:	65	Resp:	197681
Ion	Ratio	Lower	Upper
65	100		
67	53.5	0.0	109.2


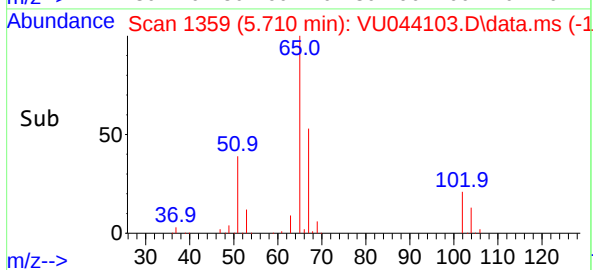
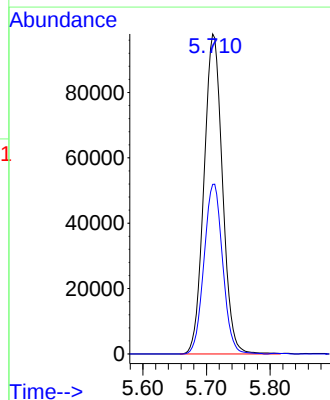
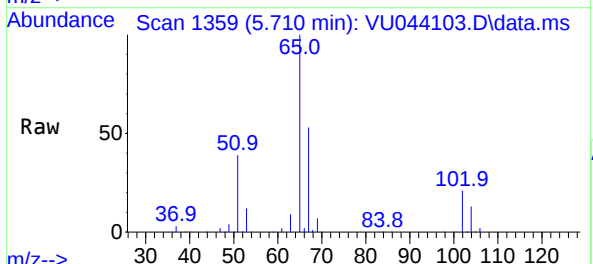


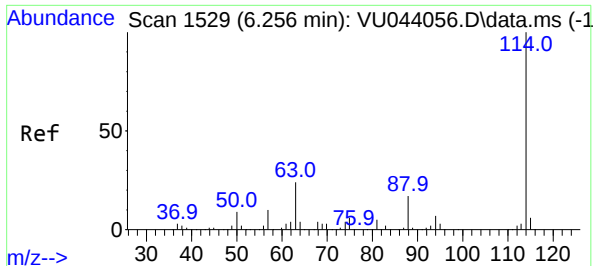

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.256 min Scan# 1529
Delta R.T. 0.000 min
Lab File: VU044103.D
Acq: 08 Jun 2021 10:20




Instrument :
MSVOA_U
ClientSampleId :
18-B12(134-138)


Tgt Ion:114 Resp: 435996
Ion Ratio Lower Upper
114 100
63 23.1 0.0 48.4
88 17.2 0.0 34.4

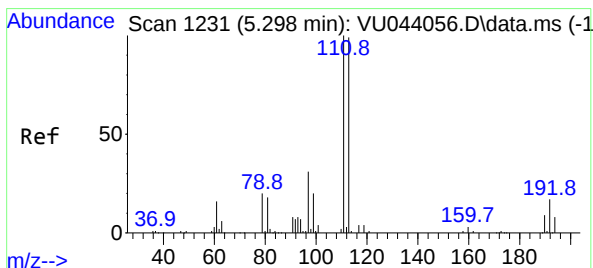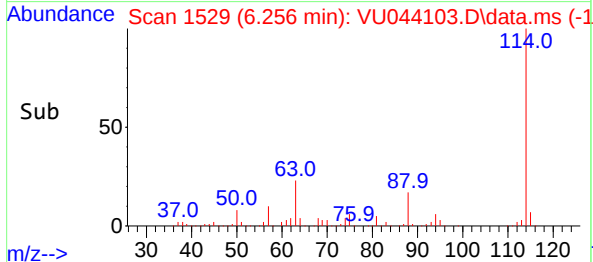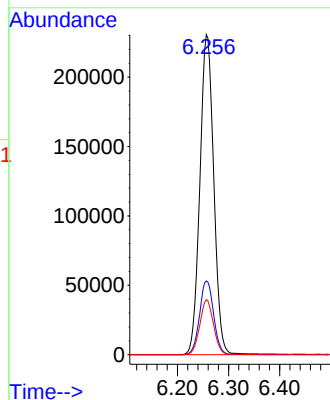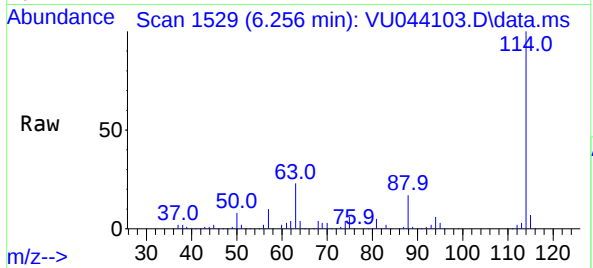

#35
Dibromofluoromethane
Concen: 48.695 ug/l
RT: 5.298 min Scan# 1231
Delta R.T. 0.000 min
Lab File: VU044103.D
Acq: 08 Jun 2021 10:20

Tgt Ion:113 Resp: 151506
Ion Ratio Lower Upper
113 100
111 102.4 82.1 123.1
192 18.0 13.8 20.8


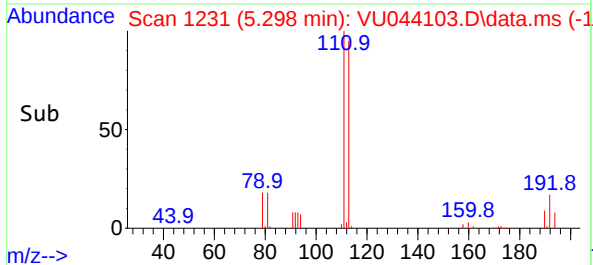
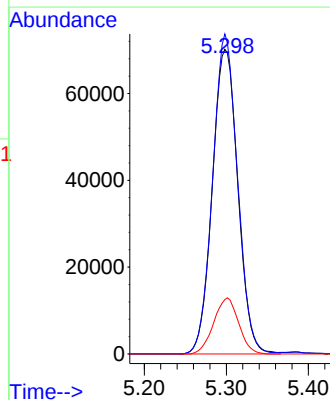
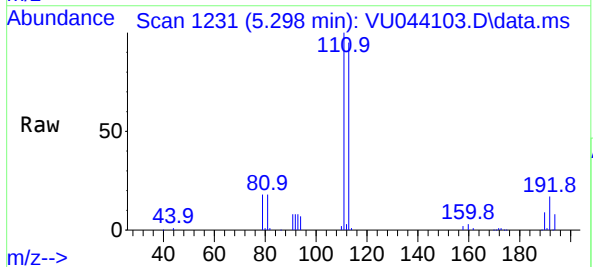


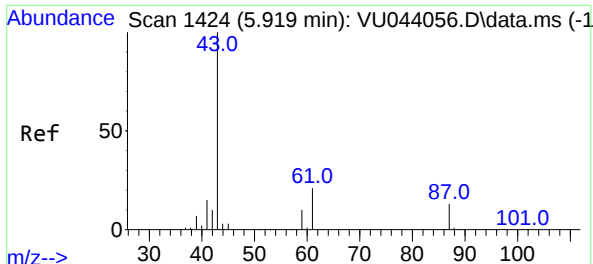

#43
Isopropyl Acetate
Concen: 3.050 ug/l
RT: 5.919 min Scan# 1424
Delta R.T. -0.000 min
Lab File: VU044103.D
Acq: 08 Jun 2021 10:20




Instrument :
MSVOA_U
ClientSampleId :
18-B12(134-138)


Tgt Ion: 43	Resp: 26692
Ion Ratio	Lower Upper
43 100	
61 22.2	16.8 25.2
87 13.6	10.2 15.2

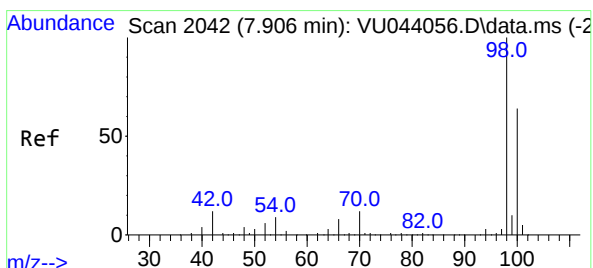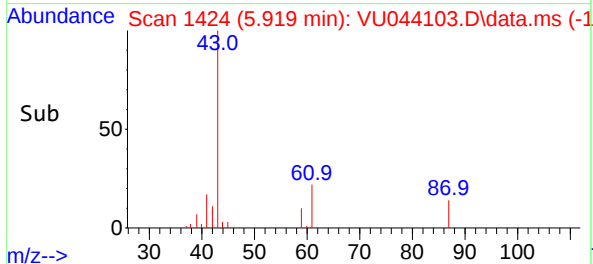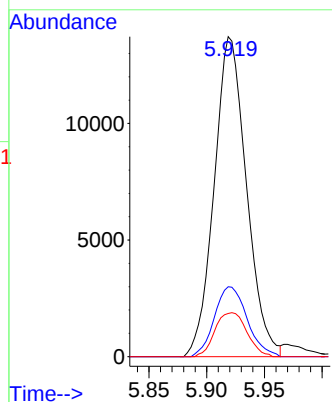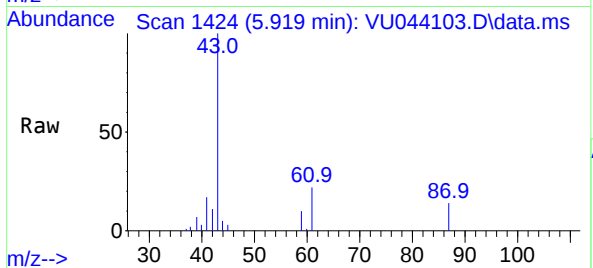

#50
Toluene-d8
Concen: 50.307 ug/l
RT: 7.906 min Scan# 2042
Delta R.T. -0.000 min
Lab File: VU044103.D
Acq: 08 Jun 2021 10:20

Tgt Ion: 98	Resp: 603737
Ion Ratio	Lower Upper
98 100	
100 64.6	51.6 77.4

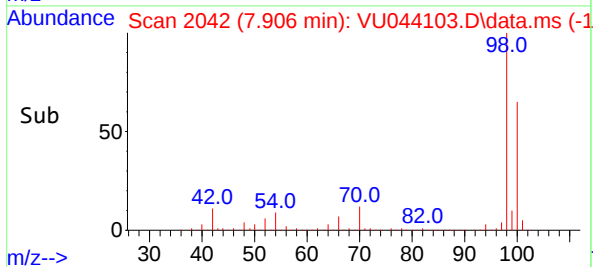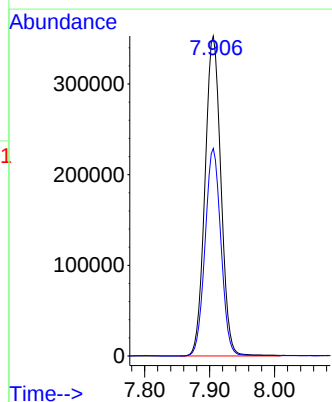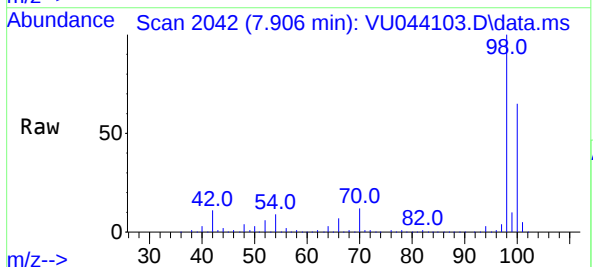




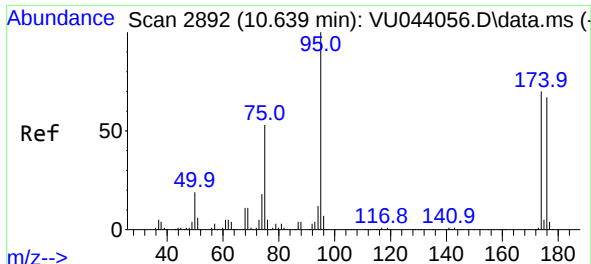


#62
4-Bromofluorobenzene
Concen: 47.197 ug/l
RT: 10.639 min Scan# 2892
Delta R.T. -0.000 min
Lab File: VU044103.D
Acq: 08 Jun 2021 10:20

Instrument :
MSVOA_U
ClientSampleId :
18-B12(134-138)

Tgt Ion: 95 Resp: 224254




Ion	Ratio	Lower	Upper
95	100		
174	73.2	0.0	141.0
176	69.7	0.0	135.2

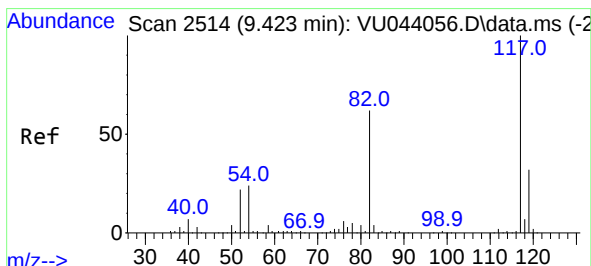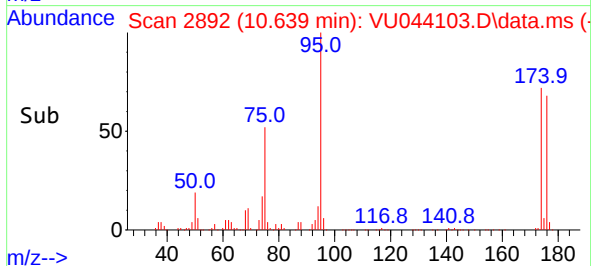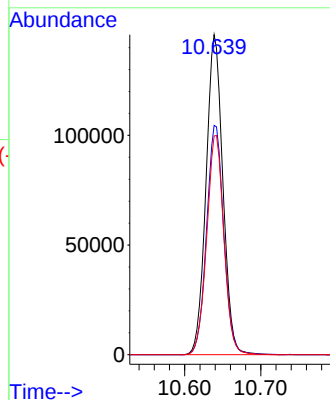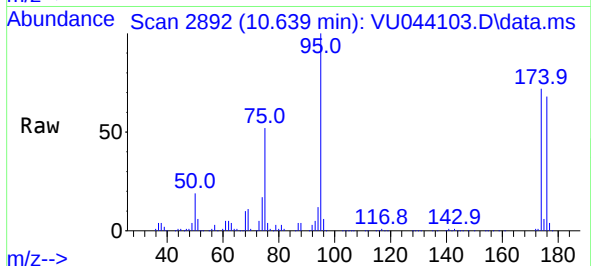


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.423 min Scan# 2514
Delta R.T. 0.000 min
Lab File: VU044103.D
Acq: 08 Jun 2021 10:20

Tgt Ion: 117 Resp: 460544

Ion	Ratio	Lower	Upper
117	100		
82	60.6	50.0	75.0
119	31.7	25.9	38.9

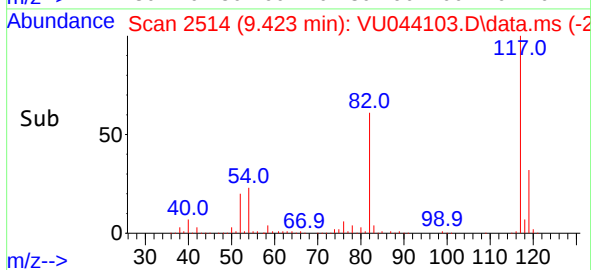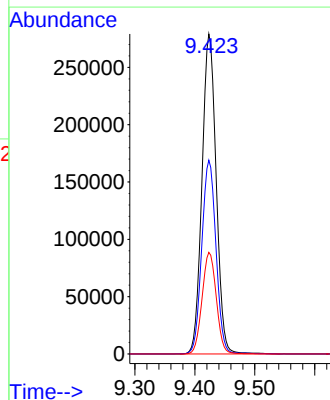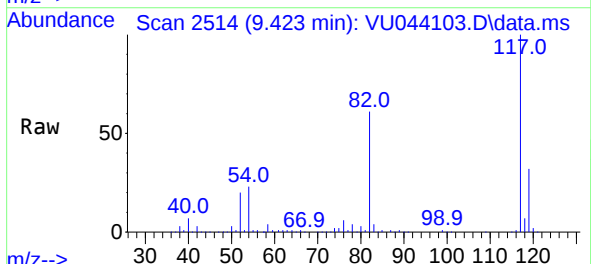

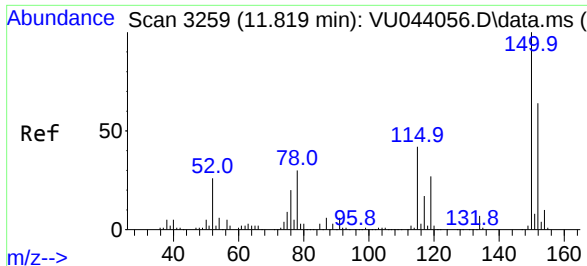

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 11.819 min Scan# 3259
 Delta R.T. -0.000 min
 Lab File: VU044103.D
 Acq: 08 Jun 2021 10:20

Instrument :
 MSVOA_U
 ClientSampleId :
 18-B12(134-138)

Tgt Ion:152 Resp: 214581
 Ion Ratio Lower Upper
 152 100
 115 63.1 44.6 134.0
 150 157.8 0.0 347.8

