


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060821\
 Data File : VU044086.D
 Acq On : 08 Jun 2021 03:42
 Operator : SY/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U060721W.M
 Title : SW846 8260
 Last Update : Tue Jun 08 17:38:51 2021

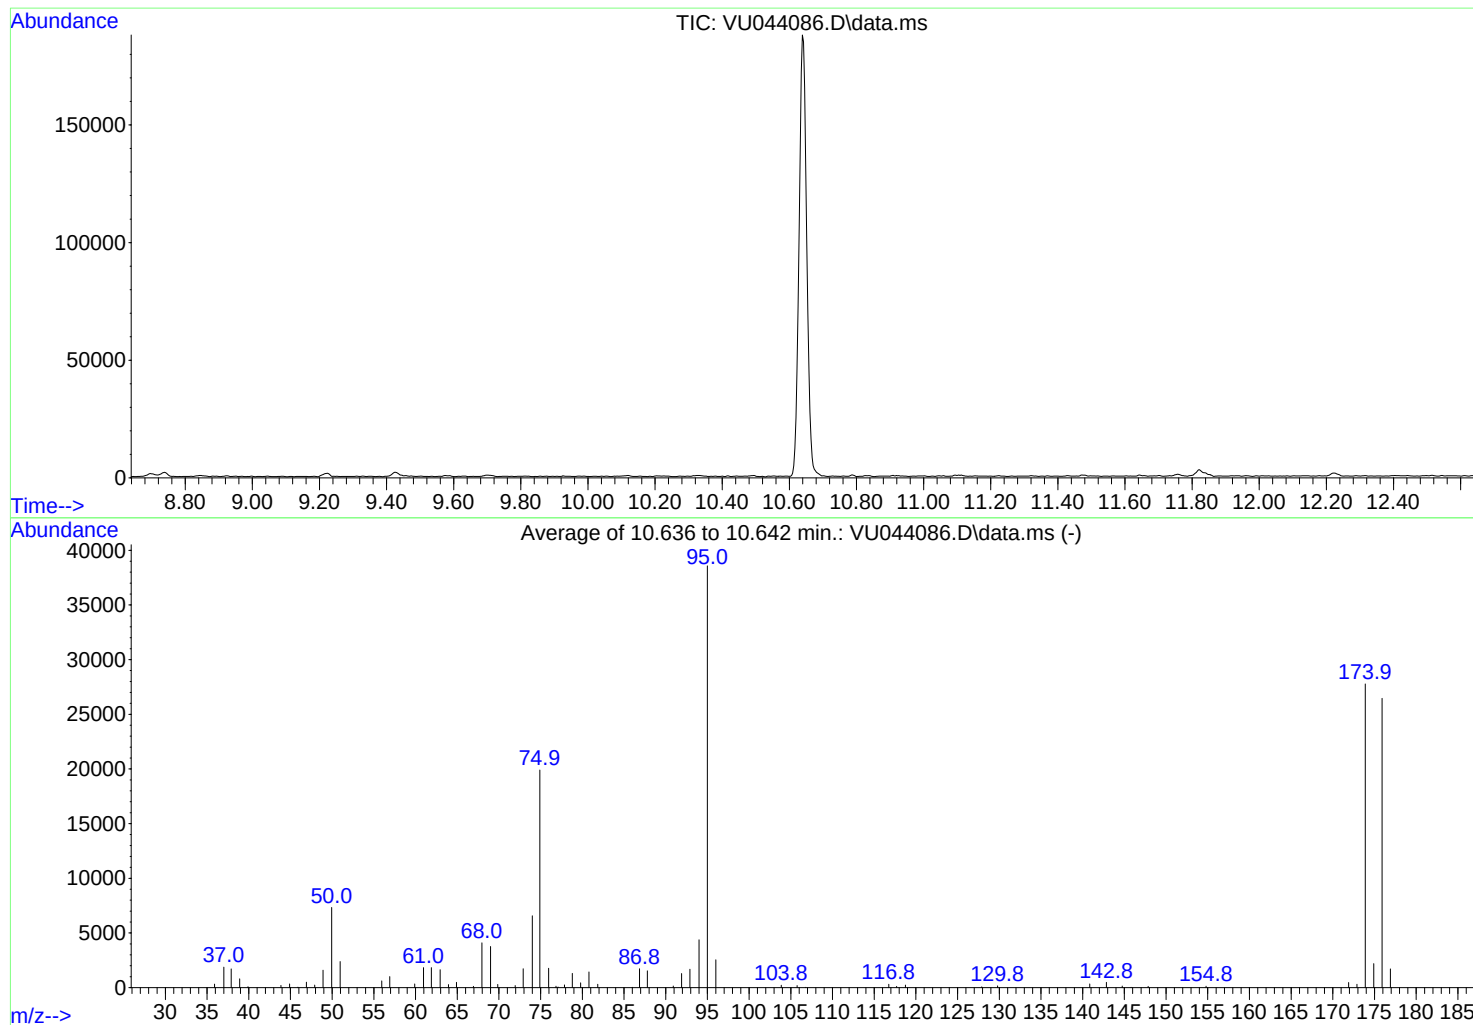

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	7328	PASS
75	95	30	60	51.6	19909	PASS
95	95	100	100	100.0	38579	PASS
96	95	5	9	6.6	2554	PASS
173	174	0.00	2	1.1	315	PASS
174	95	50	100	72.0	27781	PASS
175	174	5	9	7.9	2191	PASS
176	174	95	101	95.2	26459	PASS
177	176	5	9	6.5	1708	PASS