
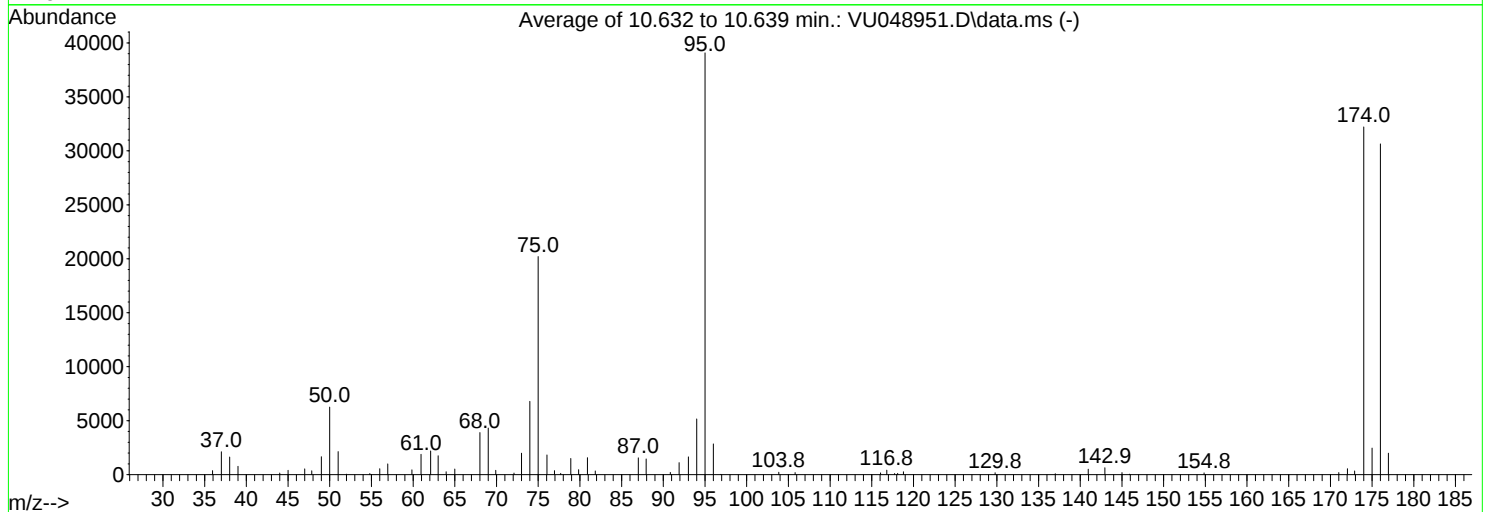


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060822\
 Data File : VU048951.D
 Acq On : 08 Jun 2022 08:58
 Operator : SY/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U052622W.M
 Title : SW846 8260
 Last Update : Fri May 27 06:42:31 2022

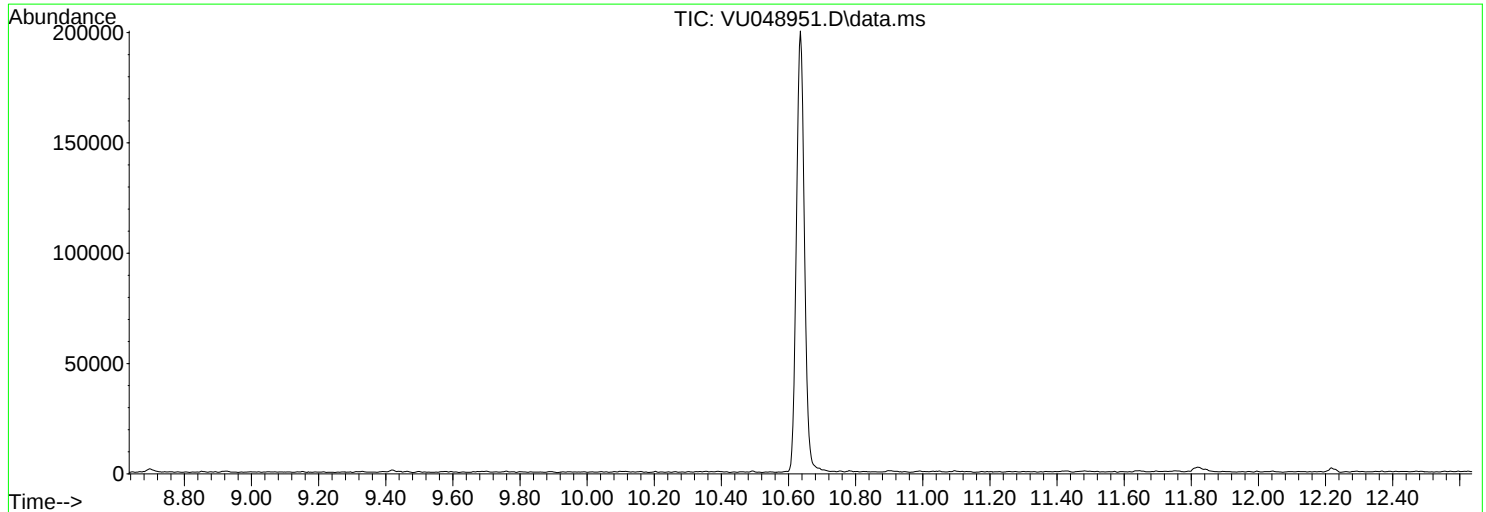

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	6258	PASS
75	95	30	60	51.7	20200	PASS
95	95	100	100	100.0	39080	PASS
96	95	5	9	7.3	2845	PASS
173	174	0.00	2	1.1	339	PASS
174	95	50	100	82.4	32216	PASS
175	174	5	9	7.6	2463	PASS
176	174	95	101	95.1	30640	PASS
177	176	5	9	6.5	1990	PASS