

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060823\
 Data File : VU054438.D
 Acq On : 08 Jun 2023 16:02
 Operator : MD/SY
 Sample : 03105-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0FD1

Quant Time: Jun 09 05:23:13 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jun 08 01:20:50 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	632614	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	589401	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	289236	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.599	65	77175	1.917	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	38.400%#
7) Chloroethane-d5	1.914	69	78033	2.070	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	41.400%#
11) 1,1-Dichloroethene-d2	2.563	65	36589	2.035	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	40.600%#
20) 2-Butanone-d5	4.628	46	286991	25.354	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	50.700%
24) Chloroform-d	5.059	84	185754	2.207	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	44.200%#
26) 1,2-Dichloroethane-d4	5.698	65	96330	2.348	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	47.000%#
32) Benzene-d6	5.724	84	364753	2.226	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	44.600%#
36) 1,2-Dichloropropane-d6	6.689	67	129823	2.373	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	47.400%#
41) Toluene-d8	7.894	98	320142	2.202	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	44.000%#
43) trans-1,3-Dichloroprop...	8.177	79	41320	2.172	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	43.400%#
46) 2-Hexanone-d5	8.631	63	193475	24.237	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	48.480%
56) 1,1,2,2-Tetrachloroeth...	10.750	84	98451	2.413	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	48.200%#
66) 1,2-Dichlorobenzene-d4	12.190	152	116802	2.394	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	47.800%#
Target Compounds					Qvalue	
37) 1,2-Dichloropropane	6.689	63	14171	0.247	ug/L	# 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060823\
Data File : VU054438.D
Acq On : 08 Jun 2023 16:02
Operator : MD/SY
Sample : 03105-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FD1

Quant Time: Jun 09 05:23:13 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jun 08 01:20:50 2023
Response via : Initial Calibration

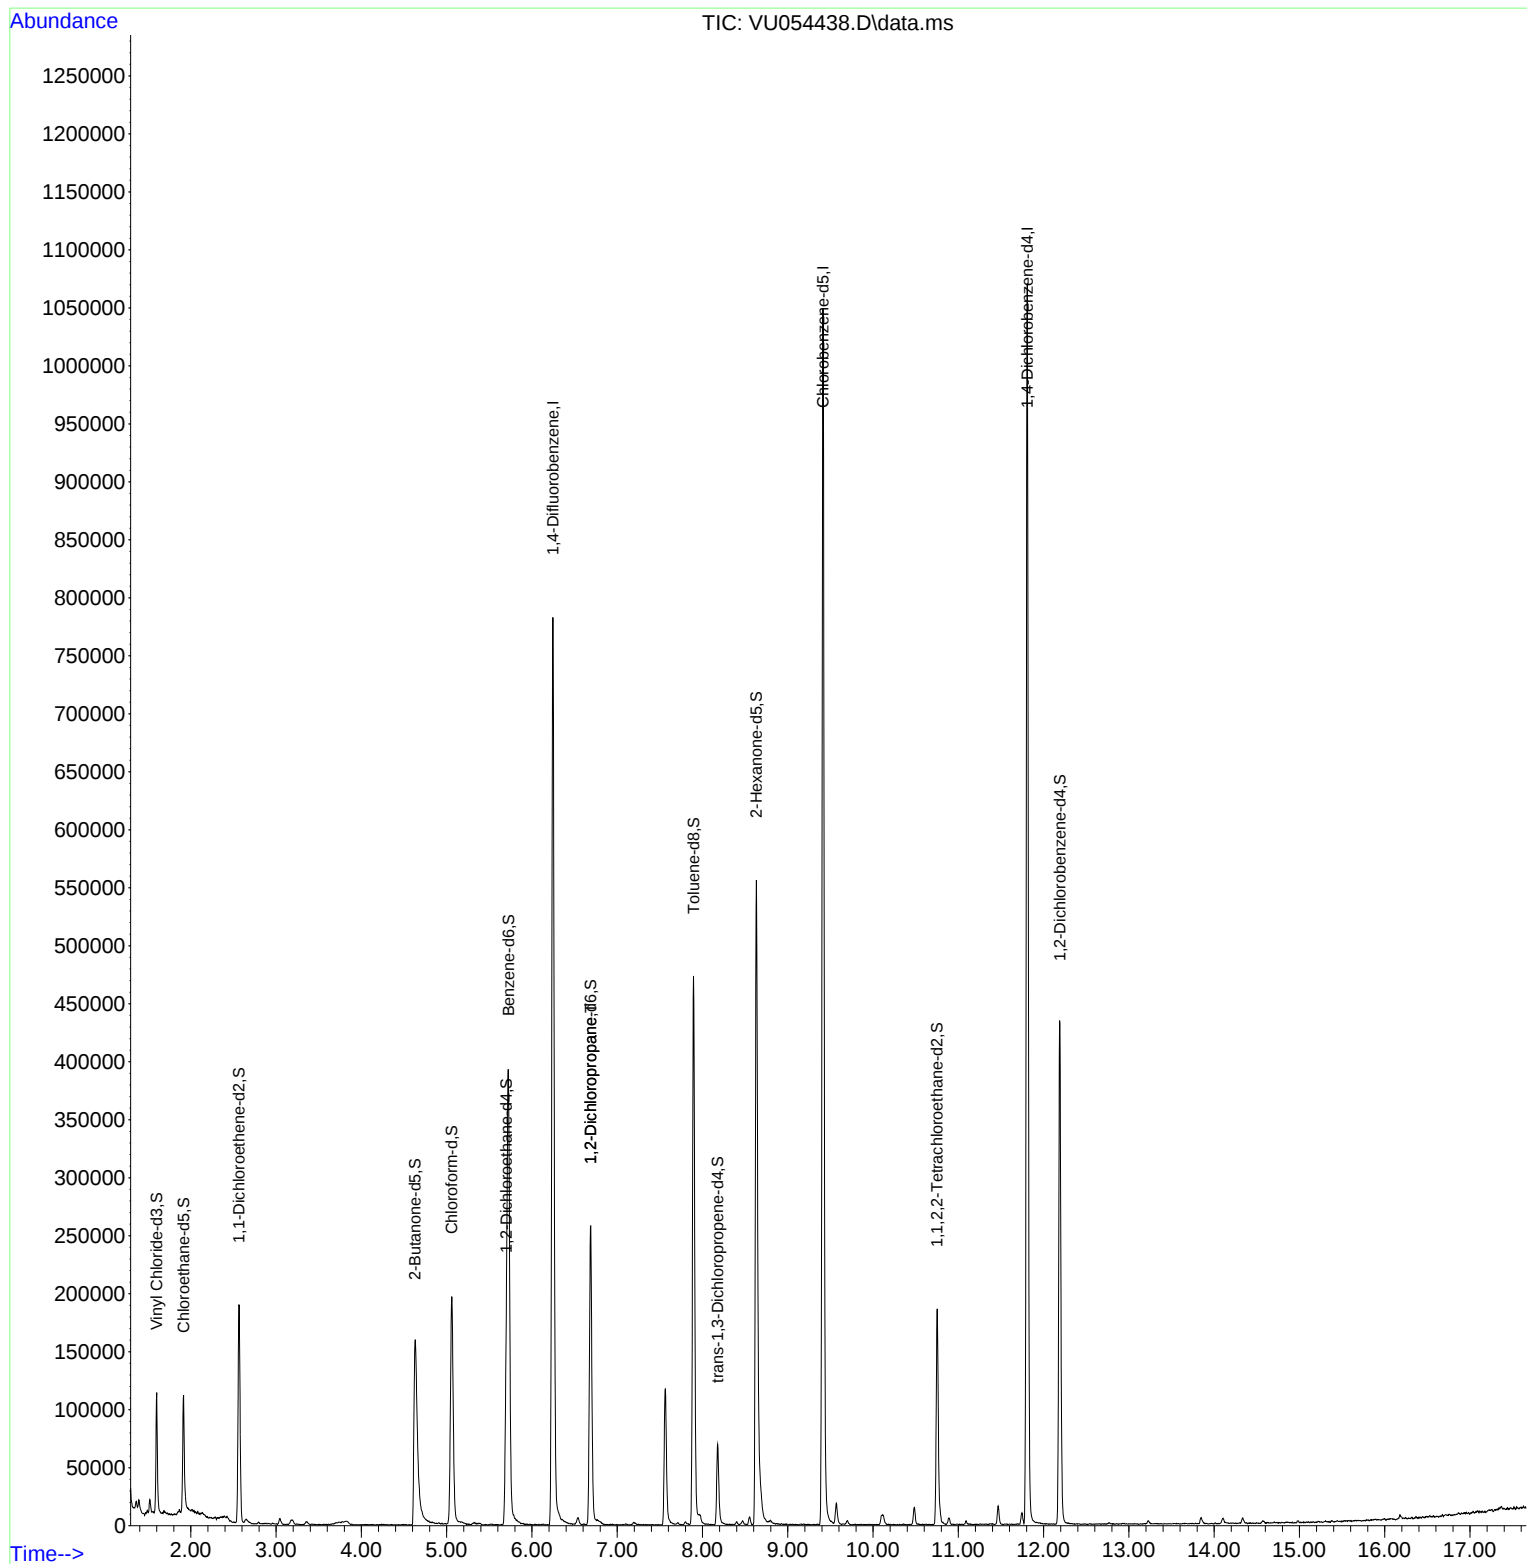

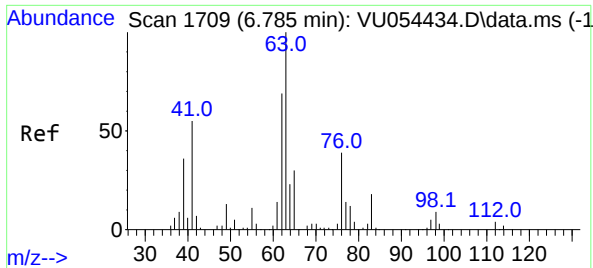

#37
1,2-Dichloropropane
Concen: 0.247 ug/L
RT: 6.689 min Scan# 1
Delta R.T. -0.096 min
Lab File: VU054438.D
Acq: 08 Jun 2023 16:02

Instrument :
MSVOA_U
ClientSampleId :
C0FD1

Tgt Ion: 63 Resp: 14171
Ion Ratio Lower Upper
63 100
112 0.6 3.0 4.6#

