

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060823\
 Data File : VU054438.D
 Acq On : 08 Jun 2023 16:02
 Operator : MD/SY
 Sample : 03105-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0FD1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054438.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	113	rVB	104194	126559	7.09%	1.103%
2	1.914	185	194	208	rBV	100681	142948	8.01%	1.245%
3	2.563	385	396	414	rVB	187773	306330	17.17%	2.669%
4	4.631	1027	1039	1079	rBV2	159510	472665	26.50%	4.118%
5	5.059	1152	1172	1194	rBV	196275	446480	25.03%	3.890%
6	5.721	1357	1378	1396	rBV2	392670	1017878	57.06%	8.868%
7	6.245	1525	1541	1571	rBV	782385	1520527	85.23%	13.247%
8	6.689	1663	1679	1700	rBV	257755	513817	28.80%	4.477%
9	7.563	1937	1951	1970	rBV	117586	216908	12.16%	1.890%
10	7.894	2038	2054	2071	rBV	472997	826647	46.34%	7.202%
11	8.177	2131	2142	2162	rBV	68952	125505	7.04%	1.093%
12	8.631	2271	2283	2322	rBV2	555524	1099268	61.62%	9.577%
13	9.412	2511	2526	2554	rBV	1048776	1783938	100.00%	15.542%
14	9.570	2565	2575	2594	rVB	18372	32402	1.82%	0.282%
15	10.483	2846	2859	2869	rBV3	14841	23854	1.34%	0.208%
16	10.753	2928	2943	2962	rBV	185768	322815	18.10%	2.812%
17	11.467	3150	3165	3179	rBV2	16020	25028	1.40%	0.218%
18	11.807	3259	3271	3302	rVV	1069142	1733237	97.16%	15.101%
19	12.187	3375	3389	3411	rBV	434191	741195	41.55%	6.458%




Sum of corrected areas: 11478001

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060823\
Data File : VU054438.D
Acq On : 08 Jun 2023 16:02
Operator : MD/SY
Sample : 03105-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

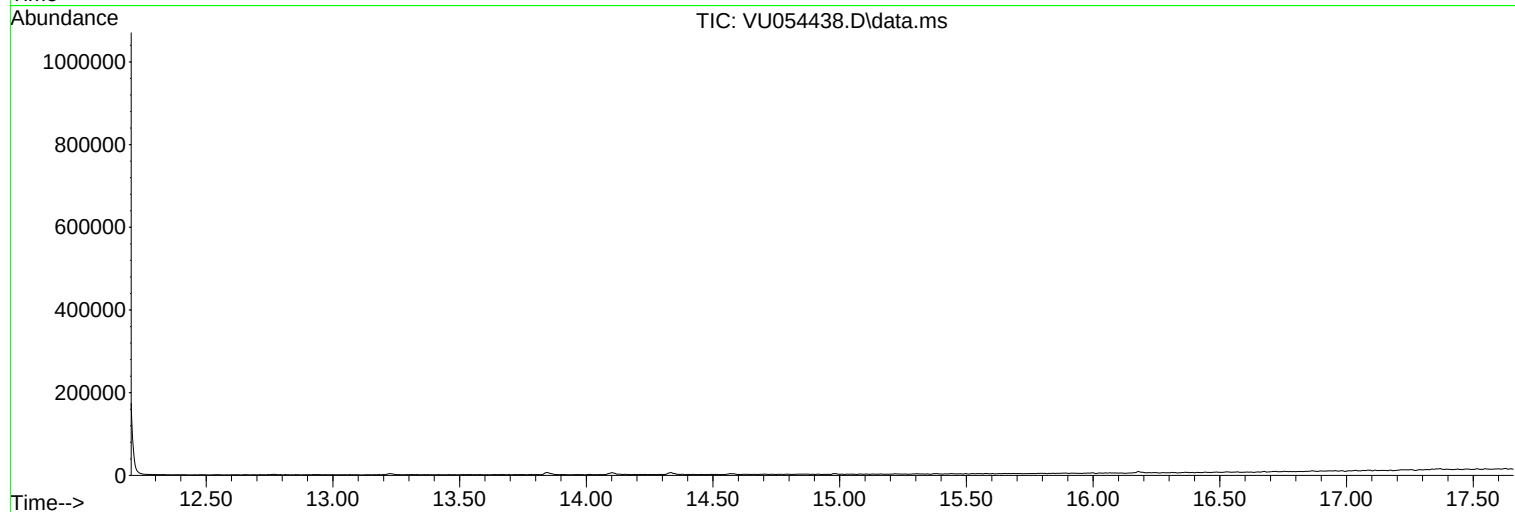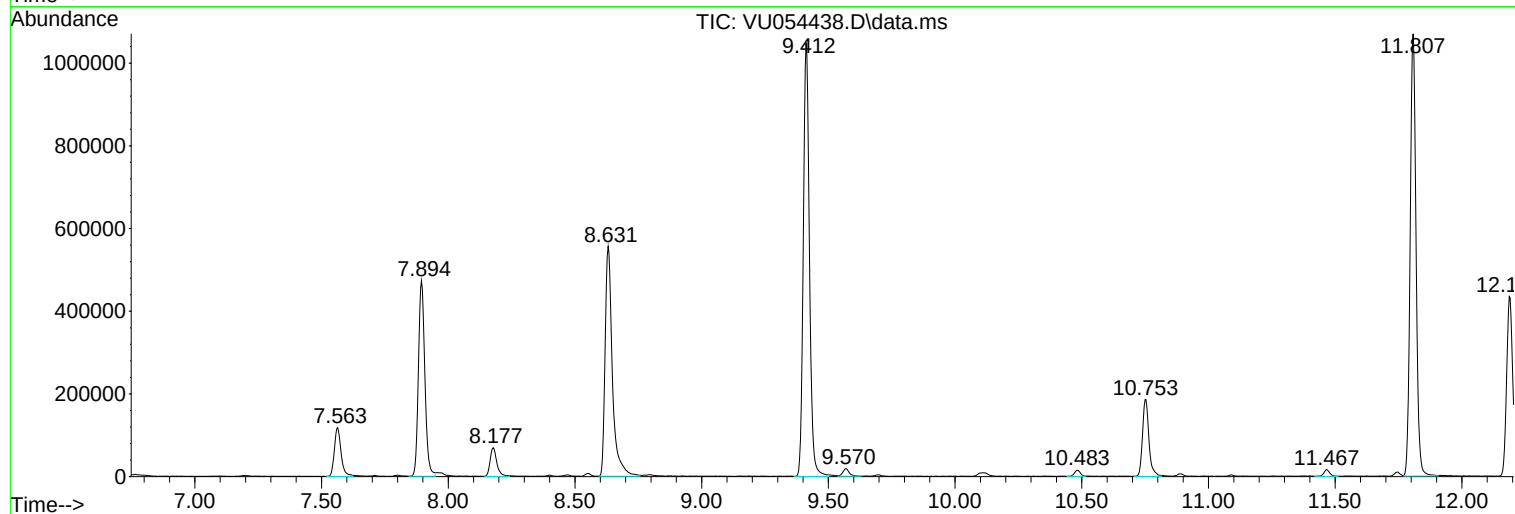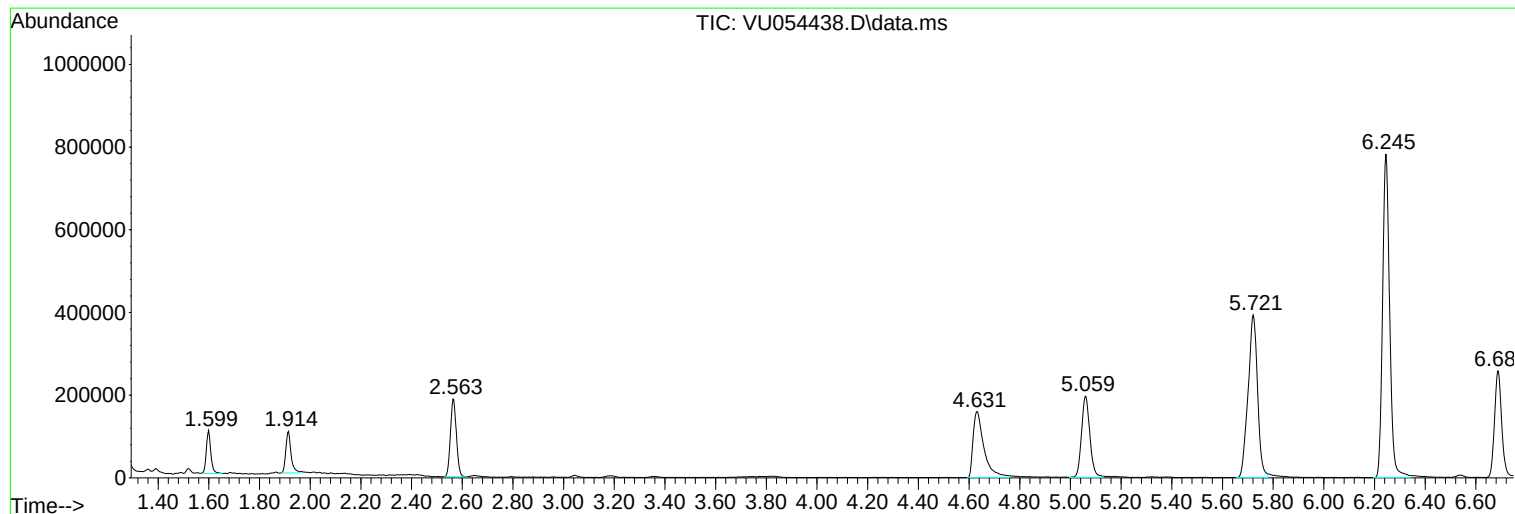

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060823\
Data File : VU054438.D
Acq On : 08 Jun 2023 16:02
Operator : MD/SY
Sample : 03105-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060823\
Data File : VU054438.D
Acq On : 08 Jun 2023 16:02
Operator : MD/SY
Sample : 03105-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc