

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060823\
 Data File : VU054441.D
 Acq On : 08 Jun 2023 17:14
 Operator : MD/SY
 Sample : 03105-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0FE0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054441.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.519	66	71	81	rVB	12579	14863	1.33%	0.167%
2	1.599	87	96	108	rVB	97223	120960	10.83%	1.357%
3	1.914	186	194	210	rBV	102257	142363	12.74%	1.598%
4	2.564	384	396	412	rBV2	184236	308933	27.66%	3.467%
5	4.631	1027	1039	1080	rBV	162557	515887	46.18%	5.790%
6	5.059	1158	1172	1199	rBV	204273	489878	43.86%	5.498%
7	5.721	1358	1378	1414	rBV2	396146	1040392	93.14%	11.676%
8	6.245	1525	1541	1564	rBV	364856	712430	63.78%	7.995%
9	6.686	1663	1678	1701	rBV	258022	510812	45.73%	5.733%
10	7.563	1938	1951	1973	rBV	115890	217366	19.46%	2.439%
11	7.895	2040	2054	2085	rBV	458667	829094	74.22%	9.305%
12	8.178	2129	2142	2163	rBV2	70564	125880	11.27%	1.413%
13	8.631	2271	2283	2321	rBV2	555236	1117012	100.00%	12.536%
14	9.412	2513	2526	2551	rBV	504808	859595	76.95%	9.647%
15	10.753	2930	2943	2963	rBV	188554	312168	27.95%	3.503%
16	10.888	2974	2985	2993	rBV2	7530	11644	1.04%	0.131%
17	11.808	3259	3271	3288	rBV	506260	820684	73.47%	9.210%
18	12.187	3377	3389	3417	rBV	450567	747269	66.90%	8.386%
19	13.853	3897	3907	3920	rBV9	6975	13291	1.19%	0.149%




Sum of corrected areas: 8910521

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060823\
Data File : VU054441.D
Acq On : 08 Jun 2023 17:14
Operator : MD/SY
Sample : 03105-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

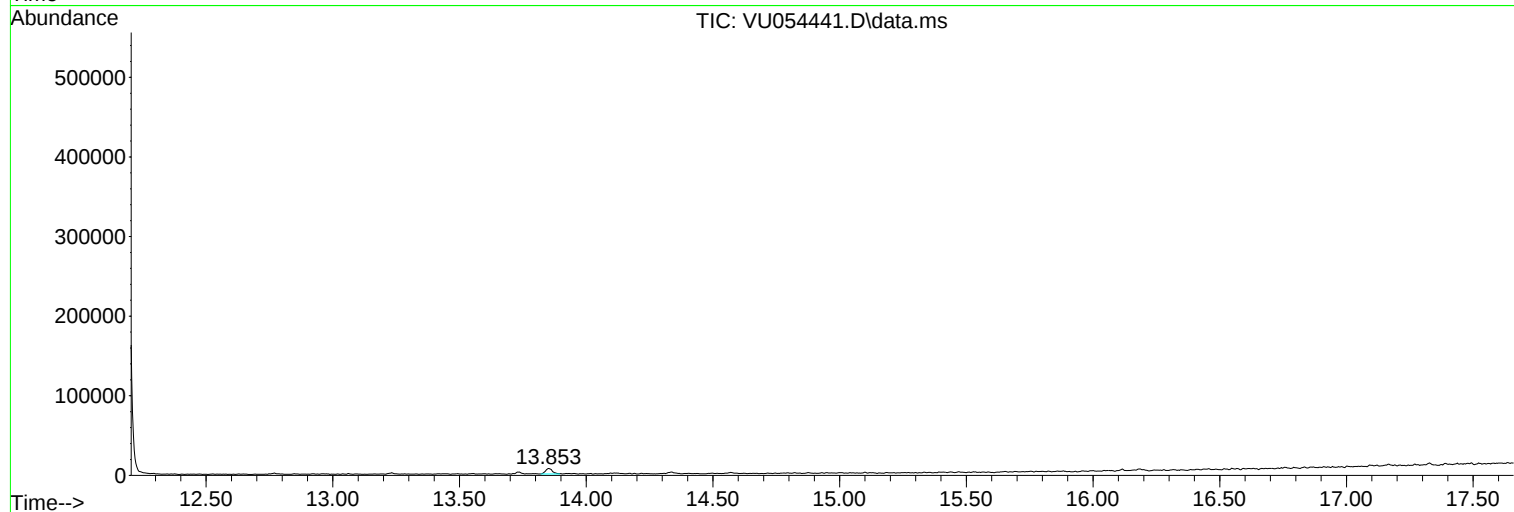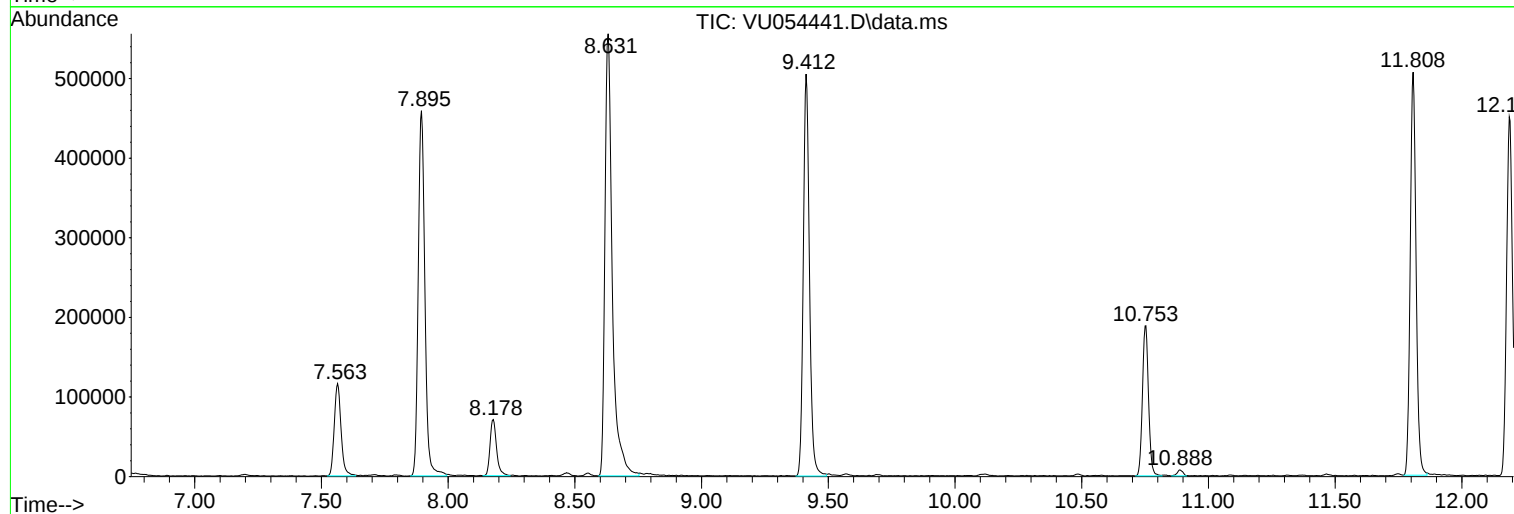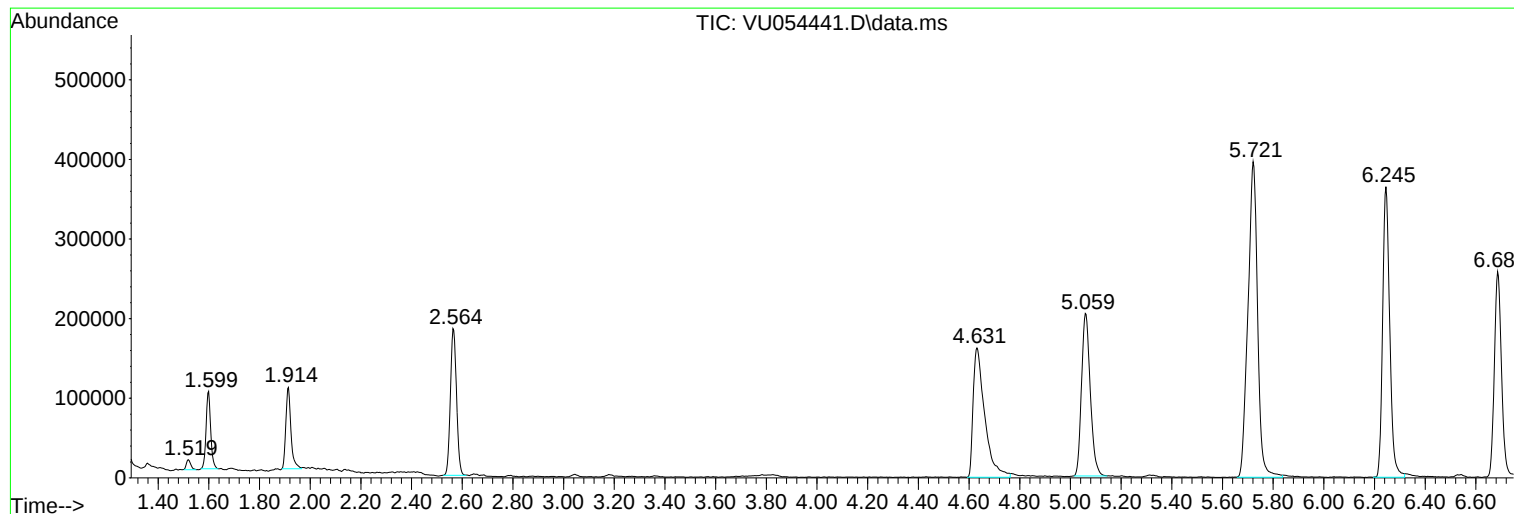

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060823\
Data File : VU054441.D
Acq On : 08 Jun 2023 17:14
Operator : MD/SY
Sample : 03105-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060823\
Data File : VU054441.D
Acq On : 08 Jun 2023 17:14
Operator : MD/SY
Sample : 03105-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
