

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060823\
 Data File : VU054443.D
 Acq On : 08 Jun 2023 18:03
 Operator : MD/SY
 Sample : 03105-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0FE6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054443.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.357	17	21	29	rVB3	12174	12752	1.15%	0.146%
2	1.518	65	71	81	rVB	18746	22093	1.99%	0.252%
3	1.599	86	96	108	rVV	95179	121490	10.93%	1.388%
4	1.914	186	194	208	rBV	93108	133106	11.98%	1.521%
5	2.563	385	396	412	rVB	172300	286058	25.74%	3.269%
6	2.792	456	467	483	rVB	16855	30694	2.76%	0.351%
7	3.187	575	590	602	rBV4	4449	11250	1.01%	0.129%
8	4.631	1027	1039	1071	rBV2	163906	464973	41.84%	5.313%
9	5.058	1156	1172	1193	rBV	195921	437338	39.35%	4.998%
10	5.721	1357	1378	1398	rBV2	387240	1012382	91.10%	11.569%
11	6.245	1528	1541	1569	rBV	379561	738001	66.41%	8.433%
12	6.685	1664	1678	1698	rBV	251885	503544	45.31%	5.754%
13	7.563	1938	1951	1976	rBV2	114429	213153	19.18%	2.436%
14	7.894	2038	2054	2075	rBV	447944	792270	71.29%	9.053%
15	8.177	2129	2142	2159	rBV2	69278	122900	11.06%	1.404%
16	8.630	2270	2283	2319	rBV2	546538	1111340	100.00%	12.699%
17	9.412	2514	2526	2550	rBV	504020	871477	78.42%	9.958%
18	10.753	2930	2943	2964	rBV	182994	305817	27.52%	3.495%
19	11.807	3258	3271	3295	rBV	518232	840290	75.61%	9.602%
20	12.190	3377	3390	3413	rBV	435090	720188	64.80%	8.230%




Sum of corrected areas: 8751116

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060823\
Data File : VU054443.D
Acq On : 08 Jun 2023 18:03
Operator : MD/SY
Sample : 03105-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FE6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

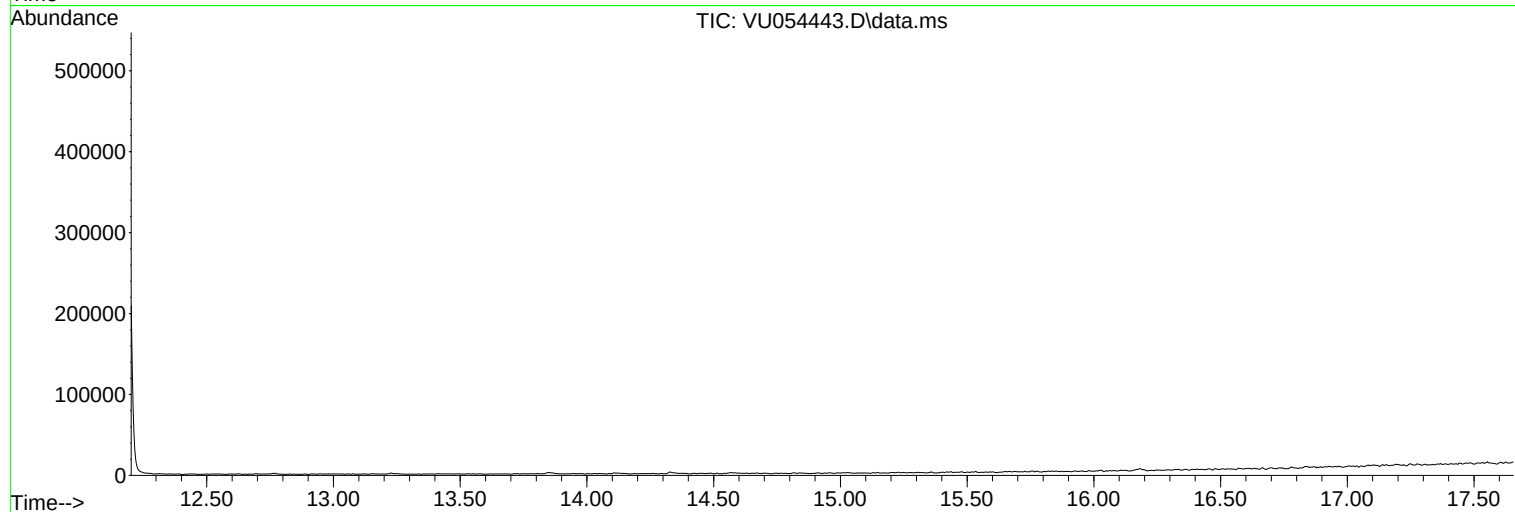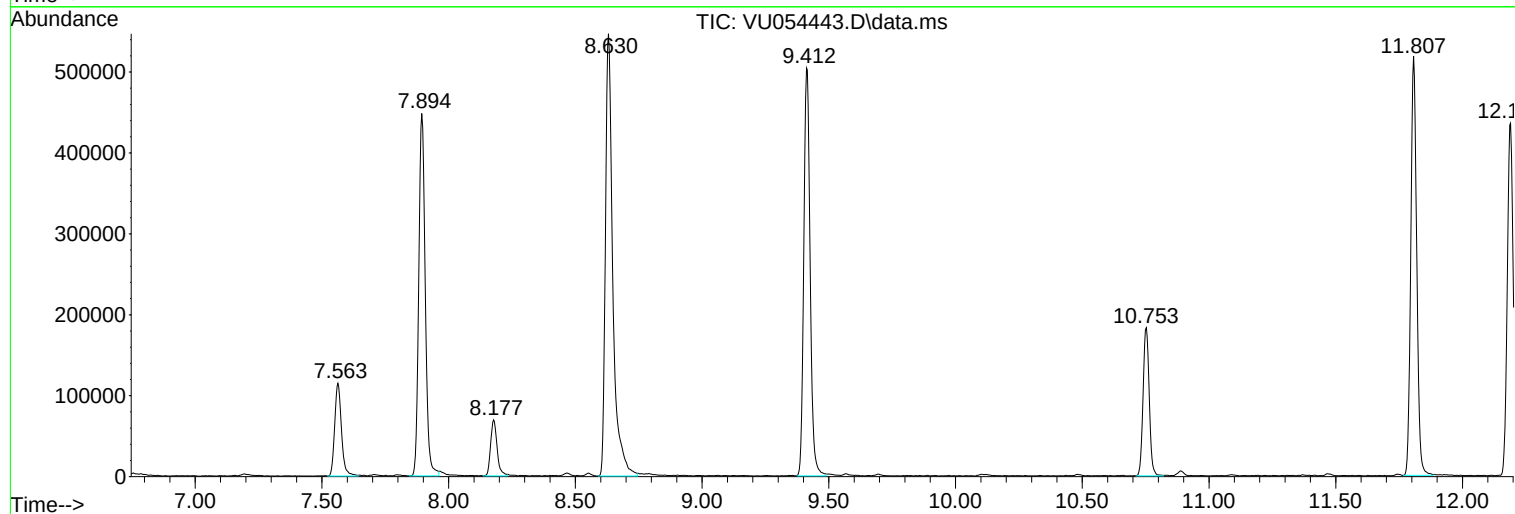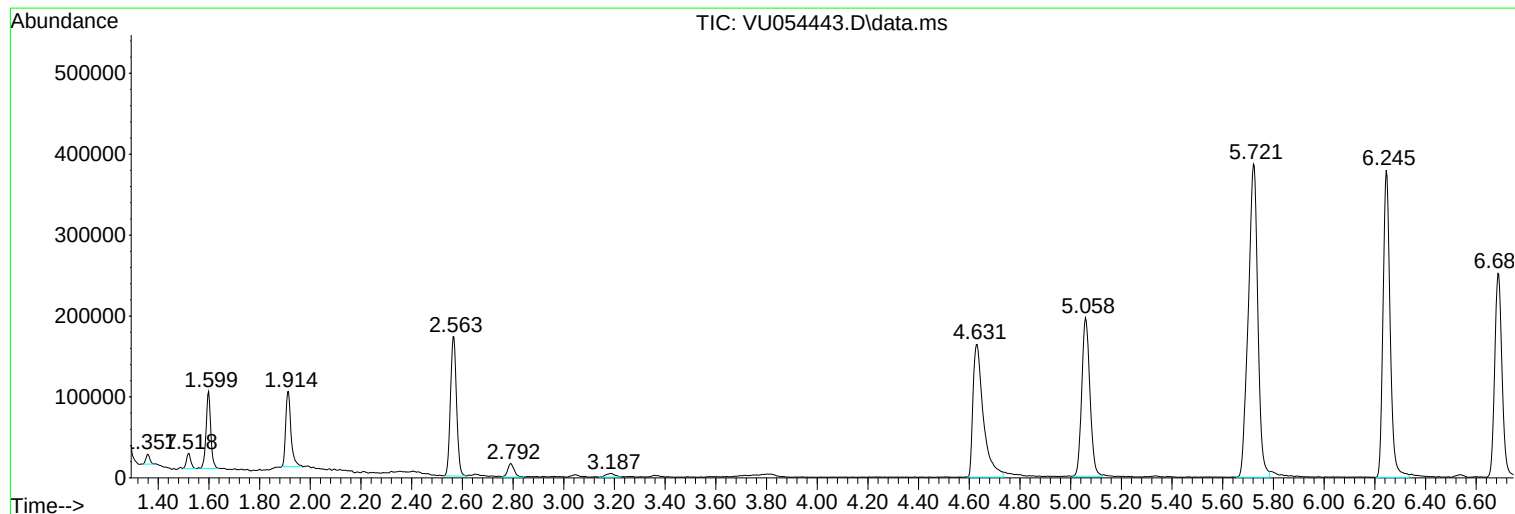

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060823\
Data File : VU054443.D
Acq On : 08 Jun 2023 18:03
Operator : MD/SY
Sample : 03105-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FE6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060823\
Data File : VU054443.D
Acq On : 08 Jun 2023 18:03
Operator : MD/SY
Sample : 03105-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0FE6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc