
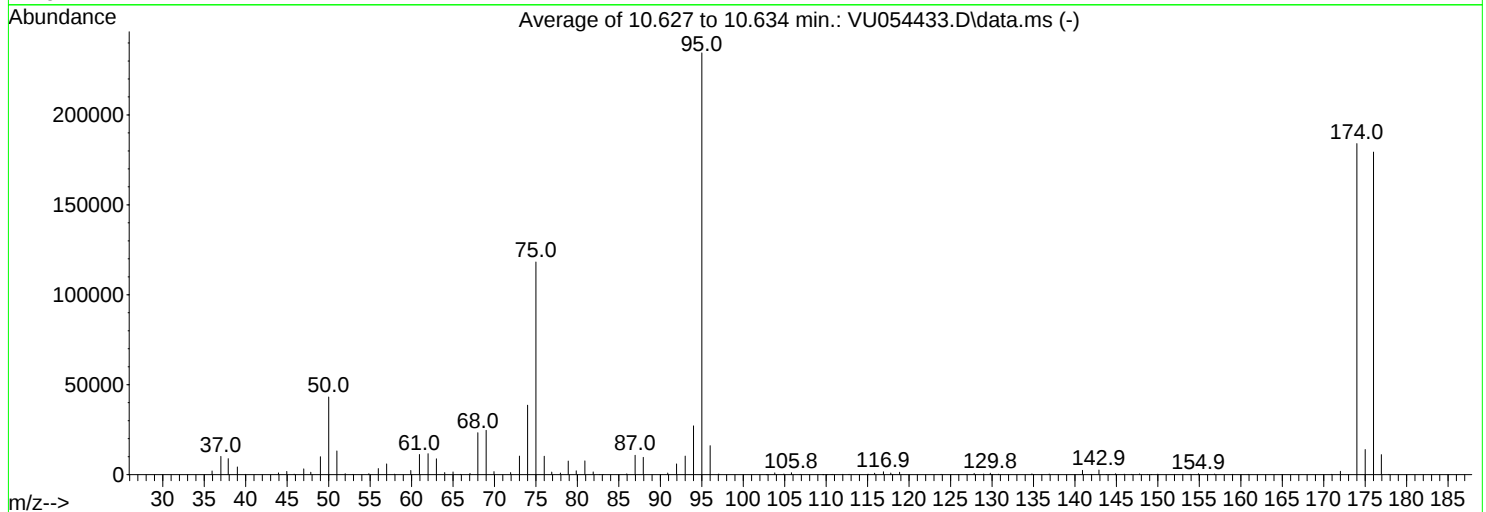


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060823\
 Data File : VU054433.D
 Acq On : 08 Jun 2023 08:40
 Operator : MD/SY
 Sample : BFB015
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB015

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Jun 08 01:20:50 2023

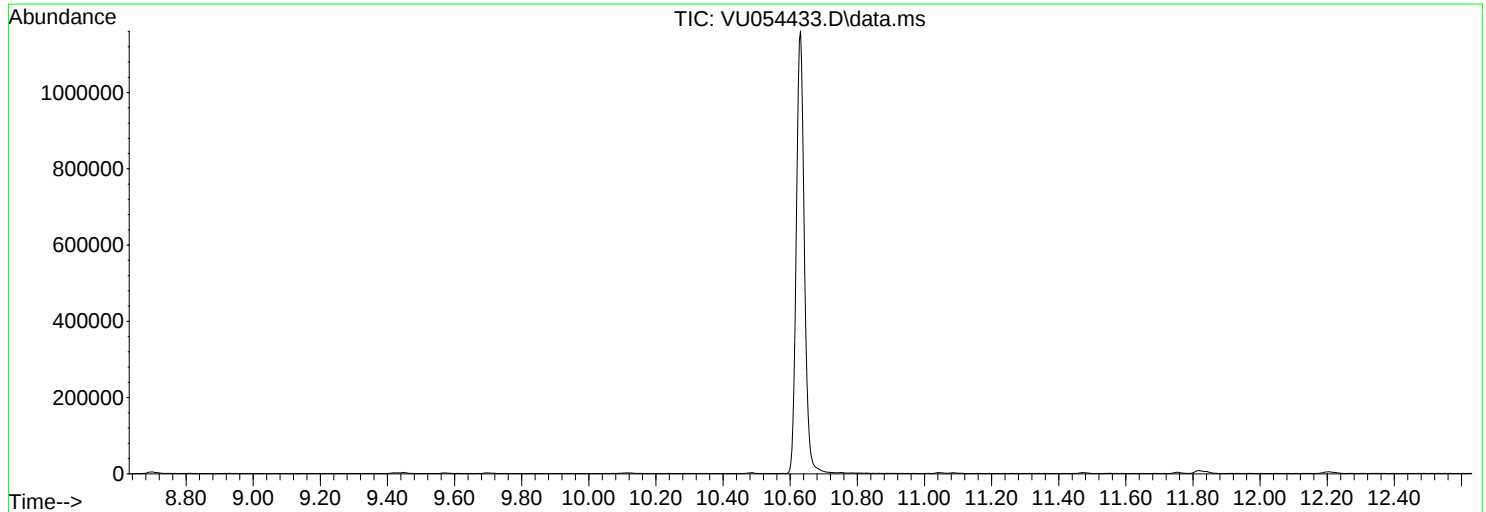

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	43125	PASS
75	95	30	80	50.4	118277	PASS
95	95	100	100	100.0	234517	PASS
96	95	5	9	6.9	16093	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.5	184021	PASS
175	174	5	9	7.6	13952	PASS
176	174	95	101	97.4	179328	PASS
177	176	5	9	6.2	11091	PASS

m/z	Abundance
39.90	194.0
41.00	145.0
42.80	106.0
43.90	710.0

Instrument :
MSVOA_U
ClientSampleId :
BFB015

m/z	Abundance
35.90	2206.0
37.00	10820.0
37.90	9100.0
39.00	4617.0
40.00	387.0
44.00	1766.0
44.90	1984.0
45.90	246.0
47.00	3530.0
47.90	1357.0
49.00	10281.0
50.00	45160.0
51.00	13745.0
52.00	628.0
53.00	208.0
54.90	633.0
56.00	3425.0
57.00	6057.0
57.90	292.0
59.90	2235.0
61.00	11174.0
62.00	11706.0
63.00	9000.0
64.00	1308.0
65.00	1550.0
65.90	229.0
67.10	726.0
68.00	23752.0
69.00	24904.0
69.90	1918.0
72.00	1154.0
73.00	10274.0
74.00	39144.0
75.00	121560.0
76.00	10477.0
76.90	1402.0
78.00	967.0
78.90	7629.0
79.80	2122.0
80.90	8173.0
81.90	1397.0
82.70	125.0
83.10	106.0
86.00	422.0
86.90	11287.0
87.90	9966.0
90.90	1066.0
92.00	6084.0
93.00	10219.0
94.00	27680.0
95.00	237504.0
96.00	16632.0
97.00	417.0
102.80	117.0
103.80	1028.0
104.90	378.0
105.80	1050.0
106.80	180.0
109.60	130.0
110.60	167.0
112.00	178.0
112.70	211.0
115.10	184.0
115.80	739.0
116.90	1618.0
117.80	961.0
118.80	1228.0
123.90	140.0
126.00	100.0
127.90	773.0
129.00	396.0
129.70	780.0
130.80	333.0
134.80	444.0
136.90	391.0
140.90	2471.0
142.00	347.0
142.90	2679.0
144.20	142.0
144.90	508.0
146.00	344.0
146.90	183.0
147.90	460.0
148.70	122.0
149.20	150.0
150.00	320.0
152.00	160.0
153.00	183.0
153.90	219.0
154.90	519.0
155.80	107.0
156.90	437.0

Instrument :
MSVOA_U
ClientSampleId :
BFB015

159.00	198.0
160.90	220.0
171.00	289.0
172.00	1866.0
174.00	183552.0
175.00	13910.0
176.00	175680.0
176.90	10833.0
177.90	238.0

Instrument :
MSVOA_U
ClientSampleId :
BFB015

m/z	Abundance
36.00	2075.0
37.00	10432.0
37.90	9320.0
39.00	4428.0
40.00	409.0
44.00	1759.0
44.90	1926.0
45.90	269.0
47.00	3290.0
47.90	1453.0
49.00	10379.0
50.00	44384.0
51.00	13573.0
52.00	595.0
53.00	209.0
54.90	564.0
56.00	3542.0
57.00	6227.0
57.90	253.0
59.90	2446.0
61.00	11565.0
62.00	12137.0
63.00	9145.0
64.00	1184.0
65.00	1519.0
65.90	182.0
67.00	784.0
68.00	24168.0
69.00	25528.0
70.00	1745.0
71.90	1225.0
73.00	10583.0
74.00	39640.0
75.00	121648.0
76.00	10420.0
76.90	1498.0
78.00	896.0
78.90	7854.0
79.80	2244.0
80.90	7853.0
81.90	1564.0
82.70	137.0
83.10	146.0
85.90	477.0
87.00	11025.0
88.00	9791.0
90.90	954.0
92.00	6061.0
93.00	10748.0
94.00	27704.0
95.00	241792.0
96.00	16704.0
97.00	377.0
103.80	1025.0
104.90	388.0
105.80	1091.0
106.80	218.0
110.80	190.0
112.00	149.0
112.70	239.0
115.10	262.0
115.90	818.0
116.90	1642.0
117.80	922.0
118.80	1407.0
123.80	154.0
126.00	104.0
126.90	148.0
127.90	782.0
129.00	372.0
129.80	727.0
130.80	290.0
134.80	423.0
136.90	376.0
140.00	111.0
140.90	2507.0
142.90	2715.0
144.10	166.0
144.90	516.0
146.00	326.0
146.80	184.0
147.80	467.0
148.70	151.0
149.20	150.0
150.00	280.0
152.00	192.0
153.00	158.0
153.90	238.0
154.90	545.0
155.80	152.0
156.90	399.0
159.00	226.0

Instrument :
MSVOA_U
ClientSampleId :
BFB015

160.90	230.0
170.90	229.0
172.00	1943.0
174.00	189504.0
175.00	14350.0
176.00	185472.0
176.90	11292.0
177.80	222.0

Instrument :
MSVOA_U
ClientSampleId :
BFB015

m/z	Abundance
36.00	1840.0
37.00	9075.0
37.90	8410.0
39.00	3750.0
40.00	361.0
44.00	1595.0
45.00	1576.0
45.80	224.0
47.00	2819.0
47.80	1299.0
49.00	9337.0
50.00	39832.0
51.00	12205.0
52.00	482.0
52.90	204.0
54.80	471.0
56.00	3260.0
57.00	5718.0
58.00	207.0
59.90	2268.0
60.90	10923.0
62.00	11204.0
63.00	8275.0
64.00	965.0
65.00	1386.0
66.00	126.0
67.00	721.0
68.00	21984.0
69.00	23616.0
70.00	1504.0
71.90	1214.0
73.00	10114.0
74.00	37072.0
75.00	111624.0
76.00	9847.0
76.90	1447.0
77.90	784.0
78.90	7162.0
79.90	2067.0
80.90	6887.0
81.90	1584.0
82.70	140.0
83.10	146.0
85.90	447.0
87.00	9922.0
88.00	9164.0
90.90	786.0
91.90	5711.0
93.00	10053.0
94.00	26016.0
95.00	224256.0
96.00	14943.0
97.10	340.0
103.80	978.0
104.90	333.0
105.80	1181.0
106.90	207.0
110.00	141.0
110.80	260.0
112.00	107.0
112.80	178.0
114.90	261.0
115.90	769.0
116.90	1613.0
117.80	816.0
118.90	1419.0
123.80	144.0
125.90	114.0
126.90	150.0
127.80	714.0
129.00	297.0
129.90	780.0
130.80	280.0
134.80	375.0
136.90	337.0
140.00	117.0
140.90	2207.0
141.90	224.0
142.90	2418.0
143.80	151.0
144.90	481.0
145.90	280.0
146.80	157.0
147.70	462.0
148.80	142.0
149.90	184.0
152.00	139.0
152.80	121.0
153.10	112.0
153.90	220.0
154.90	497.0
155.80	152.0

Instrument :
MSVOA_U
ClientSampleId :
BFB015

156.80	370.0
159.00	198.0
160.90	238.0
170.90	172.0
172.00	1800.0
174.00	179008.0
175.00	13595.0
176.00	176832.0
177.00	11149.0
177.90	215.0

Instrument :
MSVOA_U
ClientSampleId :
BFB015