

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060920\
 Data File : VU038683.D
 Acq On : 08 Jun 2020 21:48
 Operator : SY/MD
 Sample : L2896-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETW44

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	78	85	97	rVB	292351	323893	10.54%	1.481%
2	1.932	176	184	197	rVB	211695	273601	8.90%	1.251%
3	2.594	378	390	422	rVB	494312	844426	27.47%	3.861%
4	3.018	520	522	525	rVB	688	336	0.01%	0.002%
5	3.038	525	528	529	rBV	463	266	0.01%	0.001%
6	3.070	534	538	545	rVV7	905	1222	0.04%	0.006%
7	3.282	601	604	605	rBV	346	155	0.01%	0.001%
8	3.388	626	637	649	rBV3	12626	24841	0.81%	0.114%
9	3.481	664	666	669	rBV2	358	175	0.01%	0.001%
10	3.587	698	699	700	rBV2	224	71	0.00%	0.000%
11	3.668	723	724	726	rVB	548	184	0.01%	0.001%
12	3.690	726	731	733	rBV2	425	409	0.01%	0.002%
13	3.732	742	744	746	rBV	221	71	0.00%	0.000%
14	3.857	774	783	789	rBV4	657	1004	0.03%	0.005%
15	3.896	793	795	796	rBV	453	160	0.01%	0.001%
16	4.031	826	837	839	rBV6	720	990	0.03%	0.005%
17	4.083	850	853	856	rBV2	231	163	0.01%	0.001%
18	4.105	856	860	864	rVV2	277	205	0.01%	0.001%
19	4.140	869	871	874	rVV2	503	229	0.01%	0.001%
20	4.160	874	877	880	rVB2	286	189	0.01%	0.001%
21	4.211	891	893	895	rBV	120	79	0.00%	0.000%
22	4.263	904	909	912	rBV2	207	205	0.01%	0.001%
23	4.282	912	915	918	rVV2	201	120	0.00%	0.001%
24	4.298	918	920	922	rBV2	161	84	0.00%	0.000%
25	4.346	933	935	940	rVB3	195	128	0.00%	0.001%
26	4.372	940	943	945	rBV	334	247	0.01%	0.001%
27	4.404	949	953	956	rBV3	404	327	0.01%	0.001%
28	4.449	964	967	969	rBV	165	92	0.00%	0.000%
29	4.494	978	981	982	rBV2	202	117	0.00%	0.001%
30	4.507	982	985	994	rVV4	342	406	0.01%	0.002%
31	4.549	995	998	1003	rVB2	518	396	0.01%	0.002%
32	4.578	1003	1007	1010	rBV3	372	339	0.01%	0.002%
33	4.706	1018	1047	1076	rBV2	1139393	3073613	100.00%	14.052%
34	5.102	1153	1170	1192	rBV	388985	851014	27.69%	3.891%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060920\
 Data File : VU038683.D
 Acq On : 08 Jun 2020 21:48
 Operator : SY/MD
 Sample : L2896-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETW44

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis

35	5.391	1255	1260	1261	rBV2	599	481	0.02%	0.002%
36	5.439	1274	1275	1276	rBV2	270	56	0.00%	0.000%
37	5.449	1276	1278	1281	rBV	339	200	0.01%	0.001%
38	5.488	1288	1290	1292	rBV	226	93	0.00%	0.000%
39	5.513	1294	1298	1302	rBV3	274	243	0.01%	0.001%
40	5.574	1315	1317	1319	rBV	256	111	0.00%	0.001%
41	5.626	1331	1333	1335	rBV	199	66	0.00%	0.000%
42	5.681	1346	1350	1352	rBV	342	243	0.01%	0.001%
43	5.758	1352	1374	1408	rBV2	832105	2237091	72.78%	10.228%
44	6.147	1489	1495	1498	rBV3	1193	1175	0.04%	0.005%
45	6.279	1521	1536	1568	rBV	677220	1310021	42.62%	5.989%
46	6.571	1611	1627	1647	rBV	574260	1091136	35.50%	4.988%
47	6.719	1659	1673	1692	rBV	493382	962471	31.31%	4.400%
48	6.976	1752	1753	1754	rBV	338	119	0.00%	0.001%
49	7.008	1761	1763	1765	rVB2	293	88	0.00%	0.000%
50	7.041	1771	1773	1775	rVB3	329	133	0.00%	0.001%
51	7.099	1786	1791	1793	rVB	352	222	0.01%	0.001%
52	7.118	1795	1797	1799	rVB	133	36	0.00%	0.000%
53	7.169	1808	1813	1815	rBV2	377	379	0.01%	0.002%
54	7.185	1815	1818	1819	rBV2	573	253	0.01%	0.001%
55	7.198	1820	1822	1825	rBV4	741	595	0.02%	0.003%
56	7.237	1832	1834	1835	rBV2	227	64	0.00%	0.000%
57	7.272	1843	1845	1847	rBV	340	186	0.01%	0.001%
58	7.320	1857	1860	1862	rBV2	444	269	0.01%	0.001%
59	7.365	1870	1874	1877	rBV	416	290	0.01%	0.001%
60	7.410	1884	1888	1894	rBV2	400	372	0.01%	0.002%
61	7.443	1894	1898	1901	rBV2	353	320	0.01%	0.001%
62	7.484	1908	1911	1915	rBV2	432	281	0.01%	0.001%
63	7.539	1925	1928	1930	rBV	179	110	0.00%	0.001%
64	7.590	1930	1944	1962	rBV	278321	490371	15.95%	2.242%
65	7.803	2006	2010	2014	rBV3	335	253	0.01%	0.001%
66	7.851	2022	2025	2027	rBV	243	163	0.01%	0.001%
67	7.864	2027	2029	2032	rBV2	324	245	0.01%	0.001%
68	7.922	2032	2047	2087	rBV	990790	1790668	58.26%	8.187%
69	8.140	2111	2115	2117	rBV2	303	215	0.01%	0.001%
70	8.153	2117	2119	2121	rBV2	206	140	0.00%	0.001%
71	8.201	2121	2134	2152	rBV	196011	338798	11.02%	1.549%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060920\
 Data File : VU038683.D
 Acq On : 08 Jun 2020 21:48
 Operator : SY/MD
 Sample : L2896-05
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 ETW44

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis

72	8.439	2206	2208	2209	rBV	197	92	0.00%	0.000%
73	8.491	2216	2224	2234	rVB4	4270	6939	0.23%	0.032%
74	8.574	2236	2250	2263	rBV2	587564	1010569	32.88%	4.620%
75	8.655	2264	2275	2311	rVB	738802	1326768	43.17%	6.066%
76	8.896	2346	2350	2353	rVB4	397	264	0.01%	0.001%
77	8.938	2358	2363	2366	rBV2	653	679	0.02%	0.003%
78	9.057	2397	2400	2401	rBV	322	175	0.01%	0.001%
79	9.118	2417	2419	2420	rBV	195	80	0.00%	0.000%
80	9.127	2420	2422	2425	rVB	362	147	0.00%	0.001%
81	9.275	2466	2468	2471	rBV2	452	181	0.01%	0.001%
82	9.359	2490	2494	2496	rBV2	334	251	0.01%	0.001%
83	9.375	2496	2499	2504	rVV3	429	424	0.01%	0.002%
84	9.436	2504	2518	2554	rVV	946177	1634135	53.17%	7.471%
85	9.822	2635	2638	2639	rBV	273	132	0.00%	0.001%
86	10.288	2780	2783	2788	rVB	397	311	0.01%	0.001%
87	10.487	2843	2845	2846	rBV	412	169	0.01%	0.001%
88	10.600	2878	2880	2883	rBV2	263	115	0.00%	0.001%
89	10.770	2918	2933	2949	rBV	657934	1070828	34.84%	4.896%
90	10.899	2967	2973	2983	rVB4	3306	5059	0.16%	0.023%
91	10.957	2989	2991	2992	rBV4	309	168	0.01%	0.001%
92	11.211	3068	3070	3073	rBV2	295	161	0.01%	0.001%
93	11.317	3100	3103	3104	rBV2	188	106	0.00%	0.000%
94	11.417	3132	3134	3135	rBV	376	144	0.00%	0.001%
95	11.577	3182	3184	3189	rVB2	421	297	0.01%	0.001%
96	11.822	3247	3260	3277	rBV	977994	1549479	50.41%	7.084%
97	12.082	3333	3341	3353	rVB3	5905	10984	0.36%	0.050%
98	12.204	3366	3379	3396	rBV	1006948	1619937	52.70%	7.406%
99	14.114	3967	3973	3982	rVB3	4488	6975	0.23%	0.032%


Sum of corrected areas: 21873283

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU060920\
Data File : VU038683.D
Acq On : 08 Jun 2020 21:48
Operator : SY/MD
Sample : L2896-05
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETW44

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

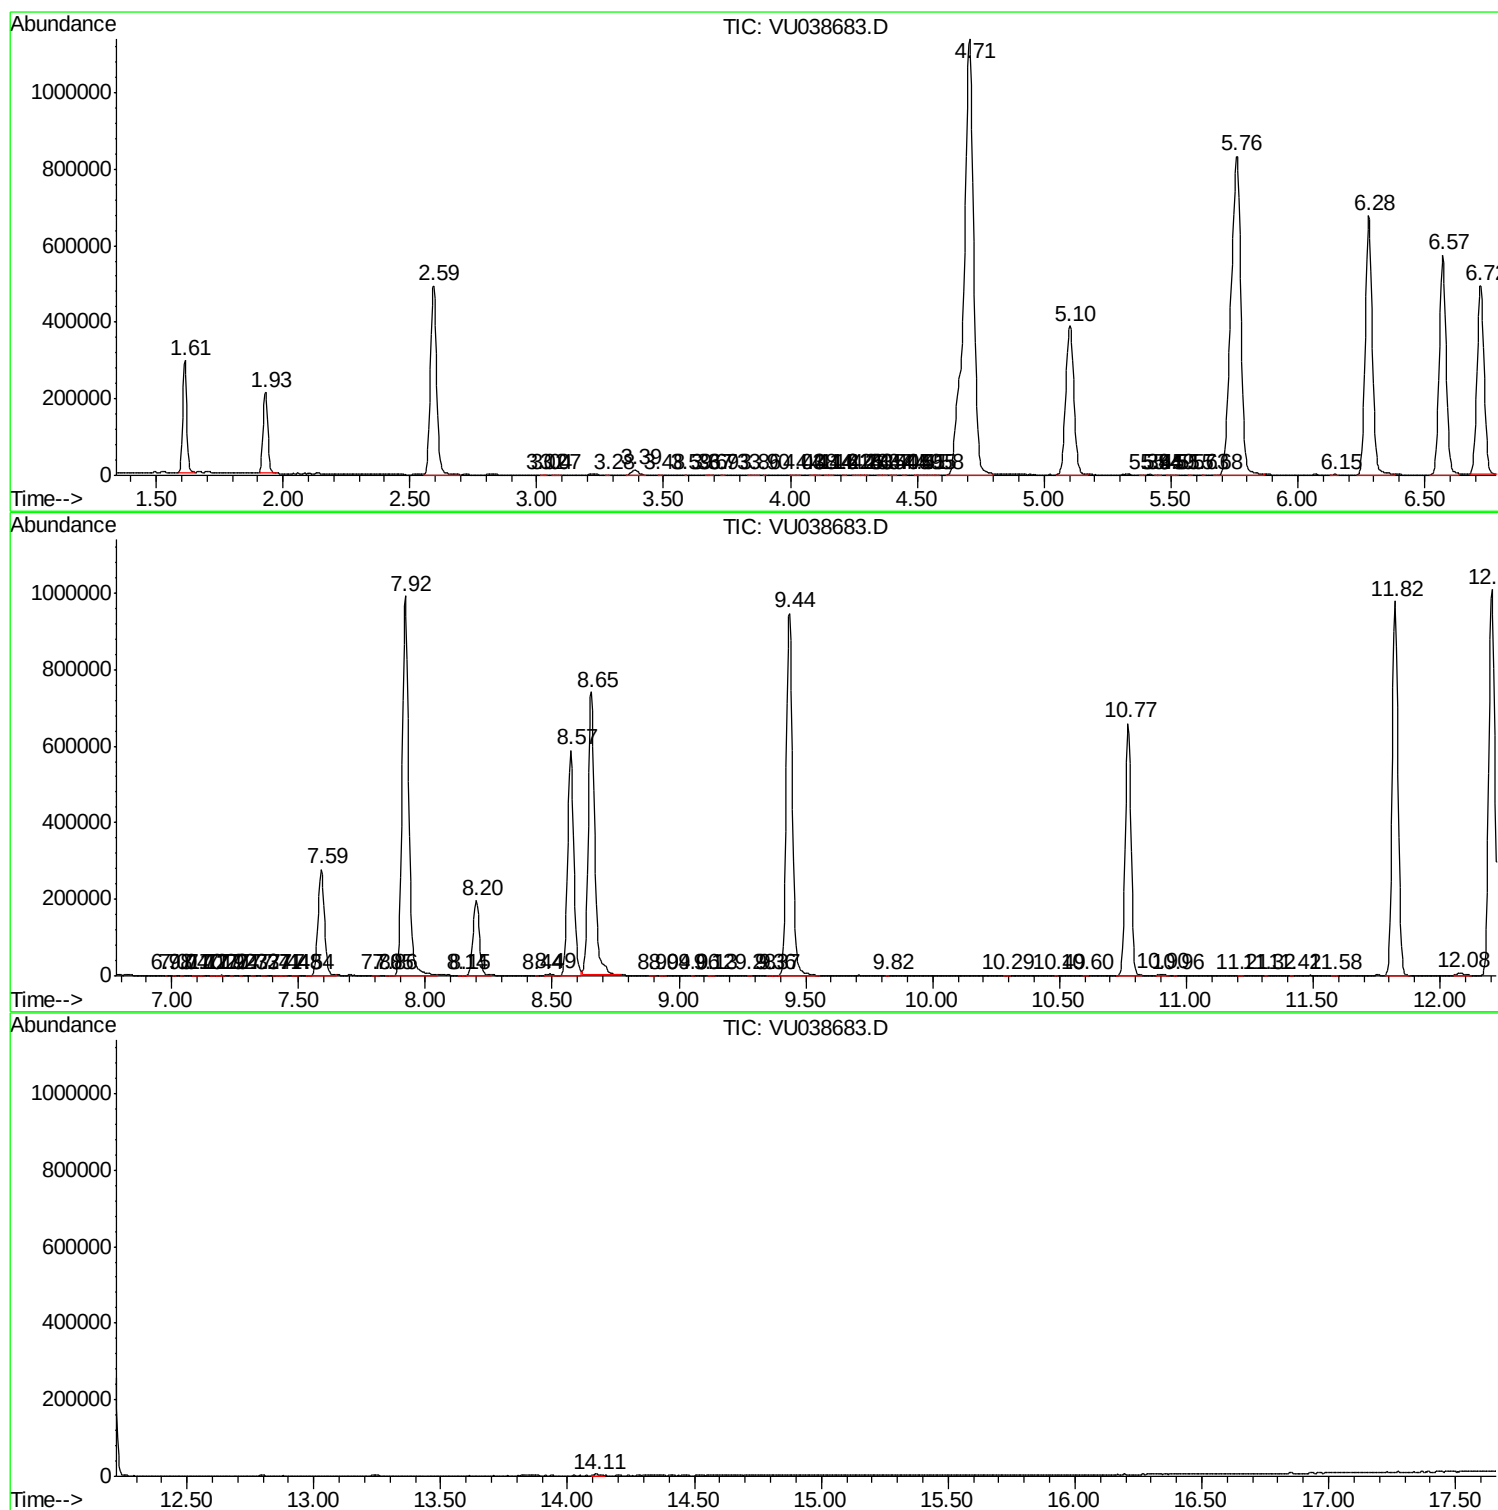

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU060920\
Data File : VU038683.D
Acq On : 08 Jun 2020 21:48
Operator : SY/MD
Sample : L2896-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETW44

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU060920\
Data File : VU038683.D
Acq On : 08 Jun 2020 21:48
Operator : SY/MD
Sample : L2896-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
ETW44

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc