

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060920\
 Data File : VU038714.D
 Acq On : 09 Jun 2020 11:24
 Operator : SY/MD
 Sample : L2913-14
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9E56

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	77	85	94	rBV	307129	334747	13.71%	1.718%
2	1.928	175	183	196	rVB	227349	295130	12.09%	1.514%
3	2.591	377	389	402	rBV	544573	889357	36.43%	4.563%
4	2.787	439	450	467	rBV	21376	42042	1.72%	0.216%
5	3.263	596	598	600	rBV	356	218	0.01%	0.001%
6	3.282	603	604	606	rVB	446	98	0.00%	0.001%
7	3.359	624	628	630	rBV2	294	264	0.01%	0.001%
8	3.391	636	638	640	rBV2	605	367	0.02%	0.002%
9	3.613	705	707	709	rVB2	268	61	0.00%	0.000%
10	3.633	711	713	715	rVB	602	157	0.01%	0.001%
11	3.645	715	717	719	rBV	150	83	0.00%	0.000%
12	3.835	774	776	779	rBV	262	153	0.01%	0.001%
13	3.864	782	785	787	rBV	309	207	0.01%	0.001%
14	4.018	830	833	837	rVB2	347	196	0.01%	0.001%
15	4.134	867	869	872	rVB	316	147	0.01%	0.001%
16	4.153	872	875	877	rBV	446	261	0.01%	0.001%
17	4.211	891	893	894	rBV	294	134	0.01%	0.001%
18	4.276	911	913	916	rVB	303	104	0.00%	0.001%
19	4.317	922	926	929	rBV2	394	324	0.01%	0.002%
20	4.346	933	935	938	rVB	349	237	0.01%	0.001%
21	4.385	945	947	948	rBV	132	57	0.00%	0.000%
22	4.395	948	950	951	rBV	197	86	0.00%	0.000%
23	4.475	973	975	977	rBV	193	91	0.00%	0.000%
24	4.501	980	983	990	rBV4	297	369	0.02%	0.002%
25	4.658	1016	1032	1067	rBV	261221	653061	26.75%	3.351%
26	4.845	1081	1090	1110	rVB2	20484	44917	1.84%	0.230%
27	4.954	1121	1124	1126	rBV3	410	228	0.01%	0.001%
28	5.044	1149	1152	1153	rBV2	443	266	0.01%	0.001%
29	5.102	1153	1170	1193	rVV	430643	934523	38.28%	4.795%
30	5.224	1206	1208	1212	rBV3	754	487	0.02%	0.002%
31	5.366	1251	1252	1254	rVB	293	95	0.00%	0.000%
32	5.417	1254	1268	1270	rBV7	5392	8185	0.34%	0.042%
33	5.465	1281	1283	1288	rBV3	425	359	0.01%	0.002%
34	5.494	1290	1292	1295	rVB	223	132	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060920\
 Data File : VU038714.D
 Acq On : 09 Jun 2020 11:24
 Operator : SY/MD
 Sample : L2913-14
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9E56

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis

35	5.510	1295	1297	1298	rBV	183	75	0.00%	0.000%
36	5.523	1298	1301	1306	rVB2	494	399	0.02%	0.002%
37	5.546	1306	1308	1310	rBV2	177	111	0.00%	0.001%
38	5.555	1310	1311	1314	rVB	221	55	0.00%	0.000%
39	5.575	1314	1317	1318	rBV	463	271	0.01%	0.001%
40	5.616	1327	1330	1336	rBV2	358	258	0.01%	0.001%
41	5.761	1351	1375	1386	rBV2	903097	2441236	100.00%	12.526%
42	6.009	1448	1452	1455	rBV3	668	515	0.02%	0.003%
43	6.227	1518	1520	1521	rBV	301	123	0.01%	0.001%
44	6.279	1521	1536	1578	rVV	811646	1550925	63.53%	7.958%
45	6.555	1612	1622	1623	rBV6	10620	10873	0.45%	0.056%
46	6.719	1658	1673	1695	rBV	547108	1062549	43.53%	5.452%
47	6.870	1718	1720	1722	rBV2	840	544	0.02%	0.003%
48	6.899	1726	1729	1730	rBV2	530	292	0.01%	0.001%
49	6.925	1735	1737	1739	rVV	447	151	0.01%	0.001%
50	6.941	1739	1742	1744	rVB2	618	374	0.02%	0.002%
51	7.018	1764	1766	1769	rBV2	375	262	0.01%	0.001%
52	7.054	1773	1777	1779	rBV	581	359	0.01%	0.002%
53	7.150	1804	1807	1810	rVB2	635	394	0.02%	0.002%
54	7.166	1810	1812	1815	rBV	438	173	0.01%	0.001%
55	7.205	1815	1824	1834	rVB7	1917	3203	0.13%	0.016%
56	7.298	1849	1853	1856	rBV	448	361	0.01%	0.002%
57	7.346	1866	1868	1874	rBV	372	303	0.01%	0.002%
58	7.423	1887	1892	1893	rBV2	319	198	0.01%	0.001%
59	7.436	1893	1896	1898	rVB	276	115	0.00%	0.001%
60	7.452	1898	1901	1903	rBV	409	251	0.01%	0.001%
61	7.504	1913	1917	1919	rBV	417	293	0.01%	0.002%
62	7.587	1930	1943	1963	rBV	301894	528600	21.65%	2.712%
63	7.758	1992	1996	2000	rBV3	769	677	0.03%	0.003%
64	7.922	2029	2047	2063	rBV	1099477	1961757	80.36%	10.066%
65	8.150	2116	2118	2120	rBV2	248	126	0.01%	0.001%
66	8.198	2120	2133	2151	rBV	214059	357172	14.63%	1.833%
67	8.391	2190	2193	2195	rBV	304	206	0.01%	0.001%
68	8.491	2216	2224	2227	rBV2	2110	2822	0.12%	0.014%
69	8.652	2261	2274	2310	rBV	825973	1454311	59.57%	7.462%
70	8.925	2354	2359	2360	rBV3	891	697	0.03%	0.004%
71	9.230	2452	2454	2457	rBV	257	126	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060920\
 Data File : VU038714.D
 Acq On : 09 Jun 2020 11:24
 Operator : SY/MD
 Sample : L2913-14
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9E56

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis

72	9.337	2483	2487	2489	rBV2	375	289	0.01%	0.001%
73	9.433	2504	2517	2541	rBV	1117810	1921026	78.69%	9.857%
74	9.587	2556	2565	2576	rBV2	15977	25701	1.05%	0.132%
75	10.002	2690	2694	2697	rBV2	433	425	0.02%	0.002%
76	10.057	2707	2711	2717	rBV2	455	472	0.02%	0.002%
77	10.115	2724	2729	2738	rVB5	4028	5666	0.23%	0.029%
78	10.288	2781	2783	2784	rBV	575	204	0.01%	0.001%
79	10.472	2838	2840	2843	rBV2	559	286	0.01%	0.001%
80	10.539	2855	2861	2872	rVB4	4395	7057	0.29%	0.036%
81	10.771	2920	2933	2951	rVB	739367	1181521	48.40%	6.062%
82	11.095	3031	3034	3036	rBV2	705	471	0.02%	0.002%
83	11.144	3047	3049	3050	rVB2	416	110	0.00%	0.001%
84	11.822	3247	3260	3278	rBV	1219810	1903235	77.96%	9.765%
85	12.079	3332	3340	3354	rBV4	14124	25732	1.05%	0.132%
86	12.205	3366	3379	3397	rVB	1123809	1828639	74.91%	9.383%
87	12.365	3427	3429	3434	rBV2	620	483	0.02%	0.002%


Sum of corrected areas: 19489617

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU060920\
Data File : VU038714.D
Acq On : 09 Jun 2020 11:24
Operator : SY/MD
Sample : L2913-14
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9E56

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

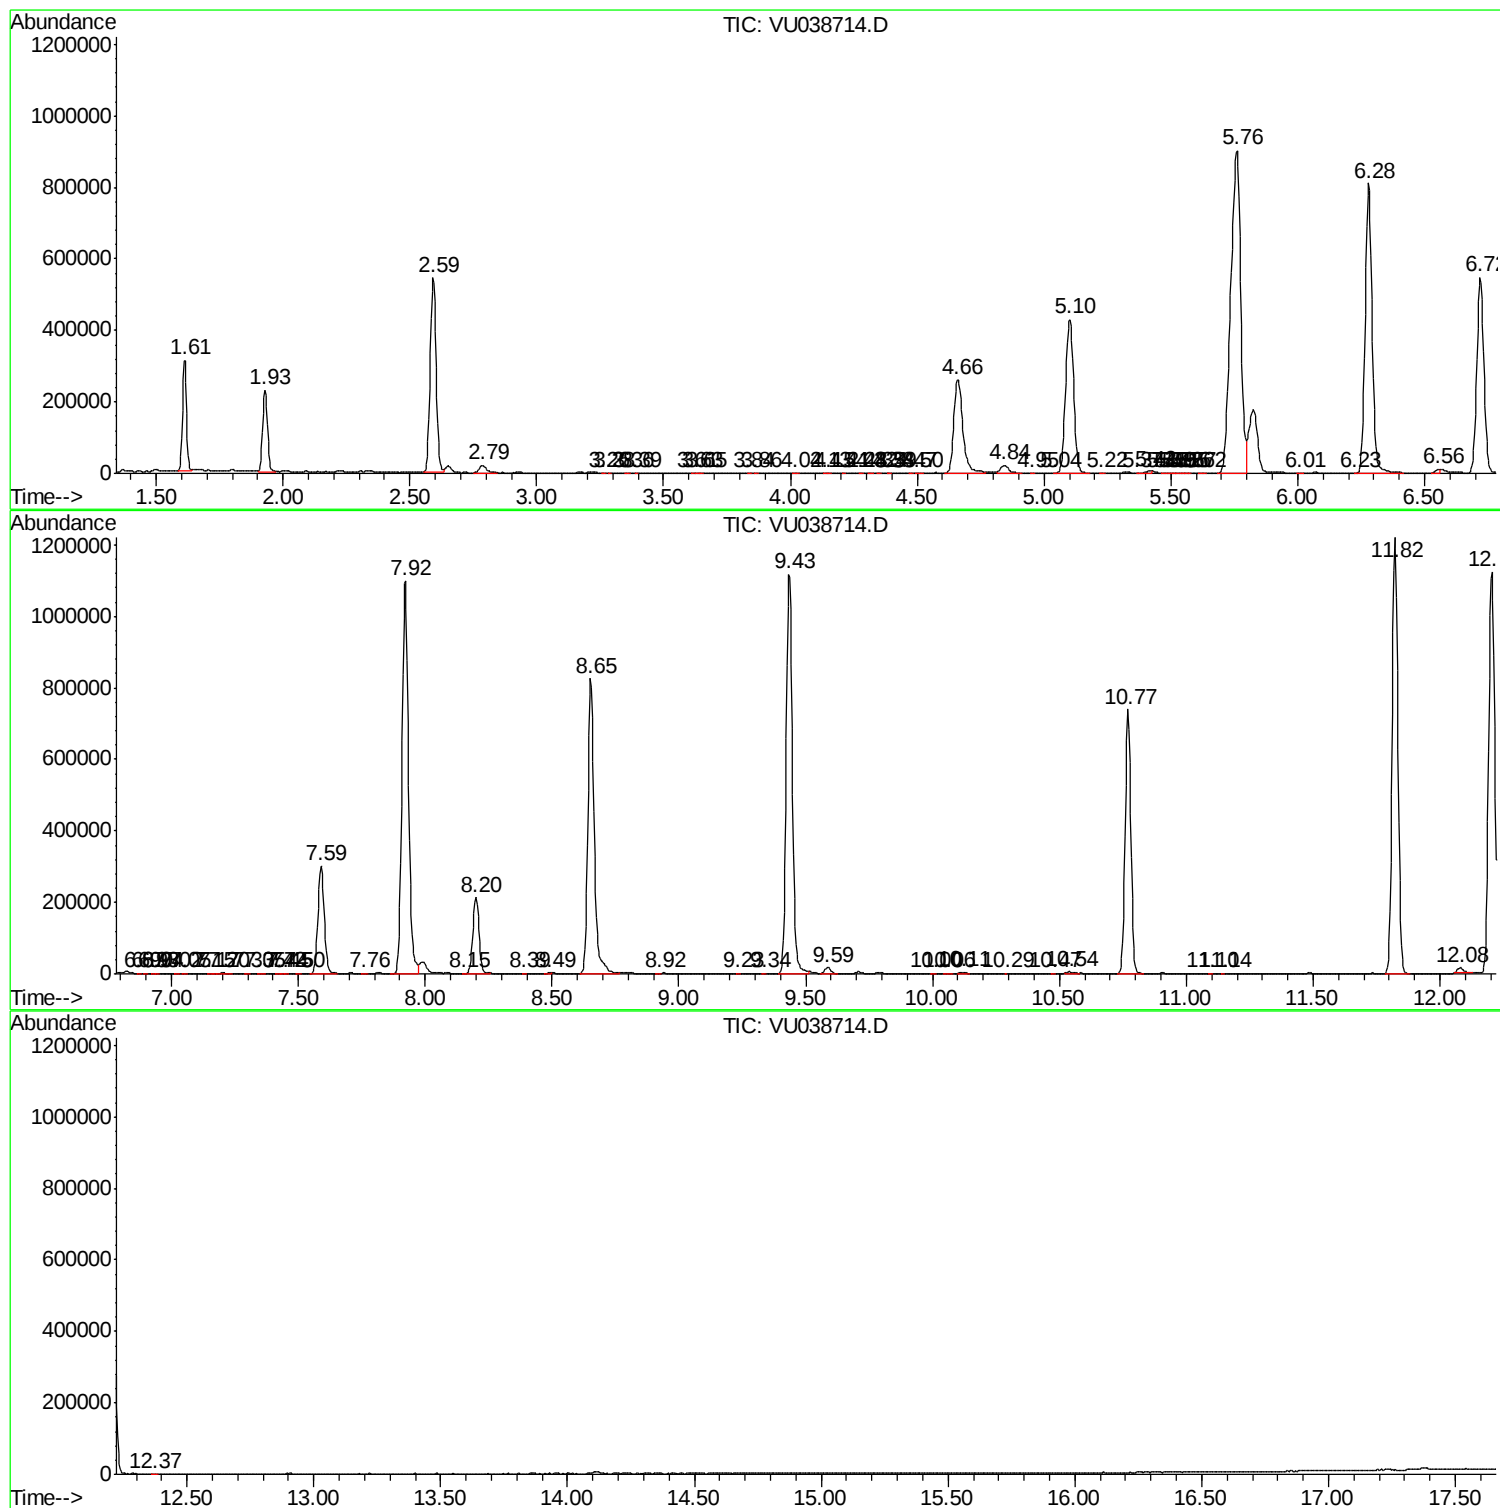

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU060920\
Data File : VU038714.D
Acq On : 09 Jun 2020 11:24
Operator : SY/MD
Sample : L2913-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9E56

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU060920\
Data File : VU038714.D
Acq On : 09 Jun 2020 11:24
Operator : SY/MD
Sample : L2913-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9E56

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc