

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060920\
 Data File : VU038717.D
 Acq On : 09 Jun 2020 12:31
 Operator : SY/MD
 Sample : L2913-17
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9E59

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.372	5	10	17	rVB	18561	17911	0.74%	0.093%
2	1.613	78	85	94	rBV	291080	329340	13.59%	1.706%
3	1.932	176	184	194	rVB	216617	277450	11.45%	1.437%
4	2.594	378	390	404	rBV	523233	879885	36.32%	4.559%
5	2.822	447	461	489	rBV2	17659	70643	2.92%	0.366%
6	3.034	524	527	528	rBV2	668	369	0.02%	0.002%
7	3.150	560	563	564	rBV2	928	484	0.02%	0.003%
8	3.333	614	620	623	rBV3	517	647	0.03%	0.003%
9	3.362	627	629	632	rBV	249	117	0.00%	0.001%
10	3.378	632	634	636	rBV	441	291	0.01%	0.002%
11	3.481	664	666	669	rBV3	408	165	0.01%	0.001%
12	3.610	704	706	710	rBV	182	113	0.00%	0.001%
13	3.678	724	727	731	rVB2	422	294	0.01%	0.002%
14	3.703	731	735	738	rBV2	376	376	0.02%	0.002%
15	3.771	753	756	759	rBV	363	289	0.01%	0.001%
16	3.813	766	769	773	rVB2	334	239	0.01%	0.001%
17	3.835	773	776	777	rBV2	159	68	0.00%	0.000%
18	3.858	781	783	786	rBV2	197	97	0.00%	0.001%
19	3.877	786	789	794	rBV2	374	261	0.01%	0.001%
20	3.906	794	798	801	rBV2	655	426	0.02%	0.002%
21	3.989	821	824	828	rBV2	468	267	0.01%	0.001%
22	4.079	850	852	855	rVB2	357	191	0.01%	0.001%
23	4.108	858	861	863	rVB	219	118	0.00%	0.001%
24	4.128	863	867	868	rBV2	189	121	0.00%	0.001%
25	4.211	891	893	895	rBV2	203	89	0.00%	0.000%
26	4.279	913	914	917	rVB	161	42	0.00%	0.000%
27	4.295	917	919	920	rBV	182	65	0.00%	0.000%
28	4.571	1002	1005	1010	rBV4	699	685	0.03%	0.004%
29	4.665	1018	1034	1064	rBV	259812	662528	27.35%	3.433%
30	4.931	1116	1117	1119	rBV	573	277	0.01%	0.001%
31	5.034	1147	1149	1152	rBV	299	119	0.00%	0.001%
32	5.102	1152	1170	1195	rBV	428909	929448	38.36%	4.815%
33	5.282	1221	1226	1228	rBV2	637	524	0.02%	0.003%
34	5.427	1258	1271	1282	rBV8	4169	8594	0.35%	0.045%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060920\
 Data File : VU038717.D
 Acq On : 09 Jun 2020 12:31
 Operator : SY/MD
 Sample : L2913-17
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9E59

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis

35	5.520	1298	1300	1301	rBV8	249	87	0.00%	0.000%
36	5.571	1312	1316	1318	rBV	454	376	0.02%	0.002%
37	5.758	1351	1374	1385	rBV2	910650	2422717	100.00%	12.552%
38	6.279	1521	1536	1574	rBV	769052	1488582	61.44%	7.712%
39	6.529	1612	1614	1615	rBV	470	240	0.01%	0.001%
40	6.719	1658	1673	1691	rBV	549396	1057433	43.65%	5.479%
41	6.944	1739	1743	1744	rBV2	471	376	0.02%	0.002%
42	6.980	1753	1754	1755	rBV	181	42	0.00%	0.000%
43	7.054	1775	1777	1780	rBV	376	247	0.01%	0.001%
44	7.208	1817	1825	1832	rVB6	1794	2702	0.11%	0.014%
45	7.269	1842	1844	1849	rBV2	285	223	0.01%	0.001%
46	7.301	1853	1854	1856	rBV	265	87	0.00%	0.000%
47	7.353	1867	1870	1873	rBV2	210	154	0.01%	0.001%
48	7.375	1874	1877	1881	rVB3	414	298	0.01%	0.002%
49	7.404	1881	1886	1887	rBV	566	407	0.02%	0.002%
50	7.439	1895	1897	1898	rBV	366	135	0.01%	0.001%
51	7.591	1928	1944	1958	rBV	302087	538658	22.23%	2.791%
52	7.703	1976	1979	1986	rVB5	1879	1728	0.07%	0.009%
53	7.774	1996	2001	2005	rBV4	541	616	0.03%	0.003%
54	7.870	2029	2031	2033	rBV3	672	401	0.02%	0.002%
55	7.922	2033	2047	2064	rBV	1090847	1946183	80.33%	10.083%
56	8.198	2119	2133	2150	rBV	207210	353034	14.57%	1.829%
57	8.369	2183	2186	2190	rBV2	402	333	0.01%	0.002%
58	8.420	2198	2202	2205	rBV3	338	247	0.01%	0.001%
59	8.436	2205	2207	2209	rVB3	207	87	0.00%	0.000%
60	8.484	2218	2222	2223	rBV2	1285	843	0.03%	0.004%
61	8.655	2261	2275	2301	rBV	836390	1485895	61.33%	7.698%
62	8.906	2348	2353	2358	rBV3	824	963	0.04%	0.005%
63	9.002	2382	2383	2385	rBV3	304	154	0.01%	0.001%
64	9.172	2433	2436	2437	rBV2	350	199	0.01%	0.001%
65	9.234	2453	2455	2458	rBV	294	140	0.01%	0.001%
66	9.330	2483	2485	2486	rBV	423	156	0.01%	0.001%
67	9.436	2502	2518	2546	rBV	1075963	1859524	76.75%	9.634%
68	9.584	2558	2564	2574	rVB	11254	16424	0.68%	0.085%
69	9.658	2586	2587	2588	rVB	338	65	0.00%	0.000%
70	9.790	2620	2628	2637	rBV5	2193	3668	0.15%	0.019%
71	9.848	2638	2646	2651	rBV7	4435	6092	0.25%	0.032%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU060920\
 Data File : VU038717.D
 Acq On : 09 Jun 2020 12:31
 Operator : SY/MD
 Sample : L2913-17
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F9E59

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis

72	9.944	2674	2676	2679	rBV	309	201	0.01%	0.001%
73	10.121	2722	2731	2740	rVB6	3286	4805	0.20%	0.025%
74	10.375	2803	2810	2820	rVB6	4912	7934	0.33%	0.041%
75	10.536	2853	2860	2870	rBV3	5386	8565	0.35%	0.044%
76	10.693	2906	2909	2913	rBV	924	660	0.03%	0.003%
77	10.770	2921	2933	2955	rVB	752910	1203043	49.66%	6.233%
78	10.909	2969	2976	2981	rBV7	1844	2331	0.10%	0.012%
79	11.188	3060	3063	3067	rBV	620	509	0.02%	0.003%
80	11.291	3086	3095	3106	rVB7	2772	4946	0.20%	0.026%
81	11.475	3148	3152	3153	rBV2	1469	1006	0.04%	0.005%
82	11.536	3169	3171	3174	rBV2	674	346	0.01%	0.002%
83	11.732	3229	3232	3233	rBV2	503	292	0.01%	0.002%
84	11.822	3247	3260	3276	rBV	1148567	1818400	75.06%	9.421%
85	11.909	3284	3287	3291	rBV4	1121	912	0.04%	0.005%
86	12.079	3328	3340	3353	rBV3	21847	44194	1.82%	0.229%
87	12.204	3366	3379	3398	rVB	1142654	1823130	75.25%	9.446%
88	13.912	3907	3910	3916	rBV5	930	1111	0.05%	0.006%
89	14.114	3965	3973	3983	rVB3	4431	6833	0.28%	0.035%


Sum of corrected areas: 19301267

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU060920\
Data File : VU038717.D
Acq On : 09 Jun 2020 12:31
Operator : SY/MD
Sample : L2913-17
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9E59

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

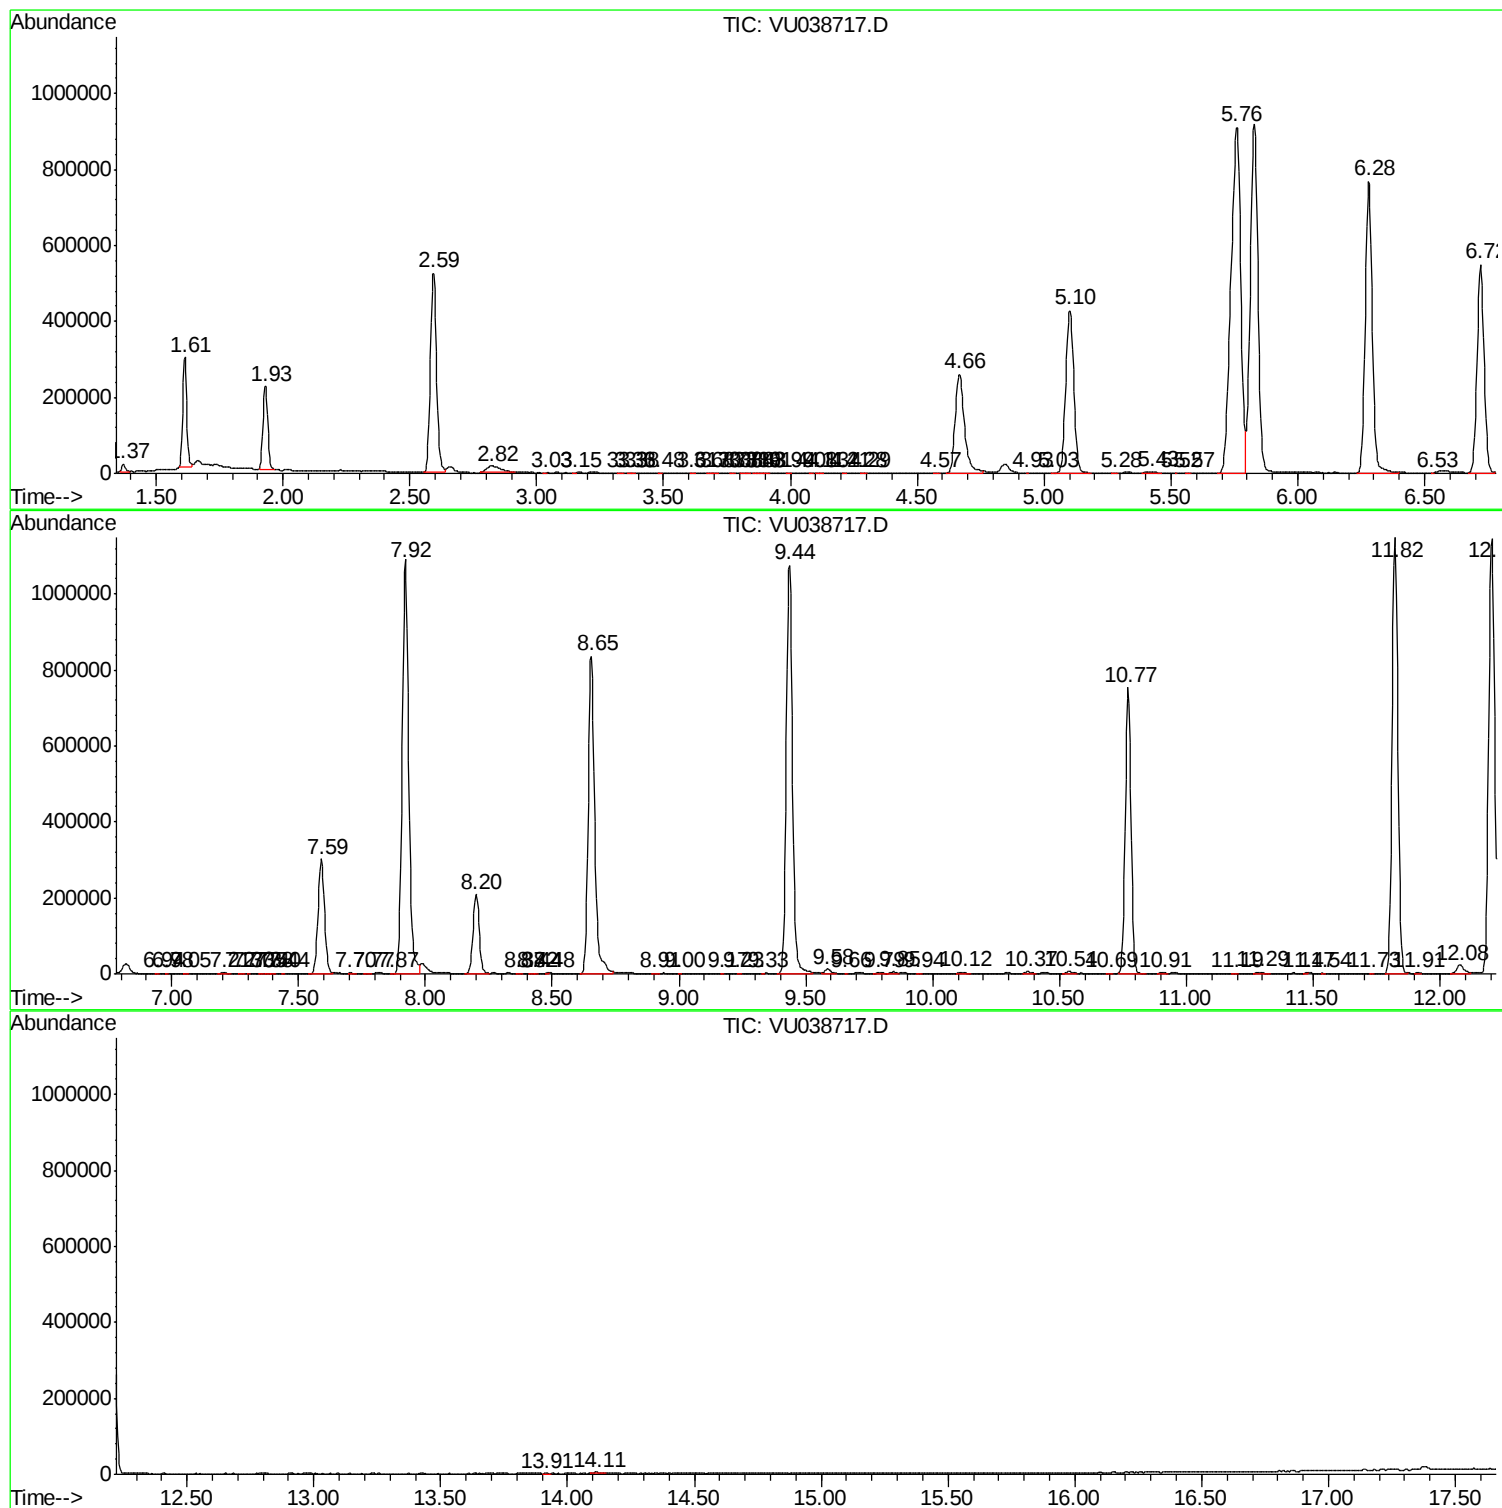

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU060920\
Data File : VU038717.D
Acq On : 09 Jun 2020 12:31
Operator : SY/MD
Sample : L2913-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9E59

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU060920\
Data File : VU038717.D
Acq On : 09 Jun 2020 12:31
Operator : SY/MD
Sample : L2913-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F9E59

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc