


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU060920\
 Data File : VU038670.D
 Acq On : 08 Jun 2020 15:23
 Operator : SY/MD
 Sample : BFB51
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB51

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM060820WMA.M
 Title : VOC Analysis
 Last Update : Thu Jun 11 13:00:07 2020

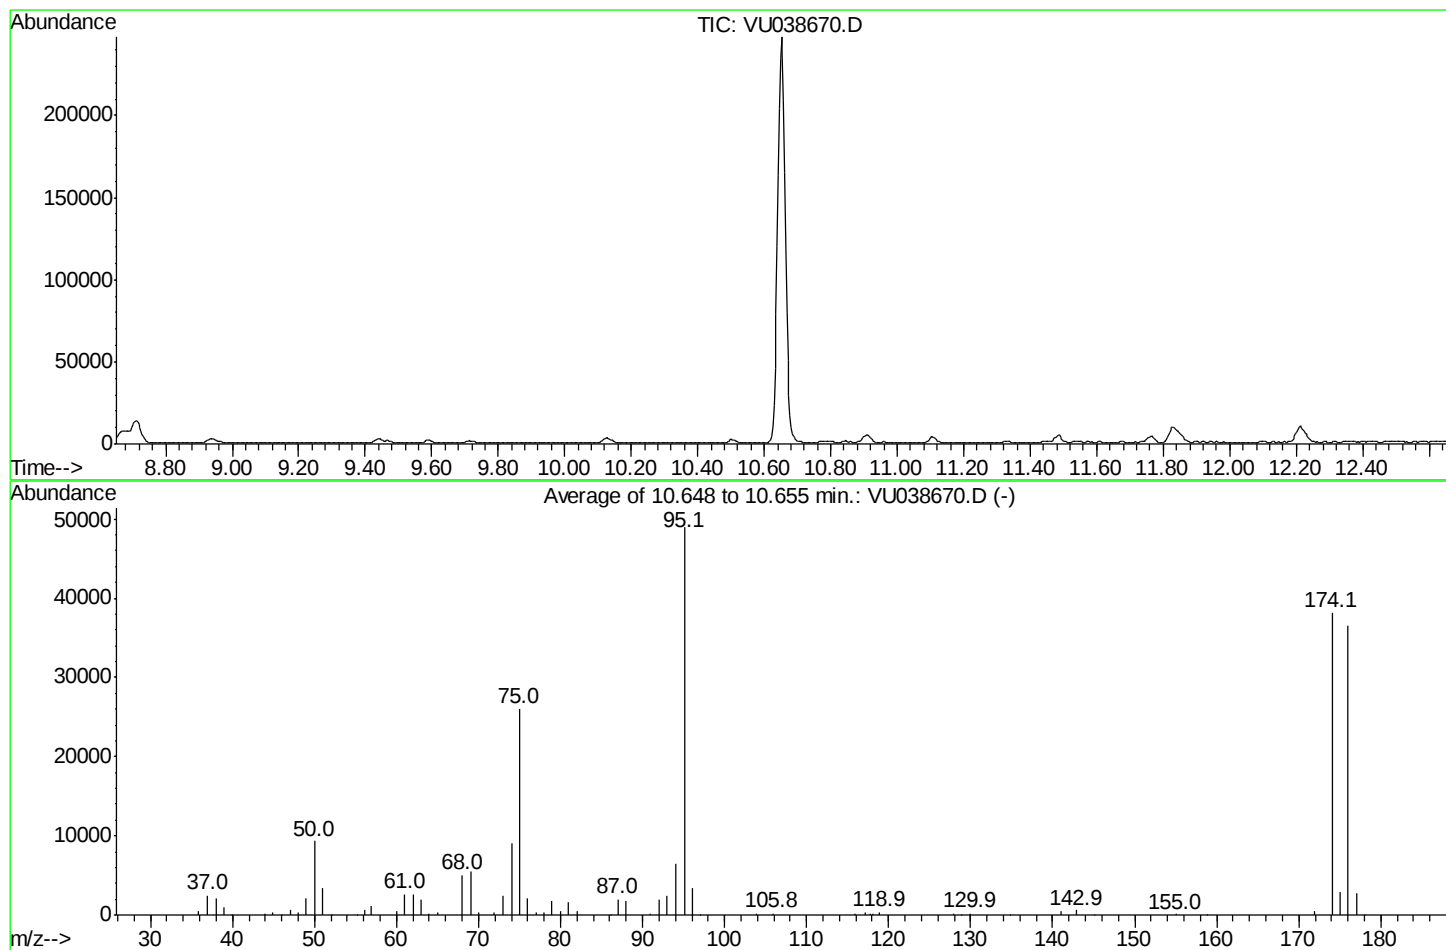

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2883

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	9351	PASS
75	95	30	80	53.2	26053	PASS
95	95	100	100	100.0	48941	PASS
96	95	5	9	7.1	3461	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.0	38154	PASS
175	174	5	9	7.6	2903	PASS
176	174	95	101	95.7	36504	PASS
177	176	5	9	7.6	2780	PASS

m/z	Abundance
35.80	440.0
37.00	2244.0
38.00	2154.0
39.00	915.0
39.90	199.0
44.00	905.0
44.90	415.0
46.00	101.0
47.10	633.0
48.10	304.0
48.90	1940.0
50.00	8690.0
51.00	3397.0
56.10	742.0
57.00	1244.0
59.90	501.0
61.00	2795.0
62.00	2366.0
63.00	1989.0
64.00	253.0
65.00	240.0
68.00	5249.0
69.00	5184.0
70.00	431.0
71.90	289.0
73.00	2482.0
74.00	8616.0
75.00	25520.0
76.00	2289.0
77.10	299.0
78.00	245.0
79.00	1844.0
80.00	579.0
81.00	1418.0
81.90	394.0
87.00	2007.0
87.90	1769.0
90.80	201.0
92.00	1826.0
93.00	2408.0
94.10	6366.0
95.10	48192.0
96.10	3489.0
97.00	100.0
103.80	194.0
105.90	174.0
115.90	143.0
117.10	350.0
117.80	141.0
118.90	329.0
127.90	112.0
130.10	182.0
134.80	115.0
141.00	470.0
142.90	663.0
155.00	139.0
158.80	101.0
171.90	410.0
174.10	36504.0
175.00	2790.0
176.00	35560.0
177.00	2621.0
178.00	102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51

m/z	Abundance
35.90	412.0
37.00	2552.0
38.00	2178.0
39.00	1002.0
40.00	172.0
43.90	885.0
44.90	369.0
47.10	730.0
48.10	293.0
48.90	2104.0
50.00	9634.0
51.00	3574.0
52.10	113.0
56.10	666.0
56.90	1221.0
60.00	512.0
61.00	2729.0
62.00	2691.0
63.00	1998.0
64.00	188.0
65.00	292.0
68.00	5217.0
69.00	5599.0
70.00	418.0
71.80	324.0
73.00	2600.0
74.00	9344.0
75.00	26840.0
76.00	2195.0
77.10	380.0
77.90	276.0
79.00	1779.0
80.00	528.0
80.90	1569.0
81.90	458.0
86.10	102.0
87.00	2122.0
87.90	1774.0
90.90	213.0
92.00	1969.0
93.00	2484.0
94.10	6629.0
95.10	50432.0
96.10	3628.0
103.80	203.0
105.80	225.0
116.00	187.0
117.10	327.0
117.80	143.0
118.00	145.0
118.90	382.0
127.90	115.0
128.90	100.0
129.90	186.0
141.00	592.0
143.00	679.0
145.10	119.0
155.00	148.0
158.80	109.0
171.90	495.0
174.10	39208.0
175.00	2923.0
176.00	37440.0
177.00	2894.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51

m/z	Abundance
35.90	388.0
37.00	2588.0
38.00	2073.0
39.00	1037.0
40.00	177.0
43.90	854.0
44.90	336.0
47.10	758.0
48.00	243.0
49.00	2057.0
50.00	9729.0
51.00	3323.0
52.00	127.0
55.20	158.0
56.10	592.0
56.90	1148.0
60.00	515.0
61.00	2367.0
62.00	2644.0
63.00	1852.0
64.00	134.0
65.00	282.0
68.00	4759.0
69.00	5498.0
70.00	344.0
71.80	291.0
73.00	2389.0
74.00	9032.0
75.00	25800.0
76.00	2010.0
77.10	417.0
77.90	236.0
78.90	1580.0
80.00	428.0
80.90	1705.0
82.00	459.0
86.10	127.0
87.00	1908.0
88.00	1655.0
90.90	214.0
92.00	1843.0
93.00	2230.0
94.00	6198.0
95.10	48200.0
96.10	3268.0
103.80	203.0
105.80	263.0
115.90	204.0
117.10	253.0
117.70	162.0
118.10	170.0
118.90	379.0
127.90	110.0
129.90	210.0
141.00	614.0
143.00	595.0
145.20	138.0
155.00	137.0
171.90	459.0
174.10	38752.0
175.00	2998.0
176.00	36512.0
177.00	2826.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51

Scan 2883 (10.610 min): VU038670.D
BFB51

m/z	Abundance
39.90	150.0
43.90	715.0

Instrument :
MSVOA_U
ClientSampleId :
BFB51