


## Chloromethane


Response Ratio

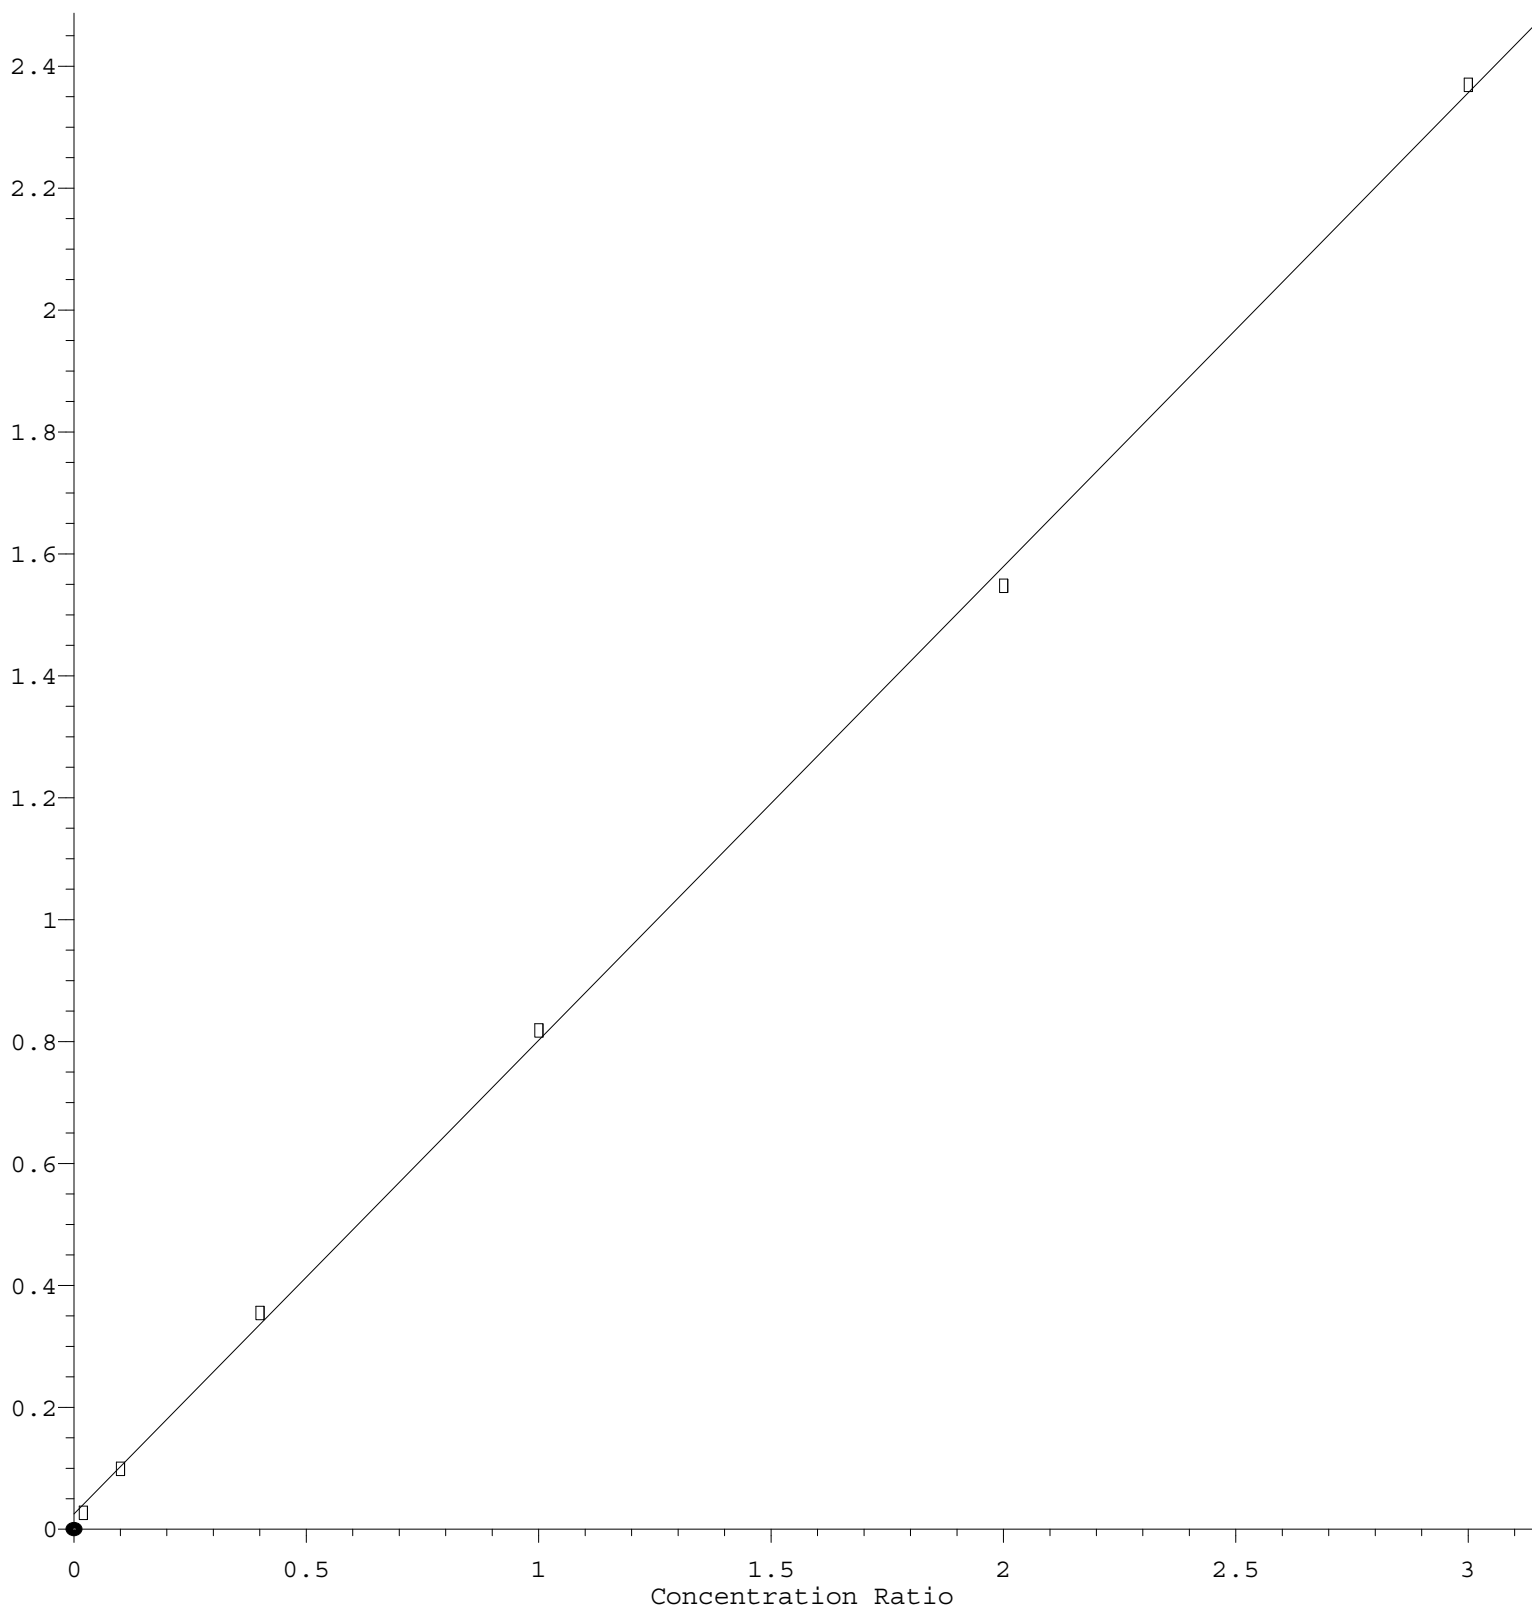

Response = 7.771e-001 \* Amt + 2.479e-002  
Coef of Det (r^2) = 0.999536 Curve Fit: Linear  
Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U060921W.M  
Calibration Table Last Updated: Thu Jun 10 05:11:37 2021

## 2-Chloroethyl Vinyl ether

Response Ratio

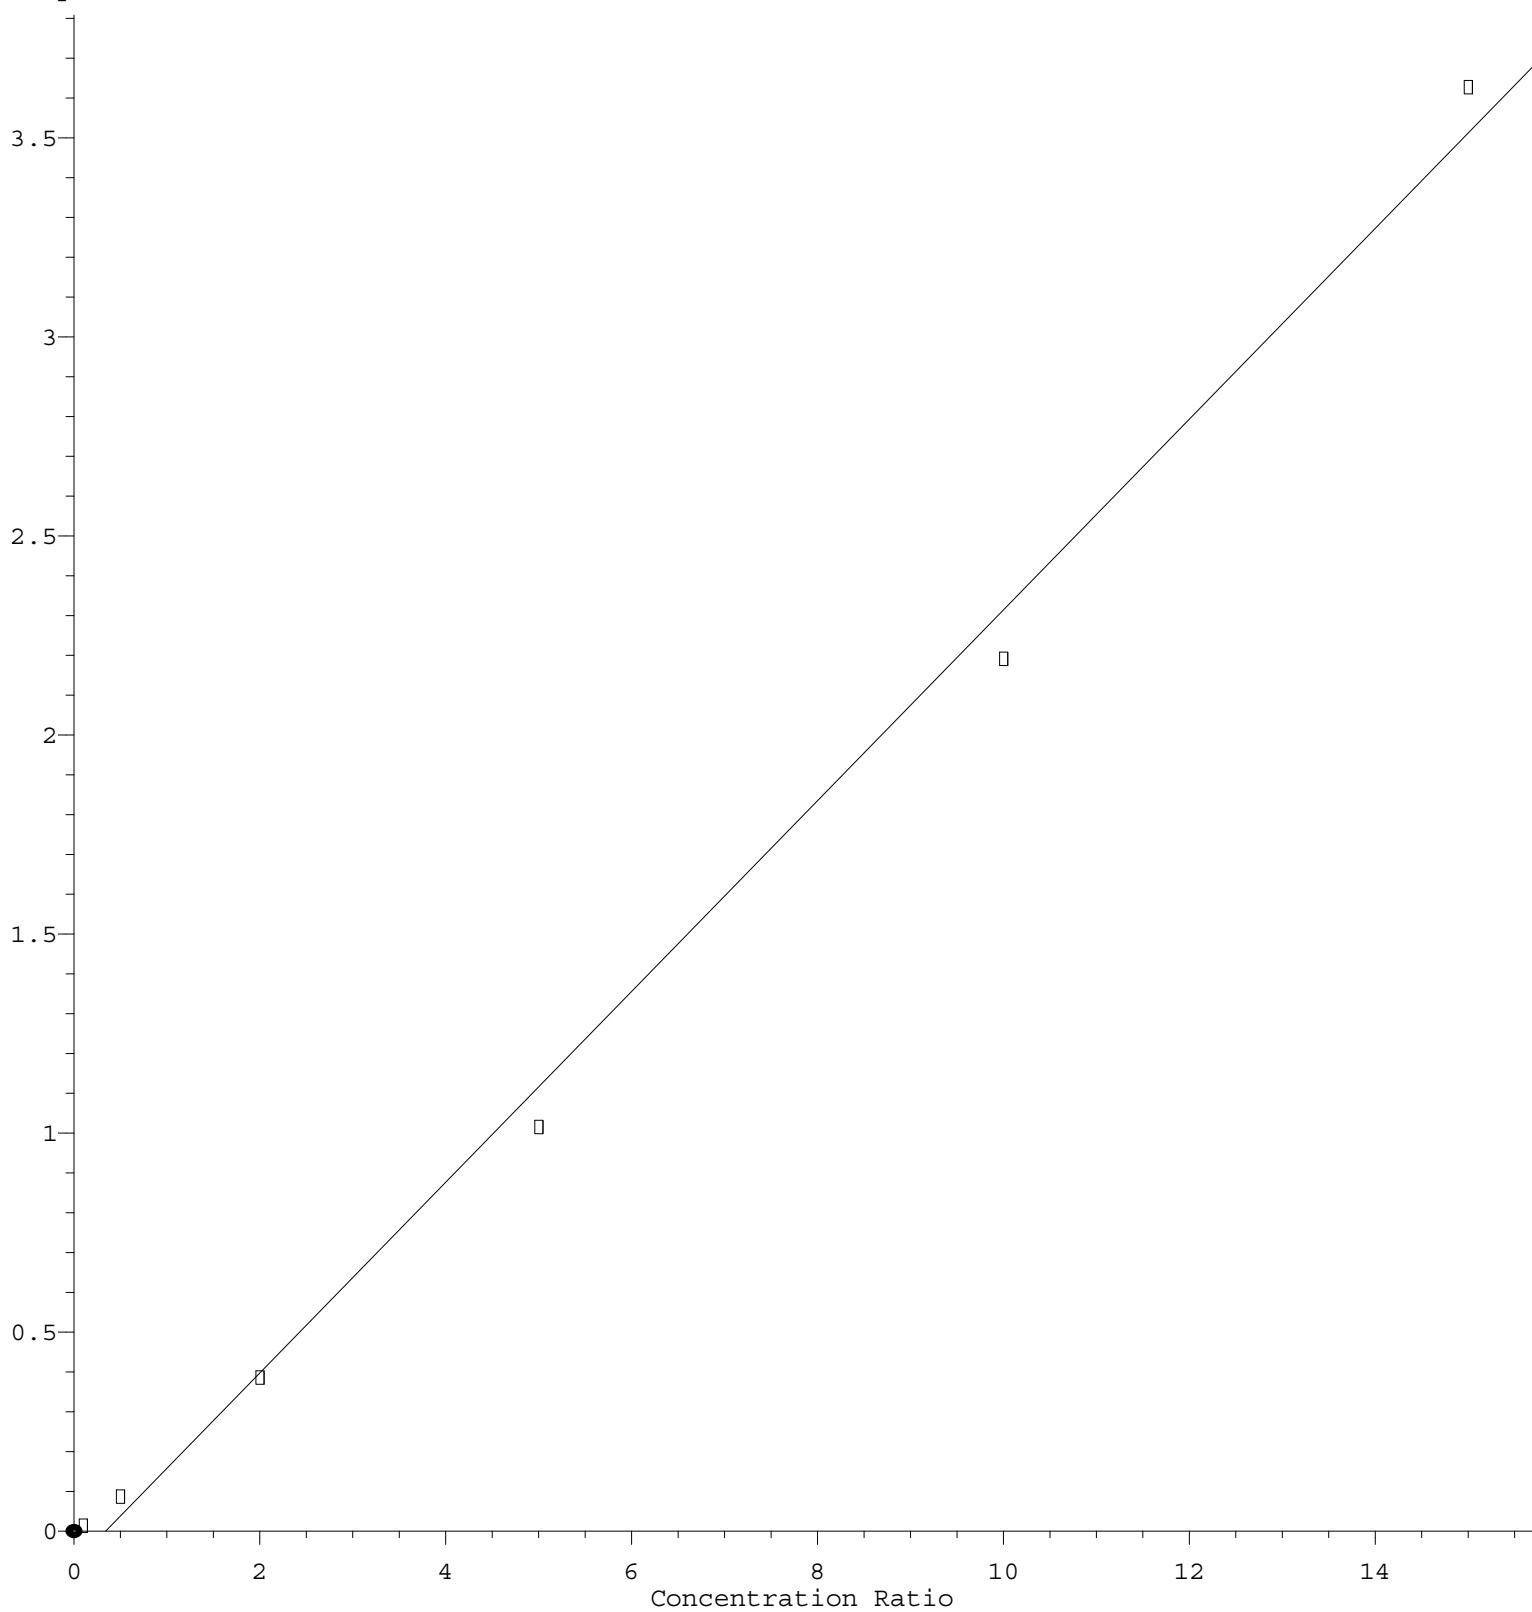

$$\text{Response} = 2.396\text{e-}001 * \text{Amt} - 8.180\text{e-}002$$


Coef of Det ( $r^2$ ) = 0.995484 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U060921W.M

Calibration Table Last Updated: Thu Jun 10 05:11:37 2021

# Naphthalene


Response Ratio

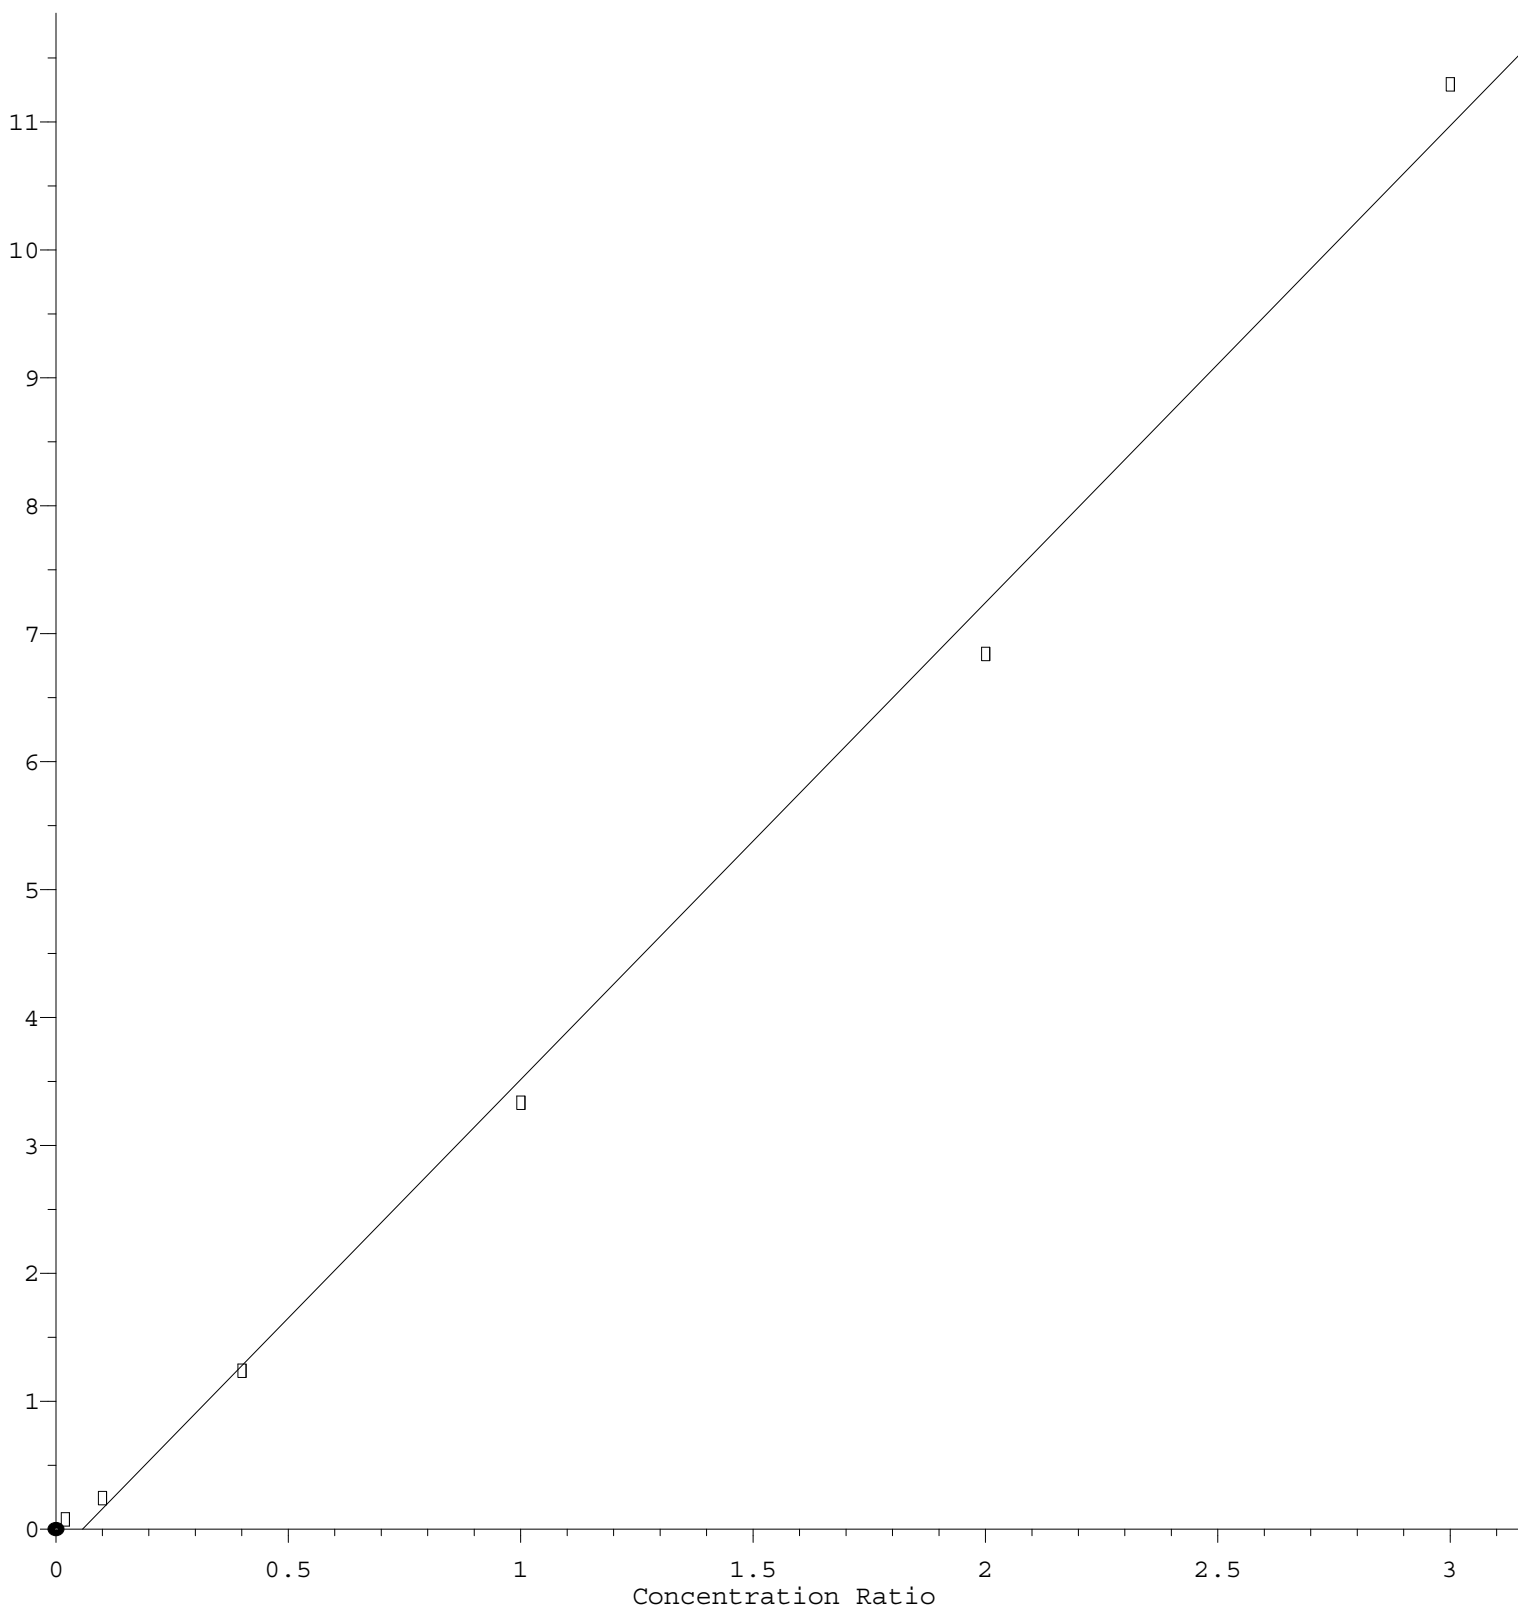

Response = 3.726e+000 \* Amt - 2.113e-001  
 Coef of Det (r^2) = 0.996424    Curve Fit: Linear  
 Method Name:    Z:\voasrv\HPCHEM1\MSVOA U\Method\82U060921W.M  
 Calibration Table Last Updated: Thu Jun 10 05:11:37 2021

# Chloroethane

Response Ratio

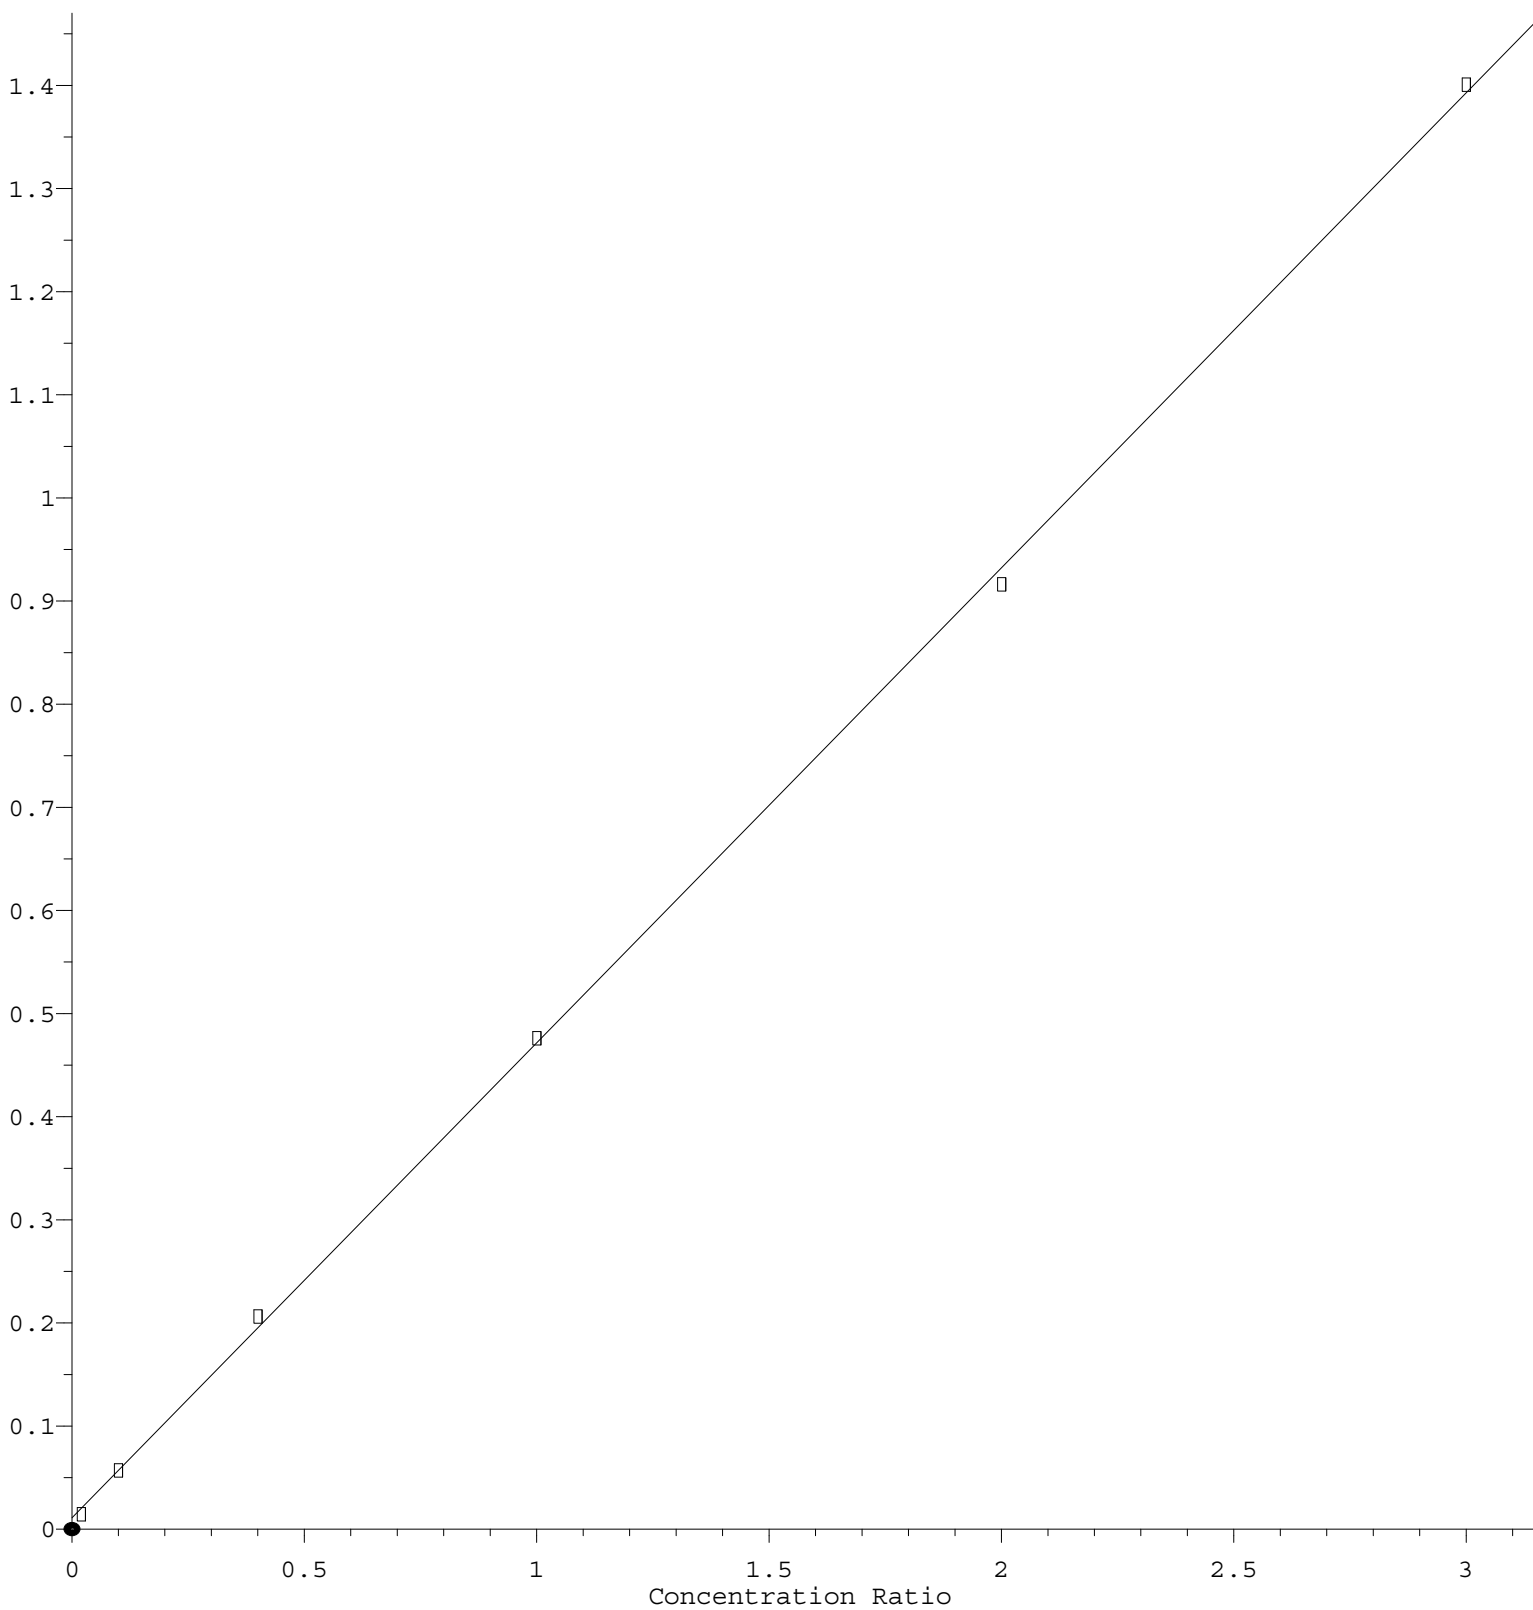

$$\text{Response} = 4.604\text{e-}001 * \text{Amt} + 1.141\text{e-}002$$


Coef of Det (r^2) = 0.999672 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U060921W.M

Calibration Table Last Updated: Thu Jun 10 05:11:37 2021

# Acrolein

Response Ratio

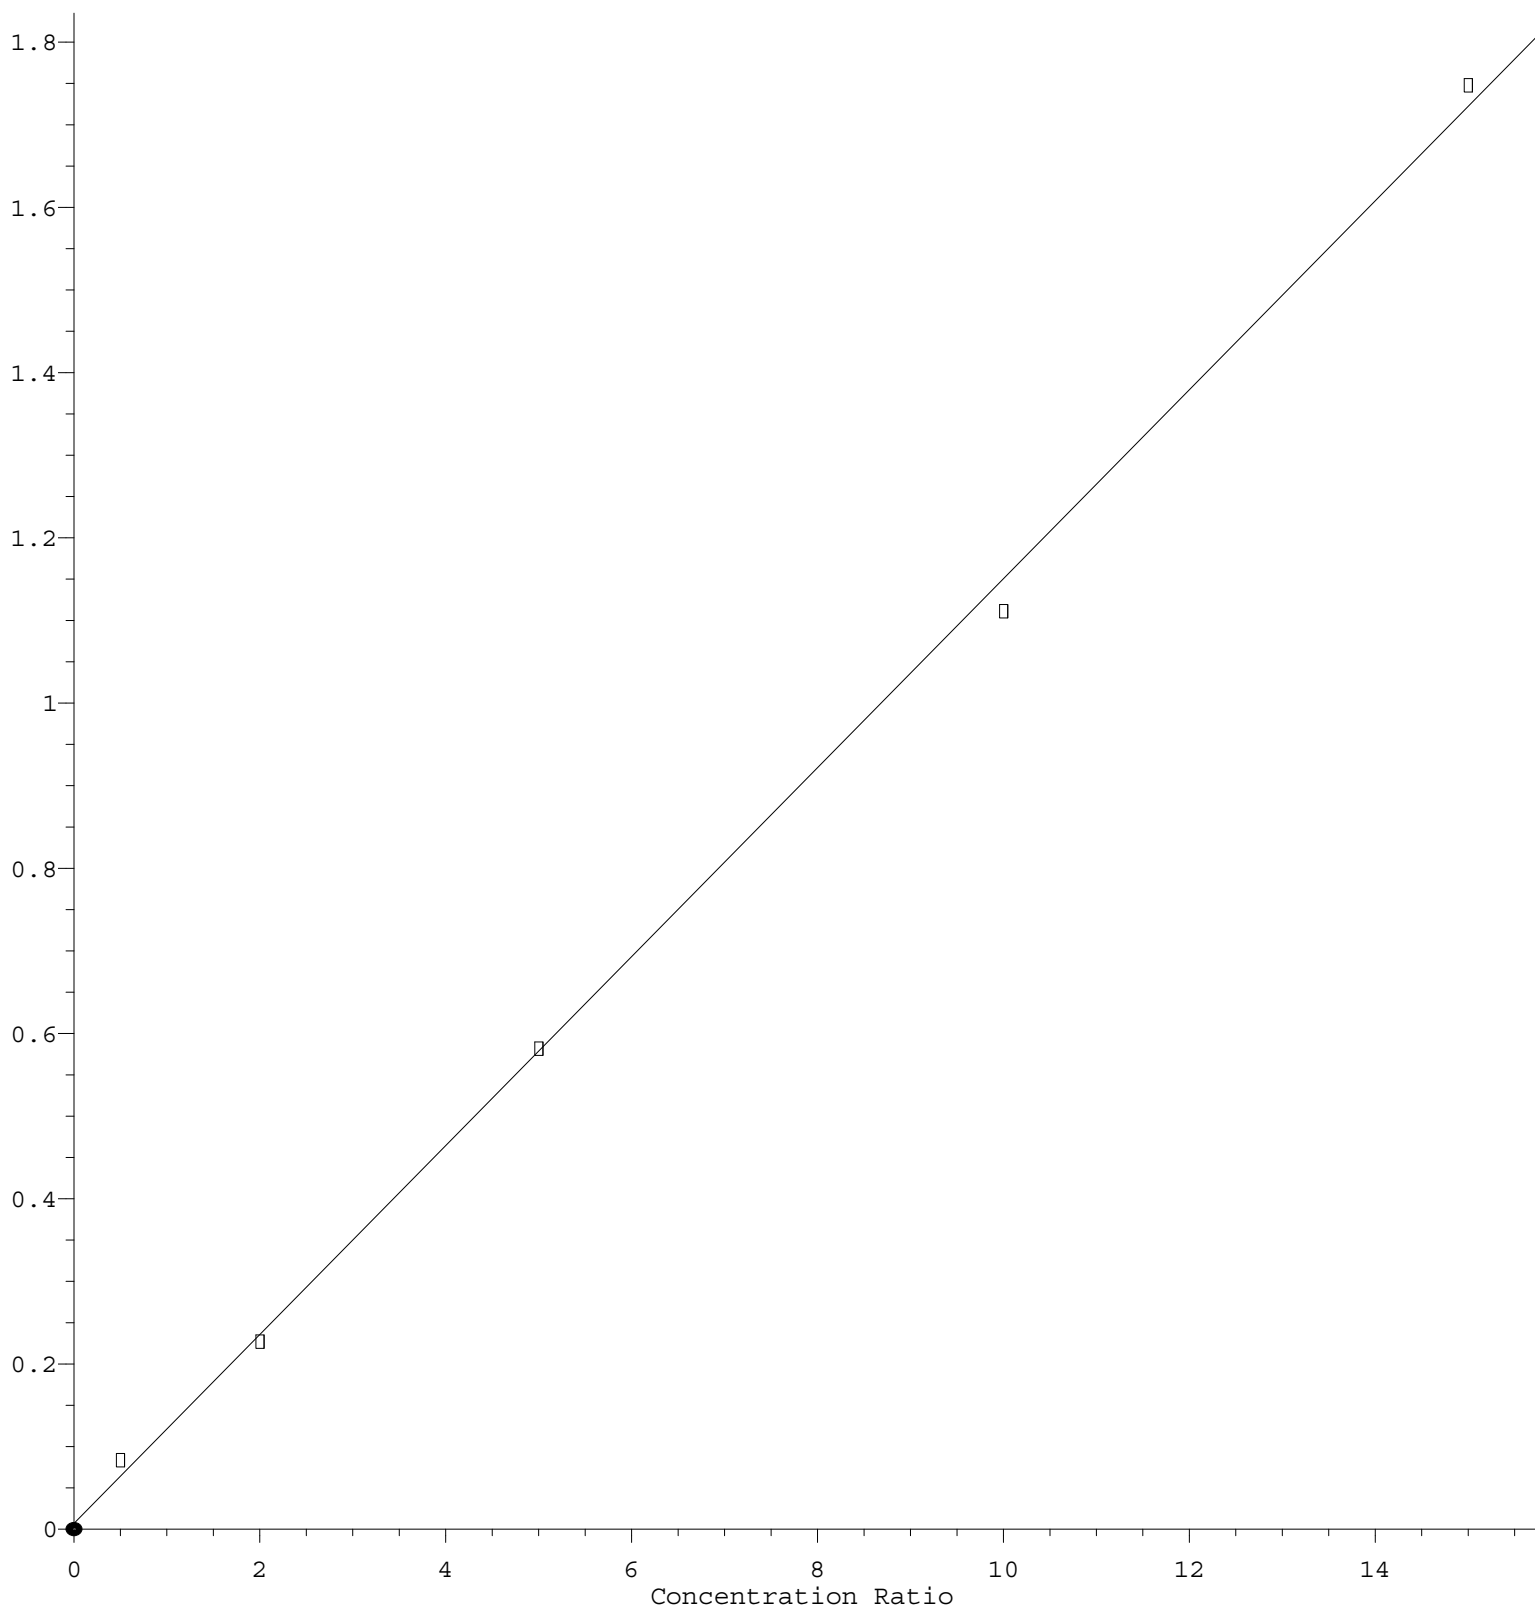

$$\text{Response} = 1.143\text{e-}001 * \text{Amt} + 6.940\text{e-}003$$


Coef of Det ( $r^2$ ) = 0.998579 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U060921W.M

Calibration Table Last Updated: Thu Jun 10 05:11:37 2021

# Acetone

Response Ratio

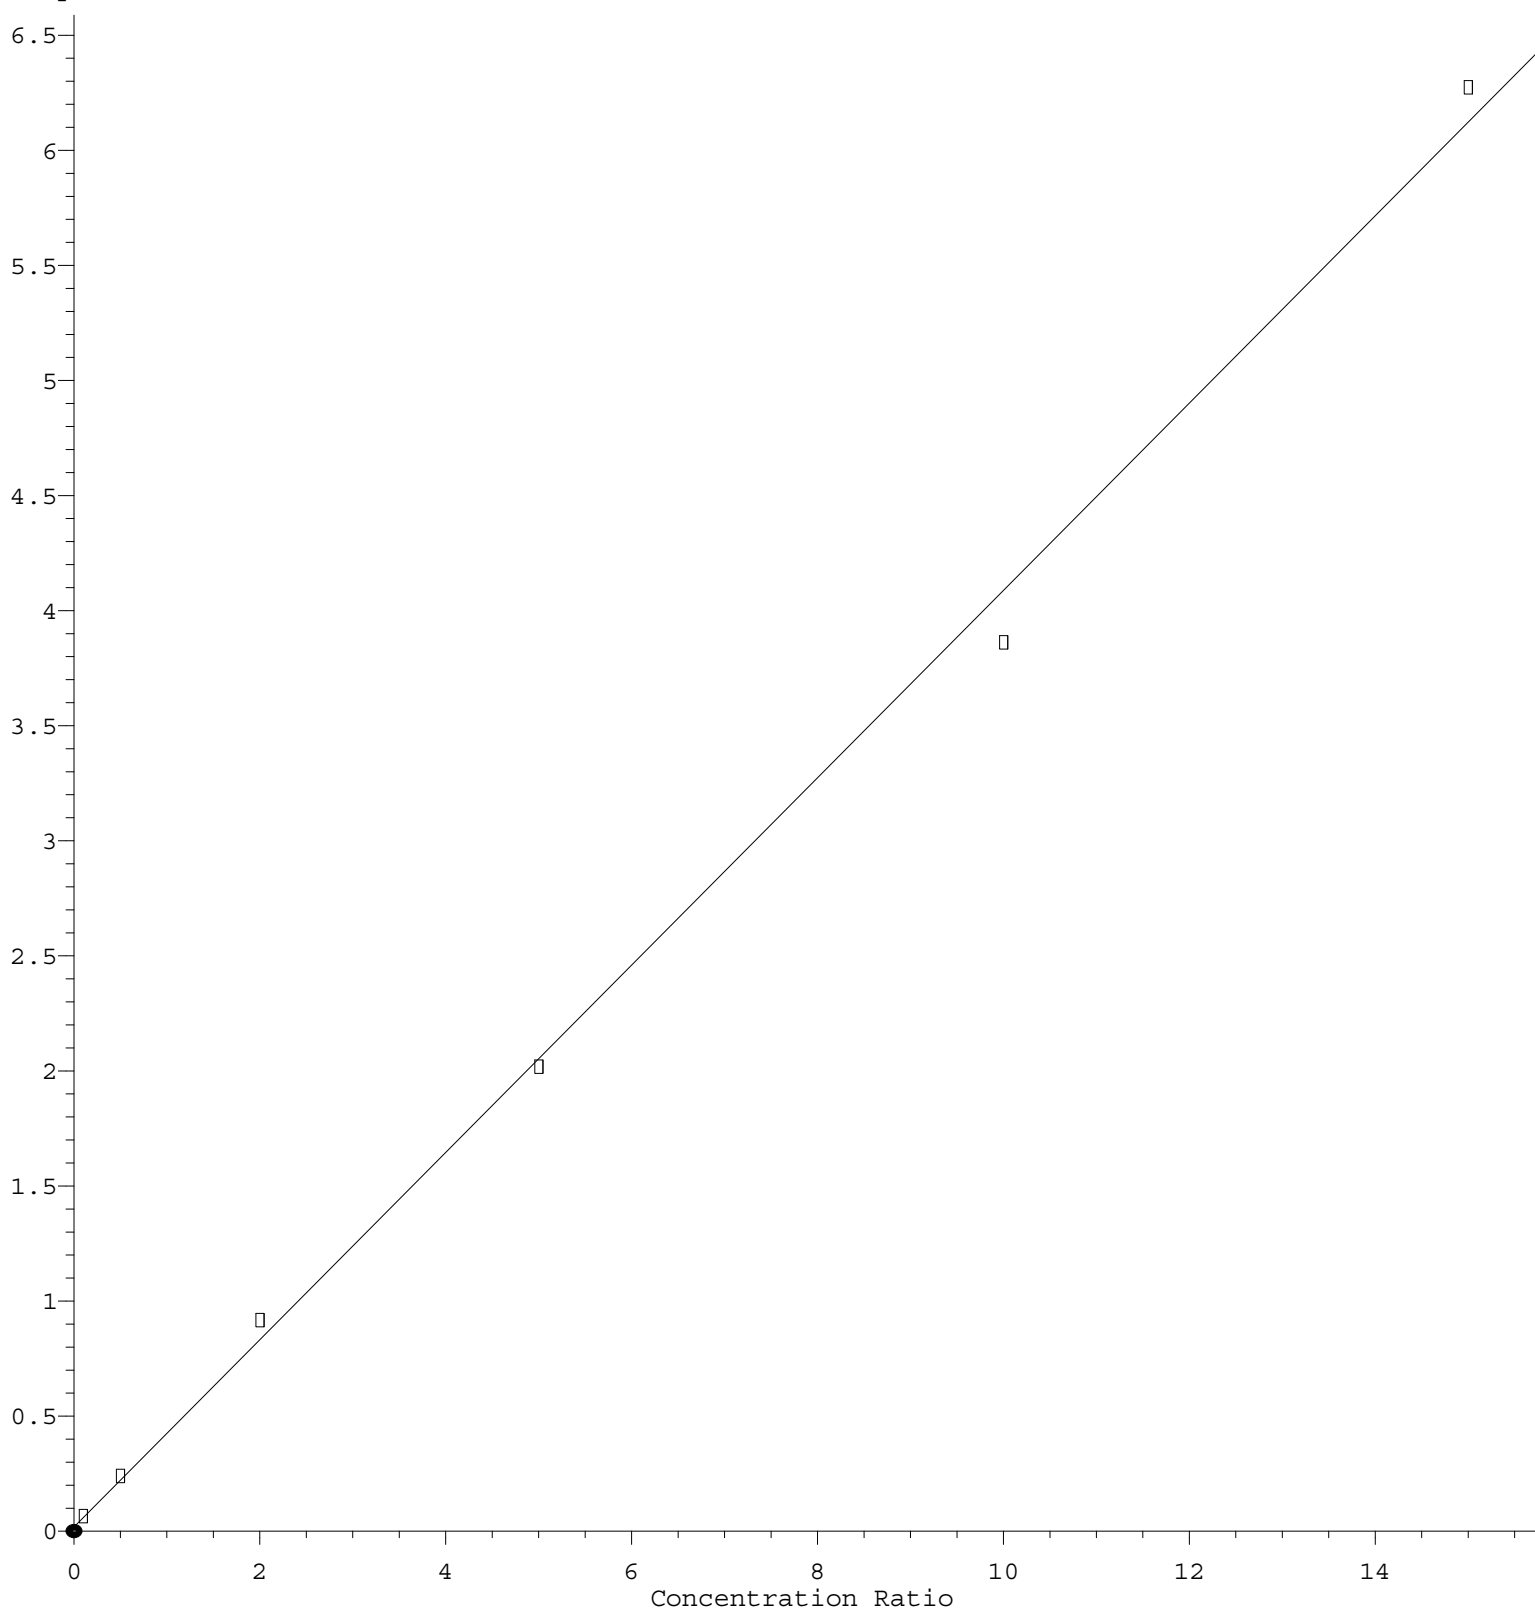

$$\text{Response} = 4.070\text{e-}001 * \text{Amt} + 1.758\text{e-}002$$


Coef of Det (r^2) = 0.997189 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U060921W.M

Calibration Table Last Updated: Thu Jun 10 05:11:37 2021

# Methylene Chloride

Response Ratio

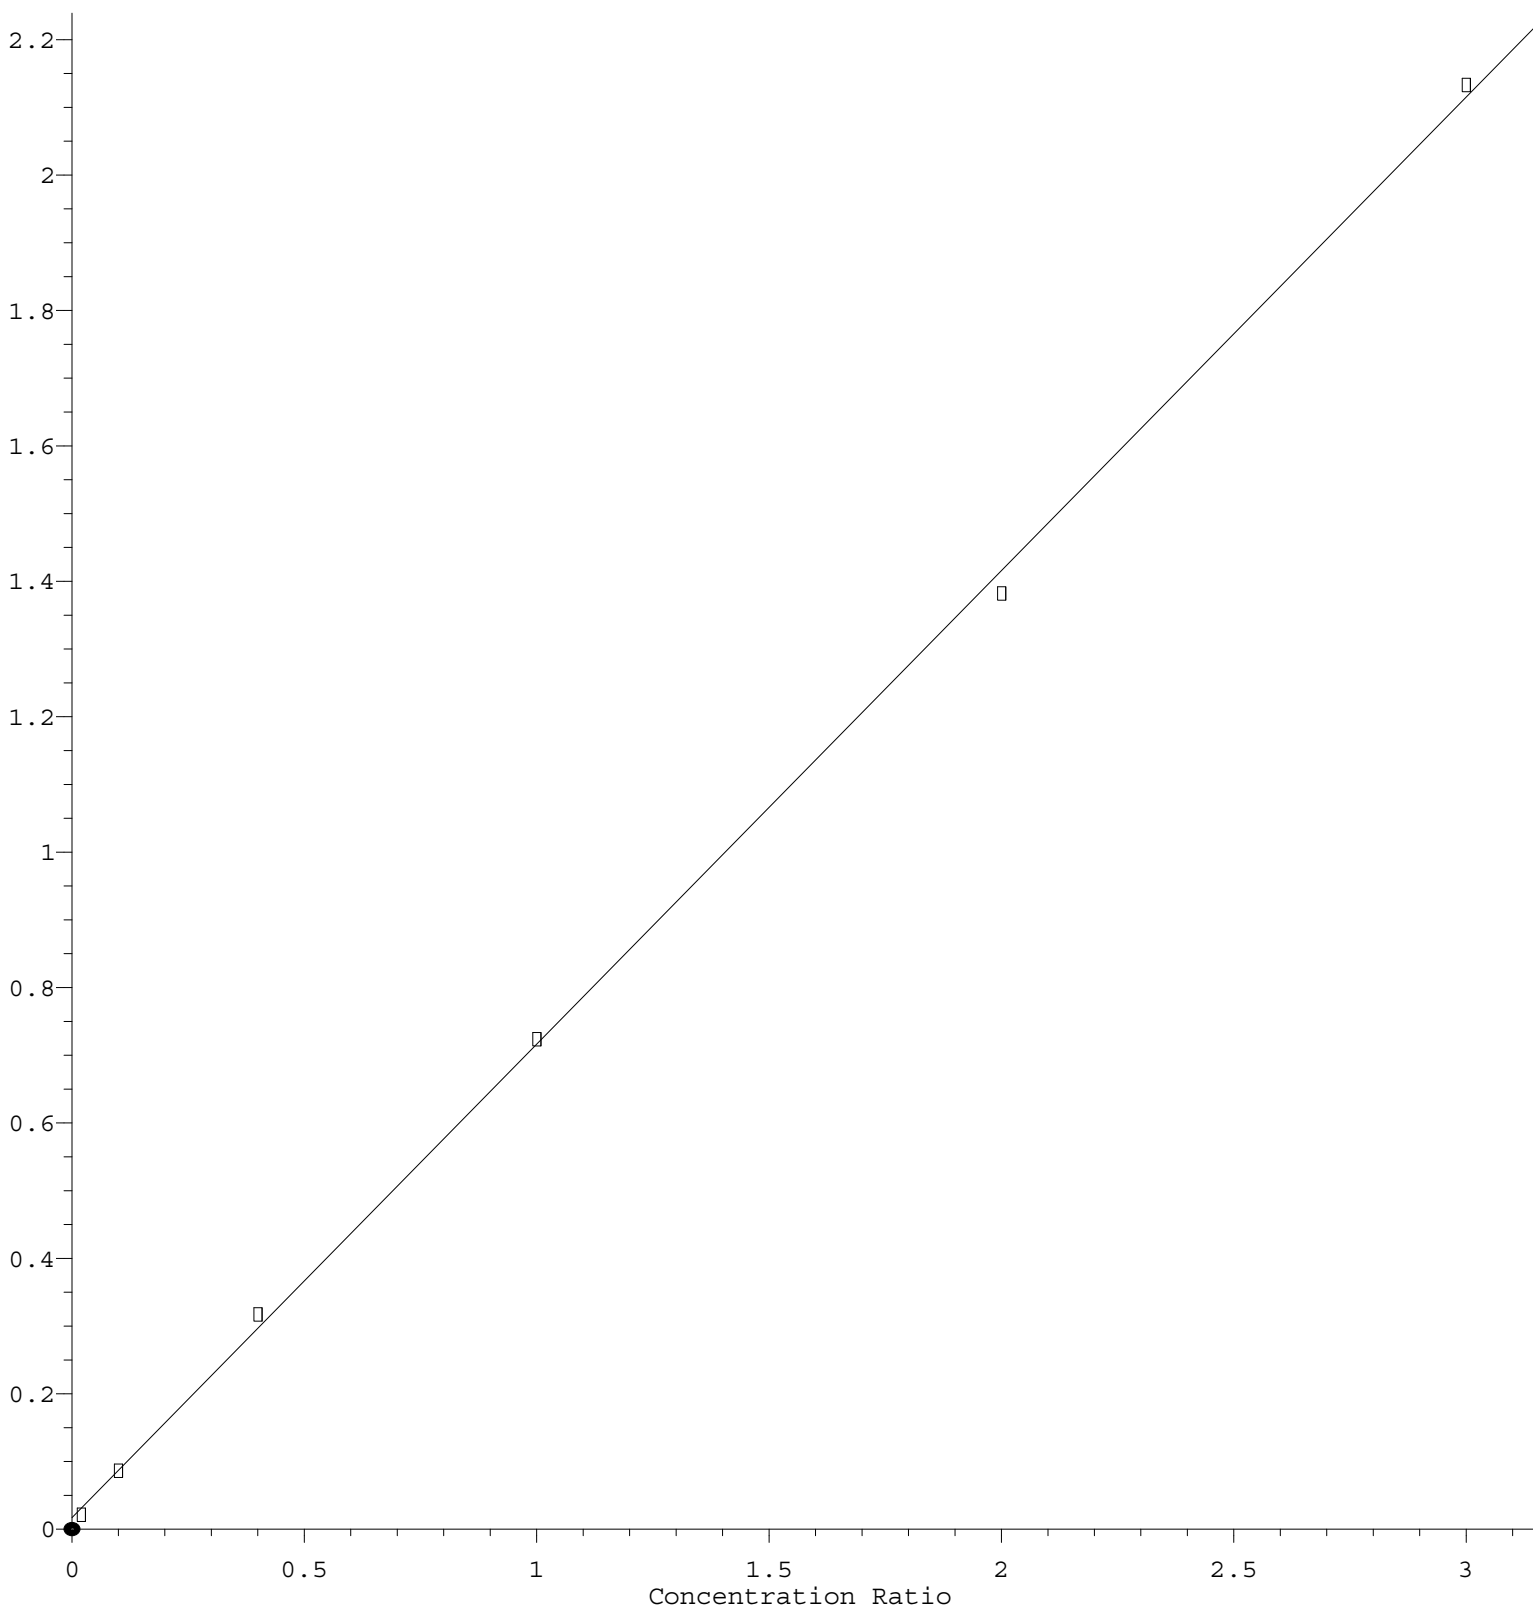

$$\text{Response} = 6.993\text{e-}001 * \text{Amt} + 1.718\text{e-}002$$

Coef of Det ( $r^2$ ) = 0.999418 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U060921W.M

Calibration Table Last Updated: Thu Jun 10 05:11:37 2021