

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\U060922\
 Data File : U048982.D
 Acq On : 09 Jun 2022 17:41
 Operator : SY/MD
 Sample : N3248-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYX7

Quant Time: Jun 10 01:04:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 10 01:01:44 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	333890	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	324896	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	180976	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	131782	64.440	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery	=	128.880%	
7) Chloroethane-d5	1.900	69	74132	48.385	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery	=	96.760%	
11) 1,1-Dichloroethene-d2	2.562	63	169048	36.551	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery	=	73.100%	
21) 2-Butanone-d5	4.623	46	223697	114.945	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery	=	114.940%	
24) Chloroform-d	5.063	84	213937	41.398	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery	=	82.800%	
26) 1,2-Dichloroethane-d4	5.700	65	140606	38.566	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery	=	77.140%	
32) Benzene-d6	5.726	84	407581	45.076	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery	=	90.160%	
36) 1,2-Dichloropropane-d6	6.690	67	141450	53.287	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery	=	106.580%	
41) Toluene-d8	7.899	98	380604	44.750	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery	=	89.500%	
43) trans-1,3-Dichloroprop...	8.179	79	67405	39.710	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery	=	79.420%	
47) 2-Hexanone-d5	8.632	63	164142	112.754	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery	=	112.750%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	223139	50.801	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery	=	101.600%	
66) 1,2-Dichlorobenzene-d4	12.195	152	164183	44.378	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery	=	88.760%	
Target Compounds						
					Qvalue	
5) Vinyl chloride	1.601	62	3962423	1682.467	ug/L	99
8) Chloroethane	1.919	64	1648851	1189.463	ug/L	98
10) 1,1,2-Trichloro-1,2,2-...	2.562	101	1494	0.637	ug/L #	17
12) 1,1-Dichloroethene	2.575	96	44772	20.610	ug/L #	64
13) Acetone	2.626	43	6381	4.036	ug/L	98
16) Methylene chloride	3.044	84	9518	3.763	ug/L	89
17) trans-1,2-Dichloroethene	3.350	96	121564	51.883	ug/L	96
19) 1,1-Dichloroethane	3.867	63	8693526	2026.650	ug/L	98
20) cis-1,2-Dichloroethene	4.665	96	5202541	1968.913	ug/L	95
22) 2-Butanone	4.710	43	9455	4.710	ug/L #	1
27) 1,2-Dichloroethane	5.793	62	59078	13.755	ug/L	96
29) Cyclohexane	5.382	56	3797	1.138	ug/L #	37
30) 1,1,1-Trichloroethane	5.314	97	782279	159.020	ug/L	98
31) Carbon tetrachloride	5.314	117	101698	22.684	ug/L	99
33) Benzene	5.774	78	119453	12.585	ug/L	100
34) Trichloroethene	6.539	95	83860	31.227	ug/L	97
35) Methylcyclohexane	6.761	83	10839	2.813	ug/L	93
39) cis-1,3-Dichloropropene	7.562	75	3814	0.941	ug/L #	68
40) 4-Methyl-2-pentanone	7.793	43	14112	3.896	ug/L #	92

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
 Data File : VU048982.D
 Acq On : 09 Jun 2022 17:41
 Operator : SY/MD
 Sample : N3248-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYX7

Quant Time: Jun 10 01:04:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jun 10 01:01:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


42) Toluene	7.970	91	976725	94.407	ug/L	99
44) trans-1,3-Dichloropropene	8.179	75	3083	0.721	ug/L	98
45) 1,1,2-Trichloroethane	8.401	97	13767	5.416	ug/L	92
46) Tetrachloroethene	8.555	164	7149	3.262	ug/L	95
49) Dibromochloromethane	8.549	129	7237	2.215	ug/L #	12
52) Ethylbenzene	9.571	91	3092993	261.606	ug/L	100
53) m,p-Xylene	9.694	106	2780071	585.111	ug/L	99
54) o-Xylene	10.102	106	1458761	320.476	ug/L	100
55) Styrene	10.102	104	71486	9.033	ug/L #	1
61) Isopropylbenzene	10.484	105	346337	31.074	ug/L	99
62) 1,3,5-Trimethylbenzene	11.089	105	2183520	344.599	ug/L	100
63) 1,2,4-Trimethylbenzene	11.472	105	10945140	1110.834	ug/L	99
67) 1,2-Dichlorobenzene	12.214	146	113424	19.402	ug/L	99
71) Naphthalene	14.086	128	561356	41.088	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
Data File : VU048982.D
Acq On : 09 Jun 2022 17:41
Operator : SY/MD
Sample : N3248-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYX7

Quant Time: Jun 10 01:04:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jun 10 01:01:44 2022
Response via : Initial Calibration




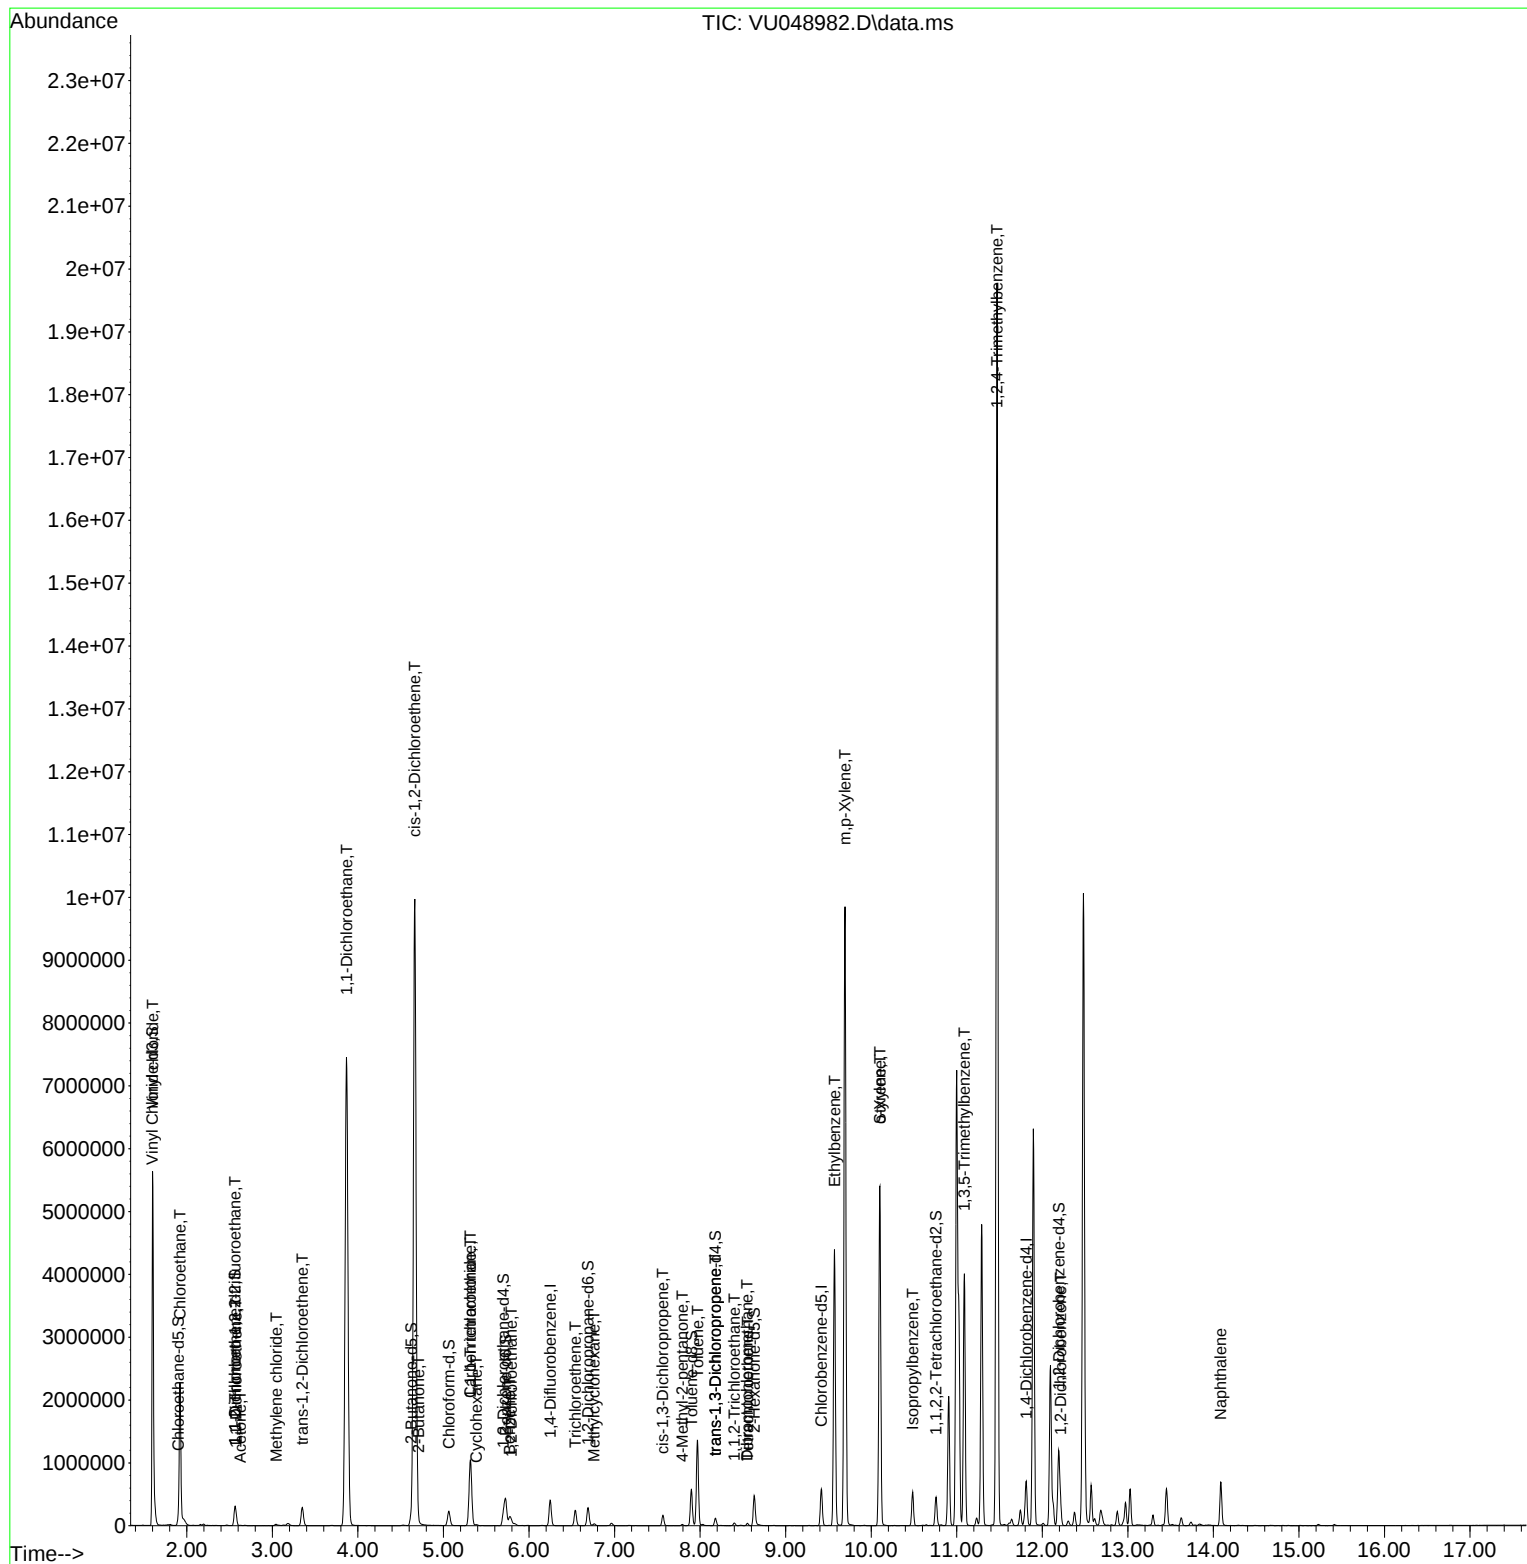


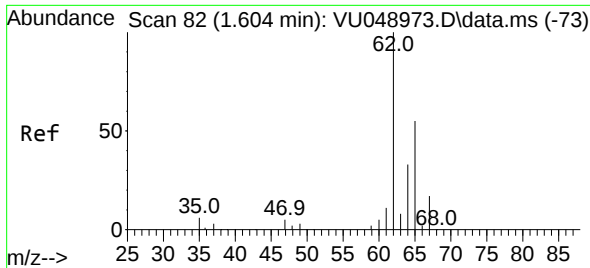

#5
 Vinyl chloride
 Concen: 1682.467 ug/L
 RT: 1.601 min Scan# 81
 Delta R.T. -0.003 min
 Lab File: VU048982.D
 Acq: 09 Jun 2022 17:41




Instrument :
 MSVOA_U
 ClientSampleId :
 EXYX7


Tgt Ion: 62 Resp: 3962423
 Ion Ratio Lower Upper
 62 100
 64 31.9 22.9 42.5

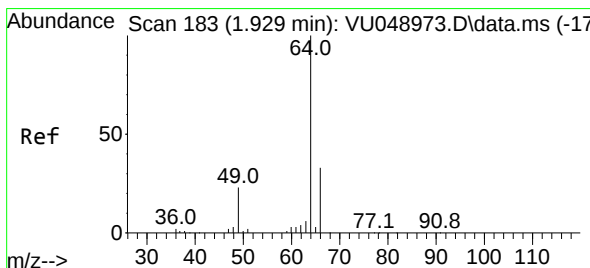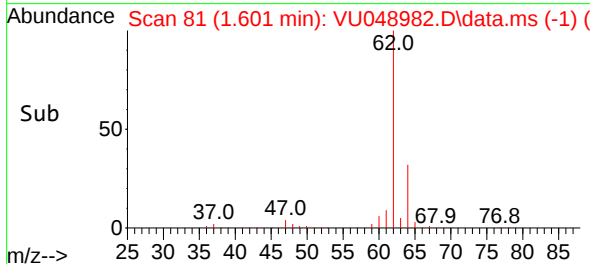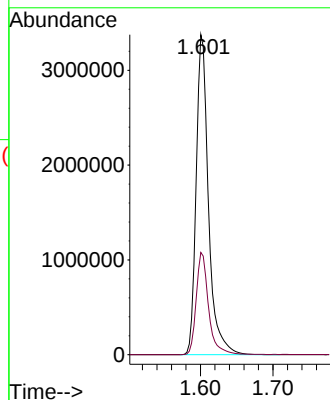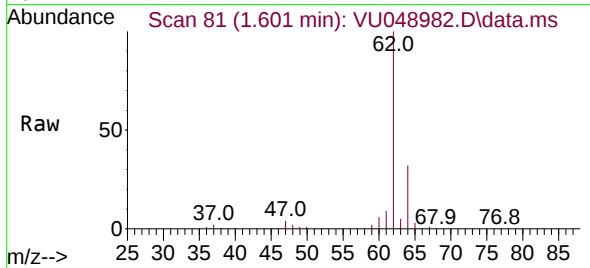

#8
 Chloroethane
 Concen: 1189.463 ug/L
 RT: 1.919 min Scan# 180
 Delta R.T. -0.010 min
 Lab File: VU048982.D
 Acq: 09 Jun 2022 17:41

Tgt Ion: 64 Resp: 1648851
 Ion Ratio Lower Upper
 64 100
 66 31.9 23.1 42.9


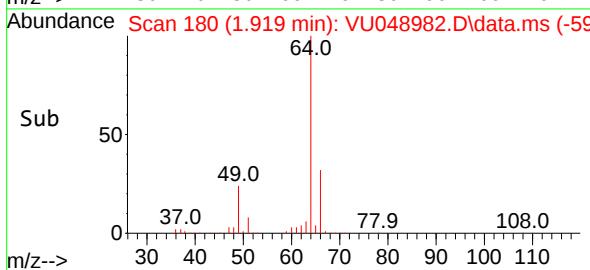
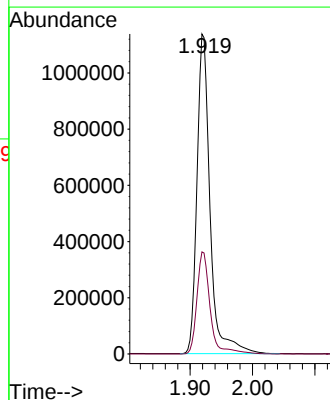
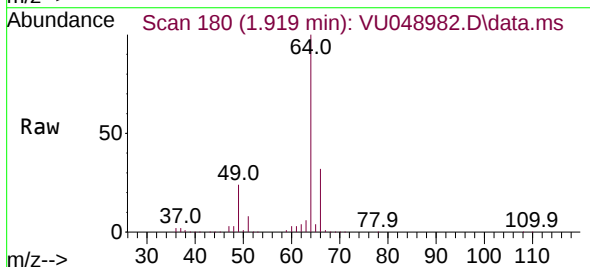




#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.637 ug/L
 RT: 2.562 min Scan# 31
 Delta R.T. -0.016 min
 Lab File: VU048982.D
 Acq: 09 Jun 2022 17:41




Instrument :
 MSVOA_U
 ClientSampleId :
 EXYX7


Tgt Ion:101 Resp: 1494
 Ion Ratio Lower Upper
 101 100
 85 0.0 35.7 53.5#
 151 0.0 64.4 96.6#

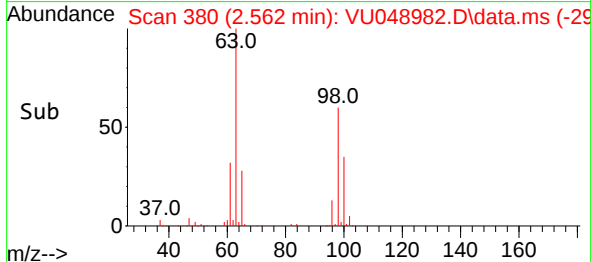

#12
 1,1-Dichloroethene
 Concen: 20.610 ug/L
 RT: 2.575 min Scan# 384
 Delta R.T. -0.003 min
 Lab File: VU048982.D
 Acq: 09 Jun 2022 17:41

Tgt Ion: 96 Resp: 44772
 Ion Ratio Lower Upper
 96 100
 61 182.6 120.6 224.0
 63 201.7 82.3 152.9#

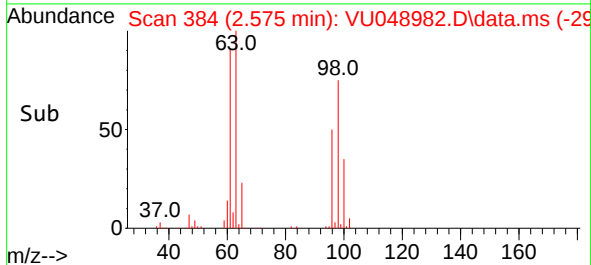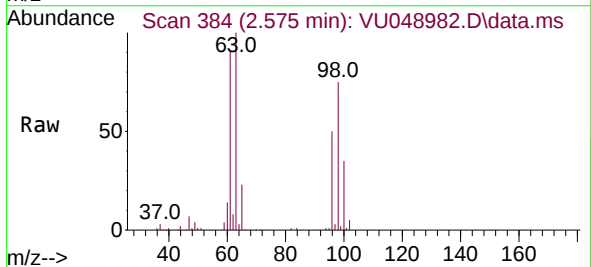



#13

Acetone

Concen: 4.036 ug/L

RT: 2.626 min Scan# 400

Delta R.T. 0.000 min

Lab File: VU048982.D

Acq: 09 Jun 2022 17:41

Instrument :

MSVOA_U

ClientSampleId :





EXYX7

Tgt Ion: 43 Resp: 6381

Ion Ratio Lower Upper

43 100

58 31.1 0.0 59.8

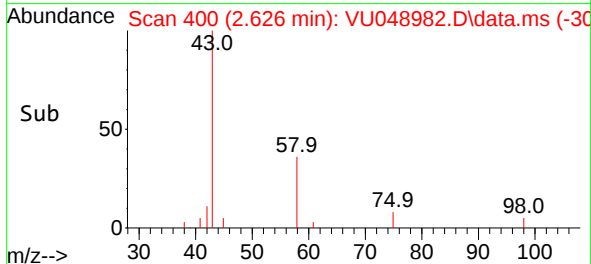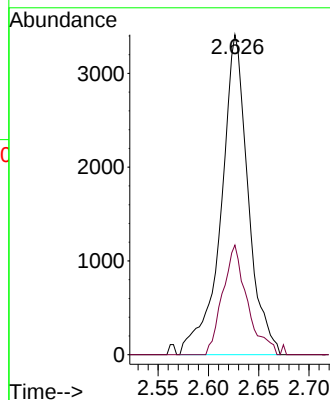

#16

Methylene chloride

Concen: 3.763 ug/L

RT: 3.044 min Scan# 530

Delta R.T. 0.000 min

Lab File: VU048982.D

Acq: 09 Jun 2022 17:41




Tgt Ion: 84 Resp: 9518


Ion Ratio Lower Upper

84 100

86 70.5 43.5 80.9

49 120.6 76.4 141.8


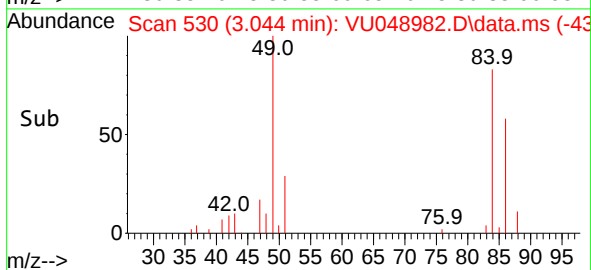
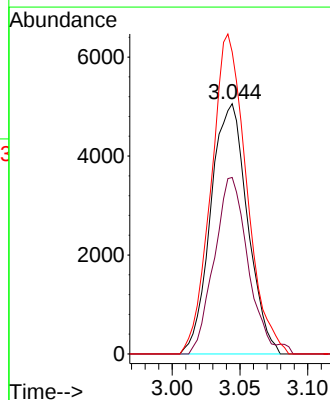
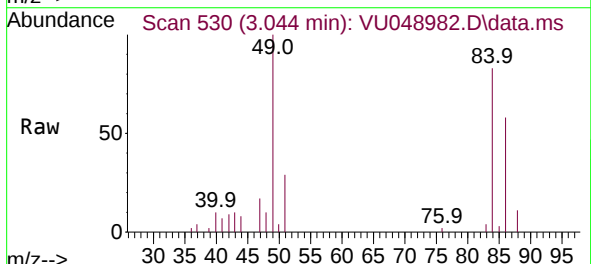




#17
trans-1,2-Dichloroethene
Concen: 51.883 ug/L
RT: 3.350 min Scan# 61
Delta R.T. -0.003 min
Lab File: VU048982.D
Acq: 09 Jun 2022 17:41




Instrument :
MSVOA_U
ClientSampleId :
EXYX7


Tgt Ion: 96 Resp: 121564
Ion Ratio Lower Upper
96 100
61 139.3 94.2 175.0
98 61.8 45.1 83.7

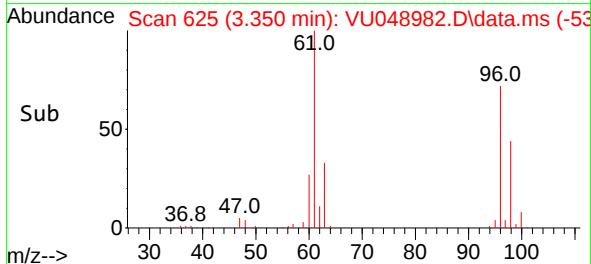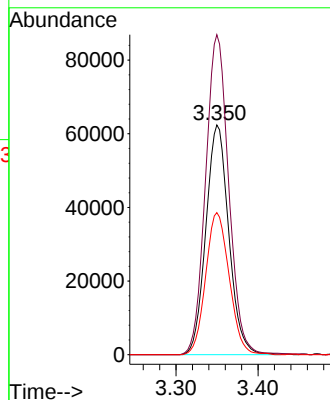

#19
1,1-Dichloroethane
Concen: 2026.650 ug/L
RT: 3.867 min Scan# 786
Delta R.T. -0.003 min
Lab File: VU048982.D
Acq: 09 Jun 2022 17:41

Tgt Ion: 63 Resp: 8693526
Ion Ratio Lower Upper
63 100
65 32.1 21.8 40.6
83 13.4 9.8 18.2

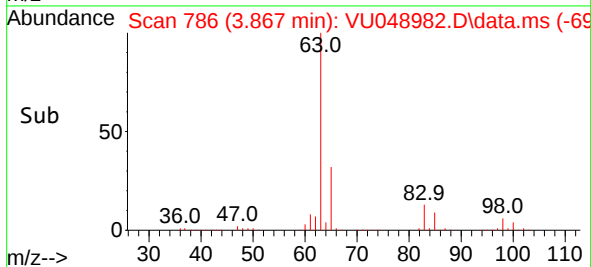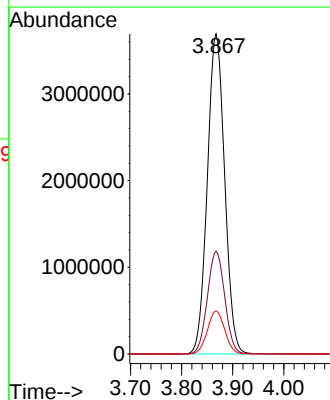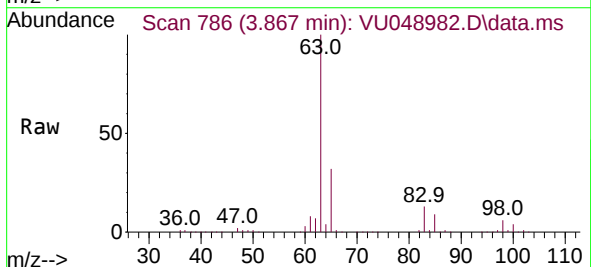







#20
 cis-1,2-Dichloroethene
 Concen: 1968.913 ug/L
 RT: 4.665 min Scan# 1034
 Delta R.T. -0.003 min
 Lab File: VU048982.D
 Acq: 09 Jun 2022 17:41

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYX7

Tgt Ion: 96 Resp: 5202541




Ion	Ratio	Lower	Upper
96	100		
61	131.4	88.3	164.1
68	0.0	0.0	0.0

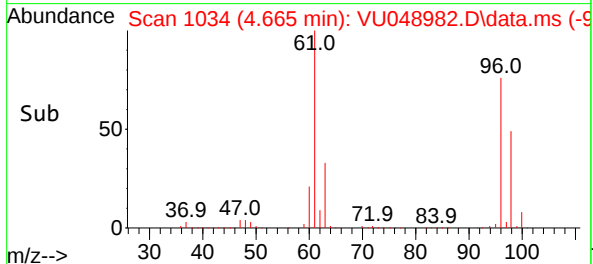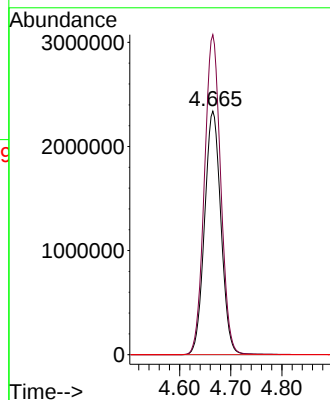


#22
 2-Butanone
 Concen: 4.710 ug/L
 RT: 4.710 min Scan# 1048
 Delta R.T. 0.006 min
 Lab File: VU048982.D
 Acq: 09 Jun 2022 17:41

Tgt Ion: 43 Resp: 9455

Ion	Ratio	Lower	Upper
43	100		
72	477.3	15.4	46.2#


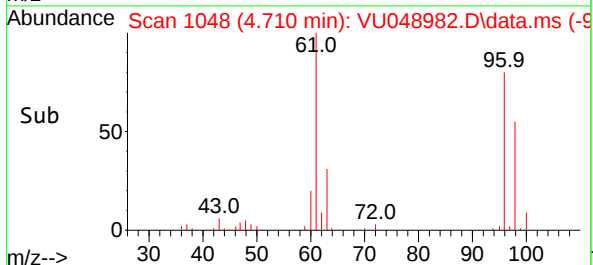
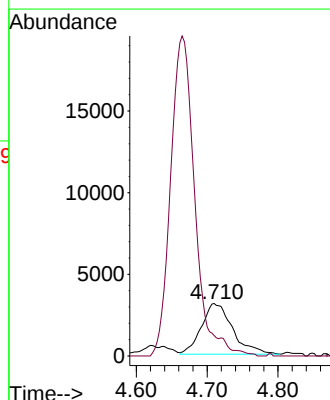
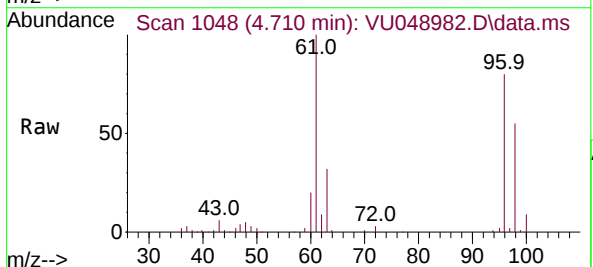




#27
1,2-Dichloroethane
Concen: 13.755 ug/L
RT: 5.793 min Scan# 11
Delta R.T. -0.003 min
Lab File: VU048982.D
Acq: 09 Jun 2022 17:41




Instrument :
MSVOA_U
ClientSampleId :
EXYX7


Tgt Ion: 62 Resp: 59078
Ion Ratio Lower Upper
62 100
98 8.8 6.0 9.0

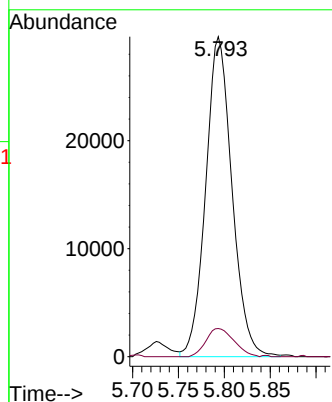

#29
Cyclohexane
Concen: 1.138 ug/L
RT: 5.382 min Scan# 1257
Delta R.T. -0.006 min
Lab File: VU048982.D
Acq: 09 Jun 2022 17:41

Tgt Ion: 56 Resp: 3797
Ion Ratio Lower Upper
56 100
69 29.1 26.5 39.7
84 178.4 78.0 117.0#

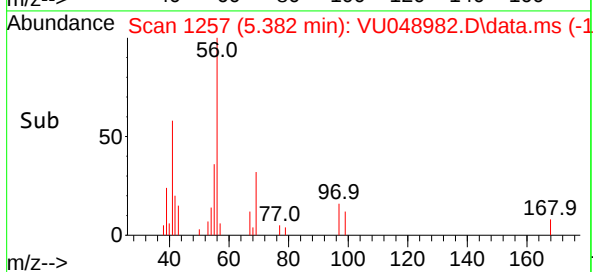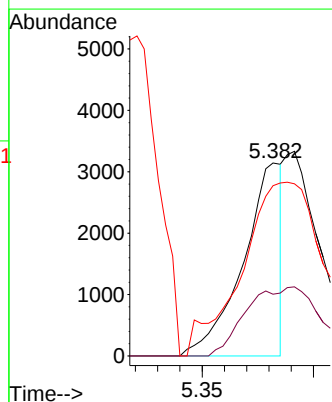



#30

1,1,1-Trichloroethane

Concen: 159.020 ug/L

RT: 5.314 min Scan# 1236

Delta R.T. -0.003 min

Lab File: VU048982.D

Acq: 09 Jun 2022 17:41

Instrument :

MSVOA_U

ClientSampleId :

EXYX7





Tgt Ion: 97 Resp: 782279

Ion Ratio Lower Upper

97 100

99 64.5 50.3 75.5

61 41.4 32.6 48.8

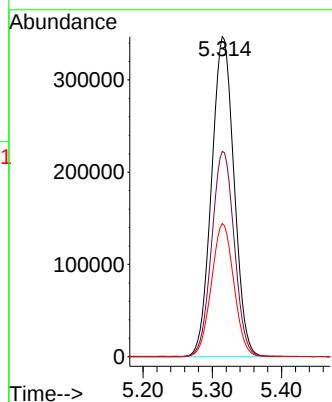

#31

Carbon tetrachloride

Concen: 22.684 ug/L

RT: 5.314 min Scan# 1236

Delta R.T. -0.209 min

Lab File: VU048982.D




Acq: 09 Jun 2022 17:41


Tgt Ion: 117 Resp: 101698

Ion Ratio Lower Upper

117 100

119 93.9 76.0 114.0


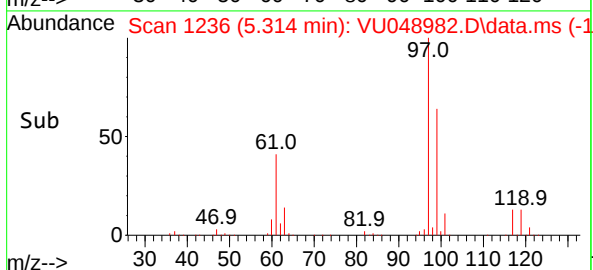






#33
Benzene
Concen: 12.585 ug/L
RT: 5.774 min Scan# 11
Delta R.T. 0.000 min
Lab File: VU048982.D
Acq: 09 Jun 2022 17:41

Instrument :
MSVOA_U
ClientSampleId :
EXYX7




Tgt Ion: 78 Resp: 119453

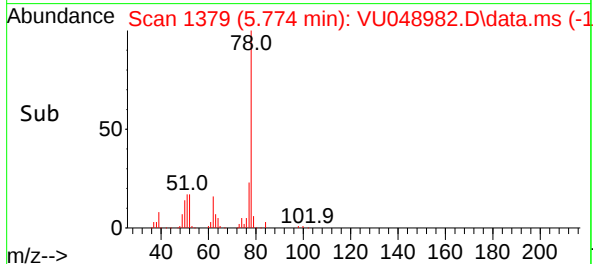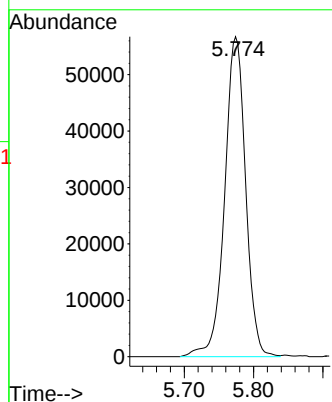


#34
Trichloroethene
Concen: 31.227 ug/L
RT: 6.539 min Scan# 1617
Delta R.T. -0.003 min
Lab File: VU048982.D
Acq: 09 Jun 2022 17:41

Tgt Ion: 95 Resp: 83860

Ion	Ratio	Lower	Upper
95	100		
97	62.0	45.2	84.0
132	93.7	67.3	124.9
130	96.5	70.7	131.3

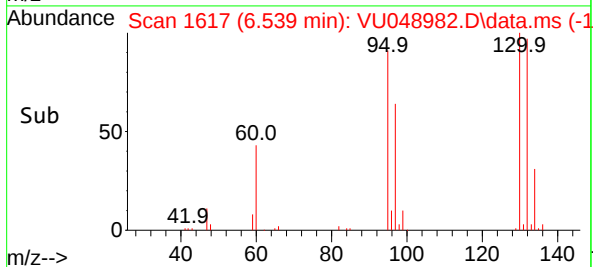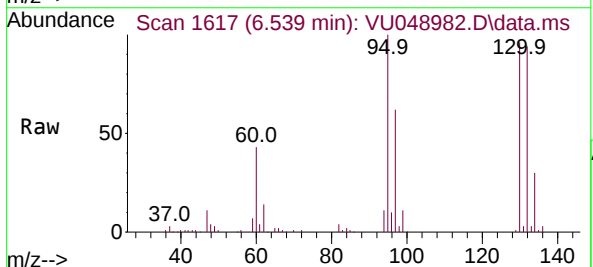



#35

Methylcyclohexane

Concen: 2.813 ug/L

RT: 6.761 min Scan# 1

Delta R.T. -0.003 min

Lab File: VU048982.D

Acq: 09 Jun 2022 17:41

Instrument :

MSVOA_U

ClientSampleId :

EXYX7





Tgt Ion: 83 Resp: 10839

Ion Ratio Lower Upper

83 100

55 79.9 56.2 84.4

98 47.2 38.2 57.2

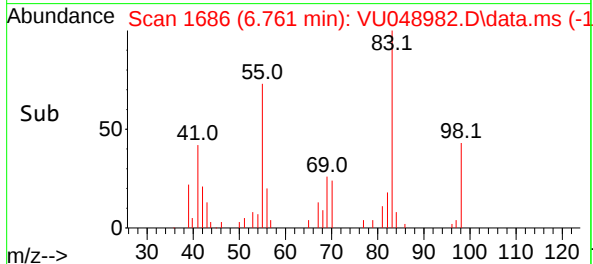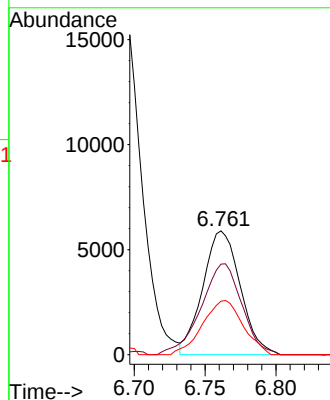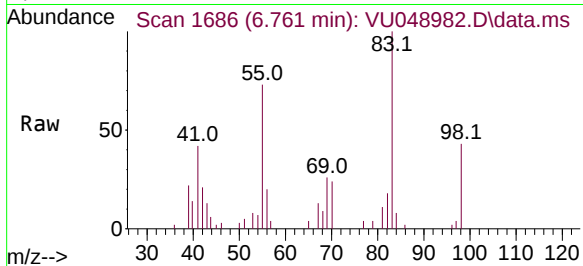

#39

cis-1,3-Dichloropropene

Concen: 0.941 ug/L

RT: 7.562 min Scan# 1935

Delta R.T. -0.045 min

Lab File: VU048982.D




Acq: 09 Jun 2022 17:41


Tgt Ion: 75 Resp: 3814

Ion Ratio Lower Upper

75 100

77 50.7 22.9 42.5#

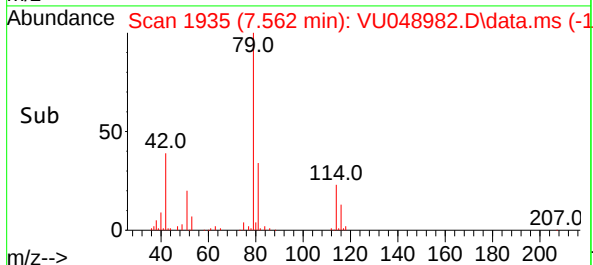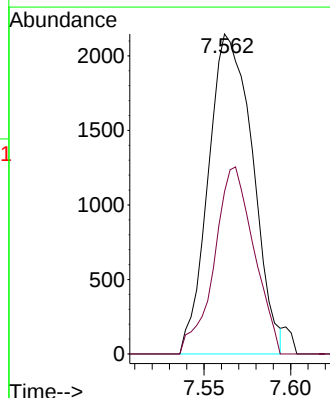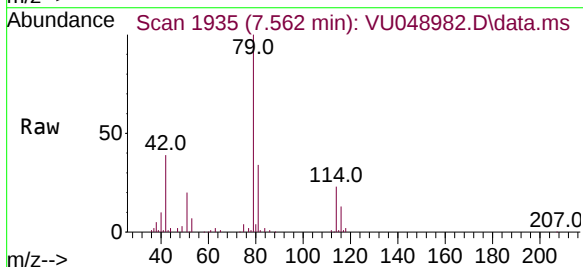



#40

4-Methyl-2-pentanone

Concen: 3.896 ug/L

RT: 7.793 min Scan# 2006

Delta R.T. 0.003 min

Lab File: VU048982.D

Acq: 09 Jun 2022 17:41

Instrument :

MSVOA_U

ClientSampleId :

EXYX7





Tgt Ion: 43 Resp: 14112

Ion Ratio Lower Upper

43 100

58 39.5 34.3 51.5

100 12.0 14.7 22.1#

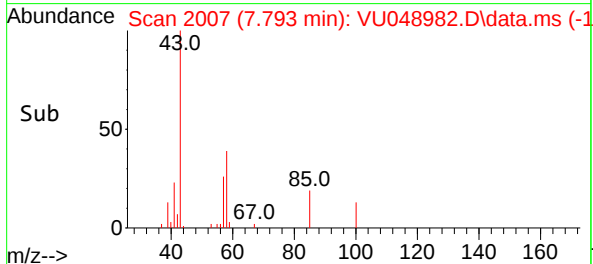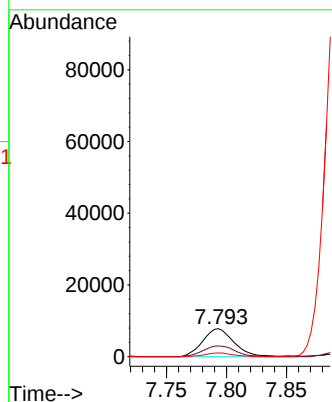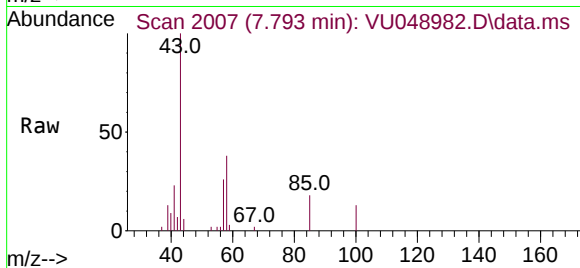

#42

Toluene

Concen: 94.407 ug/L

RT: 7.970 min Scan# 2062

Delta R.T. 0.000 min

Lab File: VU048982.D




Acq: 09 Jun 2022 17:41


Tgt Ion: 91 Resp: 976725

Ion Ratio Lower Upper

91 100

92 58.7 41.4 77.0


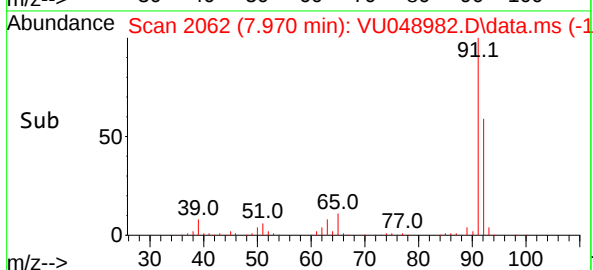

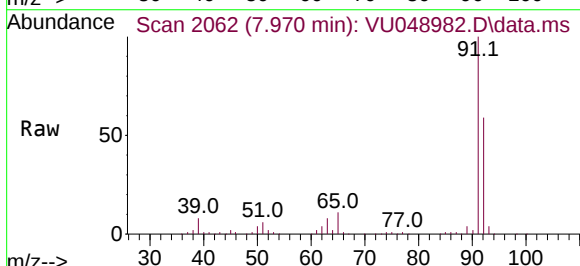




#44
trans-1,3-Dichloropropene
Concen: 0.721 ug/L
RT: 8.179 min Scan# 2137
Delta R.T. -0.032 min
Lab File: VU048982.D
Acq: 09 Jun 2022 17:41




Instrument :
MSVOA_U
ClientSampleId :
EXYX7


Tgt Ion: 75 Resp: 3083
Ion Ratio Lower Upper
75 100
77 31.4 22.7 42.1

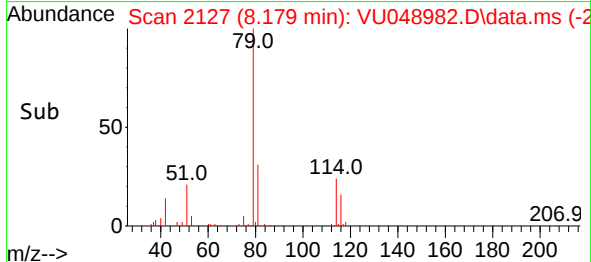

#45
1,1,2-Trichloroethane
Concen: 5.416 ug/L
RT: 8.401 min Scan# 2196
Delta R.T. 0.000 min
Lab File: VU048982.D
Acq: 09 Jun 2022 17:41

Tgt Ion: 97 Resp: 13767
Ion Ratio Lower Upper
97 100
99 66.6 42.2 78.4
83 93.5 58.4 108.6
85 55.8 38.2 71.0


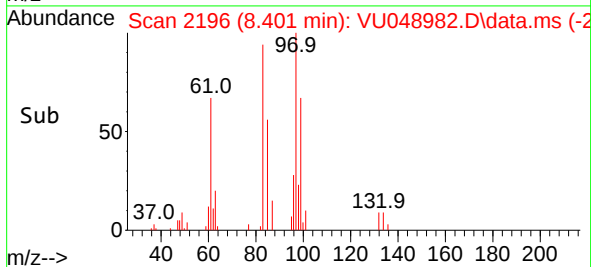
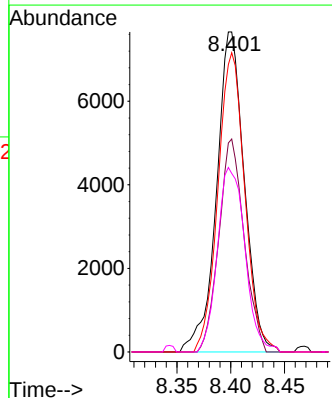
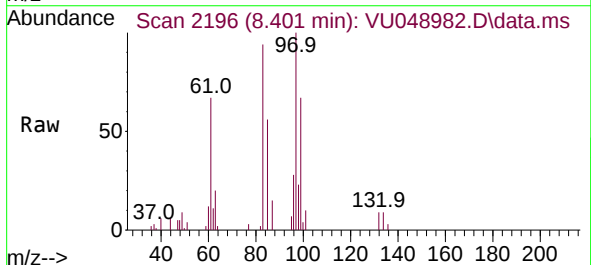




#46
Tetrachloroethene
Concen: 3.262 ug/L
RT: 8.555 min Scan# 2149
Delta R.T. 0.000 min
Lab File: VU048982.D
Acq: 09 Jun 2022 17:41




Instrument :
MSVOA_U
ClientSampleId :
EXYX7


Tgt Ion:164 Resp: 7149
Ion Ratio Lower Upper
164 100
129 82.3 64.3 119.3
131 88.0 64.5 119.7
166 122.3 87.5 162.5

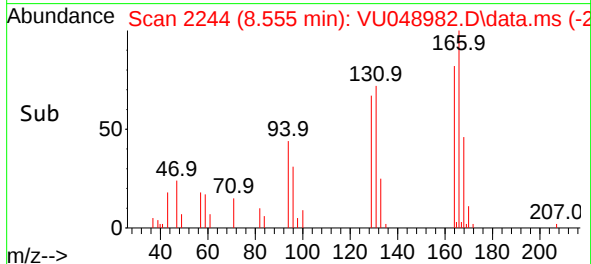

#49
Dibromochloromethane
Concen: 2.215 ug/L
RT: 8.549 min Scan# 2242
Delta R.T. -0.260 min
Lab File: VU048982.D
Acq: 09 Jun 2022 17:41

Tgt Ion:129 Resp: 7237
Ion Ratio Lower Upper
129 100
127 0.0 53.1 98.5#


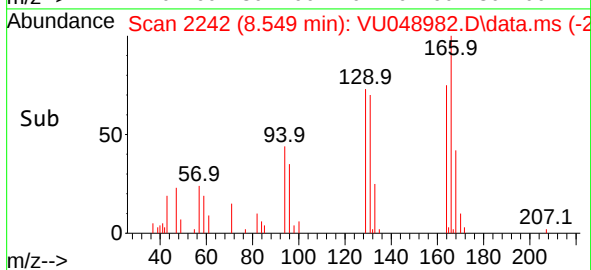

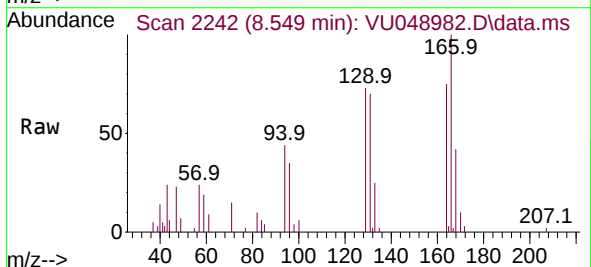




#52
Ethylbenzene
Concen: 261.606 ug/L
RT: 9.571 min Scan# 2560
Delta R.T. 0.000 min
Lab File: VU048982.D
Acq: 09 Jun 2022 17:41




Instrument :
MSVOA_U
ClientSampleId :
EXYX7


Tgt Ion: 91 Resp: 3092993
Ion Ratio Lower Upper
91 100
106 31.3 21.8 40.6

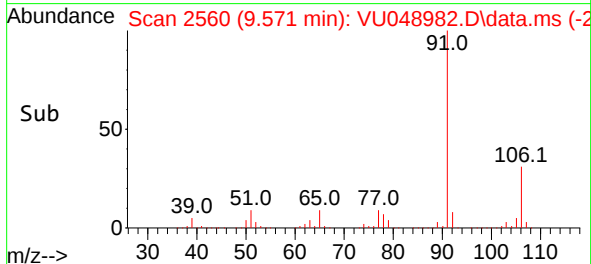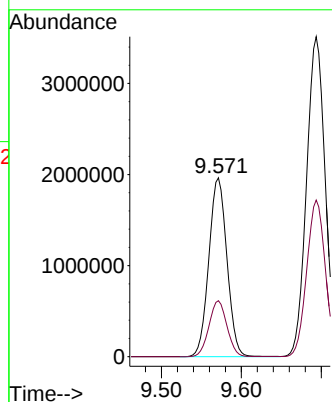

#53
m,p-Xylene
Concen: 585.111 ug/L
RT: 9.694 min Scan# 2598
Delta R.T. 0.000 min
Lab File: VU048982.D
Acq: 09 Jun 2022 17:41

Tgt Ion: 106 Resp: 2780071
Ion Ratio Lower Upper
106 100
91 204.3 141.8 263.4




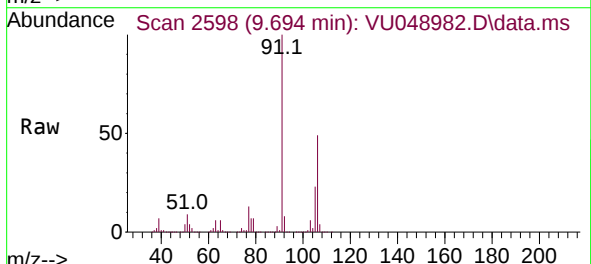




#54
o-Xylene
Concen: 320.476 ug/L
RT: 10.102 min Scan# 2725
Delta R.T. 0.000 min
Lab File: VU048982.D
Acq: 09 Jun 2022 17:41




Instrument :
MSVOA_U
ClientSampleId :
EXYX7


Tgt Ion:106 Resp: 1458761
Ion Ratio Lower Upper
106 100
91 214.4 150.1 278.9

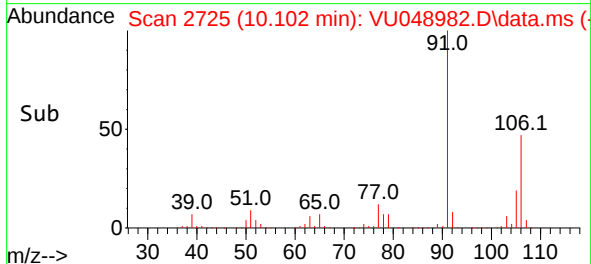

#55
Styrene
Concen: 9.033 ug/L
RT: 10.102 min Scan# 2725
Delta R.T. -0.013 min
Lab File: VU048982.D
Acq: 09 Jun 2022 17:41

Tgt Ion:104 Resp: 71486
Ion Ratio Lower Upper
104 100
78 302.7 32.7 60.7#




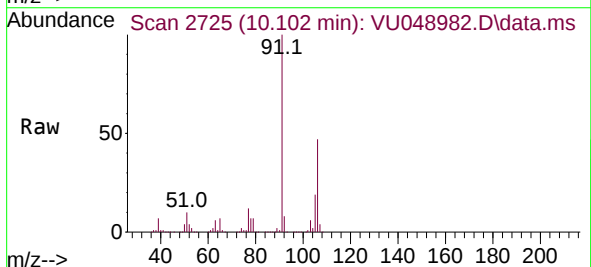


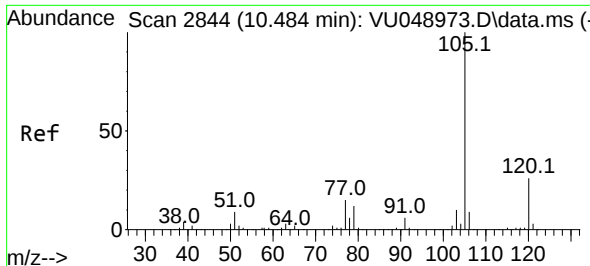

#61
Isopropylbenzene
Concen: 31.074 ug/L
RT: 10.484 min Scan# 21
Delta R.T. 0.000 min
Lab File: VU048982.D
Acq: 09 Jun 2022 17:41




Instrument :
MSVOA_U
ClientSampleId :
EXYX7


Tgt Ion:105 Resp: 346337
Ion Ratio Lower Upper
105 100
120 25.8 21.0 31.6
77 15.5 12.5 18.7

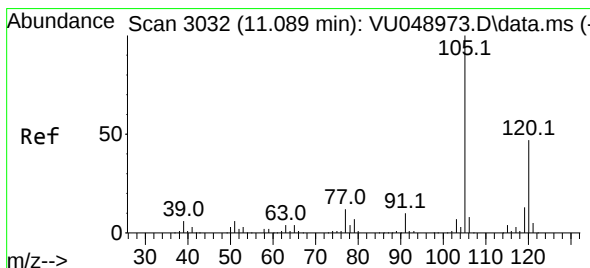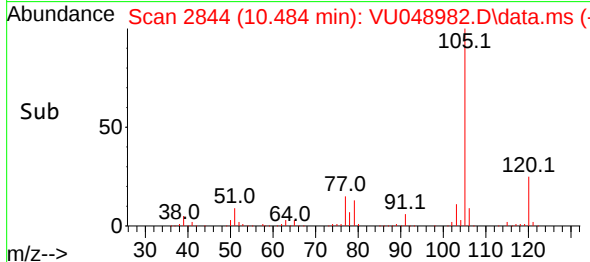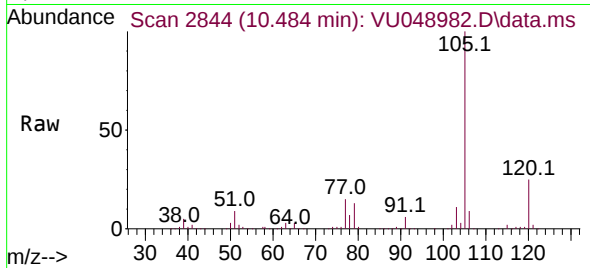

#62
1,3,5-Trimethylbenzene
Concen: 344.599 ug/L
RT: 11.089 min Scan# 3032
Delta R.T. 0.000 min
Lab File: VU048982.D
Acq: 09 Jun 2022 17:41

Tgt Ion:105 Resp: 2183520
Ion Ratio Lower Upper
105 100
120 48.2 38.5 57.7

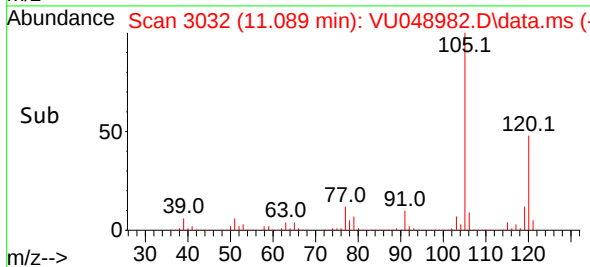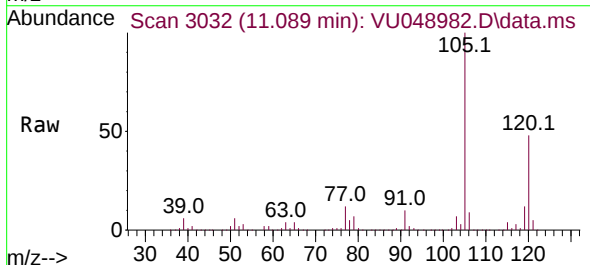



#63

1,2,4-Trimethylbenzene

Concen: 1110.834 ug/L

RT: 11.472 min Scan# 3151

Delta R.T. 0.003 min

Lab File: VU048982.D

Acq: 09 Jun 2022 17:41

Instrument :

MSVOA_U

ClientSampleId :





EXYX7

Tgt Ion:105 Resp:10945140

Ion Ratio Lower Upper

105 100

120 44.7 35.4 53.2

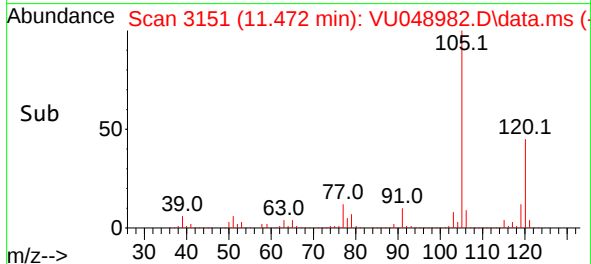

#67

1,2-Dichlorobenzene

Concen: 19.402 ug/L

RT: 12.214 min Scan# 3382

Delta R.T. 0.003 min

Lab File: VU048982.D

Acq: 09 Jun 2022 17:41




Tgt Ion:146 Resp: 113424


Ion Ratio Lower Upper

146 100

111 41.2 34.1 51.1


148 63.7 50.9 76.3

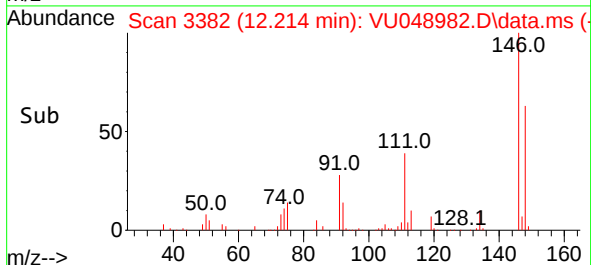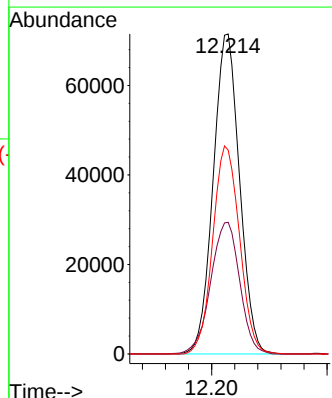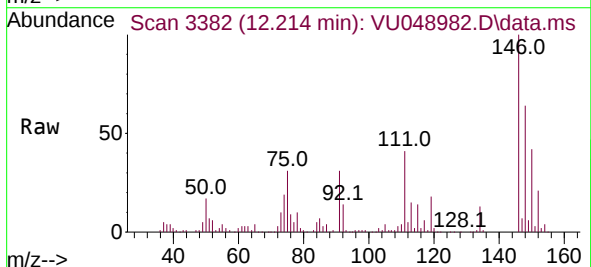



#71
Naphthalene
Concen: 41.088 ug/L
RT: 14.086 min Scan# 3964
Delta R.T. 0.000 min
Lab File: VU048982.D
Acq: 09 Jun 2022 17:41

Instrument :
MSVOA_U
ClientSampleId :
EXYX7

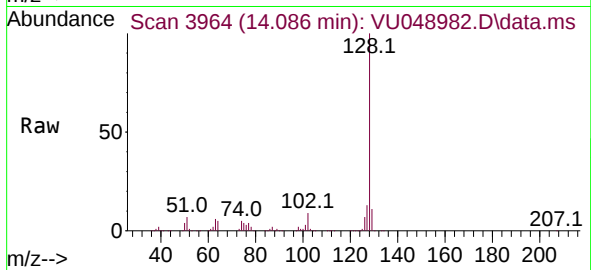

Tgt Ion:	128	Resp:	561356
Ion	Ratio	Lower	Upper
128	100		
127	12.6	10.6	16.0
129	10.9	8.8	13.2

