

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
 Data File : VU048975.D
 Acq On : 09 Jun 2022 13:33
 Operator : SY/MD
 Sample : N3248-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYW6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048975.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rBV	158525	181630	13.28%	1.443%
2	1.893	165	172	187	rVB	113542	150310	10.99%	1.194%
3	2.562	367	380	396	rBV2	284703	497693	36.40%	3.955%
4	2.861	470	473	476	rBV2	363	223	0.02%	0.002%
5	3.009	516	519	522	rBV2	279	201	0.01%	0.002%
6	3.044	522	530	537	rBV4	1242	1975	0.14%	0.016%
7	3.182	559	573	591	rVB	17202	39922	2.92%	0.317%
8	3.350	613	625	640	rBV2	22339	44585	3.26%	0.354%
9	3.449	654	656	657	rBV2	263	105	0.01%	0.001%
10	3.588	696	699	700	rBV	431	184	0.01%	0.001%
11	3.639	712	715	716	rBV	191	119	0.01%	0.001%
12	3.674	723	726	727	rBV	253	166	0.01%	0.001%
13	3.774	754	757	763	rVB2	352	322	0.02%	0.003%
14	3.800	763	765	766	rBV	123	54	0.00%	0.000%
15	3.867	767	786	806	rVV	167305	396100	28.97%	3.147%
16	3.980	819	821	823	rVB	140	57	0.00%	0.000%
17	4.006	823	829	831	rBV	461	424	0.03%	0.003%
18	4.279	911	914	917	rVB	424	248	0.02%	0.002%
19	4.298	917	920	924	rBV2	289	215	0.02%	0.002%
20	4.362	938	940	943	rBV	331	167	0.01%	0.001%
21	4.414	954	956	959	rVB	409	213	0.02%	0.002%
22	4.620	1000	1020	1024	rBV	166166	309380	22.62%	2.458%
23	5.060	1141	1157	1182	rBV	244234	539892	39.48%	4.290%
24	5.208	1198	1203	1207	rVB2	420	388	0.03%	0.003%
25	5.234	1208	1211	1213	rBV	181	88	0.01%	0.001%
26	5.314	1219	1236	1261	rBV	603150	1367438	100.00%	10.866%
27	5.456	1278	1280	1284	rVB	358	207	0.02%	0.002%
28	5.494	1289	1292	1294	rVB2	284	151	0.01%	0.001%
29	5.523	1294	1301	1307	rBV4	749	1099	0.08%	0.009%
30	5.594	1321	1323	1326	rBV2	289	149	0.01%	0.001%
31	5.723	1342	1363	1382	rBV2	476681	1316543	96.28%	10.461%
32	5.925	1424	1426	1427	rBV2	247	102	0.01%	0.001%
33	5.967	1437	1439	1440	rBV2	358	154	0.01%	0.001%
34	6.050	1462	1465	1467	rVB	760	448	0.03%	0.004%
35	6.070	1467	1471	1475	rBV2	282	294	0.02%	0.002%
36	6.182	1505	1506	1507	rBV	274	57	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
 Data File : VU048975.D
 Acq On : 09 Jun 2022 13:33
 Operator : SY/MD
 Sample : N3248-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYW6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

37	6.250	1513	1527	1549	rBV	404349	766258	56.04%	6.089%
38	6.542	1605	1618	1630	rBV6	15321	29889	2.19%	0.237%
39	6.690	1650	1664	1685	rBV	311292	605924	44.31%	4.815%
40	6.787	1691	1694	1695	rBV	445	300	0.02%	0.002%
41	6.796	1695	1697	1705	rVV5	1012	1151	0.08%	0.009%
42	6.883	1722	1724	1727	rBV	236	150	0.01%	0.001%
43	6.944	1741	1743	1744	rBV	187	65	0.00%	0.001%
44	6.986	1753	1756	1760	rBV	312	263	0.02%	0.002%
45	7.002	1760	1761	1763	rBV	187	86	0.01%	0.001%
46	7.182	1807	1817	1826	rBV6	3104	6271	0.46%	0.050%
47	7.237	1832	1834	1836	rBV	217	80	0.01%	0.001%
48	7.366	1873	1874	1877	rVB	282	115	0.01%	0.001%
49	7.385	1877	1880	1881	rBV2	405	152	0.01%	0.001%
50	7.446	1896	1899	1900	rBV	276	183	0.01%	0.001%
51	7.478	1904	1909	1910	rBV	239	181	0.01%	0.001%
52	7.513	1917	1920	1922	rBV	288	144	0.01%	0.001%
53	7.565	1923	1936	1958	rVV	177088	306026	22.38%	2.432%
54	7.658	1963	1965	1968	rVB2	501	218	0.02%	0.002%
55	7.687	1969	1974	1982	rBV5	1497	2366	0.17%	0.019%
56	7.732	1986	1988	1991	rVB	436	187	0.01%	0.001%
57	7.755	1993	1995	2000	rBV	378	251	0.02%	0.002%
58	7.800	2000	2009	2015	rBV6	2050	3029	0.22%	0.024%
59	7.841	2020	2022	2026	rBV2	406	295	0.02%	0.002%
60	7.899	2026	2040	2055	rBV	594731	1030077	75.33%	8.185%
61	8.108	2103	2105	2106	rBV2	220	85	0.01%	0.001%
62	8.179	2111	2127	2148	rBV2	132270	245245	17.93%	1.949%
63	8.398	2188	2195	2206	rBV7	3074	5164	0.38%	0.041%
64	8.475	2208	2219	2231	rVB2	32260	55480	4.06%	0.441%
65	8.555	2232	2244	2256	rBV2	83028	136600	9.99%	1.085%
66	8.632	2257	2268	2295	rBV	454440	835881	61.13%	6.642%
67	8.880	2343	2345	2351	rVB4	487	286	0.02%	0.002%
68	8.960	2367	2370	2373	rVB2	631	354	0.03%	0.003%
69	8.980	2373	2376	2381	rBV2	490	454	0.03%	0.004%
70	9.259	2459	2463	2466	rBV	348	323	0.02%	0.003%
71	9.295	2471	2474	2476	rVB2	215	100	0.01%	0.001%
72	9.417	2499	2512	2548	rBV	556824	931800	68.14%	7.404%
73	9.562	2554	2557	2560	rBV2	721	740	0.05%	0.006%
74	9.619	2572	2575	2579	rBV2	263	195	0.01%	0.002%
75	9.697	2591	2599	2609	rBV4	1409	2435	0.18%	0.019%
76	9.915	2664	2667	2671	rVB2	378	244	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
 Data File : VU048975.D
 Acq On : 09 Jun 2022 13:33
 Operator : SY/MD
 Sample : N3248-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYW6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

77	9.938	2671	2674	2676	rBV2	248	157	0.01%	0.001%
78	10.185	2749	2751	2757	rVB2	321	253	0.02%	0.002%
79	10.336	2797	2798	2801	rBV	483	119	0.01%	0.001%
80	10.381	2809	2812	2814	rBV3	402	258	0.02%	0.002%
81	10.475	2839	2841	2843	rBV2	742	348	0.03%	0.003%
82	10.558	2864	2867	2869	rBV	342	197	0.01%	0.002%
83	10.639	2888	2892	2896	rVB3	725	701	0.05%	0.006%
84	10.674	2897	2903	2911	rVV6	1814	2524	0.18%	0.020%
85	10.758	2916	2929	2946	rBV	491219	779657	57.02%	6.195%
86	10.893	2960	2971	2984	rVB2	38762	64525	4.72%	0.513%
87	10.999	3001	3004	3007	rBV2	373	238	0.02%	0.002%
88	11.066	3021	3025	3027	rBV2	582	427	0.03%	0.003%
89	11.217	3070	3072	3075	rVB	427	196	0.01%	0.002%
90	11.295	3093	3096	3099	rBV2	377	262	0.02%	0.002%
91	11.353	3111	3114	3120	rBV2	523	569	0.04%	0.005%
92	11.385	3122	3124	3126	rBV	425	209	0.02%	0.002%
93	11.751	3232	3238	3244	rVB3	1711	2054	0.15%	0.016%
94	11.812	3245	3257	3273	rBV	575086	913453	66.80%	7.258%
95	12.195	3363	3376	3397	rBV	607613	978637	71.57%	7.776%
96	12.369	3429	3430	3431	rBV	510	124	0.01%	0.001%
97	12.777	3548	3557	3567	rVB	11887	19731	1.44%	0.157%




Sum of corrected areas: 12584989

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
Data File : VU048975.D
Acq On : 09 Jun 2022 13:33
Operator : SY/MD
Sample : N3248-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYW6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

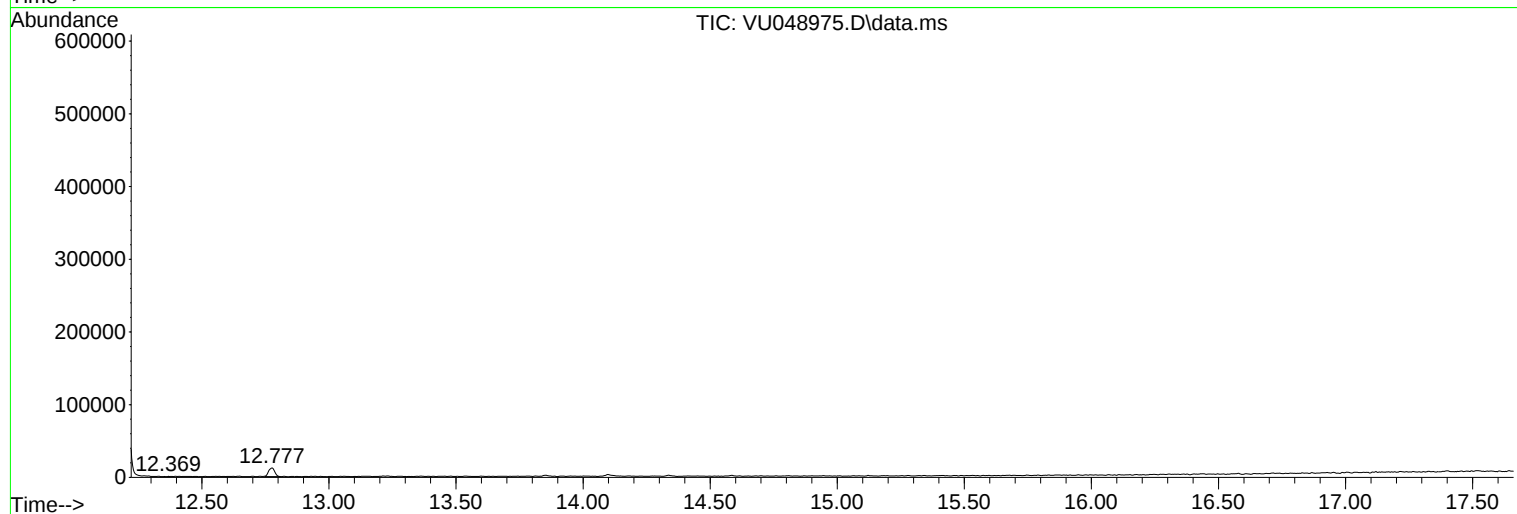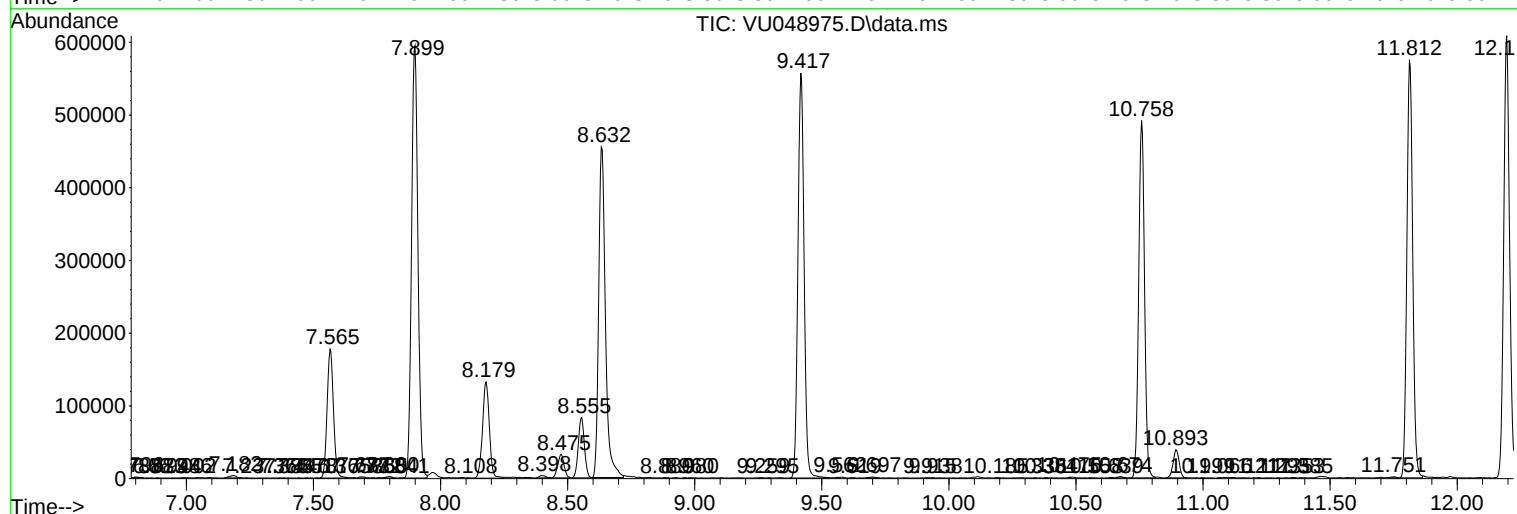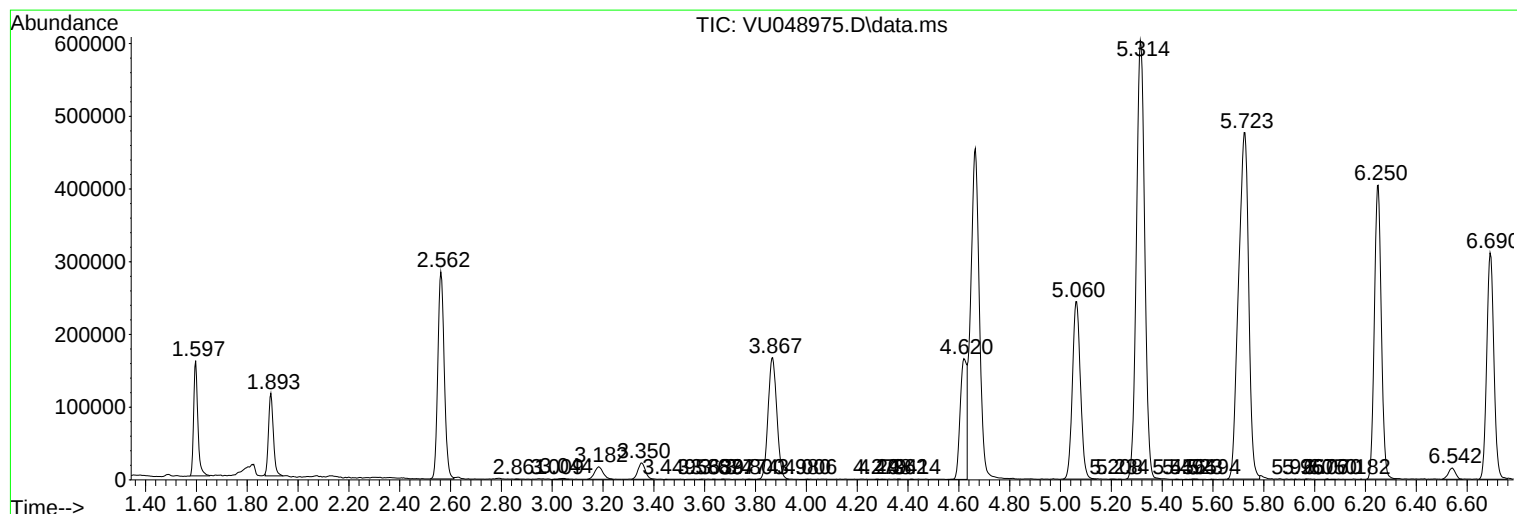

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
Data File : VU048975.D
Acq On : 09 Jun 2022 13:33
Operator : SY/MD
Sample : N3248-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYW6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
Data File : VU048975.D
Acq On : 09 Jun 2022 13:33
Operator : SY/MD
Sample : N3248-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYW6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------