

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
 Data File : VU048976.D
 Acq On : 09 Jun 2022 13:56
 Operator : SY/MD
 Sample : N3248-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYW7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048976.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	98	rBV	176061	194673	3.13%	0.856%
2	1.903	166	175	195	rVB	118874	164600	2.65%	0.723%
3	2.076	223	229	237	rVB	12349	15347	0.25%	0.067%
4	2.134	239	247	252	rBV	16472	23232	0.37%	0.102%
5	2.575	368	384	419	rVB4	1053211	1926625	30.99%	8.468%
6	2.896	479	484	487	rVB2	458	399	0.01%	0.002%
7	2.922	488	492	494	rBV	370	287	0.00%	0.001%
8	2.948	498	500	508	rVV2	641	565	0.01%	0.002%
9	3.041	523	529	539	rVV6	1364	2266	0.04%	0.010%
10	3.183	562	573	587	rBV2	3073	6427	0.10%	0.028%
11	3.353	612	626	642	rBV	34063	66133	1.06%	0.291%
12	3.453	652	657	660	rBV2	404	362	0.01%	0.002%
13	3.674	722	726	729	rVB2	473	333	0.01%	0.001%
14	3.867	768	786	815	rBV	762669	1803163	29.00%	7.925%
15	3.993	823	825	831	rVB3	671	516	0.01%	0.002%
16	4.086	852	854	862	rVB2	712	718	0.01%	0.003%
17	4.125	862	866	868	rBV2	453	374	0.01%	0.002%
18	4.269	905	911	915	rBV	331	373	0.01%	0.002%
19	4.510	982	986	989	rVB	395	284	0.00%	0.001%
20	4.620	1007	1020	1024	rBV	176752	322542	5.19%	1.418%
21	4.951	1119	1123	1129	rVB3	302	329	0.01%	0.001%
22	5.064	1141	1158	1184	rBV	265291	606867	9.76%	2.667%
23	5.211	1200	1204	1207	rVB2	402	350	0.01%	0.002%
24	5.314	1216	1236	1270	rBV	2764580	6217665	100.00%	27.328%
25	5.507	1289	1296	1298	rBV5	1685	1802	0.03%	0.008%
26	5.723	1342	1363	1383	rBV2	512227	1379903	22.19%	6.065%
27	5.935	1425	1429	1433	rVV3	302	309	0.00%	0.001%
28	5.957	1433	1436	1440	rVV5	402	390	0.01%	0.002%
29	5.986	1443	1445	1449	rVB	487	285	0.00%	0.001%
30	6.031	1455	1459	1460	rBV3	497	339	0.01%	0.001%
31	6.105	1477	1482	1485	rBV3	421	406	0.01%	0.002%
32	6.153	1493	1497	1500	rBV	490	299	0.00%	0.001%
33	6.250	1512	1527	1544	rBV	403240	756124	12.16%	3.323%
34	6.414	1576	1578	1581	rVB2	494	302	0.00%	0.001%
35	6.543	1602	1618	1634	rBV	523622	984953	15.84%	4.329%
36	6.690	1650	1664	1685	rBV	334158	648410	10.43%	2.850%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
 Data File : VU048976.D
 Acq On : 09 Jun 2022 13:56
 Operator : SY/MD
 Sample : N3248-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYW7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

37	6.768	1685	1688	1693	rVB5	934	650	0.01%	0.003%
38	6.973	1745	1752	1756	rBV3	707	919	0.01%	0.004%
39	7.028	1766	1769	1772	rBV	400	301	0.00%	0.001%
40	7.044	1772	1774	1779	rVV2	322	293	0.00%	0.001%
41	7.073	1779	1783	1788	rVV3	477	459	0.01%	0.002%
42	7.176	1811	1815	1822	rVB4	752	955	0.02%	0.004%
43	7.324	1859	1861	1865	rVB2	499	348	0.01%	0.002%
44	7.391	1877	1882	1883	rBV	316	283	0.00%	0.001%
45	7.462	1897	1904	1907	rBV	480	543	0.01%	0.002%
46	7.565	1923	1936	1953	rBV	195329	339840	5.47%	1.494%
47	7.684	1971	1973	1980	rVB5	1013	991	0.02%	0.004%
48	7.797	2005	2008	2011	rVB2	635	479	0.01%	0.002%
49	7.842	2018	2022	2025	rBV3	493	395	0.01%	0.002%
50	7.896	2025	2039	2059	rBV	648738	1112579	17.89%	4.890%
51	8.118	2105	2108	2115	rVB3	365	406	0.01%	0.002%
52	8.179	2115	2127	2142	rBV	138846	230393	3.71%	1.013%
53	8.311	2164	2168	2171	rBV2	639	584	0.01%	0.003%
54	8.346	2177	2179	2186	rVB3	707	657	0.01%	0.003%
55	8.401	2186	2196	2208	rVB2	22793	38159	0.61%	0.168%
56	8.469	2208	2217	2226	rBV2	5166	8653	0.14%	0.038%
57	8.552	2230	2243	2257	rBV	849598	1416765	22.79%	6.227%
58	8.632	2257	2268	2305	rVB	475361	867709	13.96%	3.814%
59	8.825	2326	2328	2332	rVB3	520	307	0.00%	0.001%
60	8.864	2336	2340	2343	rBV2	314	304	0.00%	0.001%
61	8.919	2355	2357	2365	rVB3	307	303	0.00%	0.001%
62	9.031	2389	2392	2396	rVB	387	303	0.00%	0.001%
63	9.057	2396	2400	2403	rBV3	329	347	0.01%	0.002%
64	9.169	2432	2435	2439	rVB2	356	278	0.00%	0.001%
65	9.340	2484	2488	2491	rBV2	412	316	0.01%	0.001%
66	9.417	2499	2512	2542	rBV	533639	898649	14.45%	3.950%
67	9.591	2565	2566	2572	rVB3	443	323	0.01%	0.001%
68	9.642	2578	2582	2590	rVB3	562	670	0.01%	0.003%
69	9.793	2624	2629	2633	rBV2	397	438	0.01%	0.002%
70	10.243	2766	2769	2775	rVB3	325	283	0.00%	0.001%
71	10.356	2800	2804	2805	rBV2	413	288	0.00%	0.001%
72	10.485	2839	2844	2851	rVB2	584	602	0.01%	0.003%
73	10.639	2889	2892	2897	rVB4	747	642	0.01%	0.003%
74	10.758	2913	2929	2948	rBV	486981	799434	12.86%	3.514%
75	10.896	2963	2972	2983	rVB3	7687	13239	0.21%	0.058%
76	10.957	2986	2991	2995	rBV2	525	560	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
 Data File : VU048976.D
 Acq On : 09 Jun 2022 13:56
 Operator : SY/MD
 Sample : N3248-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYW7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

77	11.021	3005	3011	3014	rBV	533	514	0.01%	0.002%
78	11.086	3025	3031	3034	rBV3	475	476	0.01%	0.002%
79	11.221	3071	3073	3082	rVB2	331	435	0.01%	0.002%
80	11.468	3144	3150	3158	rBV3	752	992	0.02%	0.004%
81	11.751	3232	3238	3240	rVV3	776	696	0.01%	0.003%
82	11.812	3244	3257	3281	rVV	537234	853655	13.73%	3.752%
83	11.899	3281	3284	3289	rVB4	1337	1199	0.02%	0.005%
84	12.144	3356	3360	3362	rVB2	432	300	0.00%	0.001%
85	12.192	3362	3375	3399	rBV	613904	1012194	16.28%	4.449%
86	12.465	3456	3460	3463	rVB2	501	333	0.01%	0.001%
87	12.774	3548	3556	3566	rVB3	3192	4764	0.08%	0.021%
88	12.886	3587	3591	3594	rBV2	524	402	0.01%	0.002%
89	13.015	3626	3631	3634	rBV2	573	572	0.01%	0.003%
90	13.134	3662	3668	3675	rBV2	431	724	0.01%	0.003%
91	13.237	3695	3700	3706	rVB3	506	598	0.01%	0.003%
92	13.381	3739	3745	3747	rBV2	593	602	0.01%	0.003%
93	13.491	3776	3779	3784	rVB3	483	383	0.01%	0.002%
94	13.793	3870	3873	3876	rBV2	428	326	0.01%	0.001%
95	13.844	3887	3889	3893	rBV4	460	415	0.01%	0.002%
96	14.095	3964	3967	3976	rBV5	1323	1732	0.03%	0.008%
97	14.246	4011	4014	4018	rBV	404	300	0.00%	0.001%
98	14.343	4037	4044	4047	rBV4	1057	1395	0.02%	0.006%
99	15.623	4440	4442	4445	rBV2	827	476	0.01%	0.002%
100	15.996	4556	4558	4562	rBV2	911	560	0.01%	0.002%




Sum of corrected areas: 22751642

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
Data File : VU048976.D
Acq On : 09 Jun 2022 13:56
Operator : SY/MD
Sample : N3248-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYW7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

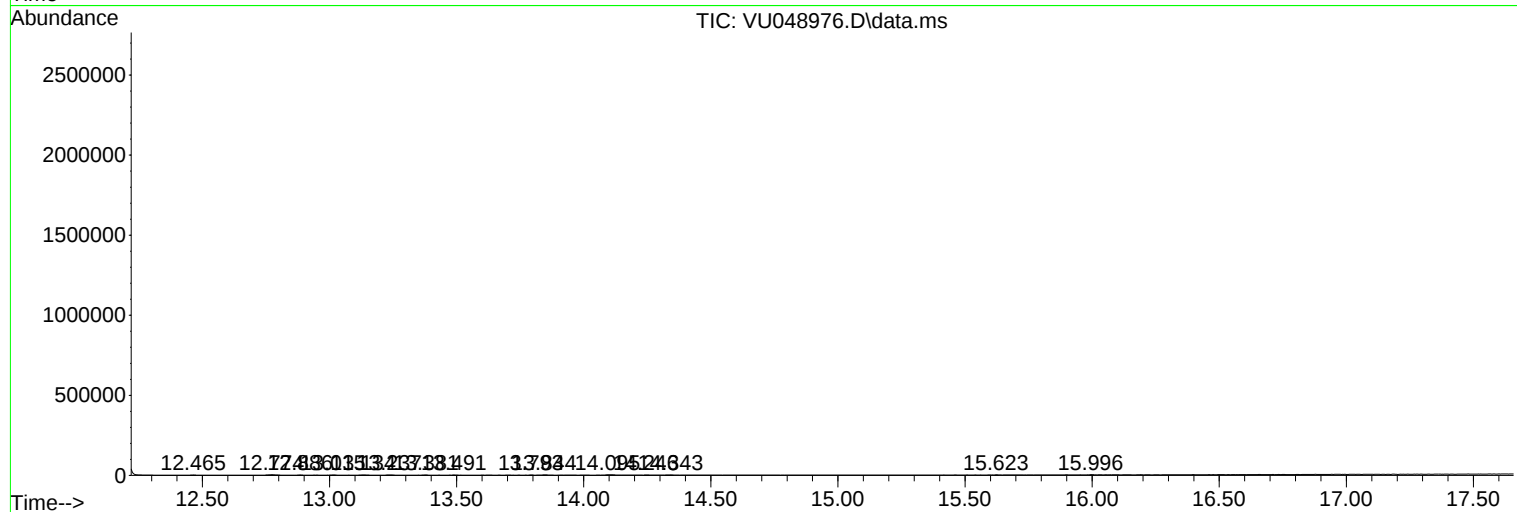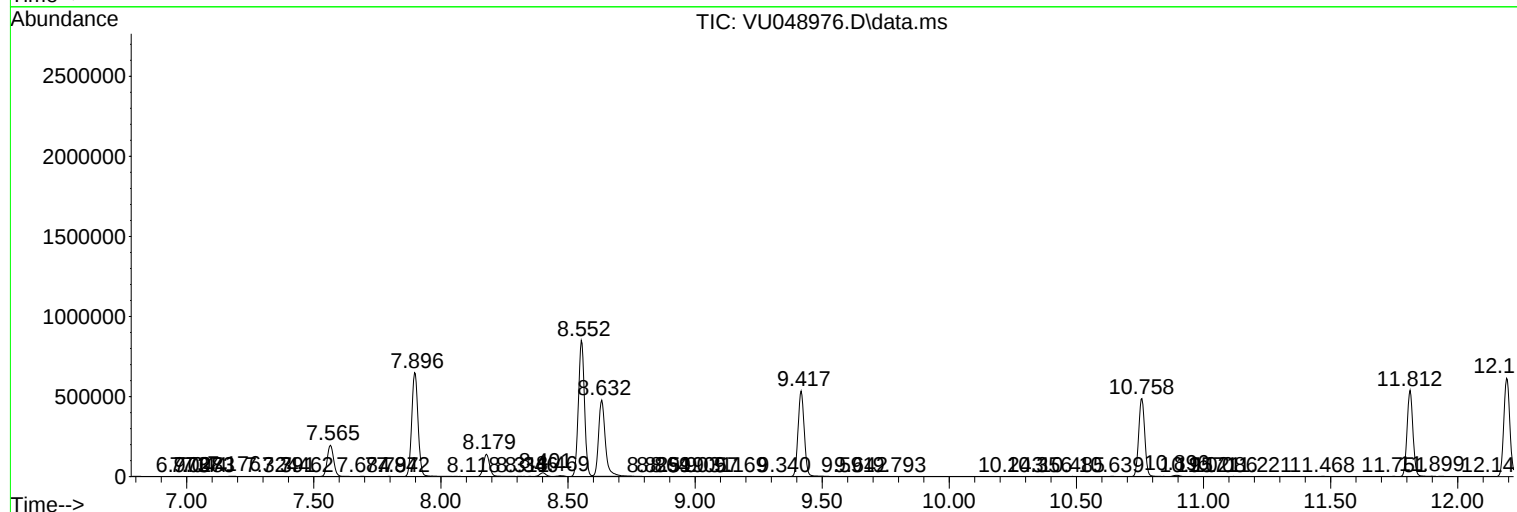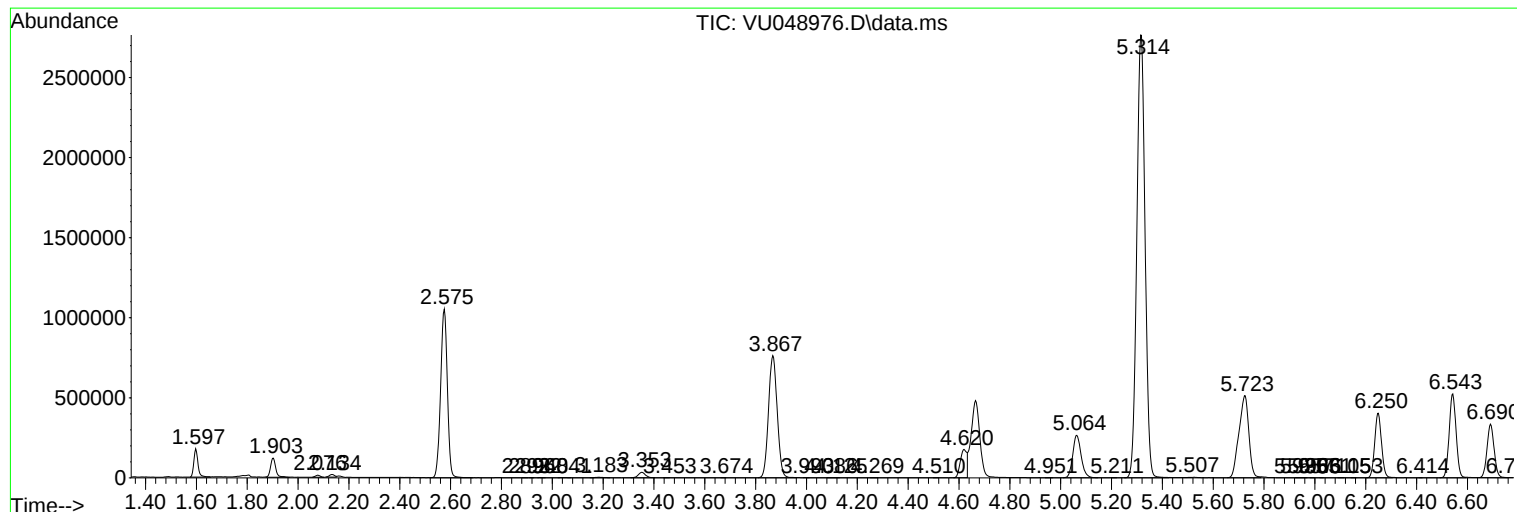

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
Data File : VU048976.D
Acq On : 09 Jun 2022 13:56
Operator : SY/MD
Sample : N3248-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYW7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
Data File : VU048976.D
Acq On : 09 Jun 2022 13:56
Operator : SY/MD
Sample : N3248-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYW7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc