

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
 Data File : VU048977.D
 Acq On : 09 Jun 2022 14:20
 Operator : SY/MD
 Sample : N3248-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYW8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

Signal : TIC: VU048977.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	100	rBV	149397	173940	3.13%	0.824%
2	1.893	164	172	186	rVB	106340	144668	2.60%	0.686%
3	2.572	368	383	412	rVB4	905354	1660783	29.86%	7.871%
4	2.819	459	460	463	rVB	479	121	0.00%	0.001%
5	2.851	467	470	474	rBV2	318	262	0.00%	0.001%
6	2.906	484	487	493	rVB3	427	307	0.01%	0.001%
7	2.951	497	501	504	rBV2	500	422	0.01%	0.002%
8	3.109	545	550	553	rBV2	425	382	0.01%	0.002%
9	3.182	564	573	588	rVB3	2572	6146	0.11%	0.029%
10	3.250	588	594	599	rBV2	315	450	0.01%	0.002%
11	3.289	603	606	610	rVV	371	265	0.00%	0.001%
12	3.353	610	626	644	rVV2	30524	61169	1.10%	0.290%
13	3.414	644	645	648	rVB	576	261	0.00%	0.001%
14	3.433	648	651	655	rVB	151	117	0.00%	0.001%
15	3.459	655	659	662	rBV	338	253	0.00%	0.001%
16	3.604	699	704	706	rBV	232	222	0.00%	0.001%
17	3.710	734	737	740	rBV	314	201	0.00%	0.001%
18	3.867	765	786	820	rBV	696104	1656467	29.78%	7.850%
19	4.099	854	858	861	rBV2	618	400	0.01%	0.002%
20	4.215	890	894	897	rBV	422	347	0.01%	0.002%
21	4.317	923	926	929	rVB2	271	145	0.00%	0.001%
22	4.340	929	933	935	rBV	290	169	0.00%	0.001%
23	4.359	937	939	943	rVB	353	151	0.00%	0.001%
24	4.404	950	953	961	rVB2	458	558	0.01%	0.003%
25	4.462	961	971	974	rBV2	427	633	0.01%	0.003%
26	4.523	988	990	994	rVB	325	167	0.00%	0.001%
27	4.549	994	998	1005	rBV2	289	313	0.01%	0.001%
28	4.623	1005	1021	1024	rBV	170993	316660	5.69%	1.501%
29	5.063	1141	1158	1184	rBV	254702	583022	10.48%	2.763%
30	5.208	1200	1203	1205	rVB2	429	229	0.00%	0.001%
31	5.314	1212	1236	1266	rBV	2487961	5561637	100.00%	26.357%
32	5.571	1315	1316	1321	rVB3	374	300	0.01%	0.001%
33	5.723	1341	1363	1384	rBV2	484972	1319005	23.72%	6.251%
34	5.970	1434	1440	1443	rBV3	1176	1237	0.02%	0.006%
35	6.044	1459	1463	1467	rBV3	600	531	0.01%	0.003%
36	6.173	1498	1503	1508	rBV4	535	589	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
 Data File : VU048977.D
 Acq On : 09 Jun 2022 14:20
 Operator : SY/MD
 Sample : N3248-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYW8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

37	6.247	1513	1526	1545	rBV	394141	731383	13.15%	3.466%
38	6.366	1560	1563	1570	rVB3	415	396	0.01%	0.002%
39	6.398	1570	1573	1576	rBV2	400	296	0.01%	0.001%
40	6.539	1603	1617	1635	rBV	468096	879412	15.81%	4.168%
41	6.690	1650	1664	1681	rBV	323357	622645	11.20%	2.951%
42	6.829	1706	1707	1712	rVB2	296	125	0.00%	0.001%
43	6.922	1735	1736	1738	rVB2	383	108	0.00%	0.001%
44	6.973	1745	1752	1758	rBV3	1165	1296	0.02%	0.006%
45	7.002	1758	1761	1762	rBV	215	142	0.00%	0.001%
46	7.044	1770	1774	1776	rBV3	245	209	0.00%	0.001%
47	7.144	1798	1805	1806	rBV2	491	380	0.01%	0.002%
48	7.237	1831	1834	1836	rBV2	230	155	0.00%	0.001%
49	7.250	1836	1838	1841	rVV2	318	183	0.00%	0.001%
50	7.269	1841	1844	1847	rVB2	343	189	0.00%	0.001%
51	7.420	1889	1891	1892	rBV	203	91	0.00%	0.000%
52	7.501	1914	1916	1921	rBV3	254	188	0.00%	0.001%
53	7.565	1923	1936	1956	rBV	189911	327203	5.88%	1.551%
54	7.690	1969	1975	1984	rVB5	936	1263	0.02%	0.006%
55	7.793	2002	2007	2010	rBV3	714	537	0.01%	0.003%
56	7.896	2024	2039	2058	rBV	614182	1050554	18.89%	4.979%
57	8.124	2108	2110	2115	rVB2	315	187	0.00%	0.001%
58	8.179	2115	2127	2141	rBV	131442	217606	3.91%	1.031%
59	8.401	2185	2196	2208	rBV	22970	37592	0.68%	0.178%
60	8.552	2230	2243	2257	rBV	746317	1255645	22.58%	5.951%
61	8.632	2257	2268	2301	rVB	506273	913735	16.43%	4.330%
62	8.851	2335	2336	2337	rBV	260	89	0.00%	0.000%
63	8.899	2348	2351	2356	rVB3	551	493	0.01%	0.002%
64	8.922	2356	2358	2360	rBV	297	157	0.00%	0.001%
65	9.070	2401	2404	2407	rVB2	355	245	0.00%	0.001%
66	9.105	2411	2415	2417	rBV2	286	241	0.00%	0.001%
67	9.169	2433	2435	2438	rBV2	300	152	0.00%	0.001%
68	9.198	2442	2444	2448	rVB2	346	197	0.00%	0.001%
69	9.253	2458	2461	2463	rBV2	338	200	0.00%	0.001%
70	9.321	2479	2482	2487	rVB2	445	328	0.01%	0.002%
71	9.417	2498	2512	2531	rBV	544056	892472	16.05%	4.229%
72	9.623	2573	2576	2577	rBV	261	130	0.00%	0.001%
73	9.693	2595	2598	2602	rBV	408	338	0.01%	0.002%
74	9.755	2613	2617	2619	rBV2	537	379	0.01%	0.002%
75	9.874	2650	2654	2655	rBV	340	174	0.00%	0.001%
76	9.890	2655	2659	2664	rVV2	262	288	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
 Data File : VU048977.D
 Acq On : 09 Jun 2022 14:20
 Operator : SY/MD
 Sample : N3248-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXYW8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
 Title : VOC Analysis

77	10.041	2702	2706	2709	rBV	372	293	0.01%	0.001%
78	10.057	2709	2711	2712	rBV	366	171	0.00%	0.001%
79	10.102	2719	2725	2729	rBV4	760	899	0.02%	0.004%
80	10.173	2741	2747	2750	rBV2	241	269	0.00%	0.001%
81	10.237	2765	2767	2774	rVB2	465	258	0.00%	0.001%
82	10.269	2774	2777	2779	rBV	286	189	0.00%	0.001%
83	10.346	2799	2801	2804	rVB2	339	153	0.00%	0.001%
84	10.407	2817	2820	2824	rVB2	159	104	0.00%	0.000%
85	10.427	2824	2826	2829	rVB2	223	104	0.00%	0.000%
86	10.446	2829	2832	2834	rBV2	225	169	0.00%	0.001%
87	10.468	2835	2839	2840	rBV2	311	213	0.00%	0.001%
88	10.597	2877	2879	2884	rBV2	239	173	0.00%	0.001%
89	10.758	2916	2929	2953	rVB	488803	795949	14.31%	3.772%
90	10.893	2960	2971	2986	rVB5	8998	15409	0.28%	0.073%
91	11.285	3091	3093	3097	rBV2	328	180	0.00%	0.001%
92	11.420	3132	3135	3138	rBV2	358	255	0.00%	0.001%
93	11.661	3206	3210	3213	rBV	360	240	0.00%	0.001%
94	11.748	3230	3237	3242	rBV5	919	1317	0.02%	0.006%
95	11.812	3245	3257	3277	rVV	531500	843595	15.17%	3.998%
96	11.992	3311	3313	3315	rBV2	298	139	0.00%	0.001%
97	12.031	3321	3325	3328	rBV	433	427	0.01%	0.002%
98	12.192	3363	3375	3400	rBV	627618	1010326	18.17%	4.788%
99	13.172	3677	3680	3683	rBV2	600	433	0.01%	0.002%
100	13.279	3712	3713	3714	rBV	500	138	0.00%	0.001%




Sum of corrected areas: 21101335

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
Data File : VU048977.D
Acq On : 09 Jun 2022 14:20
Operator : SY/MD
Sample : N3248-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYW8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

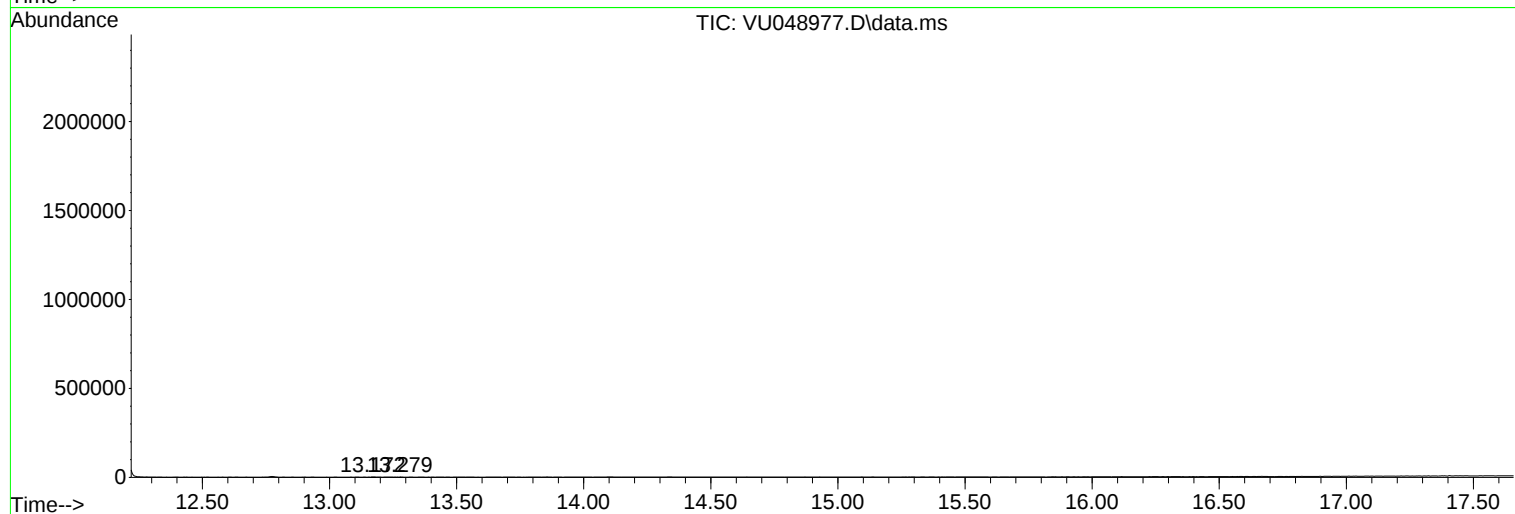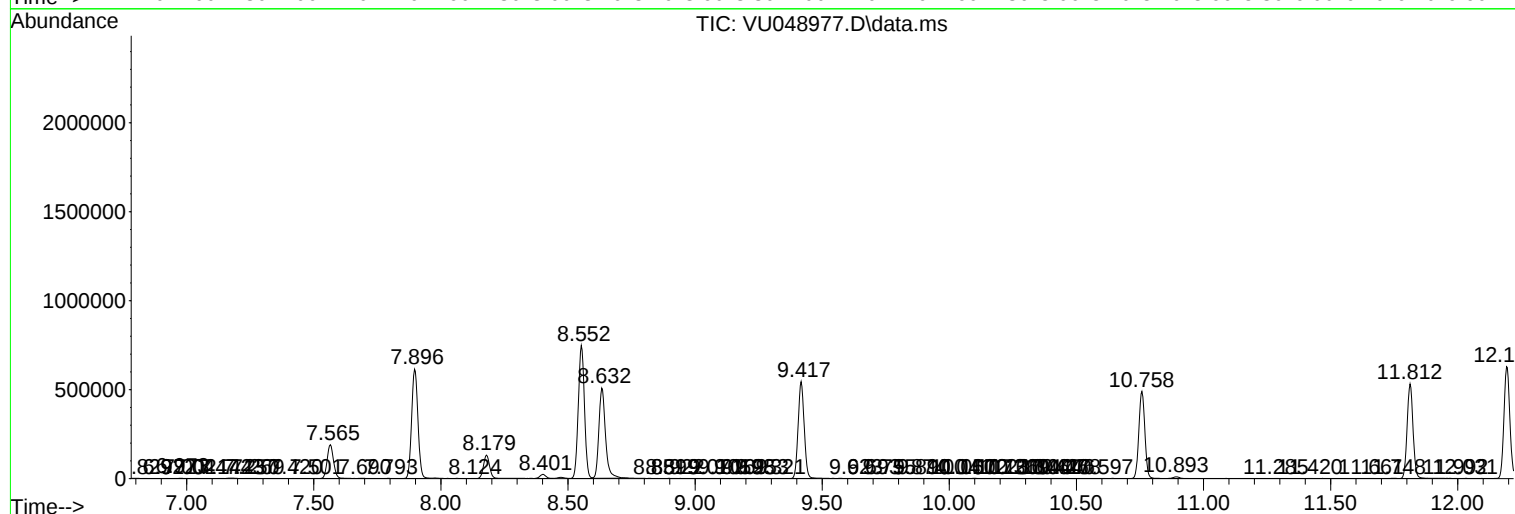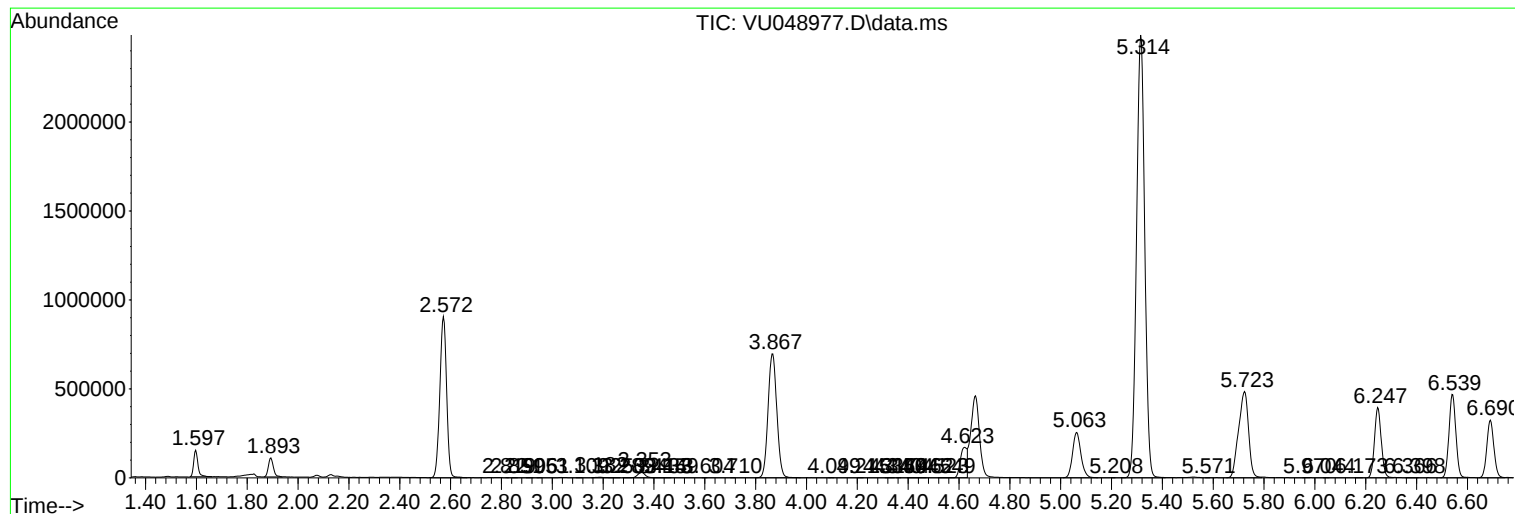

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
Data File : VU048977.D
Acq On : 09 Jun 2022 14:20
Operator : SY/MD
Sample : N3248-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYW8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU060922\
Data File : VU048977.D
Acq On : 09 Jun 2022 14:20
Operator : SY/MD
Sample : N3248-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXYW8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM051622WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------